

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028605.D
 Acq On : 14 Nov 2023 16:35
 Operator : MA/JU
 Sample : 05281-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	27	rVB3	69372	140740	1.44%	0.209%
2	3.581	80	84	91	rBV2	38720	95452	0.98%	0.142%
3	4.987	318	323	335	rBV	26527	65942	0.68%	0.098%
4	6.934	644	654	661	rBV2	35197	136423	1.40%	0.203%
5	7.040	667	672	699	rBV	383511	1140630	11.70%	1.694%
6	7.234	699	705	739	rVB	447140	1271387	13.04%	1.888%
7	7.705	778	785	813	rBV	239427	803714	8.24%	1.193%
8	8.434	902	909	928	rBV3	137616	706752	7.25%	1.049%
9	8.863	975	982	1004	rBV	595405	1758968	18.04%	2.612%
10	9.581	1097	1104	1135	rBV	440495	1353522	13.88%	2.010%
11	10.122	1189	1196	1217	rBV	495192	1652220	16.94%	2.453%
12	10.487	1252	1258	1280	rBV	614139	1429467	14.66%	2.122%
13	10.652	1280	1286	1317	rVV	323678	1392199	14.28%	2.067%
14	11.722	1461	1468	1474	rBV10	11720	27282	0.28%	0.041%
15	11.781	1474	1478	1487	rVB10	7978	22778	0.23%	0.034%
16	12.728	1634	1639	1648	rBV	16732	38430	0.39%	0.057%
17	13.257	1721	1729	1738	rBV2	27907	50322	0.52%	0.075%
18	13.663	1788	1798	1807	rBV3	18901	41577	0.43%	0.062%
19	13.763	1809	1815	1838	rBV	3117661	5013423	51.41%	7.444%
20	14.034	1854	1861	1888	rBV	3362505	5708453	58.54%	8.475%
21	14.346	1907	1914	1936	rVV	1296077	2211948	22.68%	3.284%
22	15.169	2049	2054	2061	rBV4	23045	40469	0.42%	0.060%
23	15.340	2077	2083	2100	rBV	4331591	7369306	75.57%	10.941%
24	15.463	2100	2104	2122	rVB	757494	1508816	15.47%	2.240%
25	15.793	2156	2160	2165	rVB	18619	29877	0.31%	0.044%
26	16.428	2265	2268	2272	rVB4	13721	17041	0.17%	0.025%
27	16.975	2357	2361	2367	rBV4	19343	27805	0.29%	0.041%
28	17.092	2375	2381	2392	rBV	1329376	2429589	24.92%	3.607%
29	17.192	2392	2398	2431	rVB	4801619	8214159	84.24%	12.196%
30	17.528	2453	2455	2460	rVB6	9471	10552	0.11%	0.016%
31	18.510	2619	2622	2625	rBV4	7814	10507	0.11%	0.016%
32	19.063	2711	2716	2723	rBV3	61721	105028	1.08%	0.156%
33	19.139	2725	2729	2733	rVV	36755	56148	0.58%	0.083%
34	19.498	2784	2790	2812	rBV2	6626843	9751043	100.00%	14.478%
35	21.310	3093	3098	3114	rBV	1143163	2336809	23.96%	3.470%
36	23.457	3456	3463	3475	rBV2	3791729	8060838	82.67%	11.968%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028605.D
Acq On : 14 Nov 2023 16:35
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	23.604	3483	3488	3502	rVB	1069518	2322953	23.82%	3.449%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 67352569

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028605.D
Acq On : 14 Nov 2023 16:35
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

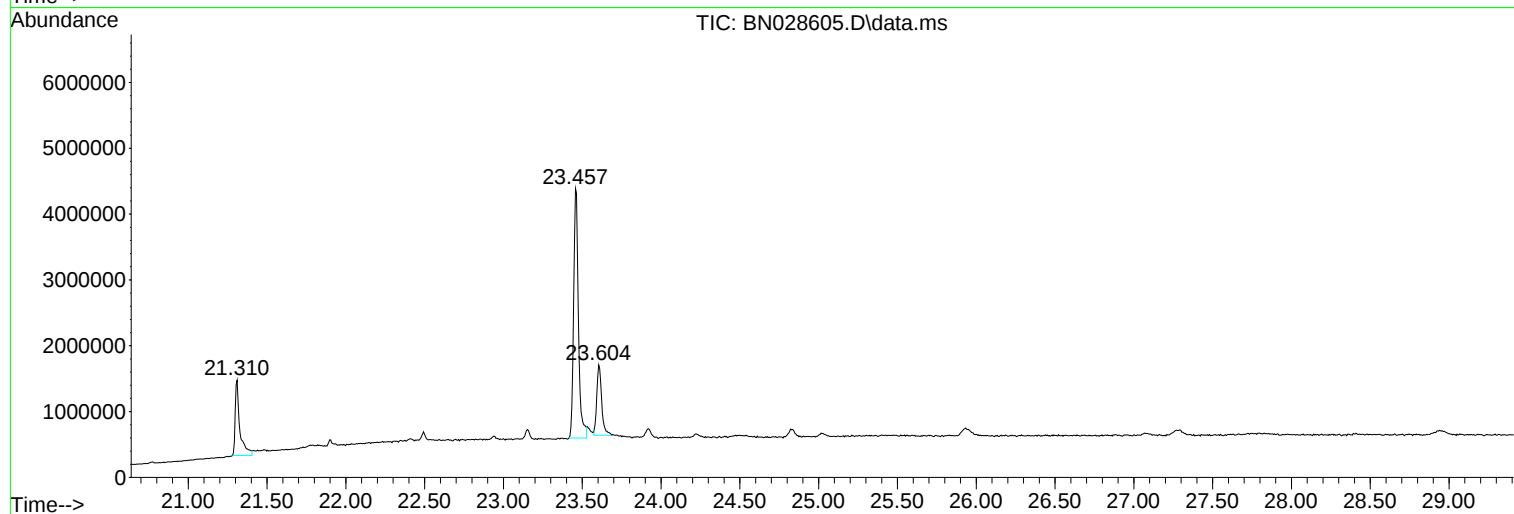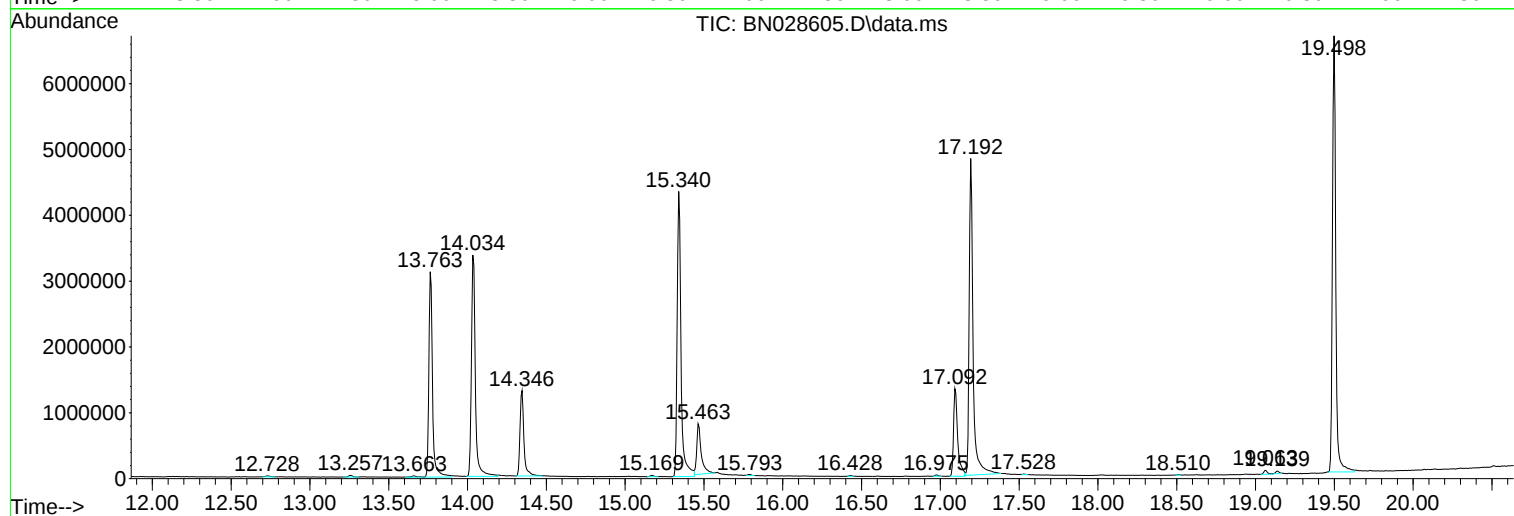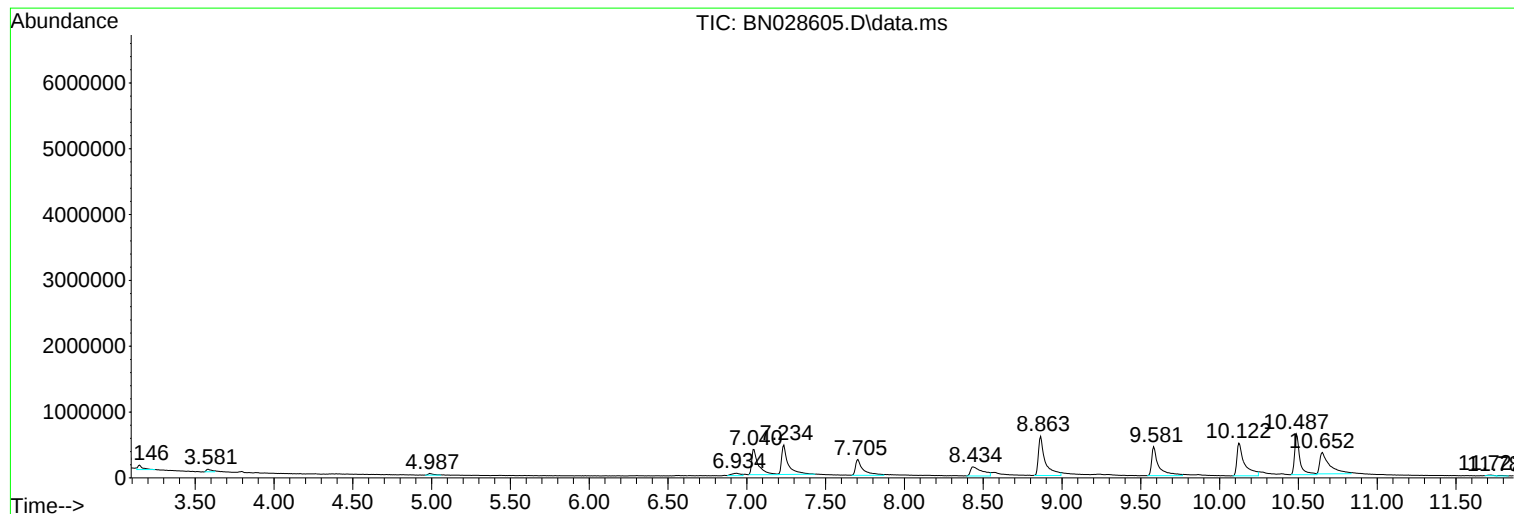

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028605.D
Acq On : 14 Nov 2023 16:35
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028605.D
Acq On : 14 Nov 2023 16:35
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc