

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028606.D
 Acq On : 14 Nov 2023 17:11
 Operator : MA/JU
 Sample : 05281-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	17	rVB	43993	62303	0.70%	0.102%
2	3.575	80	83	94	rBV	45155	134383	1.50%	0.220%
3	3.793	117	120	124	rVB3	16401	23491	0.26%	0.038%
4	4.381	215	220	221	rBV2	14107	20864	0.23%	0.034%
5	4.993	319	324	327	rBV6	9962	17270	0.19%	0.028%
6	6.869	636	643	647	rBV4	21312	54755	0.61%	0.090%
7	6.934	649	654	659	rVB6	13971	38299	0.43%	0.063%
8	7.046	667	673	695	rBV	274063	872390	9.75%	1.428%
9	7.234	699	705	738	rVB	323352	962577	10.76%	1.576%
10	7.705	777	785	810	rBV	231015	773290	8.64%	1.266%
11	8.440	902	910	928	rBV3	92489	511433	5.72%	0.837%
12	8.863	975	982	1015	rBV	433413	1532941	17.13%	2.509%
13	9.299	1051	1056	1067	rVB3	25010	59131	0.66%	0.097%
14	9.581	1098	1104	1134	rBV	312181	1035140	11.57%	1.694%
15	10.122	1188	1196	1215	rBV	356259	1236910	13.83%	2.025%
16	10.487	1252	1258	1279	rBV	602669	1411374	15.78%	2.310%
17	10.651	1279	1286	1307	rBV	309820	1260797	14.09%	2.064%
18	11.722	1462	1468	1474	rBV7	10936	26203	0.29%	0.043%
19	11.787	1477	1479	1486	rVB7	8609	13095	0.15%	0.021%
20	12.734	1630	1640	1651	rBV2	20911	55805	0.62%	0.091%
21	13.257	1723	1729	1735	rBV2	29751	55164	0.62%	0.090%
22	13.663	1793	1798	1802	rBV3	17747	30215	0.34%	0.049%
23	13.763	1809	1815	1847	rBV	2760353	4447629	49.71%	7.280%
24	14.034	1855	1861	1889	rBV	2852648	4938476	55.20%	8.083%
25	14.345	1907	1914	1933	rBV	1331031	2269305	25.37%	3.714%
26	14.763	1981	1985	1991	rVB9	4068	9754	0.11%	0.016%
27	15.169	2049	2054	2059	rBV3	19760	34212	0.38%	0.056%
28	15.339	2077	2083	2099	rBV	3725079	6291188	70.32%	10.298%
29	15.463	2099	2104	2122	rVB	623134	1300285	14.53%	2.128%
30	15.786	2156	2159	2168	rVB2	18867	32819	0.37%	0.054%
31	16.434	2264	2269	2273	rVB5	11454	17460	0.20%	0.029%
32	16.781	2325	2328	2331	rBV5	7134	9129	0.10%	0.015%
33	16.975	2357	2361	2369	rVB6	15066	26110	0.29%	0.043%
34	17.092	2375	2381	2392	rBV	1420180	2575404	28.79%	4.216%
35	17.192	2392	2398	2426	rVB	4106758	7217573	80.68%	11.814%
36	17.528	2453	2455	2464	rVB9	14873	28017	0.31%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028606.D
Acq On : 14 Nov 2023 17:11
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	18.028	2537	2540	2541	rBV3	11332	11705	0.13%	0.019%
38	19.063	2712	2716	2722	rBV2	57363	86855	0.97%	0.142%
39	19.139	2725	2729	2736	rVV3	35590	65105	0.73%	0.107%
40	19.451	2780	2782	2784	rBV2	23730	24141	0.27%	0.040%
41	19.498	2784	2790	2809	rVV	6058138	8946288	100.00%	14.644%
42	21.310	3093	3098	3110	rBV	1427794	2519861	28.17%	4.125%
43	23.463	3457	3464	3474	rBV2	3612788	7391060	82.62%	12.098%
44	23.604	3483	3488	3506	rVB	1164227	2663464	29.77%	4.360%




Sum of corrected areas: 61093670

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028606.D
Acq On : 14 Nov 2023 17:11
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

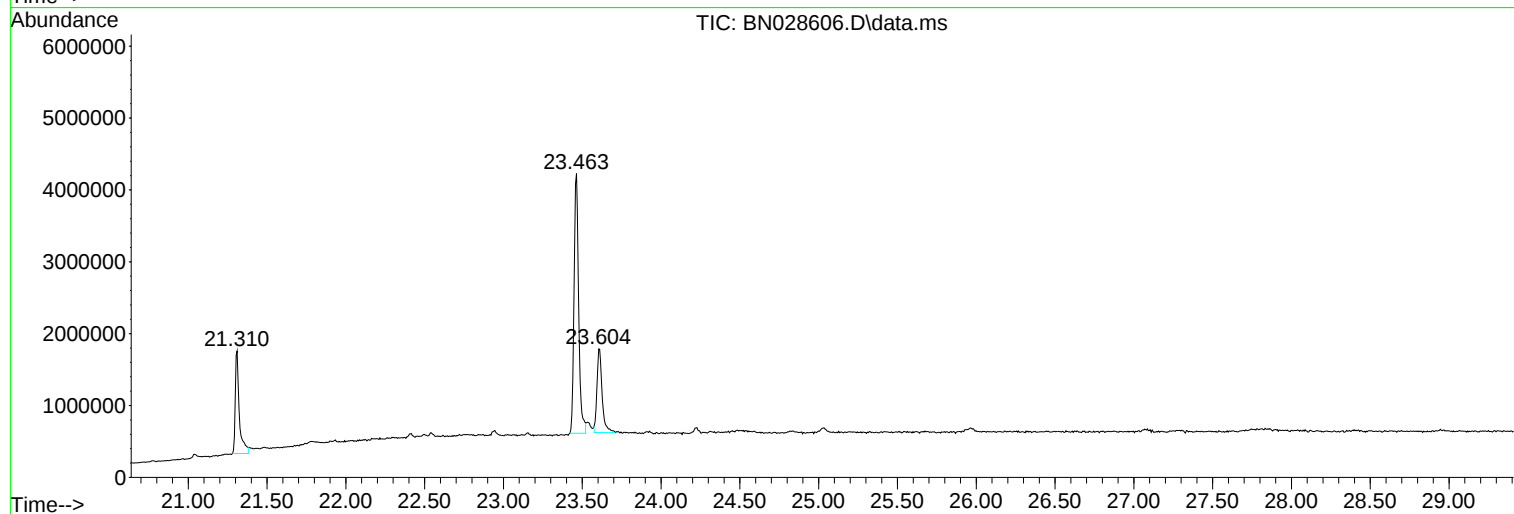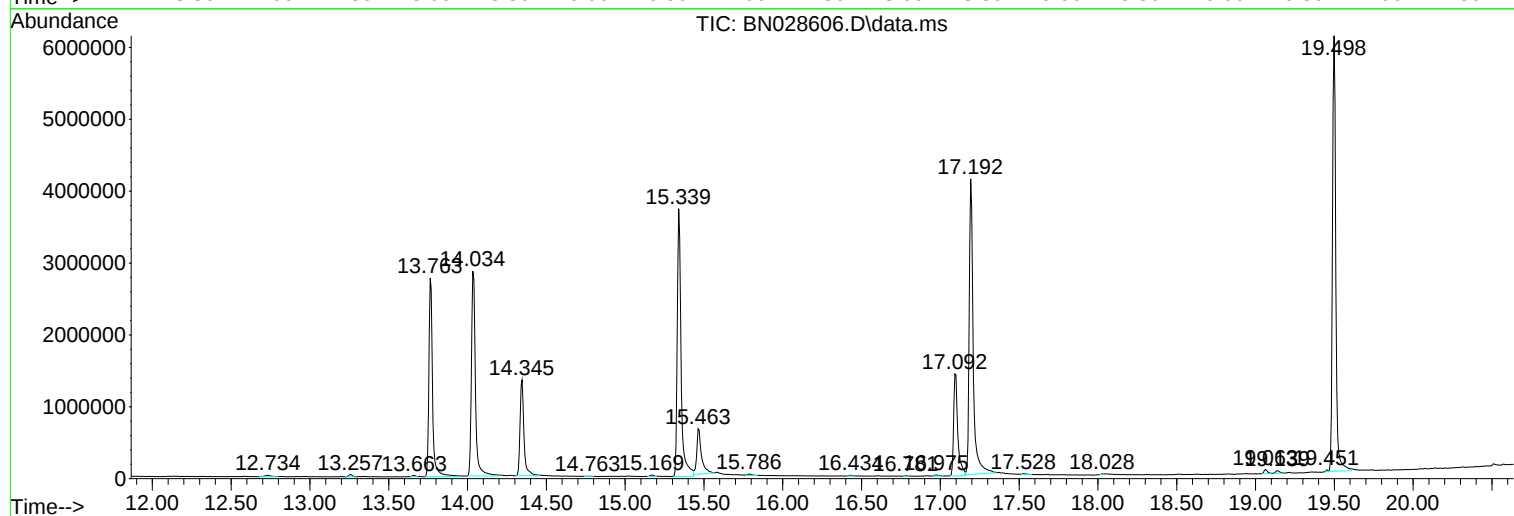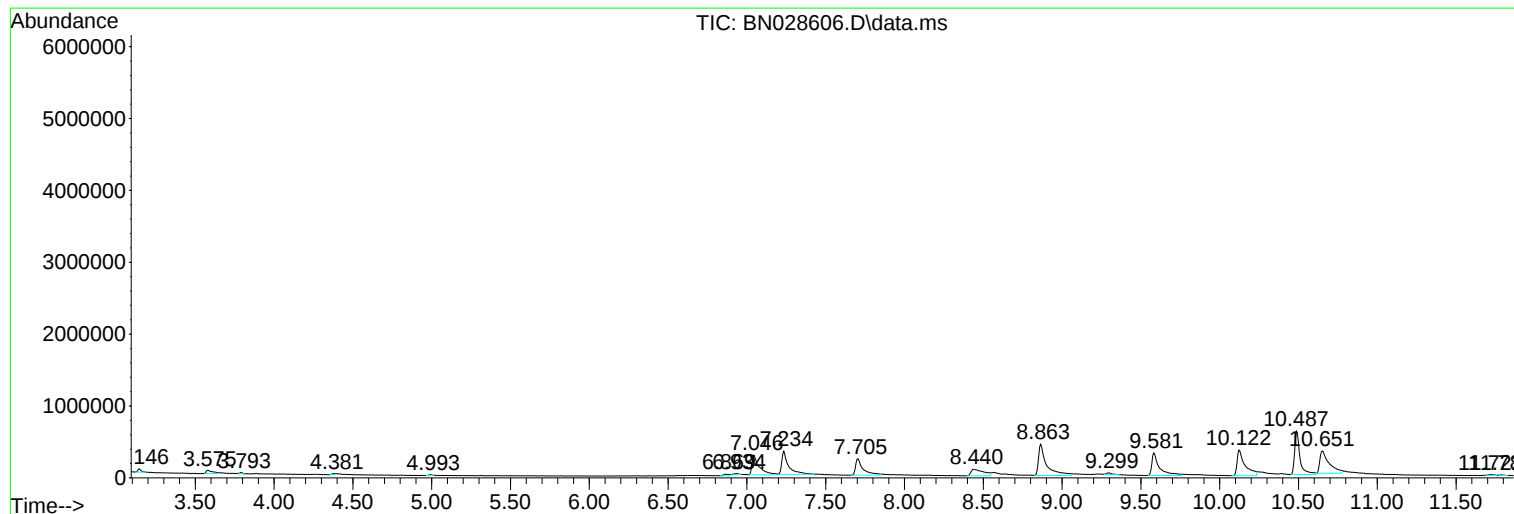

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028606.D
Acq On : 14 Nov 2023 17:11
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028606.D
Acq On : 14 Nov 2023 17:11
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc