

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028607.D
 Acq On : 14 Nov 2023 17:47
 Operator : MA/JU
 Sample : 05281-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	14	rBV	35244	39985	0.46%	0.062%
2	3.575	79	83	96	rBV	59576	186195	2.15%	0.291%
3	4.993	319	324	332	rBV2	22757	49835	0.58%	0.078%
4	5.693	440	443	448	rBV5	5609	10824	0.13%	0.017%
5	6.310	543	548	553	rBV7	4799	9861	0.11%	0.015%
6	6.928	645	653	660	rBV2	24578	86974	1.00%	0.136%
7	7.046	667	673	696	rBV	280056	888932	10.27%	1.387%
8	7.234	699	705	734	rVV	351771	989890	11.43%	1.545%
9	7.699	778	784	812	rBV	377007	1153548	13.32%	1.800%
10	8.440	901	910	927	rBV3	90782	491707	5.68%	0.767%
11	8.863	976	982	1018	rBV	447855	1523386	17.59%	2.377%
12	9.228	1038	1044	1050	rBV8	7947	20473	0.24%	0.032%
13	9.581	1097	1104	1132	rBV	328434	1059987	12.24%	1.654%
14	10.122	1190	1196	1218	rBV	362665	1318304	15.23%	2.057%
15	10.487	1251	1258	1280	rBV	939221	2074294	23.96%	3.237%
16	10.651	1280	1286	1326	rVB	240919	1182462	13.66%	1.845%
17	11.716	1461	1467	1473	rBV7	10004	23941	0.28%	0.037%
18	11.787	1475	1479	1485	rVB9	6437	11466	0.13%	0.018%
19	12.728	1632	1639	1650	rVB3	15734	41385	0.48%	0.065%
20	13.257	1724	1729	1734	rBV	25500	42919	0.50%	0.067%
21	13.657	1793	1797	1803	rVB3	14254	24512	0.28%	0.038%
22	13.763	1809	1815	1844	rBV	2740875	4343129	50.16%	6.777%
23	14.034	1855	1861	1885	rBV	2859203	4732550	54.66%	7.385%
24	14.345	1907	1914	1931	rBV	1875614	3186361	36.80%	4.972%
25	15.169	2049	2054	2060	rBV4	17848	31216	0.36%	0.049%
26	15.339	2077	2083	2099	rBV	3653809	6272876	72.45%	9.788%
27	15.463	2099	2104	2121	rVB	638133	1296941	14.98%	2.024%
28	15.786	2156	2159	2168	rVB2	17501	31931	0.37%	0.050%
29	16.428	2264	2268	2275	rVB4	10898	16852	0.19%	0.026%
30	16.780	2324	2328	2336	rVB4	6375	14445	0.17%	0.023%
31	16.975	2356	2361	2370	rBV8	19880	34101	0.39%	0.053%
32	17.092	2375	2381	2393	rBV	2046446	3546132	40.96%	5.533%
33	17.192	2393	2398	2438	rVB	4114365	7352329	84.92%	11.472%
34	18.086	2548	2550	2557	rVB5	11005	13146	0.15%	0.021%
35	18.516	2619	2623	2626	rBV5	7682	12296	0.14%	0.019%
36	19.063	2712	2716	2724	rBV2	49059	76078	0.88%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028607.D
Acq On : 14 Nov 2023 17:47
Operator : MA/JU
Sample : 05281-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.139	2725	2729	2737	rVV	31941	56290	0.65%	0.088%
38	19.451	2780	2782	2784	rBV2	13705	13778	0.16%	0.021%
39	19.498	2784	2790	2815	rVV	6018515	8658126	100.00%	13.510%
40	21.310	3093	3098	3110	rBV	1820032	3193147	36.88%	4.983%
41	23.457	3456	3463	3473	rBV	3417848	6949812	80.27%	10.844%
42	23.604	3482	3488	3498	rVB	1447065	3024226	34.93%	4.719%




Sum of corrected areas: 64086642

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028607.D
Acq On : 14 Nov 2023 17:47
Operator : MA/JU
Sample : 05281-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

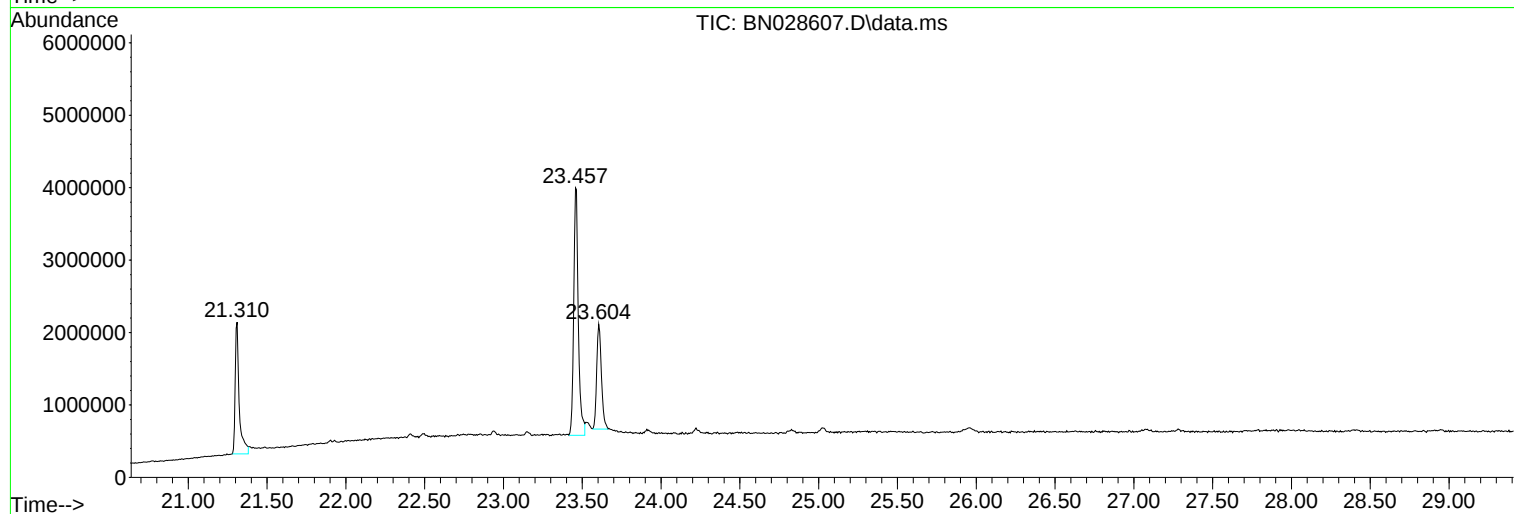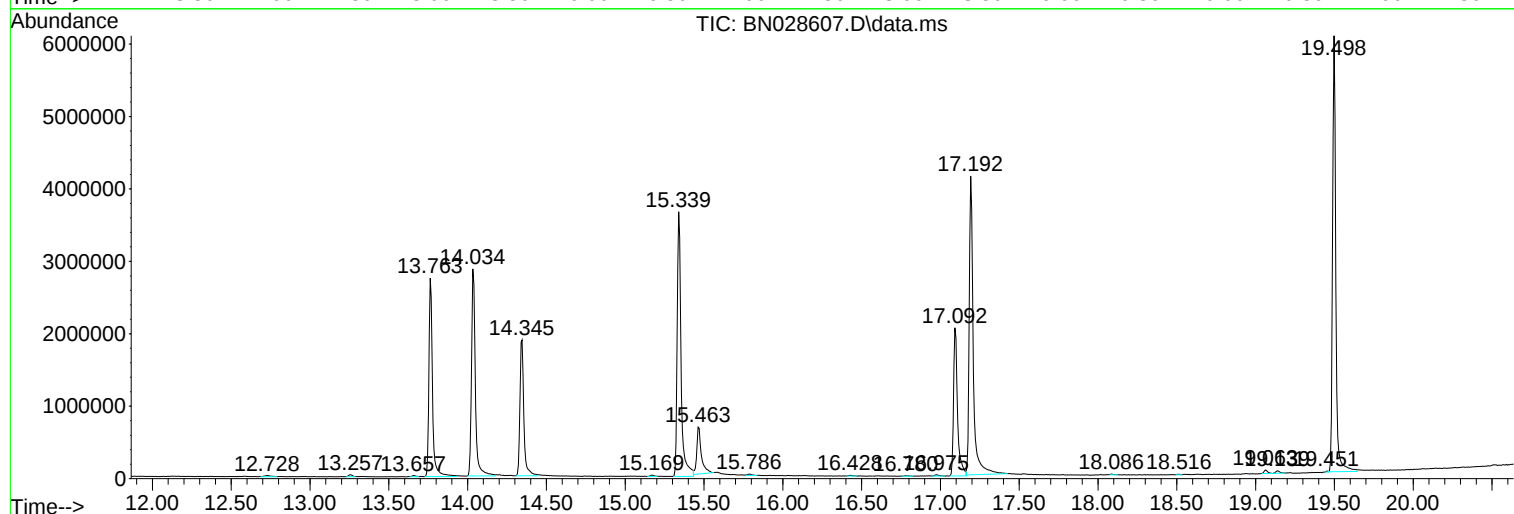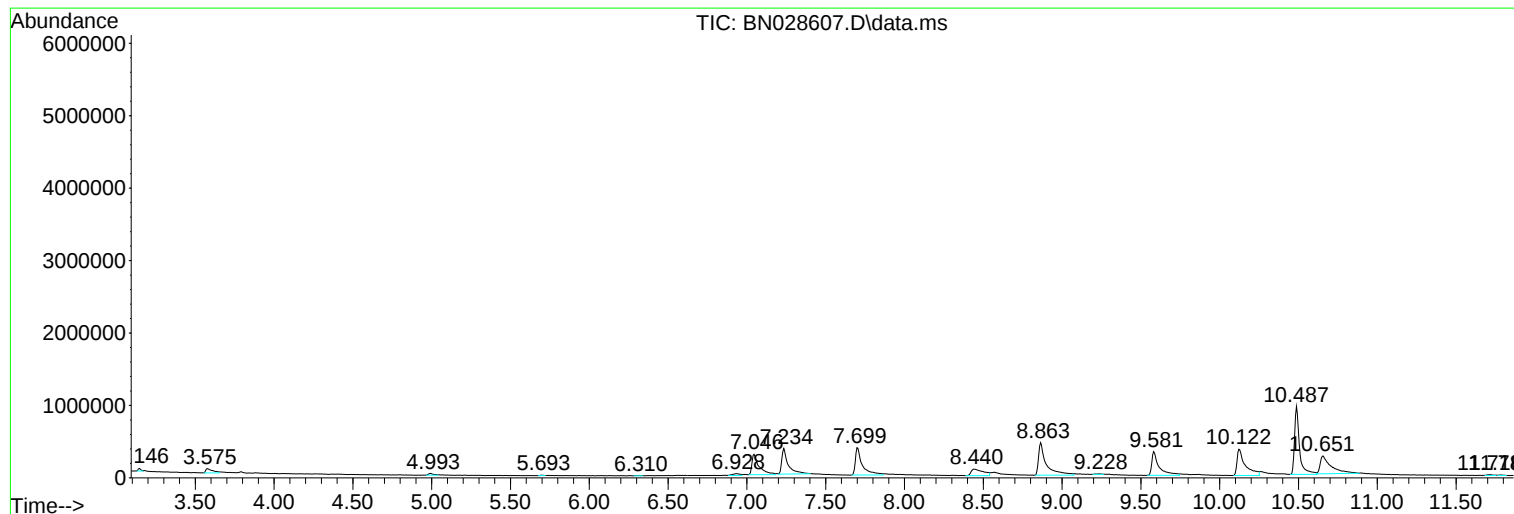

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028607.D
Acq On : 14 Nov 2023 17:47
Operator : MA/JU
Sample : 05281-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028607.D
Acq On : 14 Nov 2023 17:47
Operator : MA/JU
Sample : 05281-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc