

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028611.D
 Acq On : 14 Nov 2023 20:47
 Operator : MA/JU
 Sample : PB157093BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK093

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	20	rVB	68015	109226	1.57%	0.176%
2	3.564	77	81	99	rBV	282932	748594	10.78%	1.209%
3	6.887	639	646	667	rBV	298845	1218123	17.54%	1.968%
4	7.040	667	672	697	rVV	379866	1149643	16.56%	1.857%
5	7.228	698	704	735	rVB	575453	1511181	21.76%	2.441%
6	7.699	778	784	816	rBV	380895	1187105	17.10%	1.918%
7	8.134	852	858	860	rBV6	4197	10543	0.15%	0.017%
8	8.169	862	864	872	rVV9	7340	11267	0.16%	0.018%
9	8.422	901	907	929	rBV	425515	1550232	22.32%	2.504%
10	8.863	975	982	1014	rBV	459665	1500350	21.61%	2.424%
11	9.581	1097	1104	1130	rBV	344830	1091559	15.72%	1.763%
12	10.028	1179	1180	1186	rVB6	5326	7066	0.10%	0.011%
13	10.122	1190	1196	1218	rBV	442104	1496602	21.55%	2.418%
14	10.487	1251	1258	1280	rBV	917751	2023050	29.13%	3.268%
15	10.652	1280	1286	1312	rVV	229933	999263	14.39%	1.614%
16	11.710	1458	1466	1467	rBV8	10032	20035	0.29%	0.032%
17	12.728	1633	1639	1643	rBV	15871	27531	0.40%	0.044%
18	13.257	1724	1729	1735	rVV	33320	59710	0.86%	0.096%
19	13.657	1793	1797	1802	rBV4	14581	24850	0.36%	0.040%
20	13.763	1809	1815	1845	rBV	2412573	3950962	56.90%	6.383%
21	14.034	1854	1861	1883	rBV	2668386	4470341	64.38%	7.222%
22	14.340	1907	1913	1933	rBV	1799332	3067515	44.17%	4.956%
23	14.640	1954	1964	1966	rBV4	41220	110380	1.59%	0.178%
24	15.169	2050	2054	2058	rBV3	18540	24782	0.36%	0.040%
25	15.340	2077	2083	2099	rBV	3312684	5501045	79.22%	8.887%
26	15.463	2099	2104	2121	rVB	570273	1140462	16.42%	1.842%
27	15.787	2156	2159	2165	rVB2	17668	28107	0.40%	0.045%
28	16.428	2264	2268	2276	rVB6	13603	22556	0.32%	0.036%
29	16.969	2357	2360	2364	rBV4	12057	17221	0.25%	0.028%
30	17.092	2375	2381	2392	rBV	2104098	3466775	49.92%	5.601%
31	17.192	2392	2398	2427	rVB	3300535	5873746	84.59%	9.489%
32	18.016	2535	2538	2546	rBV7	8134	15499	0.22%	0.025%
33	18.616	2638	2640	2645	rBV6	5106	7725	0.11%	0.012%
34	19.063	2712	2716	2722	rBV2	41967	64757	0.93%	0.105%
35	19.139	2725	2729	2738	rVV2	22962	50413	0.73%	0.081%
36	19.498	2784	2790	2810	rBV	4642255	6944095	100.00%	11.218%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028611.D
Acq On : 14 Nov 2023 20:47
Operator : MA/JU
Sample : PB157093BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	21.304	3092	3097	3114	rBV	1804857	3375893	48.62%	5.454%
38	23.457	3456	3463	3473	rBV2	2815519	5878480	84.65%	9.497%
39	23.604	3482	3488	3499	rVB	1482078	3142573	45.26%	5.077%




Sum of corrected areas: 61899257

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028611.D
Acq On : 14 Nov 2023 20:47
Operator : MA/JU
Sample : PB157093BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

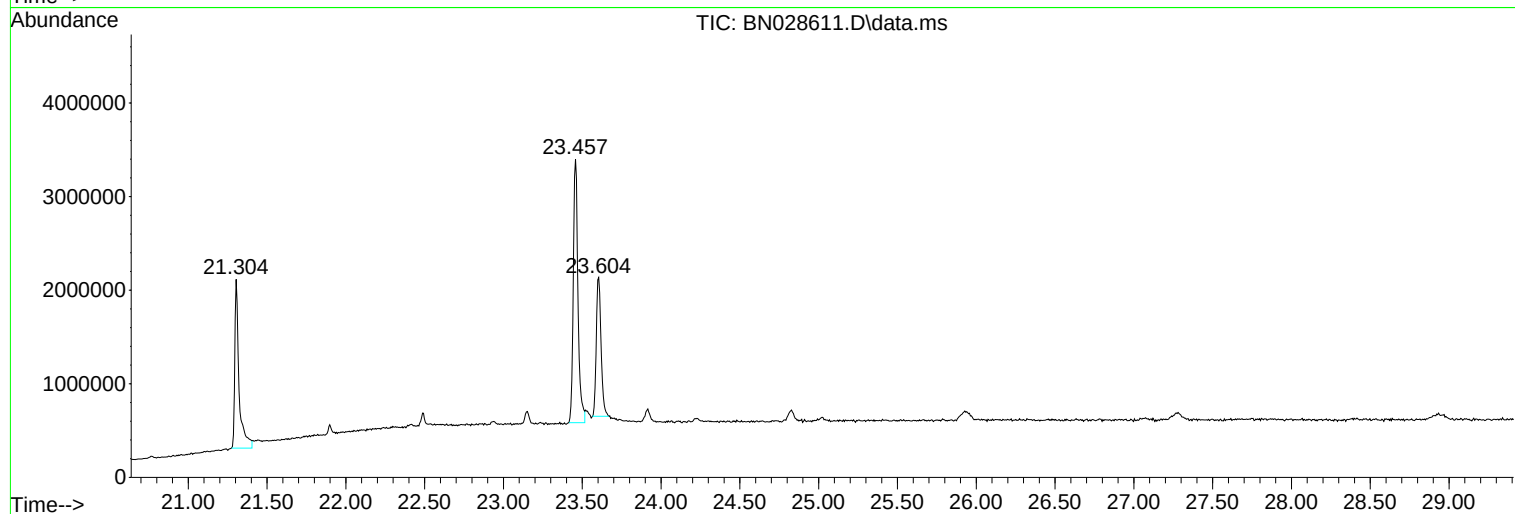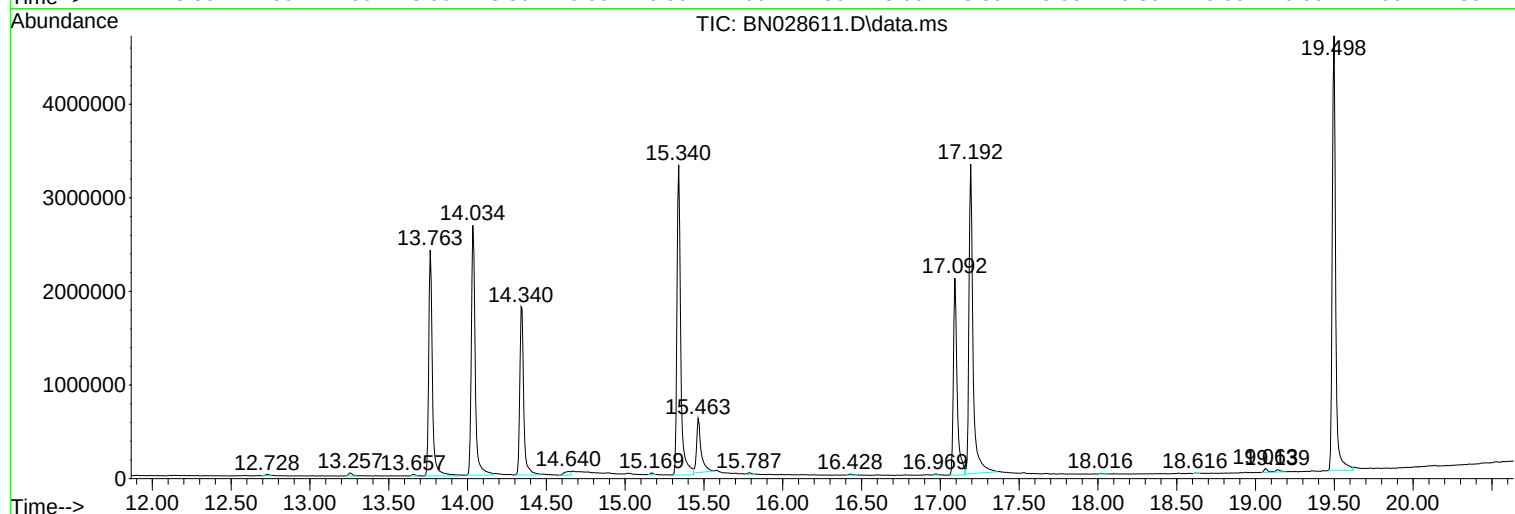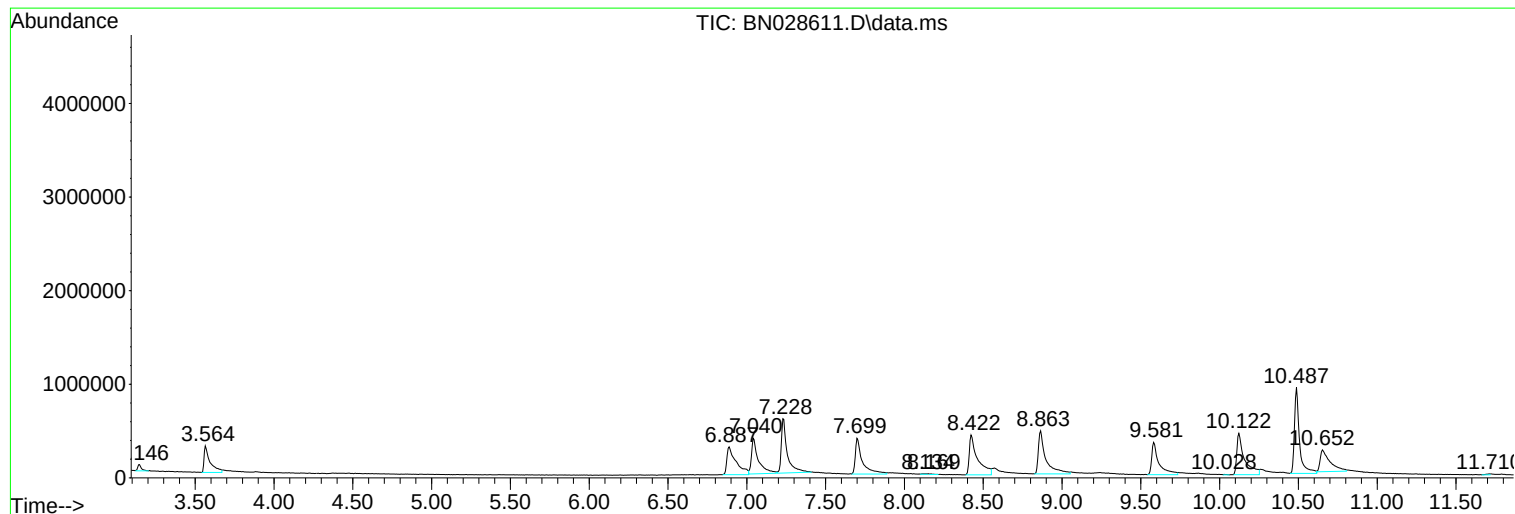

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028611.D
Acq On : 14 Nov 2023 20:47
Operator : MA/JU
Sample : PB157093BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028611.D
Acq On : 14 Nov 2023 20:47
Operator : MA/JU
Sample : PB157093BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------