

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028623.D
 Acq On : 15 Nov 2023 03:54
 Operator : MA/JU
 Sample : 05281-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	6	9	13	rBV	47249	65245	0.60%	0.078%
2	3.587	81	85	91	rBV3	24309	59767	0.55%	0.071%
3	3.787	117	119	124	rVB	17189	23049	0.21%	0.027%
4	6.928	642	653	660	rBV3	55827	230727	2.11%	0.275%
5	7.040	667	672	696	rBV	485491	1261987	11.54%	1.505%
6	7.228	698	704	731	rVV	646960	1542762	14.11%	1.840%
7	7.699	778	784	811	rBV	466375	1272852	11.64%	1.518%
8	8.422	901	907	927	rBV	286567	1037190	9.49%	1.237%
9	8.858	974	981	1009	rBV	781256	2089798	19.11%	2.492%
10	9.575	1097	1103	1129	rBV	614928	1606072	14.69%	1.915%
11	10.116	1188	1195	1216	rBV	806625	2184752	19.98%	2.605%
12	10.487	1251	1258	1274	rBV	1077682	2229282	20.39%	2.658%
13	10.646	1279	1285	1315	rVV2	259439	1064768	9.74%	1.270%
14	11.710	1462	1466	1472	rBV9	6051	12655	0.12%	0.015%
15	12.722	1628	1638	1644	rBV5	12644	32319	0.30%	0.039%
16	13.251	1724	1728	1735	rBV	28303	45167	0.41%	0.054%
17	13.657	1794	1797	1801	rBV5	9839	14416	0.13%	0.017%
18	13.763	1807	1815	1832	rBV	3884867	5721336	52.33%	6.822%
19	14.034	1854	1861	1883	rBV	4148987	6374879	58.31%	7.601%
20	14.340	1906	1913	1933	rBV	2123659	3429693	31.37%	4.089%
21	15.169	2049	2054	2059	rBV5	15018	23088	0.21%	0.028%
22	15.340	2076	2083	2099	rBV	5139404	8271513	75.65%	9.863%
23	15.463	2099	2104	2120	rVB	1240195	2130402	19.48%	2.540%
24	15.787	2156	2159	2165	rVB4	15828	22748	0.21%	0.027%
25	16.428	2263	2268	2272	rBV6	9902	15728	0.14%	0.019%
26	16.775	2324	2327	2333	rVB7	7009	13433	0.12%	0.016%
27	16.975	2356	2361	2365	rBV3	10095	14081	0.13%	0.017%
28	17.092	2375	2381	2392	rBV	2533056	3966204	36.28%	4.729%
29	17.192	2392	2398	2417	rVV	5862224	9025244	82.55%	10.761%
30	18.016	2534	2538	2548	rBV4	46745	125309	1.15%	0.149%
31	19.057	2711	2715	2720	rBV2	71525	112515	1.03%	0.134%
32	19.134	2724	2728	2738	rVV2	51283	100692	0.92%	0.120%
33	19.316	2755	2759	2763	rBV7	28115	57227	0.52%	0.068%
34	19.451	2779	2782	2784	rBV2	33657	38477	0.35%	0.046%
35	19.498	2784	2790	2810	rVV	7355420	10933584	100.00%	13.037%
36	21.033	3047	3051	3060	rBV5	116729	240490	2.20%	0.287%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028623.D
Acq On : 15 Nov 2023 03:54
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	21.304	3092	3097	3111	rBV	2614921	4148340	37.94%	4.946%
38	22.927	3370	3373	3379	rVB2	215863	296174	2.71%	0.353%
39	23.451	3455	3462	3470	rBV2	5051654	9966506	91.15%	11.884%
40	23.598	3481	3487	3502	rVB	2072750	4066967	37.20%	4.849%




Sum of corrected areas: 83867438

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028623.D
Acq On : 15 Nov 2023 03:54
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

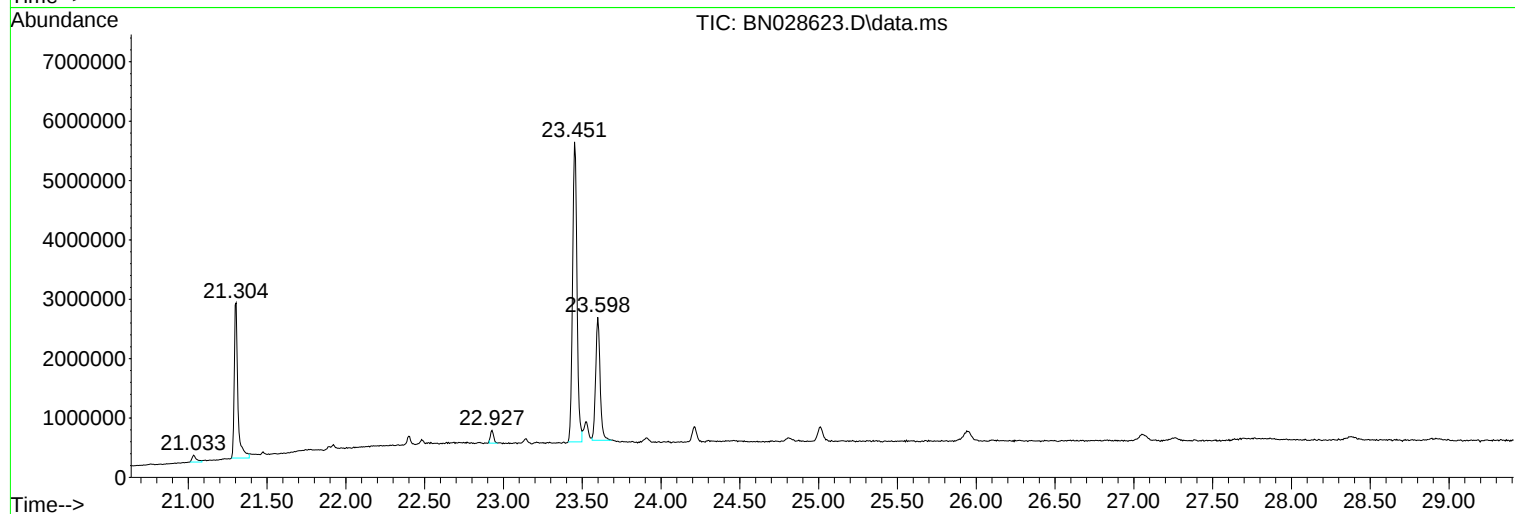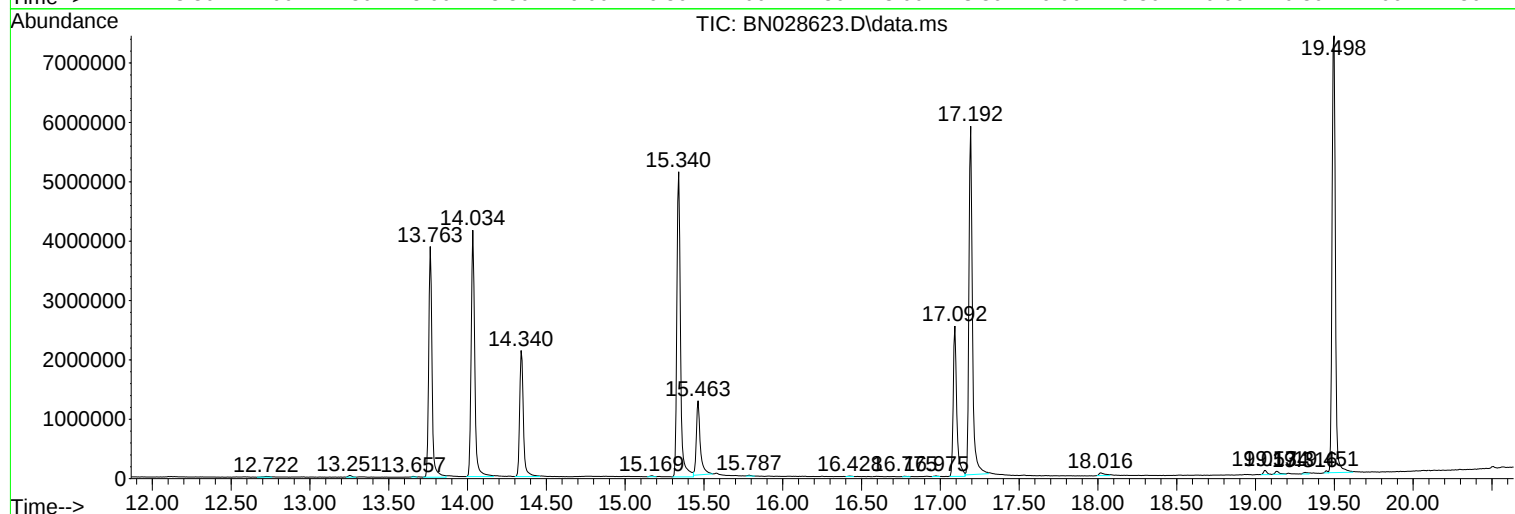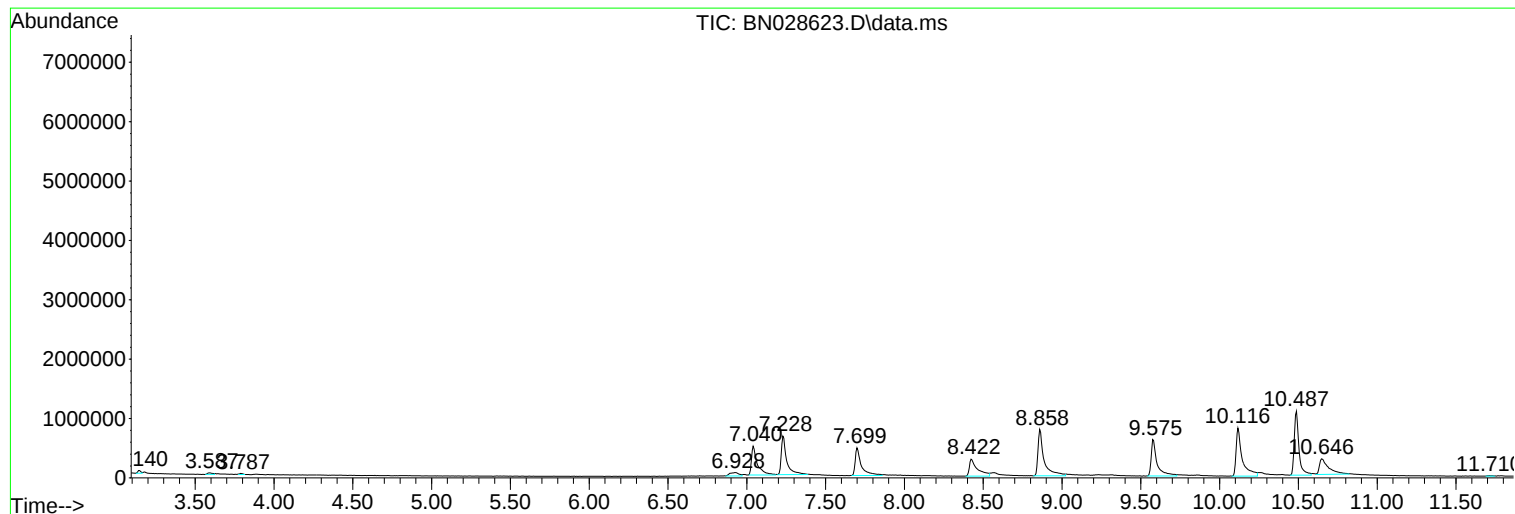

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028623.D
Acq On : 15 Nov 2023 03:54
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028623.D
Acq On : 15 Nov 2023 03:54
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc