

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028624.D
 Acq On : 15 Nov 2023 04:30
 Operator : MA/JU
 Sample : 05281-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	14	rBV	56969	76132	0.75%	0.094%
2	3.575	79	83	95	rBV	73174	217045	2.13%	0.267%
3	3.787	116	119	124	rVB2	21067	29720	0.29%	0.037%
4	4.993	318	324	333	rBV2	27271	73005	0.72%	0.090%
5	5.705	440	445	450	rBV7	8678	19952	0.20%	0.025%
6	6.905	637	649	650	rBV4	44680	81517	0.80%	0.100%
7	7.040	666	672	691	rBV	552316	1391527	13.65%	1.713%
8	7.228	698	704	736	rVB	669870	1614153	15.83%	1.987%
9	7.699	777	784	811	rBV	461998	1338918	13.13%	1.648%
10	8.428	899	908	926	rBV	248739	951185	9.33%	1.171%
11	8.857	974	981	1012	rBV	853506	2304613	22.61%	2.837%
12	9.228	1041	1044	1052	rVB7	10155	21012	0.21%	0.026%
13	9.575	1096	1103	1137	rBV	641047	1771580	17.38%	2.181%
14	10.116	1189	1195	1216	rBV	854043	2271835	22.29%	2.797%
15	10.487	1251	1258	1273	rBV	1089596	2278096	22.35%	2.805%
16	10.640	1278	1284	1321	rVB	588577	1991050	19.53%	2.451%
17	11.716	1461	1467	1472	rBV8	7654	18755	0.18%	0.023%
18	11.775	1472	1477	1485	rVB8	8972	23921	0.23%	0.029%
19	12.728	1632	1639	1643	rBV2	10738	23835	0.23%	0.029%
20	13.251	1722	1728	1737	rBV	33221	55647	0.55%	0.069%
21	13.657	1790	1797	1801	rBV5	11717	18836	0.18%	0.023%
22	13.763	1808	1815	1831	rBV	3839891	5657547	55.50%	6.966%
23	14.034	1854	1861	1883	rBV	4139247	6499755	63.76%	8.002%
24	14.263	1897	1900	1905	rVB7	6082	10420	0.10%	0.013%
25	14.339	1907	1913	1928	rBV	2127673	3365324	33.01%	4.143%
26	14.763	1978	1985	1989	rBV9	7136	18084	0.18%	0.022%
27	15.169	2048	2054	2059	rBV5	14810	25661	0.25%	0.032%
28	15.339	2076	2083	2099	rBV	4972764	8085815	79.32%	9.955%
29	15.463	2099	2104	2121	rVB	1075257	1917148	18.81%	2.360%
30	15.692	2141	2143	2148	rVB5	8256	10566	0.10%	0.013%
31	15.786	2156	2159	2164	rVB3	13644	21430	0.21%	0.026%
32	16.033	2196	2201	2208	rBV3	6334	14251	0.14%	0.018%
33	16.422	2264	2267	2273	rBV5	9432	15989	0.16%	0.020%
34	16.598	2292	2297	2301	rBV7	5065	10698	0.10%	0.013%
35	16.775	2324	2327	2334	rVB9	7267	11666	0.11%	0.014%
36	16.886	2342	2346	2351	rBV8	4965	10522	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028624.D
Acq On : 15 Nov 2023 04:30
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	16.969	2355	2360	2368	rBV5	17597	35683	0.35%	0.044%
38	17.092	2375	2381	2392	rBV	2343576	3871696	37.98%	4.767%
39	17.192	2392	2398	2427	rVB	5095170	8581897	84.18%	10.566%
40	19.063	2711	2716	2722	rBV	65119	108270	1.06%	0.133%
41	19.133	2724	2728	2736	rVV	46724	80381	0.79%	0.099%
42	19.451	2779	2782	2784	rBV3	26063	29274	0.29%	0.036%
43	19.492	2784	2789	2809	rVV	6995883	10194337	100.00%	12.551%
44	21.304	3092	3097	3108	rBV	2283633	3683678	36.13%	4.535%
45	23.451	3455	3462	3471	rBV2	4451240	8664326	84.99%	10.667%
46	23.598	3481	3487	3504	rVB	1813191	3725254	36.54%	4.587%




Sum of corrected areas: 81222006

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028624.D
Acq On : 15 Nov 2023 04:30
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

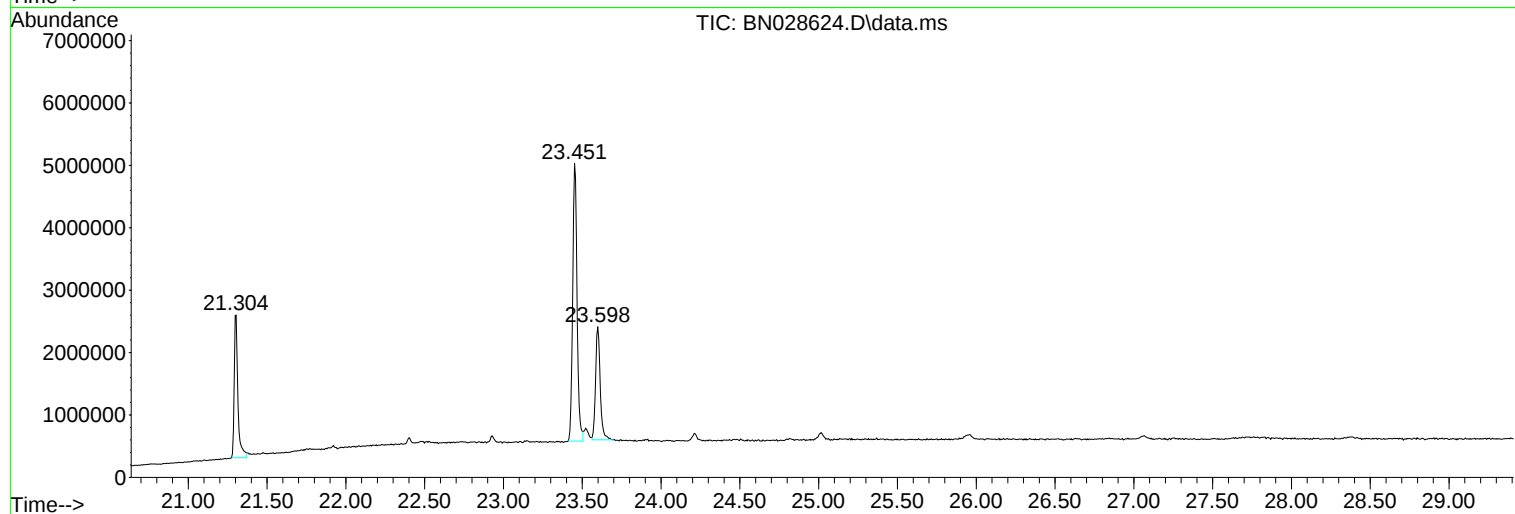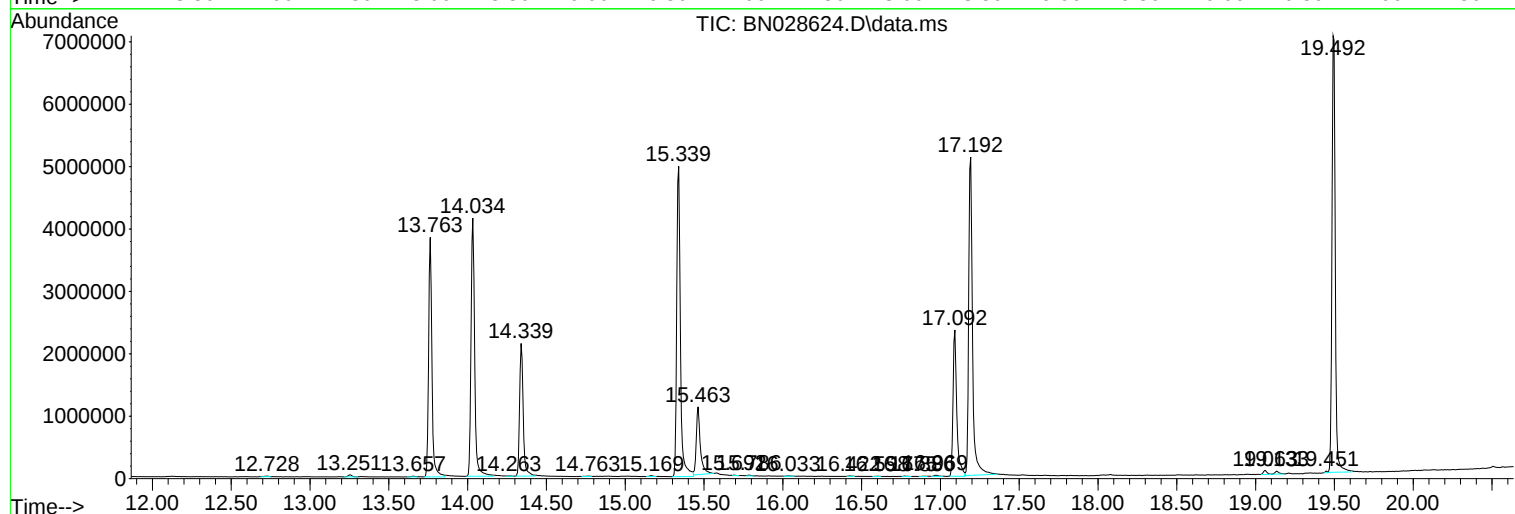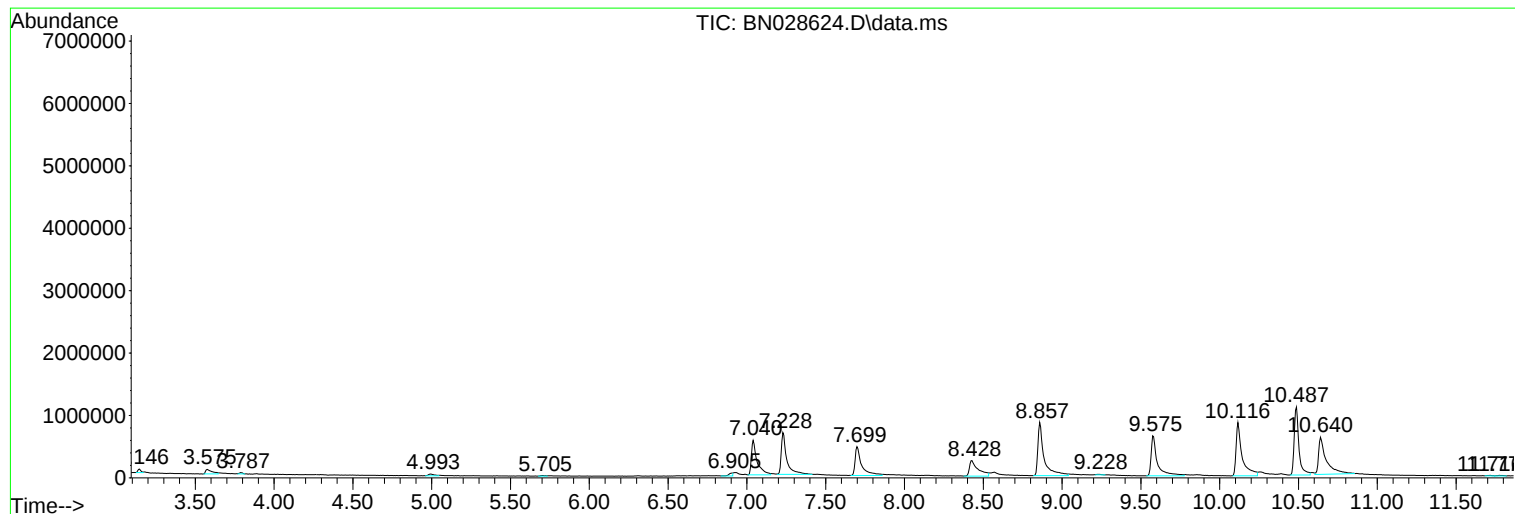

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028624.D
Acq On : 15 Nov 2023 04:30
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028624.D
Acq On : 15 Nov 2023 04:30
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc