

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028626.D
 Acq On : 15 Nov 2023 10:37
 Operator : MA/JU
 Sample : PB157091BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK091

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	5	8	16	rVB	92720	146584	1.68%	0.156%
2	3.552	75	79	106	rBV	639399	1451092	16.59%	1.547%
3	6.863	636	642	664	rBV	766727	1926928	22.03%	2.054%
4	7.028	664	670	689	rVB	698249	1514432	17.31%	1.614%
5	7.216	696	702	732	rVB	1031385	2138261	24.44%	2.279%
6	7.687	775	782	801	rBV	831169	1834165	20.97%	1.955%
7	8.405	897	904	926	rBV	986753	2476590	28.31%	2.640%
8	8.846	972	979	1015	rBV	869417	2131866	24.37%	2.272%
9	9.569	1094	1102	1128	rBV	681125	1682640	19.24%	1.794%
10	10.104	1186	1193	1213	rBV	1018898	2496865	28.54%	2.661%
11	10.475	1249	1256	1272	rBV	1618602	3045925	34.82%	3.247%
12	10.628	1277	1282	1311	rVB	737521	2055938	23.50%	2.191%
13	11.951	1500	1507	1509	rBV7	4842	10626	0.12%	0.011%
14	12.087	1526	1530	1536	rBV5	12567	31834	0.36%	0.034%
15	12.216	1544	1552	1553	rBV3	19386	39199	0.45%	0.042%
16	13.245	1721	1727	1732	rBV3	29536	56531	0.65%	0.060%
17	13.322	1738	1740	1745	rVB5	5514	9011	0.10%	0.010%
18	13.457	1753	1763	1764	rBV4	37906	88893	1.02%	0.095%
19	13.757	1808	1814	1834	rVB	3410921	5037787	57.59%	5.370%
20	14.028	1853	1860	1874	rBV	3783883	5833173	66.68%	6.218%
21	14.145	1876	1880	1883	rVV4	13621	23314	0.27%	0.025%
22	14.334	1899	1912	1934	rVB	2903126	5069071	57.95%	5.403%
23	14.575	1945	1953	1976	rBV2	192131	1030953	11.79%	1.099%
24	15.145	2041	2050	2058	rBV2	139580	381189	4.36%	0.406%
25	15.334	2071	2082	2098	rBV	4693385	7486883	85.59%	7.980%
26	15.457	2098	2103	2121	rVB	1049783	1820291	20.81%	1.940%
27	15.675	2135	2140	2145	rBV2	39338	84183	0.96%	0.090%
28	15.769	2151	2156	2162	rVB2	196423	353999	4.05%	0.377%
29	15.904	2176	2179	2182	rBV5	6901	8754	0.10%	0.009%
30	15.981	2187	2192	2197	rBV3	19044	33073	0.38%	0.035%
31	16.092	2208	2211	2215	rVB3	12662	17199	0.20%	0.018%
32	16.416	2261	2266	2275	rVV	162415	254219	2.91%	0.271%
33	16.586	2288	2295	2301	rBV2	109433	165932	1.90%	0.177%
34	16.910	2340	2350	2353	rBV3	45936	68581	0.78%	0.073%
35	16.963	2353	2359	2371	rVV2	173577	284288	3.25%	0.303%
36	17.086	2374	2380	2392	rBV	3165593	5285297	60.42%	5.634%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028626.D
 Acq On : 15 Nov 2023 10:37
 Operator : MA/JU
 Sample : PB157091BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK091

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

37	17.186	2392	2397	2426	rVB	4780350	7684714	87.85%	8.191%
38	17.522	2449	2454	2460	rVB	96449	129255	1.48%	0.138%
39	17.669	2474	2479	2483	rVB2	87330	119848	1.37%	0.128%
40	18.010	2529	2537	2545	rBV3	75739	167743	1.92%	0.179%
41	18.157	2560	2562	2568	rVB3	13917	16736	0.19%	0.018%
42	18.469	2613	2615	2617	rBV3	7486	9065	0.10%	0.010%
43	18.504	2617	2621	2625	rVV2	55443	73768	0.84%	0.079%
44	18.622	2637	2641	2646	rVB	83625	101419	1.16%	0.108%
45	18.933	2689	2694	2699	rBV3	43607	79871	0.91%	0.085%
46	19.057	2711	2715	2723	rVB3	67093	105675	1.21%	0.113%
47	19.133	2724	2728	2737	rBV3	43403	92674	1.06%	0.099%
48	19.210	2737	2741	2746	rVV3	47033	59859	0.68%	0.064%
49	19.357	2762	2766	2774	rBV5	35708	53657	0.61%	0.057%
50	19.428	2774	2778	2779	rBV	85125	91070	1.04%	0.097%
51	19.451	2779	2782	2784	rVV	124913	121733	1.39%	0.130%
52	19.492	2784	2789	2799	rVV	6059200	8747443	100.00%	9.324%
53	19.733	2827	2830	2832	rBV2	27505	28155	0.32%	0.030%
54	20.133	2895	2898	2902	rVB2	92801	104540	1.20%	0.111%
55	20.510	2958	2962	2969	rBV2	129769	176498	2.02%	0.188%
56	20.769	3002	3006	3012	rVB	130879	179238	2.05%	0.191%
57	21.304	3092	3097	3102	rBV	3819876	5095179	58.25%	5.431%
58	21.898	3195	3198	3201	rBV2	142471	199804	2.28%	0.213%
59	23.457	3456	3463	3473	rBV	4242248	8498061	97.15%	9.058%
60	23.604	3482	3488	3505	rVB2	2562797	5505093	62.93%	5.868%




Sum of corrected areas: 93816664

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028626.D
Acq On : 15 Nov 2023 10:37
Operator : MA/JU
Sample : PB157091BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK091

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

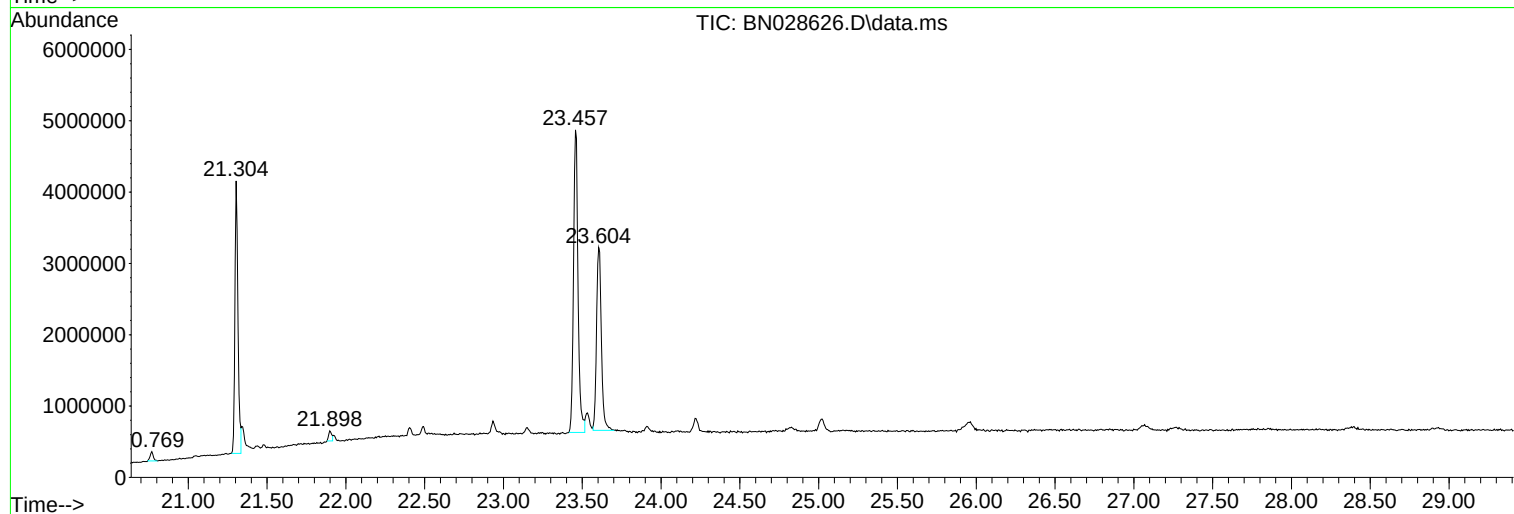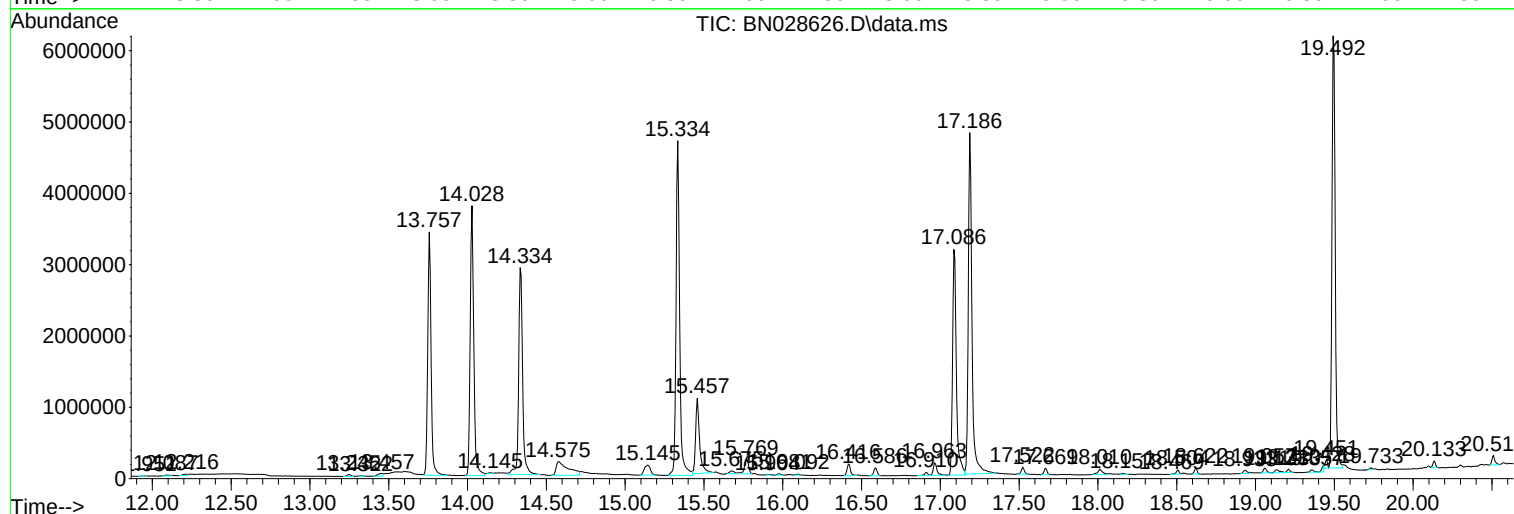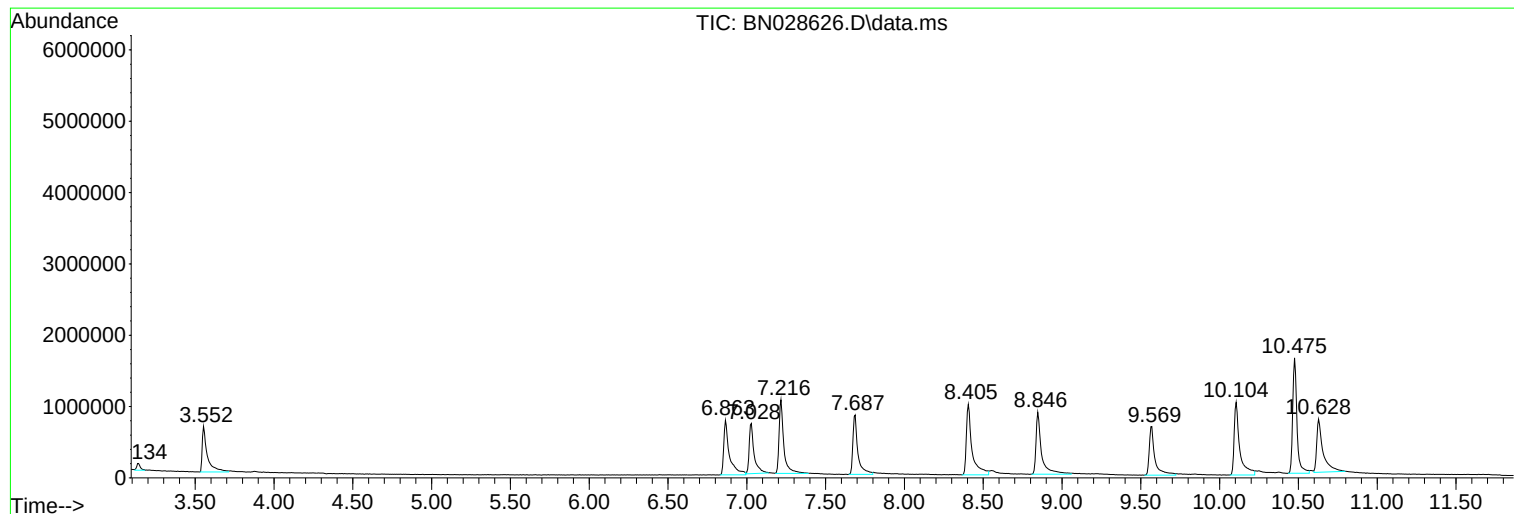

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028626.D
Acq On : 15 Nov 2023 10:37
Operator : MA/JU
Sample : PB157091BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK091

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028626.D
Acq On : 15 Nov 2023 10:37
Operator : MA/JU
Sample : PB157091BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK091

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc