

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028629.D
 Acq On : 15 Nov 2023 13:13
 Operator : MA/JU
 Sample : 05281-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	23	rVB	69656	134790	1.02%	0.133%
2	3.576	79	83	98	rBV	90457	293186	2.22%	0.289%
3	4.987	318	323	330	rBV	29229	71879	0.54%	0.071%
4	6.899	641	648	649	rBV2	59753	110527	0.84%	0.109%
5	7.034	666	671	693	rBV	698413	1686341	12.78%	1.660%
6	7.222	697	703	733	rVV	797811	1892971	14.35%	1.863%
7	7.693	777	783	805	rBV	552441	1468131	11.13%	1.445%
8	8.416	900	906	927	rBV	335613	1188638	9.01%	1.170%
9	8.852	974	980	1005	rBV	1021067	2609028	19.77%	2.568%
10	9.569	1096	1102	1130	rBV	796231	2026798	15.36%	1.995%
11	10.011	1175	1177	1187	rVB9	5960	15322	0.12%	0.015%
12	10.111	1187	1194	1215	rBV	1059742	2752646	20.86%	2.709%
13	10.481	1250	1257	1274	rBV	1309873	2597811	19.69%	2.557%
14	10.634	1278	1283	1319	rVB	706982	2278807	17.27%	2.243%
15	11.681	1454	1461	1464	rBV9	12009	28838	0.22%	0.028%
16	12.704	1631	1635	1649	rVB4	21830	59348	0.45%	0.058%
17	13.252	1722	1728	1734	rBV2	20058	36115	0.27%	0.036%
18	13.652	1792	1796	1804	rVB	23384	37862	0.29%	0.037%
19	13.763	1807	1815	1843	rBV	4619591	6999175	53.05%	6.888%
20	14.034	1854	1861	1886	rBV	4730401	7789863	59.04%	7.666%
21	14.340	1906	1913	1932	rBV	2491799	3998428	30.31%	3.935%
22	15.163	2048	2053	2058	rBV4	29726	44151	0.33%	0.043%
23	15.340	2076	2083	2098	rBV	6194062	10139677	76.85%	9.979%
24	15.463	2098	2104	2120	rVB	1529754	2668083	20.22%	2.626%
25	15.787	2155	2159	2166	rVB	28289	44600	0.34%	0.044%
26	16.428	2264	2268	2274	rVB4	19922	34312	0.26%	0.034%
27	16.598	2292	2297	2301	rVB4	13233	18736	0.14%	0.018%
28	16.781	2322	2328	2332	rBV8	10132	15794	0.12%	0.016%
29	16.969	2355	2360	2367	rBV4	29893	51636	0.39%	0.051%
30	17.087	2375	2380	2392	rBV	2692910	4536660	34.38%	4.465%
31	17.192	2392	2398	2416	rVV	6815142	11060566	83.83%	10.885%
32	17.528	2452	2455	2462	rVB6	15890	24323	0.18%	0.024%
33	18.075	2546	2548	2554	rVB3	11043	14573	0.11%	0.014%
34	18.616	2638	2640	2647	rVB7	10218	17959	0.14%	0.018%
35	19.057	2711	2715	2723	rBV	88106	134394	1.02%	0.132%
36	19.134	2723	2728	2737	rBV2	68644	136600	1.04%	0.134%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028629.D
Acq On : 15 Nov 2023 13:13
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.451	2779	2782	2784	rBV	32340	36008	0.27%	0.035%
38	19.498	2784	2790	2810	rVV	9054438	13193916	100.00%	12.984%
39	21.304	3092	3097	3112	rBV	2811425	4526412	34.31%	4.455%
40	21.898	3195	3198	3201	rBV2	99703	131186	0.99%	0.129%
41	22.486	3295	3298	3303	rVB3	171742	251731	1.91%	0.248%
42	23.457	3455	3463	3472	rBV2	5861578	11793540	89.39%	11.606%
43	23.598	3481	3487	3508	rVB	2173289	4662291	35.34%	4.588%




Sum of corrected areas: 101613652

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028629.D
Acq On : 15 Nov 2023 13:13
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

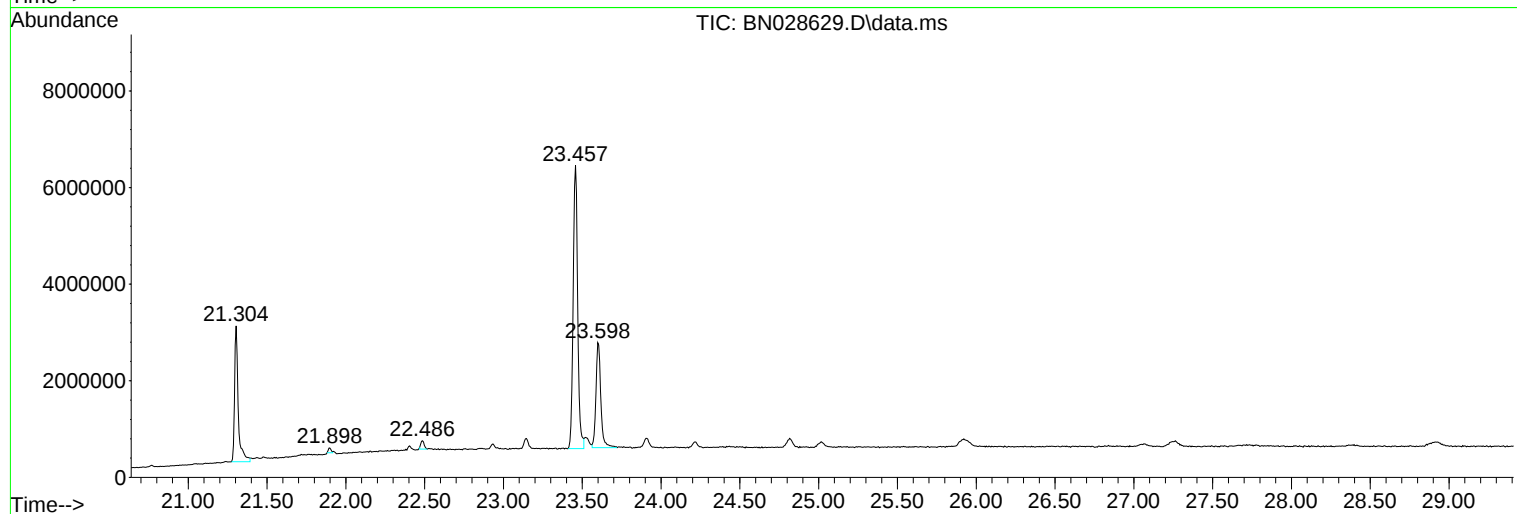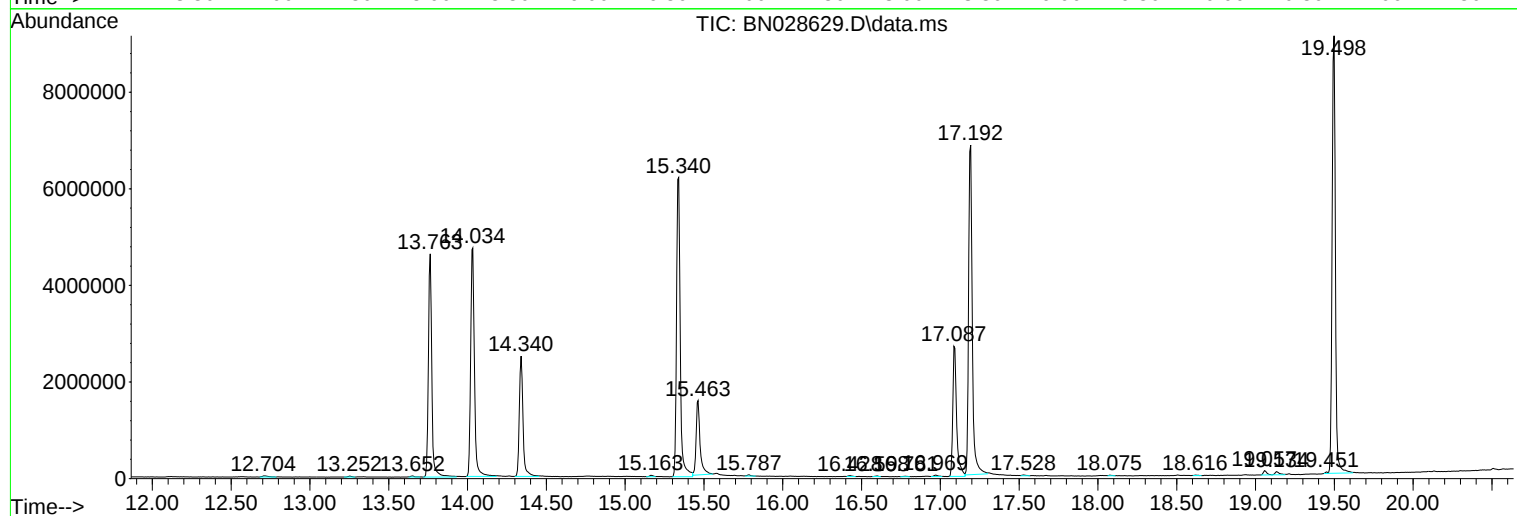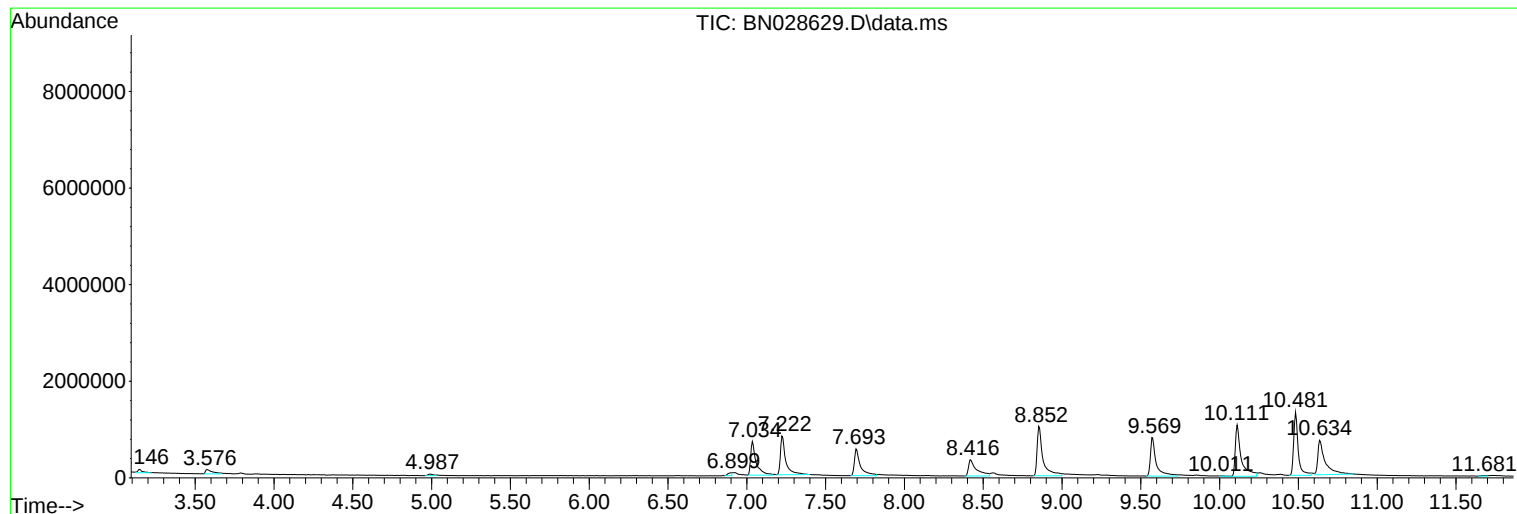

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028629.D
Acq On : 15 Nov 2023 13:13
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028629.D
Acq On : 15 Nov 2023 13:13
Operator : MA/JU
Sample : 05281-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------