

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028630.D
 Acq On : 15 Nov 2023 13:49
 Operator : MA/JU
 Sample : 05281-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	17	rVB	46692	62361	0.77%	0.095%
2	3.575	80	83	97	rBV	79731	236621	2.94%	0.361%
3	4.999	323	325	330	rVB5	6387	8462	0.10%	0.013%
4	6.922	643	652	660	rBV2	39009	143007	1.77%	0.218%
5	7.040	667	672	694	rBV	396262	1101915	13.67%	1.679%
6	7.228	698	704	736	rVB	486861	1291004	16.02%	1.967%
7	7.699	778	784	820	rBV	392972	1208297	14.99%	1.841%
8	8.428	902	908	927	rBV	164661	700022	8.69%	1.067%
9	8.857	974	981	1014	rBV	628562	1874014	23.25%	2.856%
10	9.287	1051	1054	1058	rVB2	10799	13065	0.16%	0.020%
11	9.575	1097	1103	1129	rBV	459529	1314499	16.31%	2.003%
12	9.857	1149	1151	1161	rVB9	13897	26771	0.33%	0.041%
13	10.116	1186	1195	1217	rBV	593679	1774768	22.02%	2.705%
14	10.487	1250	1258	1273	rBV	914903	1977023	24.53%	3.013%
15	10.640	1279	1284	1319	rBV	495486	1650498	20.48%	2.515%
16	11.769	1474	1476	1483	rVB7	8337	15461	0.19%	0.024%
17	12.116	1529	1535	1536	rBV6	7270	9122	0.11%	0.014%
18	12.722	1629	1638	1646	rBV7	10070	29386	0.36%	0.045%
19	13.251	1722	1728	1736	rBV5	17019	33769	0.42%	0.051%
20	13.657	1791	1797	1799	rBV5	10210	14986	0.19%	0.023%
21	13.763	1808	1815	1839	rBV	3038188	4786444	59.39%	7.294%
22	14.028	1854	1860	1882	rBV	3223562	5430682	67.38%	8.276%
23	14.339	1906	1913	1934	rBV	1775506	2921090	36.25%	4.451%
24	15.169	2047	2054	2059	rBV8	13739	27468	0.34%	0.042%
25	15.333	2076	2082	2098	rBV	4166485	6785586	84.20%	10.341%
26	15.463	2099	2104	2121	rVB	751152	1450025	17.99%	2.210%
27	15.780	2156	2158	2164	rVB3	11048	16149	0.20%	0.025%
28	16.427	2264	2268	2272	rBV7	6782	11053	0.14%	0.017%
29	16.592	2292	2296	2301	rBV8	7956	13599	0.17%	0.021%
30	16.975	2357	2361	2362	rBV4	8087	9437	0.12%	0.014%
31	17.092	2374	2381	2392	rBV	1795118	3099975	38.47%	4.724%
32	17.186	2392	2397	2430	rVB	4262479	7319561	90.82%	11.154%
33	18.022	2534	2539	2547	rBV8	23273	70435	0.87%	0.107%
34	18.504	2619	2621	2625	rBV5	7377	8274	0.10%	0.013%
35	19.057	2711	2715	2720	rBV2	52330	79584	0.99%	0.121%
36	19.133	2724	2728	2736	rBV2	37670	68215	0.85%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028630.D
Acq On : 15 Nov 2023 13:49
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.321	2756	2760	2763	rBV6	12668	25295	0.31%	0.039%
38	19.451	2779	2782	2783	rBV2	21001	19979	0.25%	0.030%
39	19.492	2783	2789	2814	rVV	5608231	8059205	100.00%	12.281%
40	21.304	3092	3097	3111	rBV	1604229	2652137	32.91%	4.042%
41	23.451	3455	3462	3472	rBV	3327885	6766865	83.96%	10.312%
42	23.598	3481	3487	3499	rVB	1211805	2514655	31.20%	3.832%




Sum of corrected areas: 65620764

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028630.D
Acq On : 15 Nov 2023 13:49
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

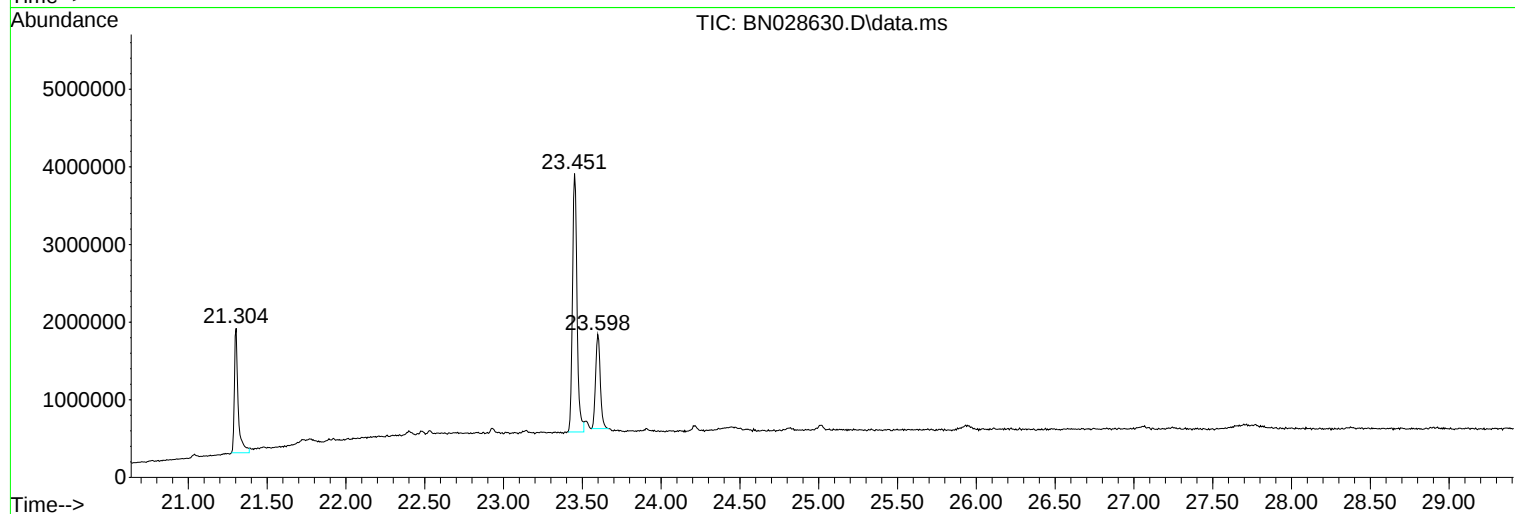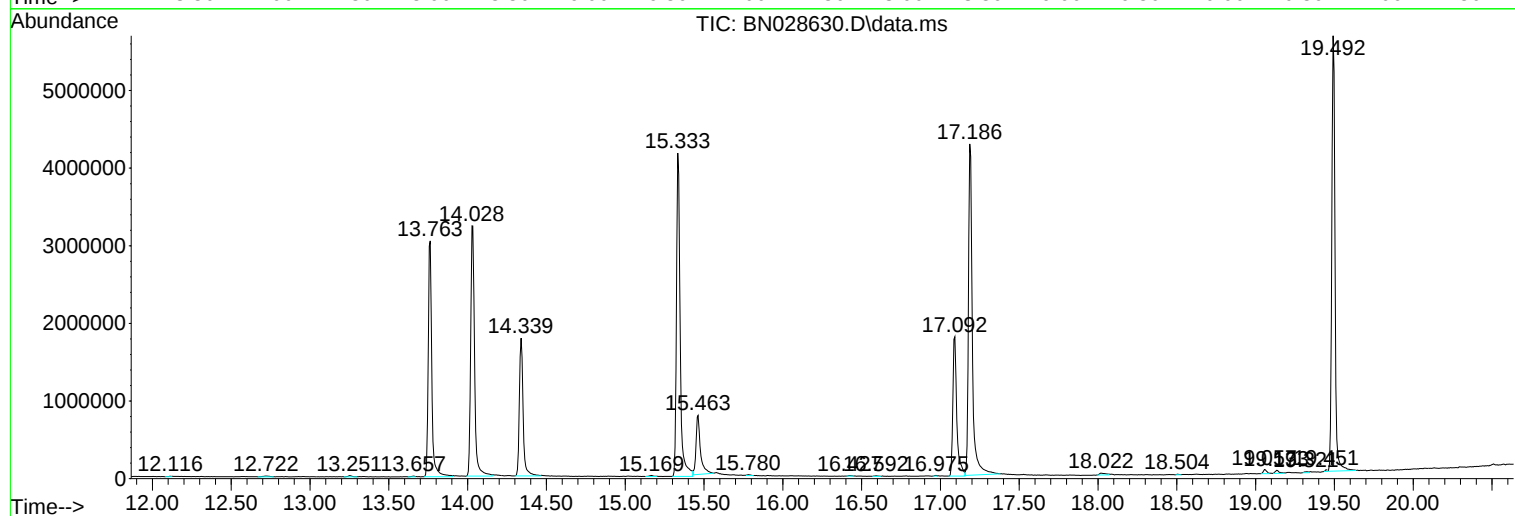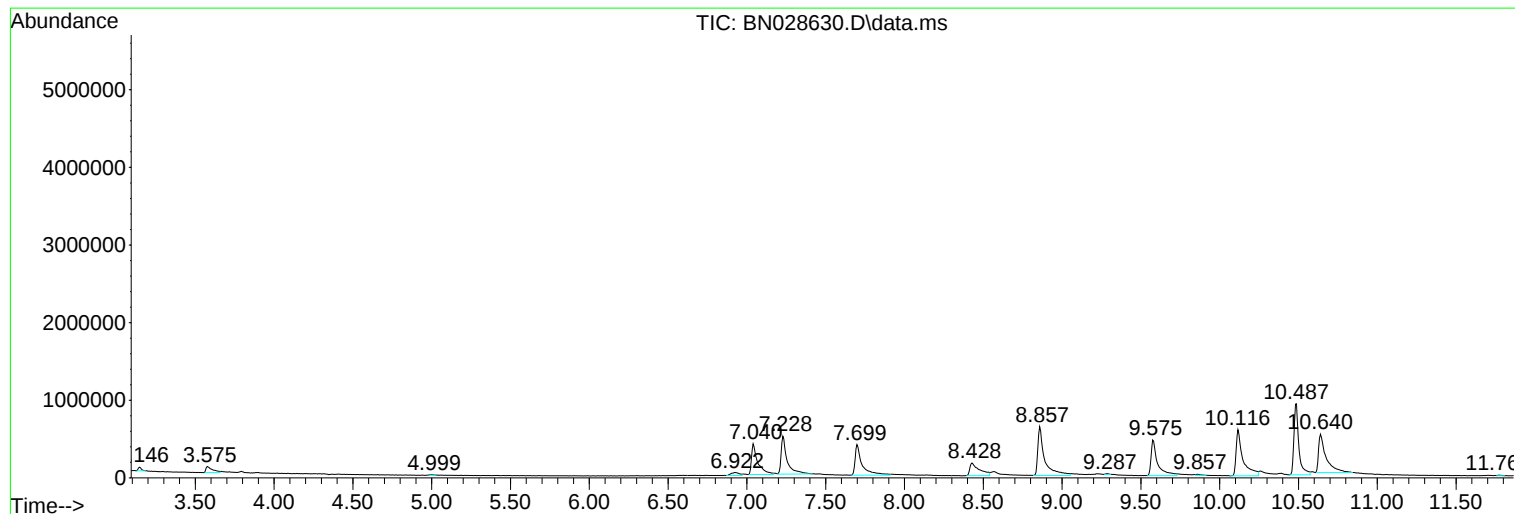

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028630.D
Acq On : 15 Nov 2023 13:49
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028630.D
Acq On : 15 Nov 2023 13:49
Operator : MA/JU
Sample : 05281-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc