

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042819.D
 Acq On : 16 Nov 2023 23:21
 Operator : MA/JU
 Sample : 05268-10
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKD2

Quant Time: Nov 16 23:56:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 22:28:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	22427	20.000	ng/ul	0.00
20) Naphthalene-d8	10.633	136	93876	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.480	164	62413	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	140574	20.000	ng/ul	0.00
79) Chrysene-d12	21.415	240	145170	20.000	ng/ul	0.00
88) Perylene-d12	23.774	264	181305	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	1818	2.544	ng/uL	0.00
4) Pyridine-d5	3.622	84	20118	11.316	ng/ul	0.00
7) Phenol-d5	6.998	99	8937	4.094	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	54578	35.585	ng/ul	0.00
11) 2-Chlorophenol-d4	7.345	132	37002	21.970	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	18404	10.709	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	24808	30.141	ng/ul	0.00
24) 2-Nitrophenol-d4	9.739	143	25562	26.549	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	41607	23.240	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	49508	21.780	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	201259	34.072	ng/ul	0.00
49) Acenaphthylene-d8	14.180	160	204351	32.333	ng/ul	0.00
54) 4-Nitrophenol-d4	14.786	143	393	0.589	ng/ul	0.05
60) Fluorene-d10	15.474	176	173803	35.532	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.621	200	23386	21.963	ng/ul	0.00
73) Anthracene-d10	17.333	188	283282	35.958	ng/ul	0.00
81) Pyrene-d10	19.627	212	398649	41.935	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.621	264	411317	37.927	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.686	128	14498	2.465	ng/ul	96
36) 2-Methylnaphthalene	12.304	142	6307	1.600	ng/ul	93
37) 1-Methylnaphthalene	12.521	142	4855	1.171	ng/ul#	89
43) 1,1'-Biphenyl	13.321	154	6145	1.181	ng/ul	90
52) Acenaphthene	14.545	153	8167	1.705	ng/ul	95
56) Dibenzofuran	14.886	168	21682	3.262	ng/ul	99
61) Fluorene	15.527	166	10902	1.932	ng/ul#	97
72) Phenanthrene	17.274	178	8929	1.017	ng/ul#	94
77) Carbazole	17.662	167	38884	5.331	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042819.D
Acq On : 16 Nov 2023 23:21
Operator : MA/JU
Sample : 05268-10
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCKD2

Quant Time: Nov 16 23:56:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 22:28:07 2023
Response via : Initial Calibration




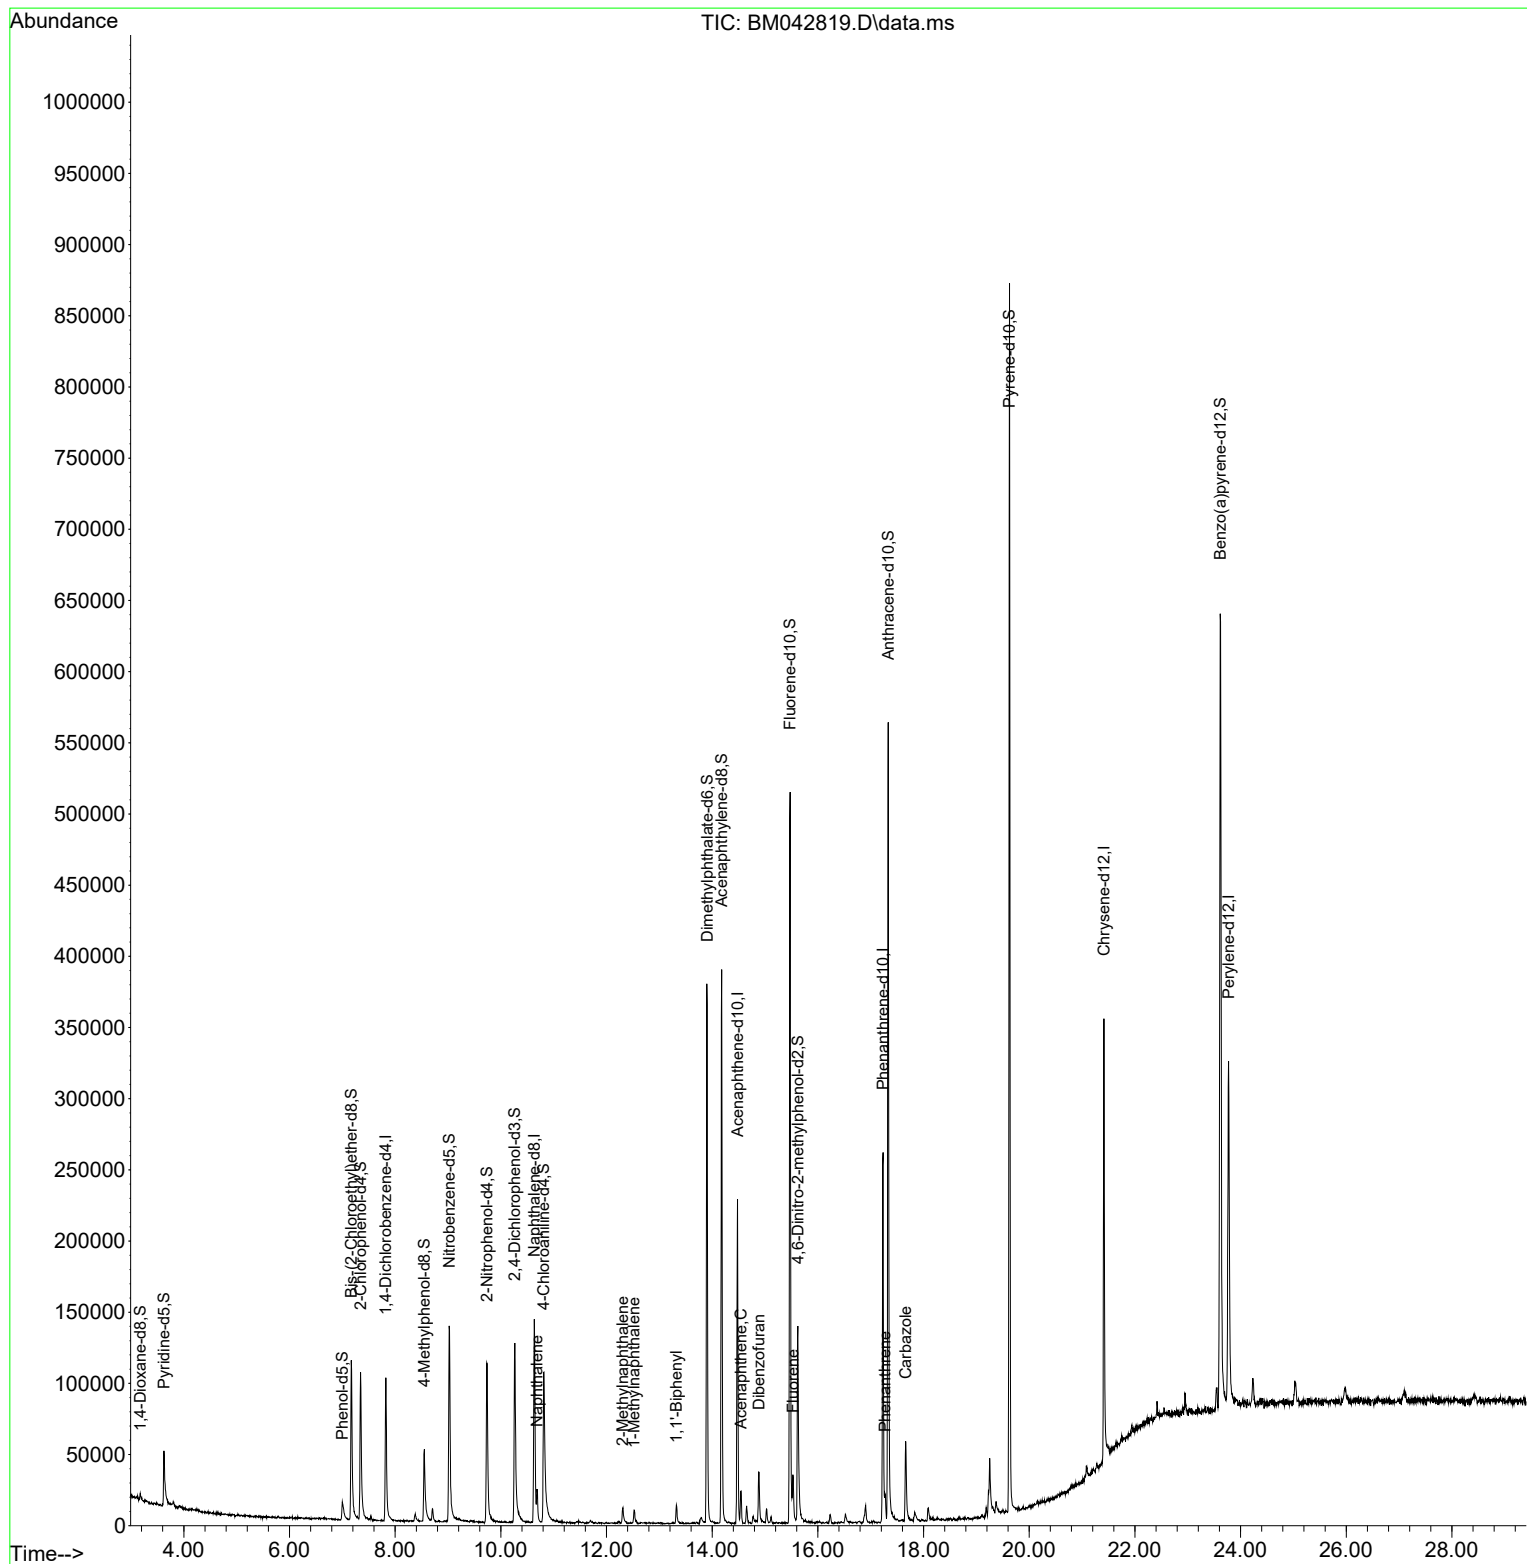


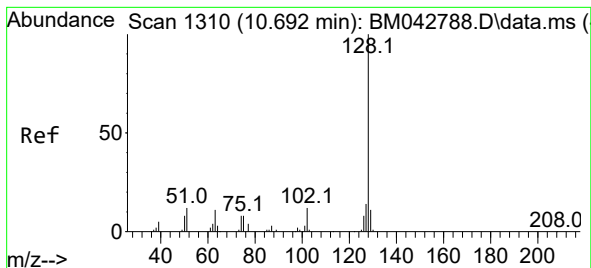

#30
Naphthalene
Concen: 2.465 ng/ul
RT: 10.686 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM042819.D
Acq: 16 Nov 2023 23:21




Instrument :
BNA_N
ClientSampleId :
DCKD2


Tgt Ion:128 Resp: 14498
Ion Ratio Lower Upper
128 100
129 11.3 8.6 13.0
127 10.6 10.5 15.7

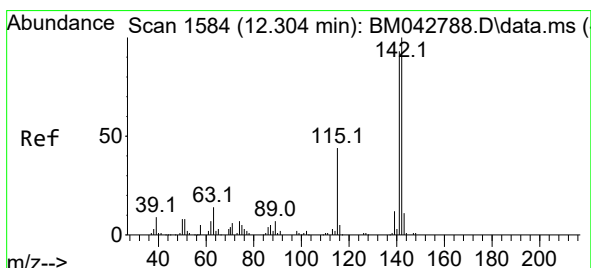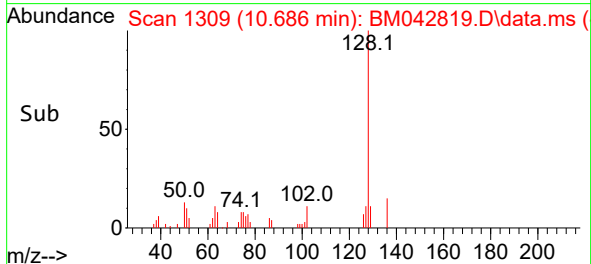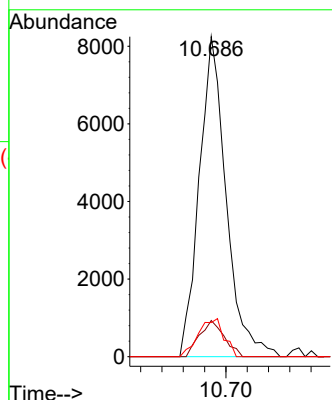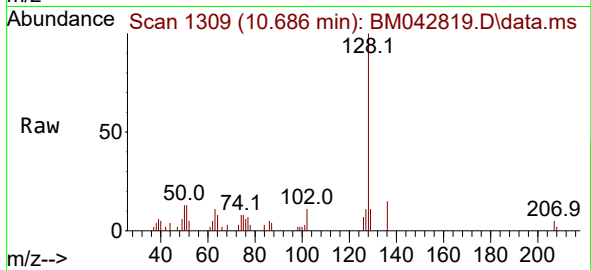

#36
2-Methylnaphthalene
Concen: 1.600 ng/ul
RT: 12.304 min Scan# 1584
Delta R.T. -0.000 min
Lab File: BM042819.D
Acq: 16 Nov 2023 23:21

Tgt Ion:142 Resp: 6307
Ion Ratio Lower Upper
142 100
141 84.9 73.6 110.4


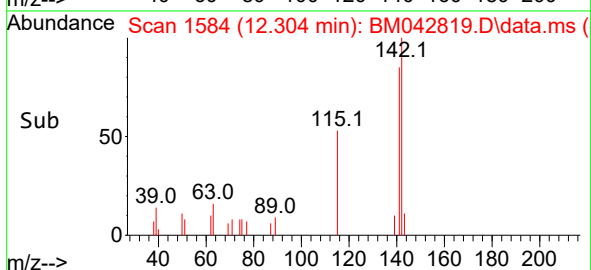
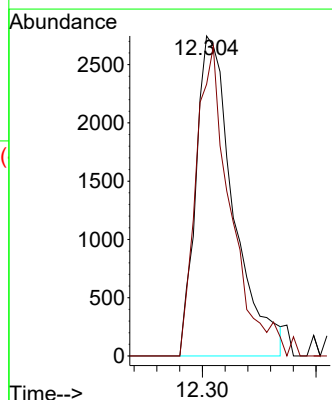
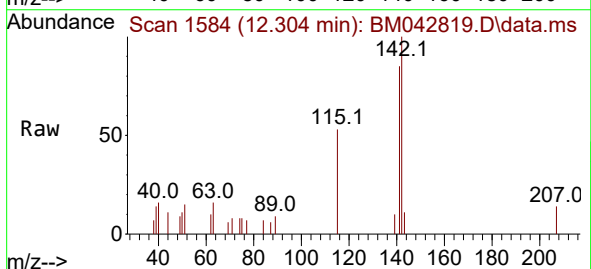


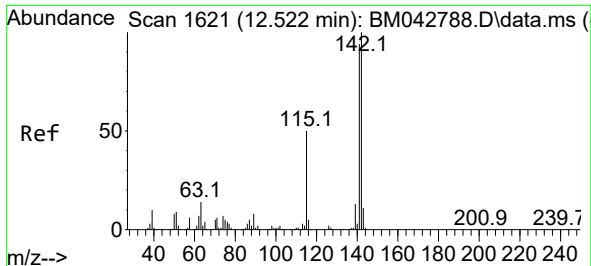

#37
1-Methylnaphthalene
Concen: 1.171 ng/ul
RT: 12.521 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM042819.D
Acq: 16 Nov 2023 23:21




Instrument :
BNA_N
ClientSampleId :
DCKD2


Tgt Ion:142 Resp: 4855
Ion Ratio Lower Upper
142 100
141 81.1 73.3 109.9
116 6.6 3.9 5.9#

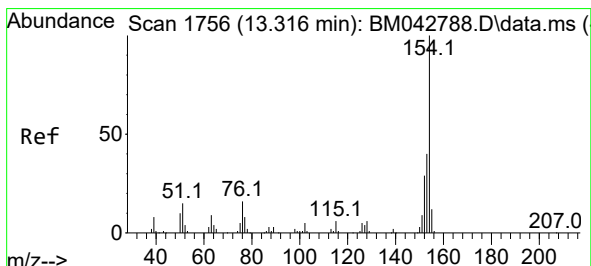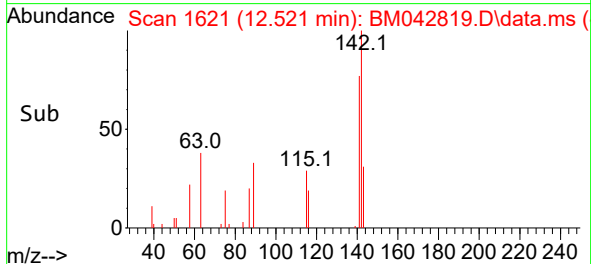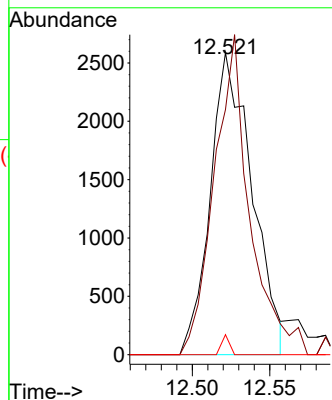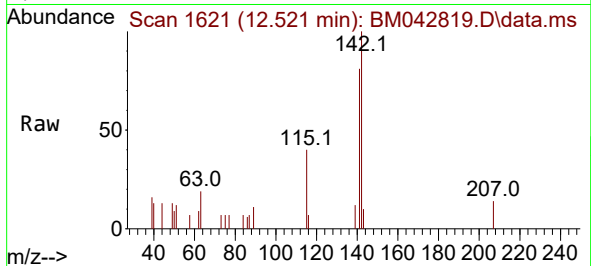

#43
1,1'-Biphenyl
Concen: 1.181 ng/ul
RT: 13.321 min Scan# 1757
Delta R.T. -0.000 min
Lab File: BM042819.D
Acq: 16 Nov 2023 23:21

Tgt Ion:154 Resp: 6145
Ion Ratio Lower Upper
154 100
153 47.4 32.4 48.6
76 15.7 10.7 16.1

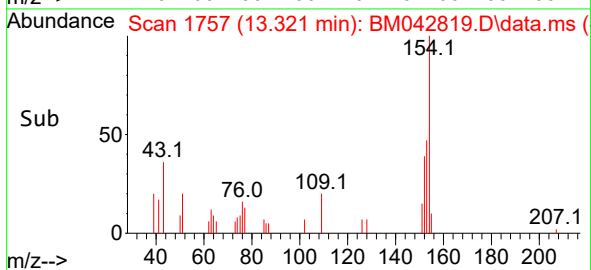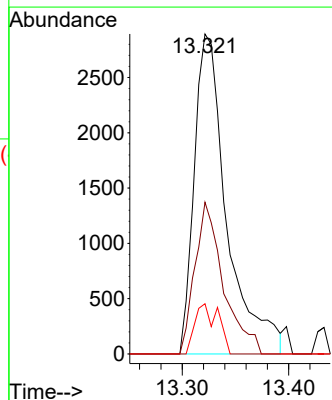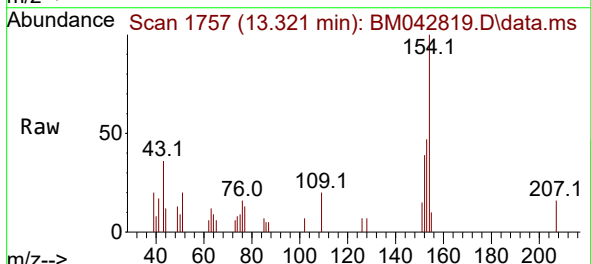

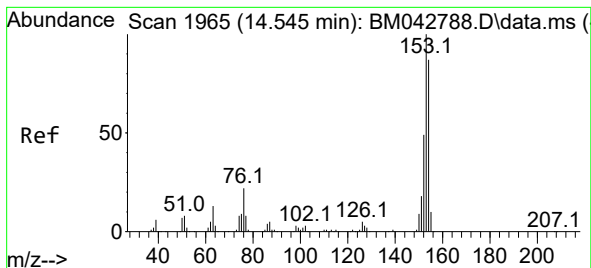

#52

Acenaphthene

Concen: 1.705 ng/u1

RT: 14.545 min Scan# 1965

Delta R.T. -0.006 min

Lab File: BM042819.D

Acq: 16 Nov 2023 23:21

Instrument :

BNA_N

ClientSampleId :

DCKD2





Tgt Ion:153 Resp: 8167

Ion Ratio Lower Upper

153 100

152 51.6 38.2 57.2

154 85.5 71.3 106.9

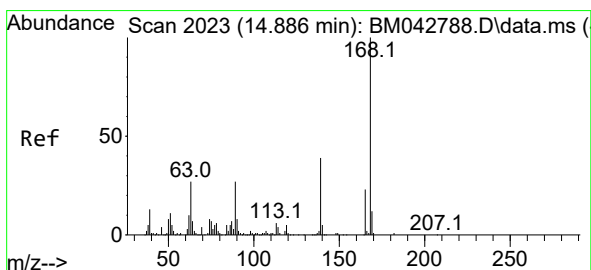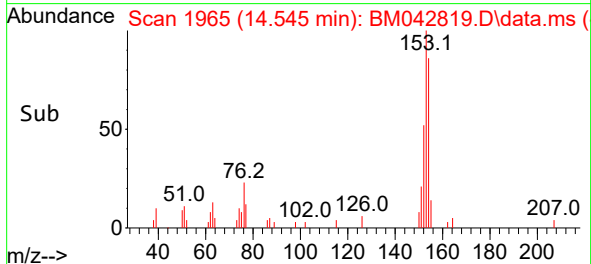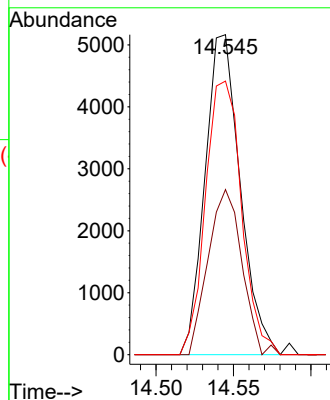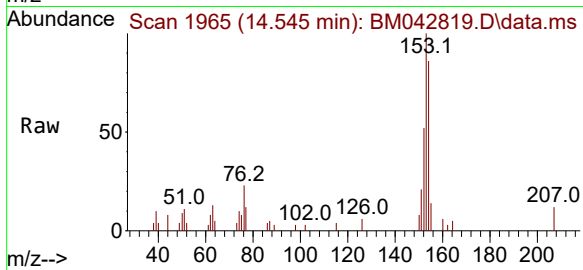

#56

Dibenzofuran

Concen: 3.262 ng/u1

RT: 14.886 min Scan# 2023

Delta R.T. -0.000 min

Lab File: BM042819.D




Acq: 16 Nov 2023 23:21


Tgt Ion:168 Resp: 21682

Ion Ratio Lower Upper

168 100

139 38.2 30.8 46.2

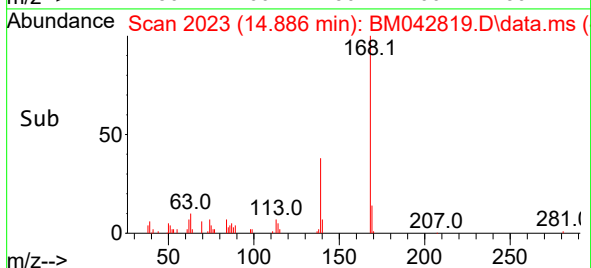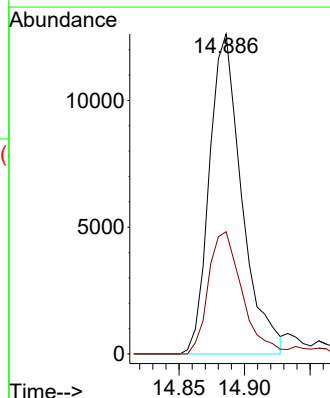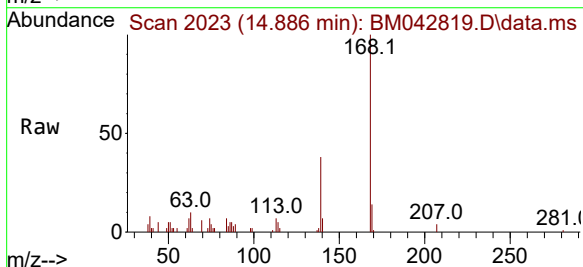

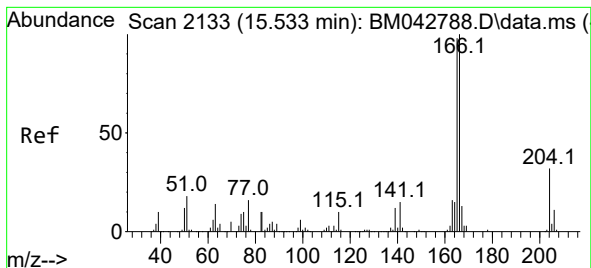

#61

Fluorene

Concen: 1.932 ng/ul

RT: 15.527 min Scan# 2133

Delta R.T. -0.006 min

Lab File: BM042819.D

Acq: 16 Nov 2023 23:21

Instrument :

BNA_N

ClientSampleId :

DCKD2





Tgt Ion:166 Resp: 10902

Ion Ratio Lower Upper

166 100

165 101.4 79.3 118.9

167 17.2 10.6 15.8#

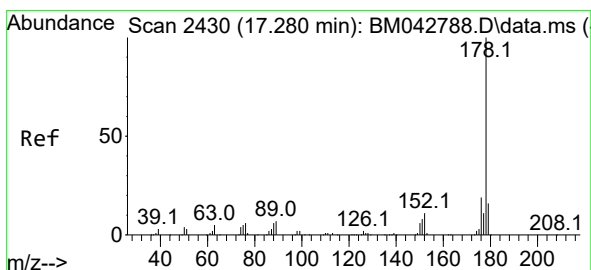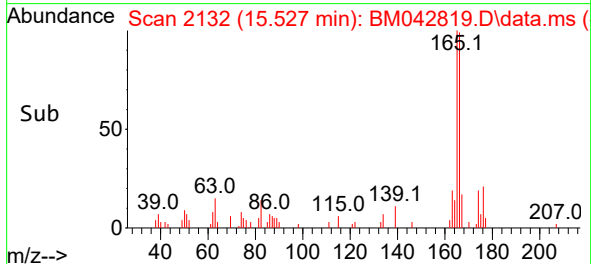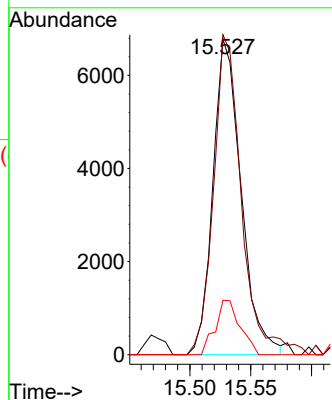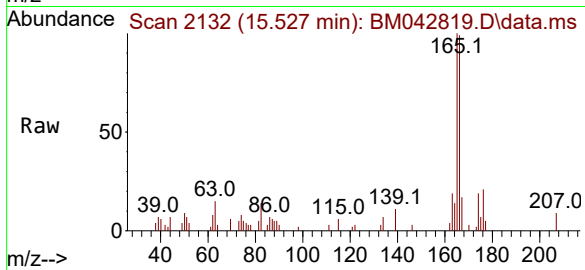

#72

Phenanthrene

Concen: 1.017 ng/ul

RT: 17.274 min Scan# 2429

Delta R.T. -0.006 min

Lab File: BM042819.D

Acq: 16 Nov 2023 23:21




Tgt Ion:178 Resp: 8929


Ion Ratio Lower Upper

178 100

179 14.8 11.4 17.2

176 15.4 15.5 23.3#

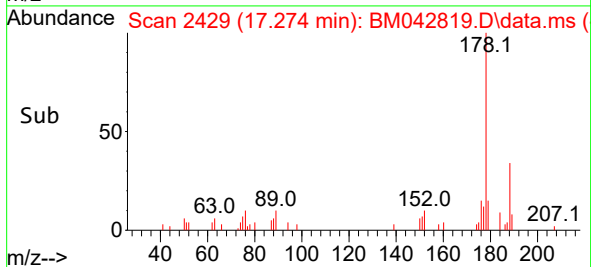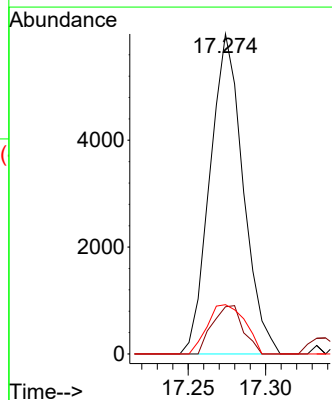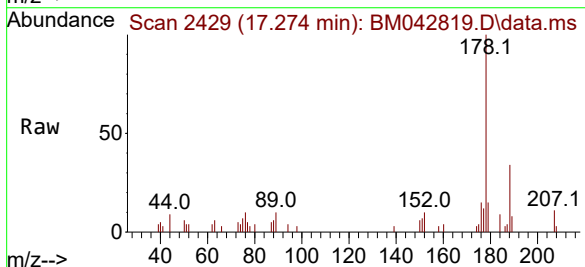

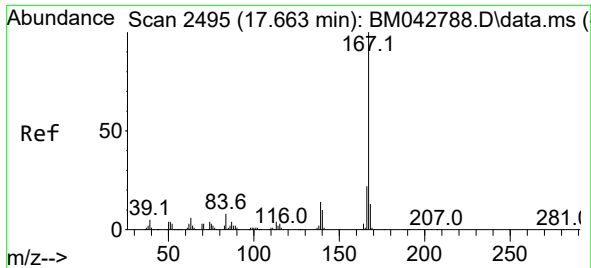

#77

Carbazole

Concen: 5.331 ng/ul

RT: 17.662 min Scan# 24

Delta R.T. -0.000 min

Lab File: BM042819.D


Acq: 16 Nov 2023 23:21

Instrument :

BNA_N

ClientSampleId :

DCKD2

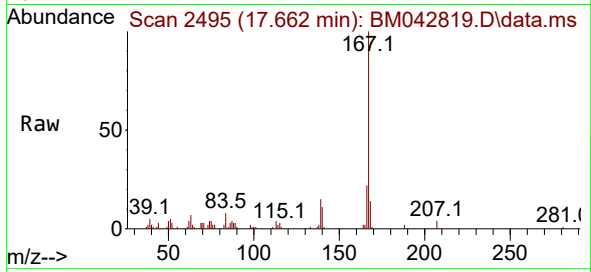

Tgt Ion:167 Resp: 38884

Ion Ratio Lower Upper

167 100

166 21.8 17.2 25.8

139 14.9 10.8 16.2

