

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028634.D
 Acq On : 15 Nov 2023 18:50
 Operator : MA/JU
 Sample : PB157056BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK056

Quant Time: Nov 15 23:01:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 15 18:38:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.696	152	6247	0.400	ng/ul	0.02
4) Naphthalene-d8	10.470	136	25063	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.322	164	13870	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.083	188	26332	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240	20270	0.400	ng/ul	# 0.00
23) Perylene-d12	23.581	264	29121	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.118	96	49142	7.118	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.109	152	3658	0.097	ng/ul	0.04
18) Fluoranthene-d10	19.119	212	18542	0.284	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.317	166	3098	0.052	ng/ul#	16
20) Pyrene	19.477	202	3476	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.426	252	7231	0.070	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028634.D
Acq On : 15 Nov 2023 18:50
Operator : MA/JU
Sample : PB157056BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK056

Quant Time: Nov 15 23:01:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 18:38:25 2023
Response via : Initial Calibration




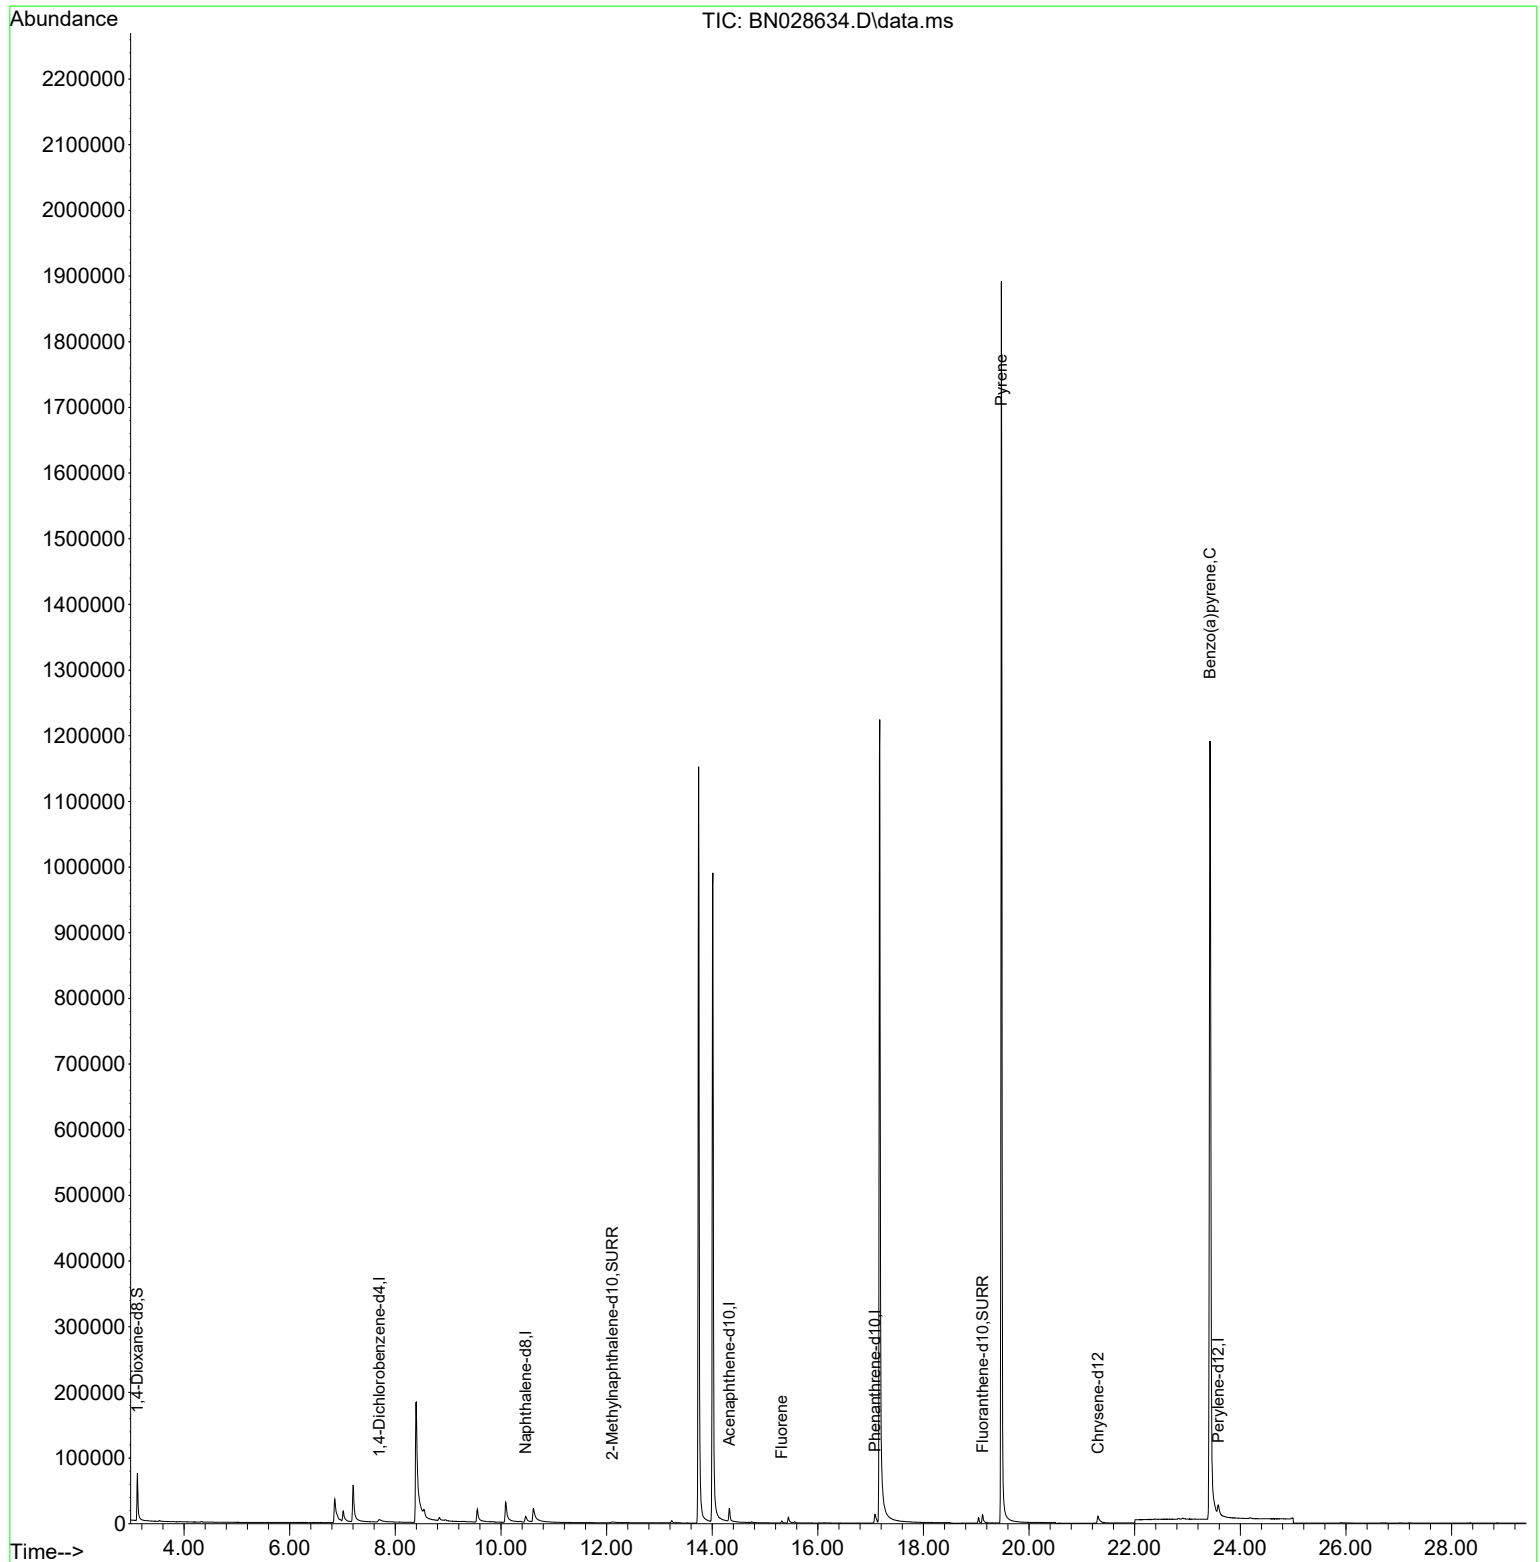


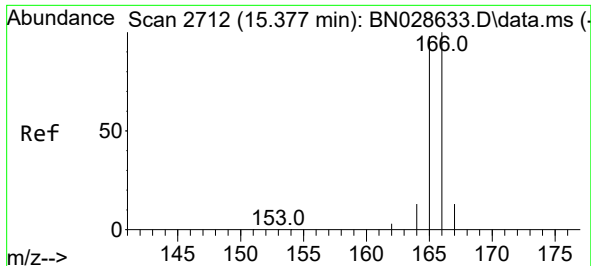

#12
Fluorene
Concen: 0.052 ng/ul
RT: 15.317 min Scan# 2699
Delta R.T. -0.060 min
Lab File: BN028634.D
Acq: 15 Nov 2023 18:50




Instrument :
BNA_N
ClientSampleId :
SBLK056


Tgt Ion:166 Resp: 3098
Ion Ratio Lower Upper
166 100
165 9.4 78.6 118.0#
167 30.7 11.0 16.6#

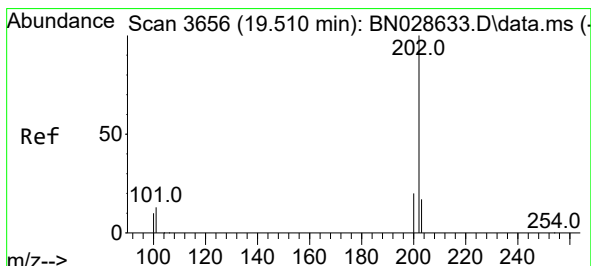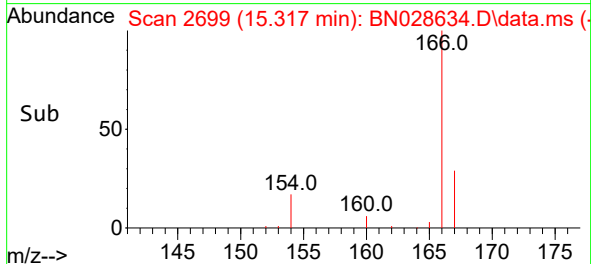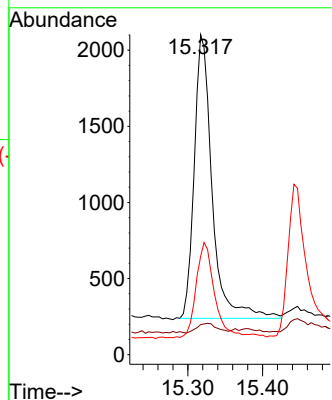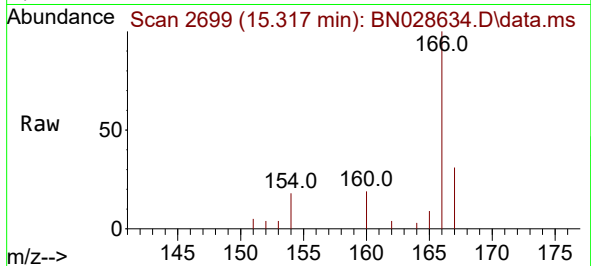

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.477 min Scan# 3649
Delta R.T. -0.033 min
Lab File: BN028634.D
Acq: 15 Nov 2023 18:50


Tgt Ion:202 Resp: 3476
Ion Ratio Lower Upper
202 100
101 153.6 10.3 15.5#
100 1102.5 8.2 12.2#

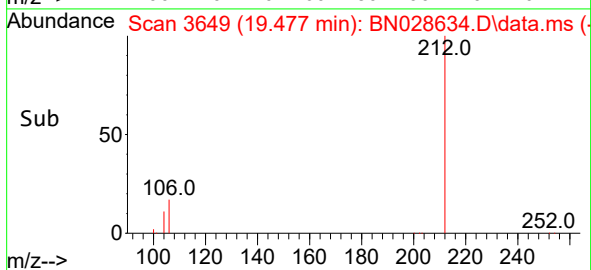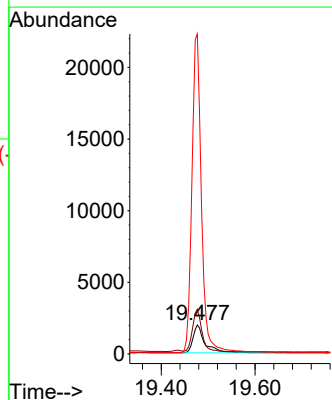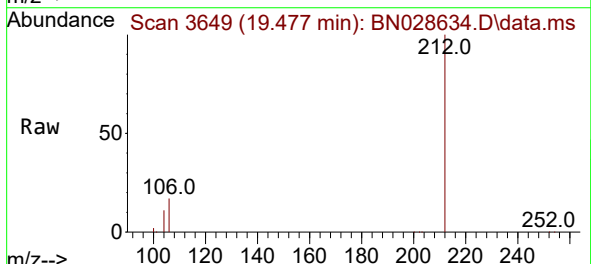

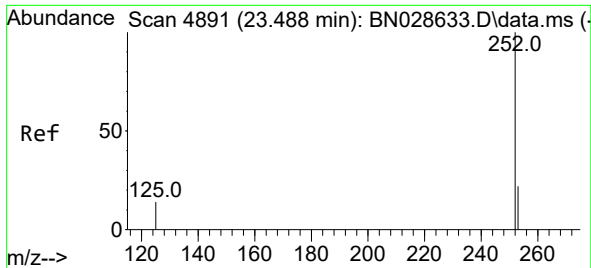

#26
Benzo(a)pyrene
Concen: 0.070 ng/ul
RT: 23.426 min Scan# 41
Delta R.T. -0.062 min
Lab File: BN028634.D
Acq: 15 Nov 2023 18:50

Instrument :
BNA_N
ClientSampleId :
SBLK056

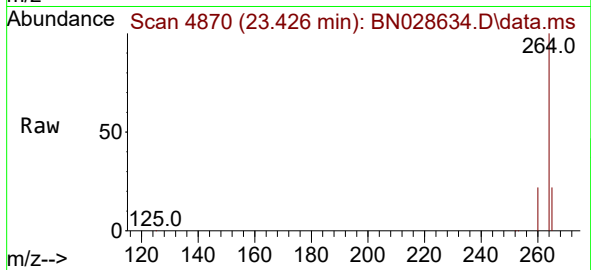

Tgt Ion:252 Resp: 7231
Ion Ratio Lower Upper
252 100
253 47.7 19.0 28.6#
125 43.4 13.2 19.8#

