

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028636.D
 Acq On : 15 Nov 2023 20:10
 Operator : MA/JU
 Sample : 05337-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ1

Quant Time: Nov 15 23:02:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 15 18:38:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	5553	0.400	ng/ul	0.02
4) Naphthalene-d8	10.470	136	23624	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.327	164	13136	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.083	188	23687	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.301	240	16777	0.400	ng/ul	# 0.00
23) Perylene-d12	23.584	264	23315	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.118	96	36537	5.953	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.092	152	5495	0.155	ng/ul	0.03
18) Fluoranthene-d10	19.119	212	26065	0.483	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.156	88	2108	0.311	ng/ul#	87
20) Pyrene	19.477	202	4331	0.059	ng/ul#	1
26) Benzo(a)pyrene	23.429	252	8084	0.098	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028636.D
Acq On : 15 Nov 2023 20:10
Operator : MA/JU
Sample : 05337-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDJ1

Quant Time: Nov 15 23:02:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 18:38:25 2023
Response via : Initial Calibration




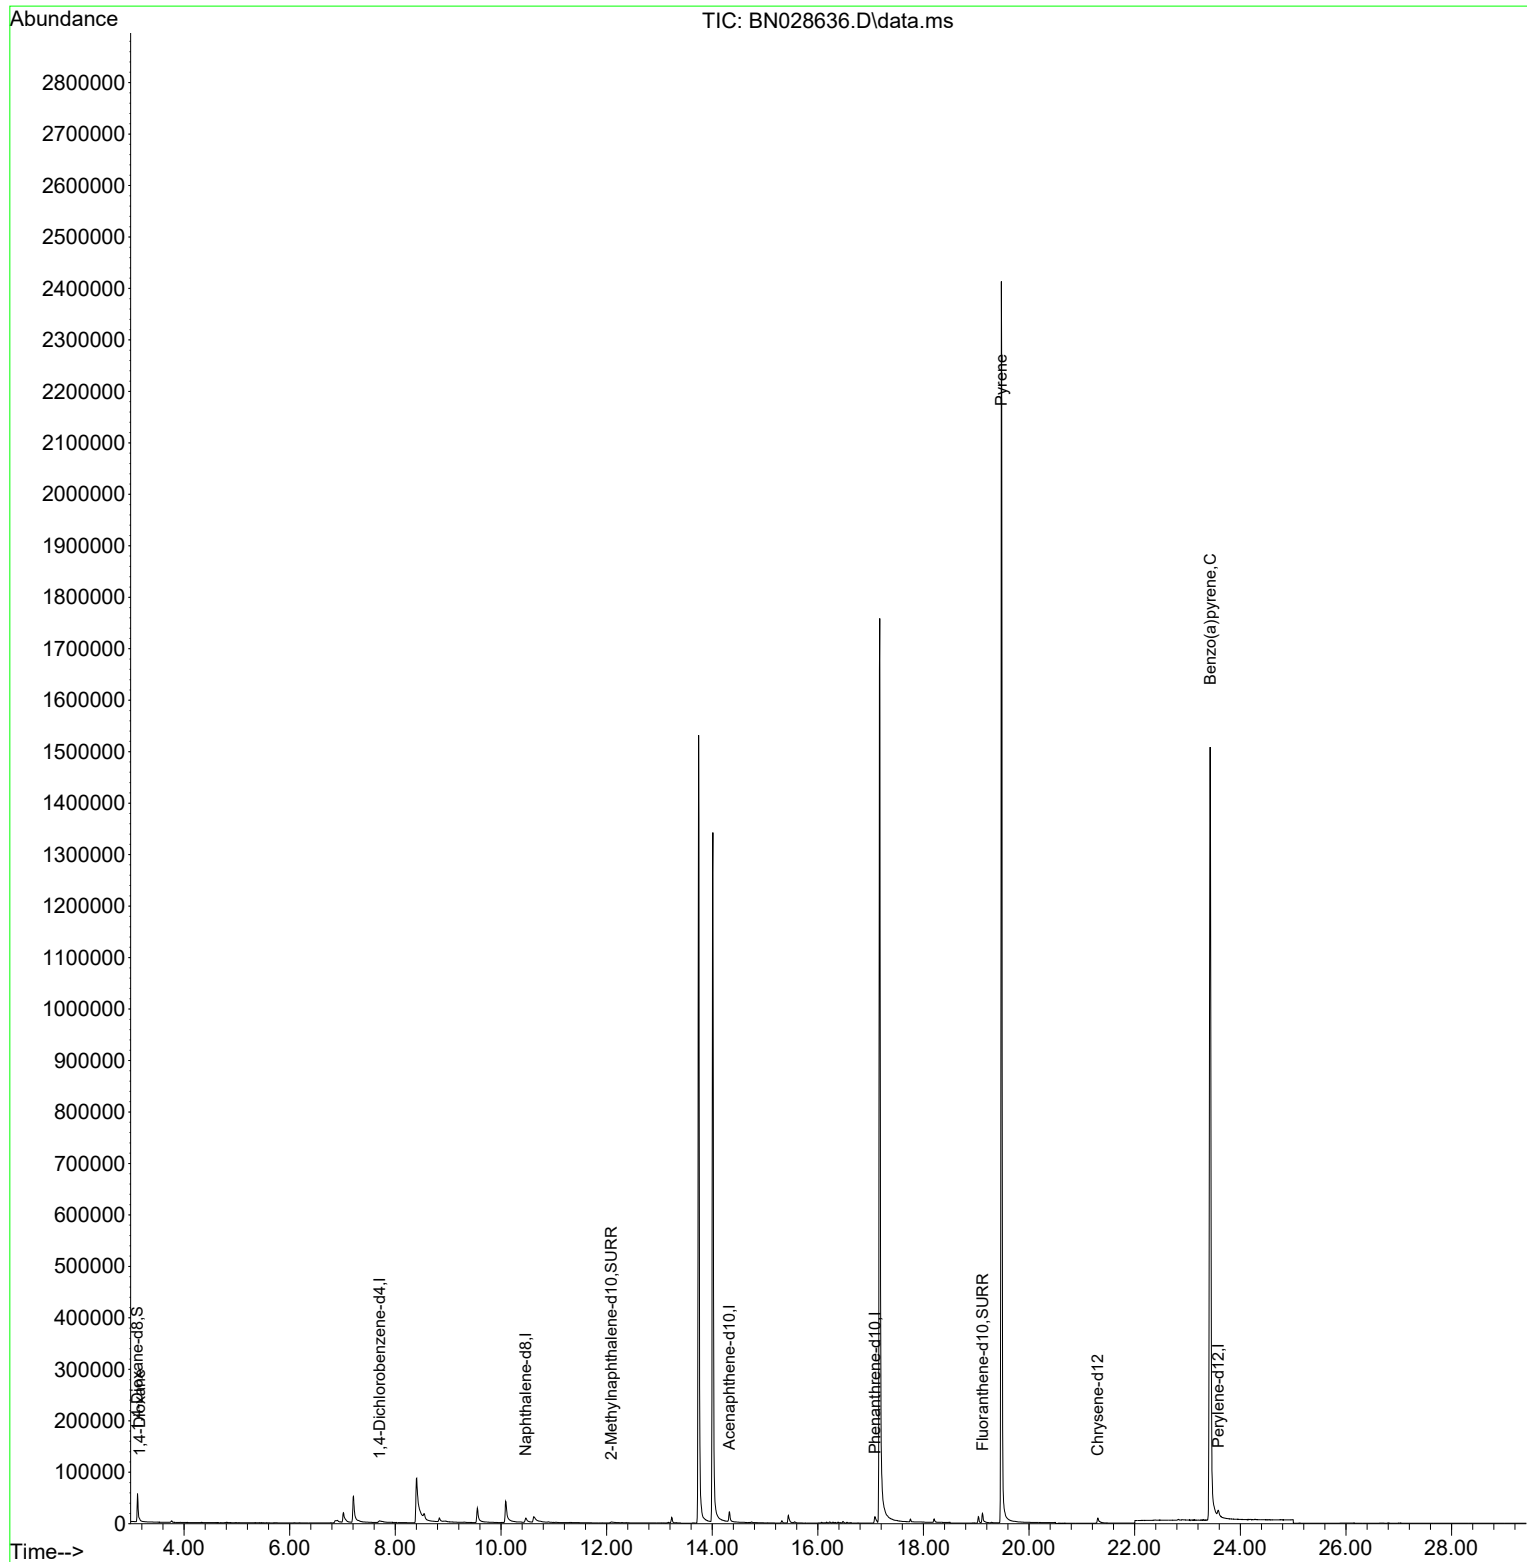


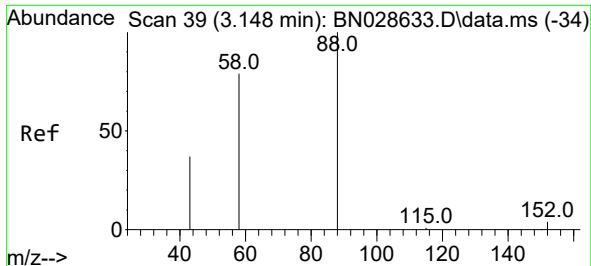

#2
1,4-Dioxane
Concen: 0.311 ng/ul
RT: 3.156 min Scan# 41
Delta R.T. 0.008 min
Lab File: BN028636.D
Acq: 15 Nov 2023 20:10




Instrument :
BNA_N
ClientSampleId :
GCDJ1


Tgt Ion: 88 Resp: 2108
Ion Ratio Lower Upper
88 100
43 42.2 32.9 49.3
58 36.3 41.8 62.8#

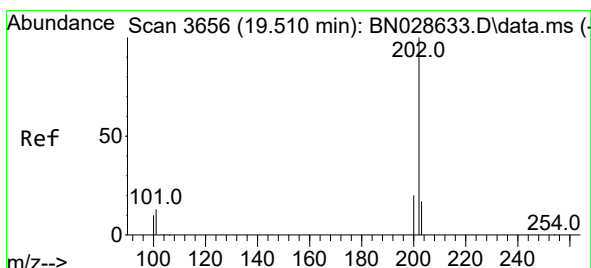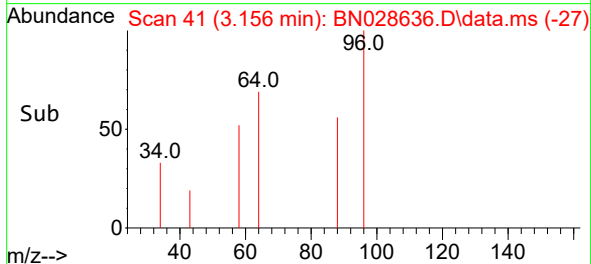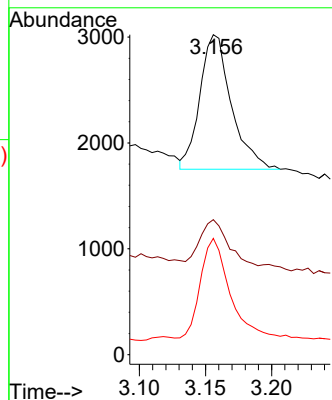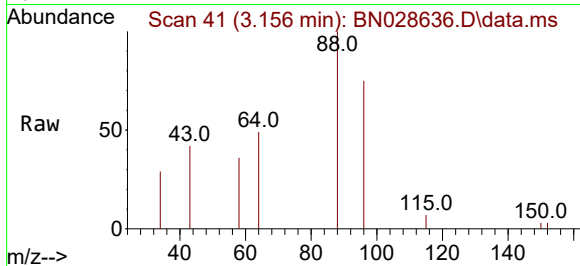

#20
Pyrene
Concen: 0.059 ng/ul
RT: 19.477 min Scan# 3649
Delta R.T. -0.033 min
Lab File: BN028636.D
Acq: 15 Nov 2023 20:10


Tgt Ion: 202 Resp: 4331
Ion Ratio Lower Upper
202 100
101 153.2 10.3 15.5#
100 1116.2 8.2 12.2#

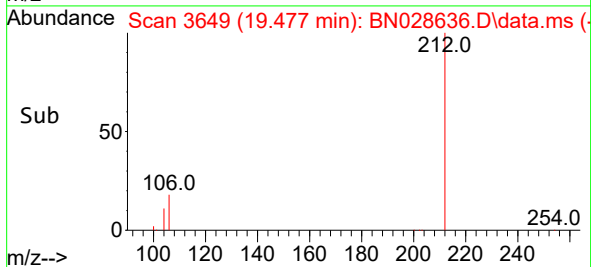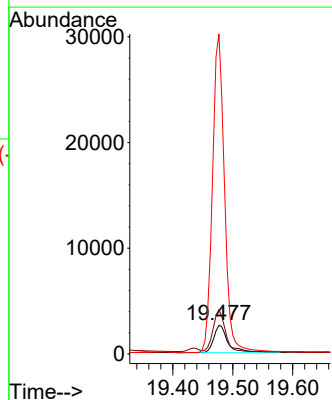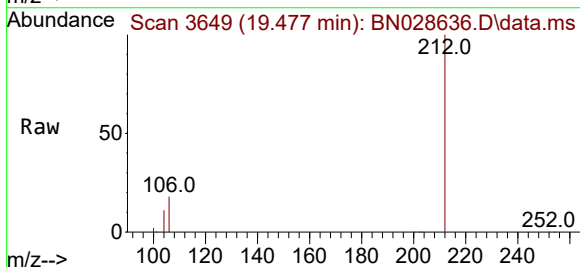

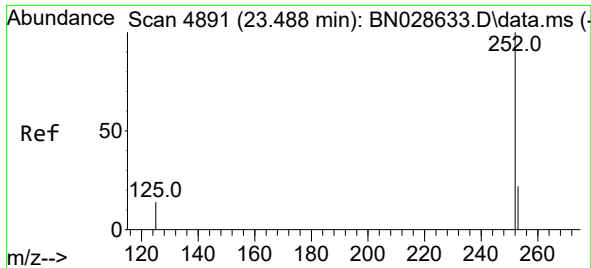

#26
 Benzo(a)pyrene
 Concen: 0.098 ng/ul
 RT: 23.429 min Scan# 4871
 Delta R.T. -0.059 min
 Lab File: BN028636.D
 Acq: 15 Nov 2023 20:10

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ1

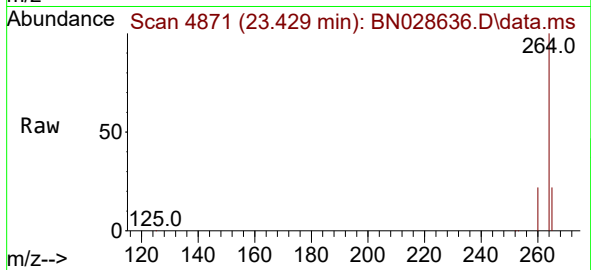

Tgt Ion:252 Resp: 8084
 Ion Ratio Lower Upper
 252 100
 253 44.2 19.0 28.6#
 125 40.8 13.2 19.8#

