

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028667.D
 Acq On : 16 Nov 2023 16:59
 Operator : MA/JU
 Sample : 05349-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BPOW5-3-20231108

Quant Time: Nov 16 18:09:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 14:20:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.879	152	1743	0.400	ng/ul	# 0.08
4) Naphthalene-d8	10.549	136	8045	0.400	ng/ul	# 0.06
9) Acenaphthene-d10	14.334	164	9369	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.097	188	13809	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.303	240	14501	0.400	ng/ul	# 0.00
23) Perylene-d12	23.583	264	14293	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.141	96	17	0.009	ng/ul	0.02
6) 2-Methylnaphthalene-d10	12.149	152	3106	0.256	ng/ul	0.04
18) Fluoranthene-d10	19.121	212	20097	0.431	ng/ul	0.00
Target Compounds				Qvalue		
2) 1,4-Dioxane	3.154	88	5340	2.508	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028667.D
Acq On : 16 Nov 2023 16:59
Operator : MA/JU
Sample : 05349-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BPOW5-3-20231108

Quant Time: Nov 16 18:09:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 14:20:35 2023
Response via : Initial Calibration

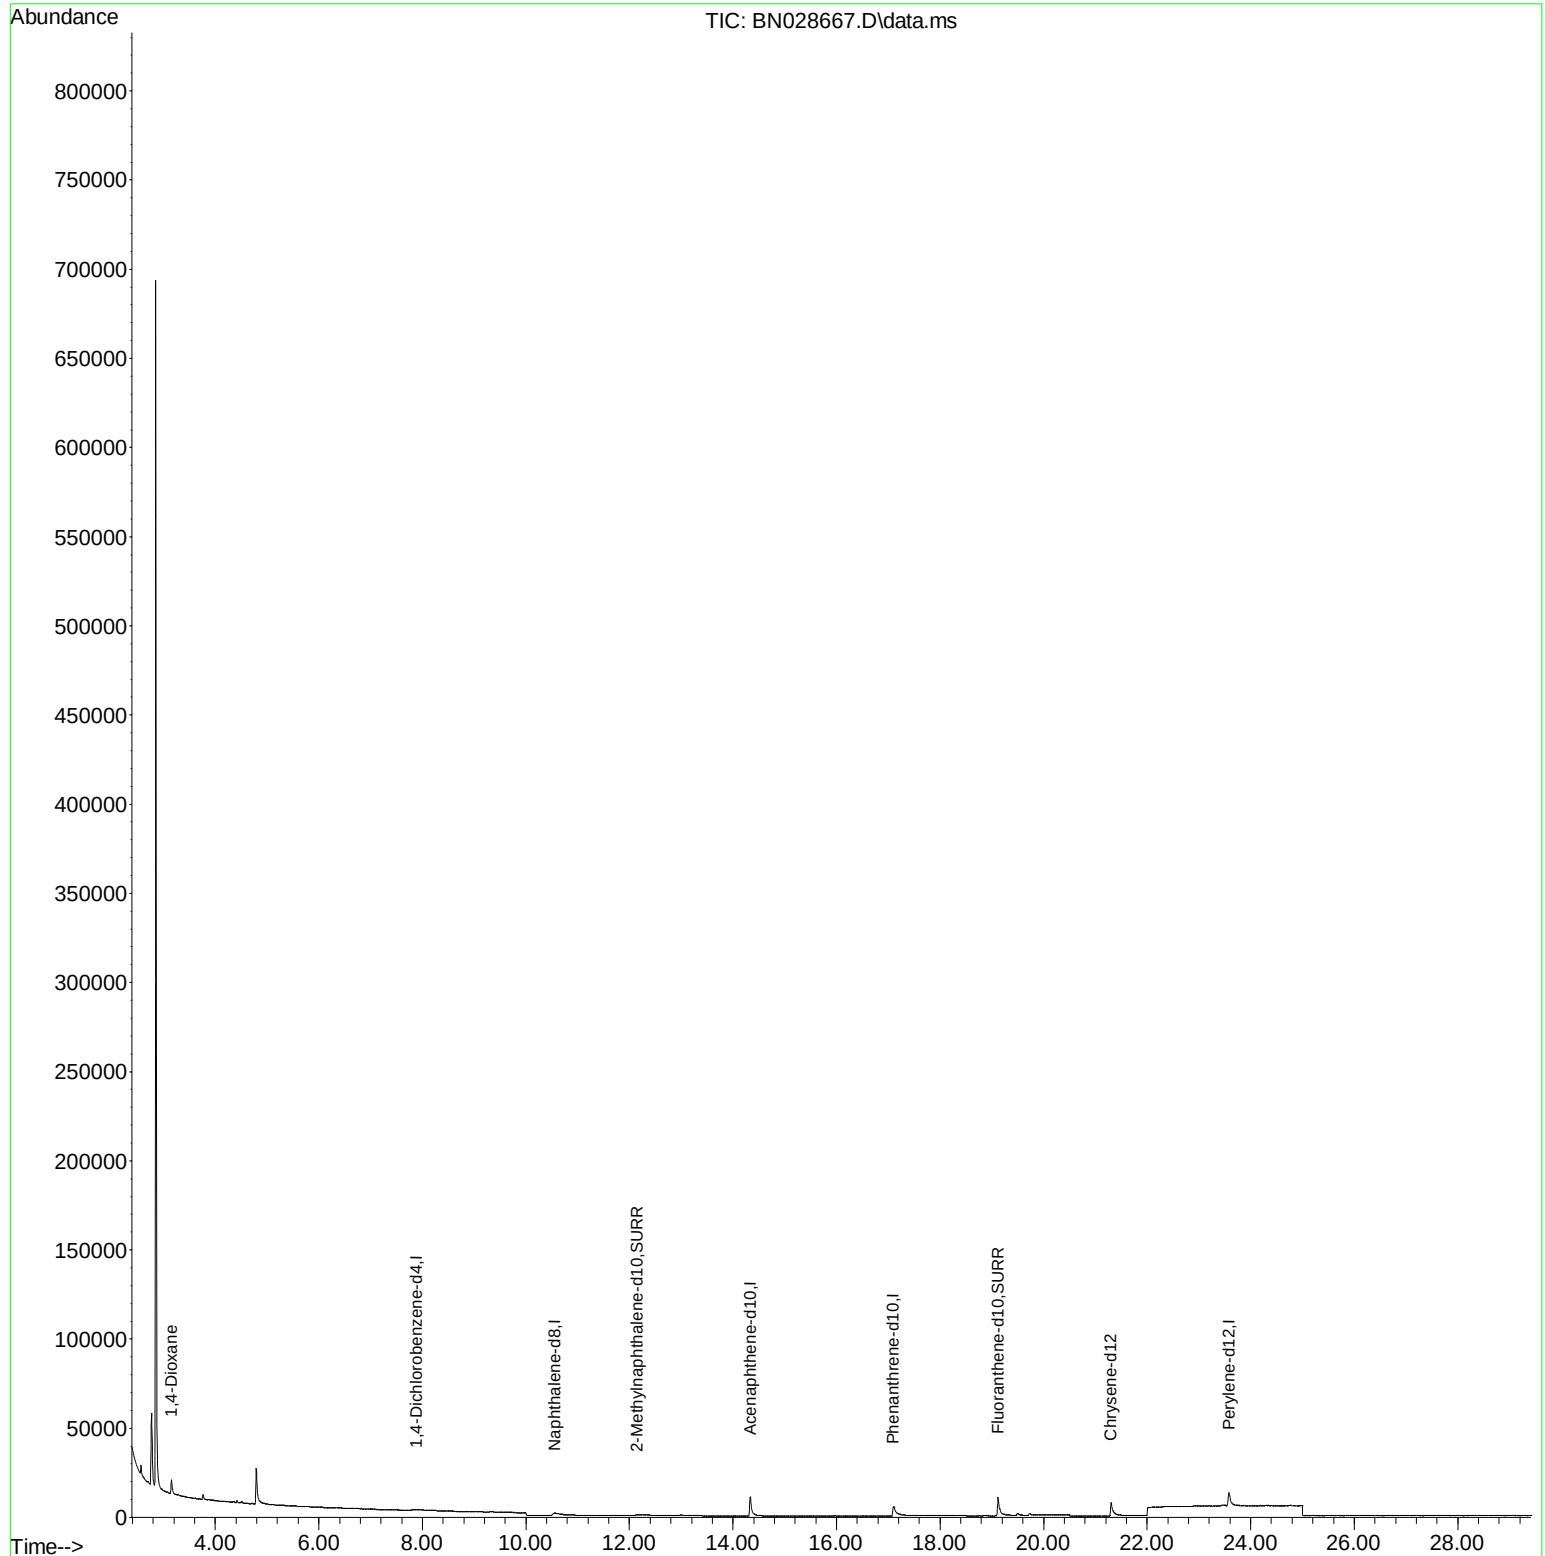

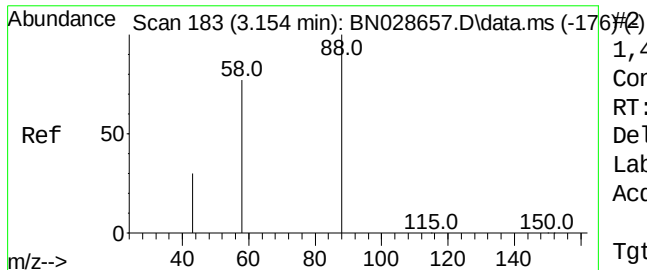

1,4-Dioxane

Concen: 2.508 ng/ul

RT: 3.154 min Scan#

Delta R.T. -0.000 min

Lab File: BN028667.D


Acq: 16 Nov 2023 16:59

Instrument :

BNA_N

ClientSampleId :

BPOW5-3-20231108

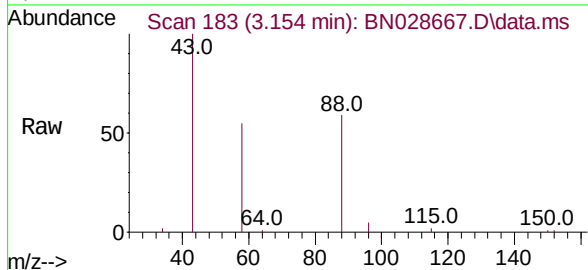

Tgt Ion: 88 Resp: 5340

Ion Ratio Lower Upper

88 100

43 170.1 32.9 49.3#

58 93.9 41.8 62.8#

