




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028646.D
 Acq On : 16 Nov 2023 02:44
 Operator : MA/JU
 Sample : PB157060BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK060

Manual IntegrationsAPPROVED

Quant Time: Nov 16 04:37:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 04:34:21 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/20/2023

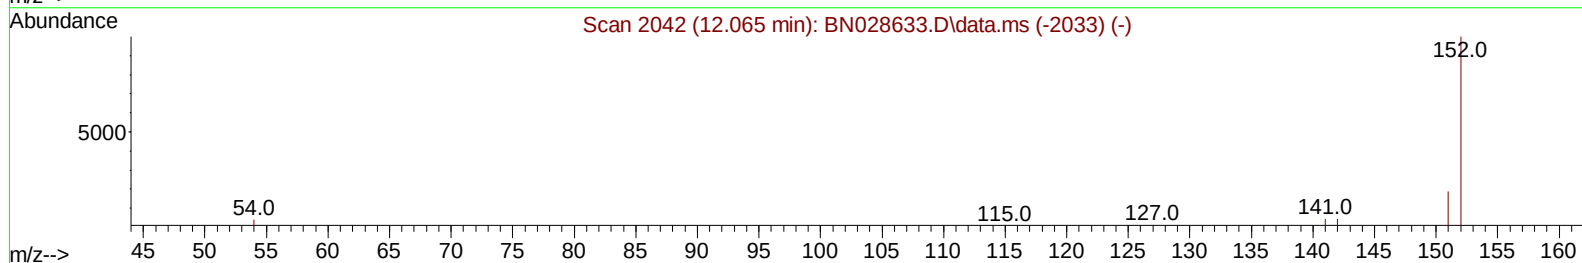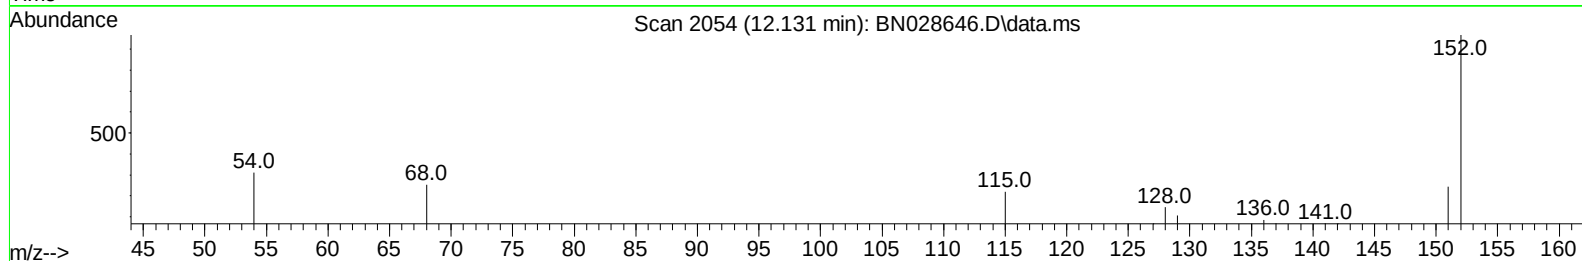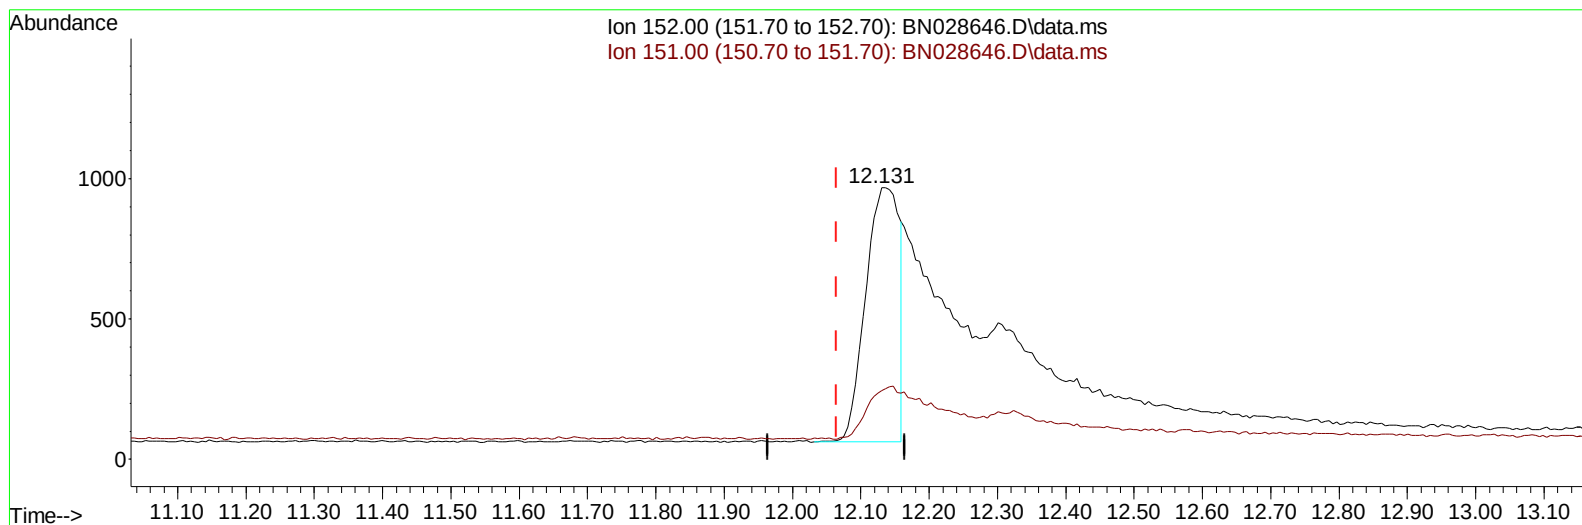

TIC: BN028646.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.131min (+ 0.066) 0.07 ng/u1

response 3079

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	19.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028646.D
 Acq On : 16 Nov 2023 02:44
 Operator : MA/JU
 Sample : PB157060BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK060

Manual IntegrationsAPPROVED

Quant Time: Nov 16 04:37:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 04:34:21 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/20/2023

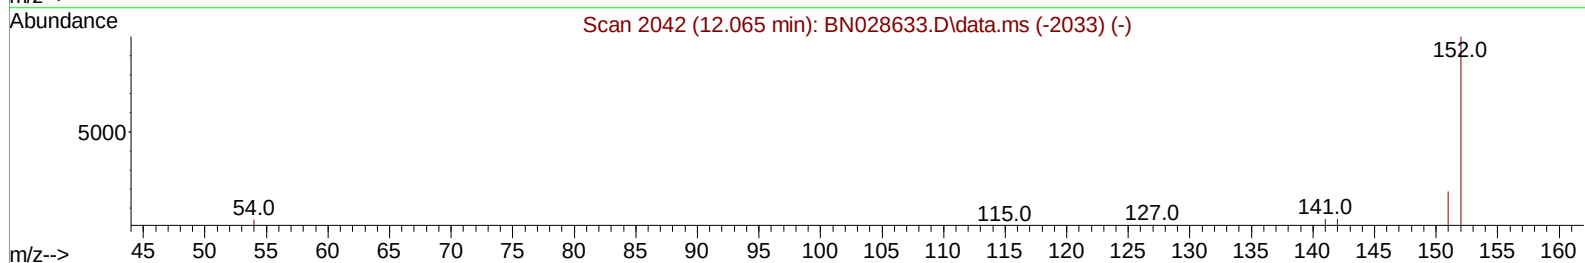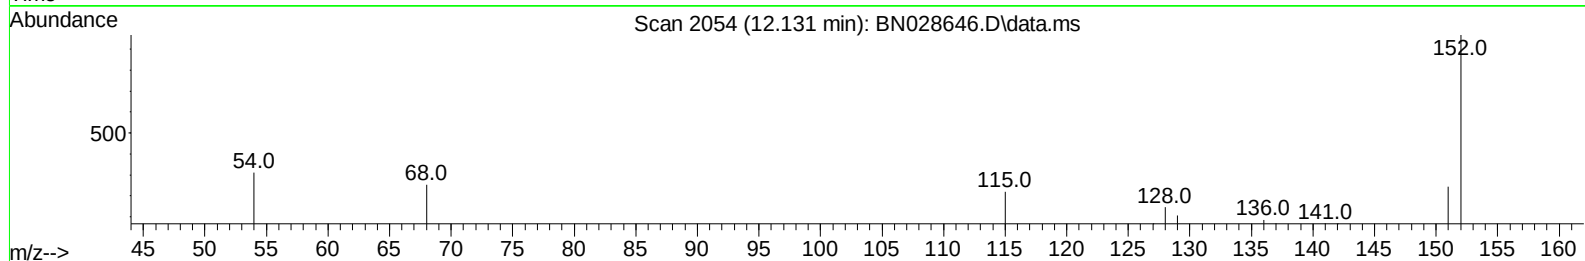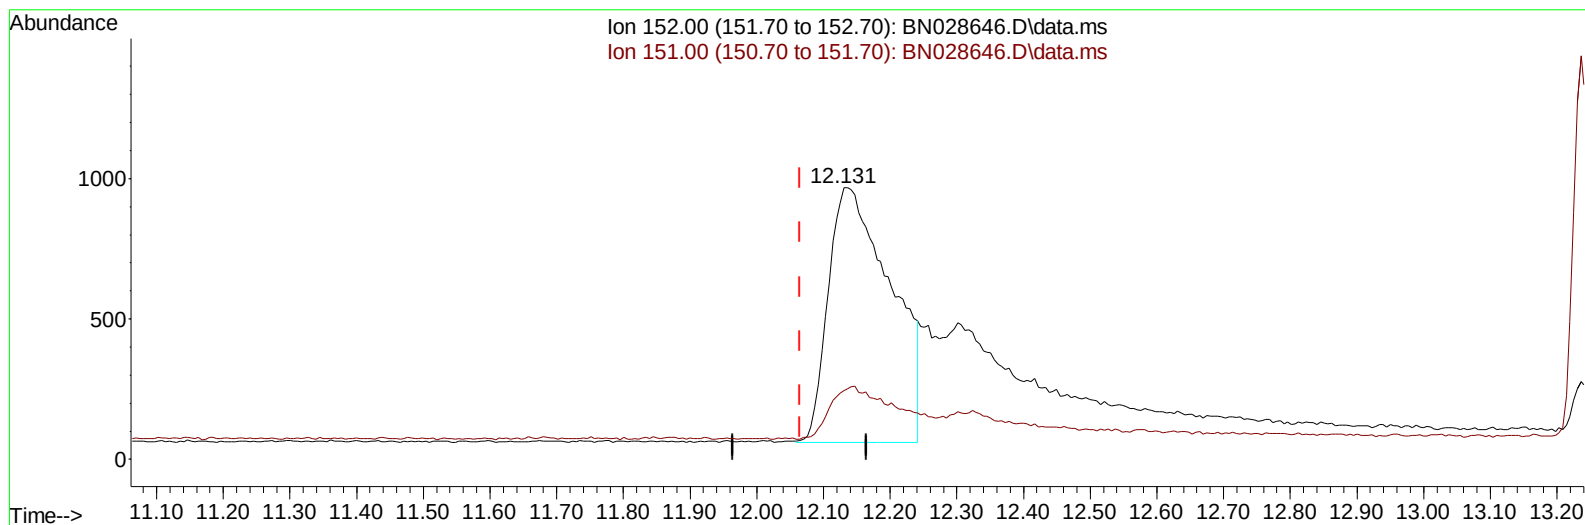

TIC: BN028646.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.131min (+ 0.066) 0.13 ng/ul m

response 5930

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	10.32#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028646.D
 Acq On : 16 Nov 2023 02:44
 Operator : MA/JU
 Sample : PB157060BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK060

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 16 04:37:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 04:34:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.713	152	6170	0.400	ng/ul	0.03
4) Naphthalene-d8	10.475	136	29413	0.400	ng/ul #	0.01
9) Acenaphthene-d10	14.327	164	18260	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.083	188	36217	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240	24854	0.400	ng/ul #	0.00
23) Perylene-d12	23.575	264	37381	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.114	96	48075	7.050	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.131	152	5930m	0.134	ng/ul	0.07
18) Fluoranthene-d10	19.119	212	25376	0.317	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028646.D
Acq On : 16 Nov 2023 02:44
Operator : MA/JU
Sample : PB157060BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK060

Manual IntegrationsAPPROVED

Quant Time: Nov 16 04:37:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 04:34:21 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2023
Supervised By :mohammad ahmed 11/20/2023

