




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028658.D
Acq On : 16 Nov 2023 11:36
Operator : MA/JU
Sample : PB157172BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK172

Manual IntegrationsAPPROVED

Quant Time: Nov 16 22:45:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

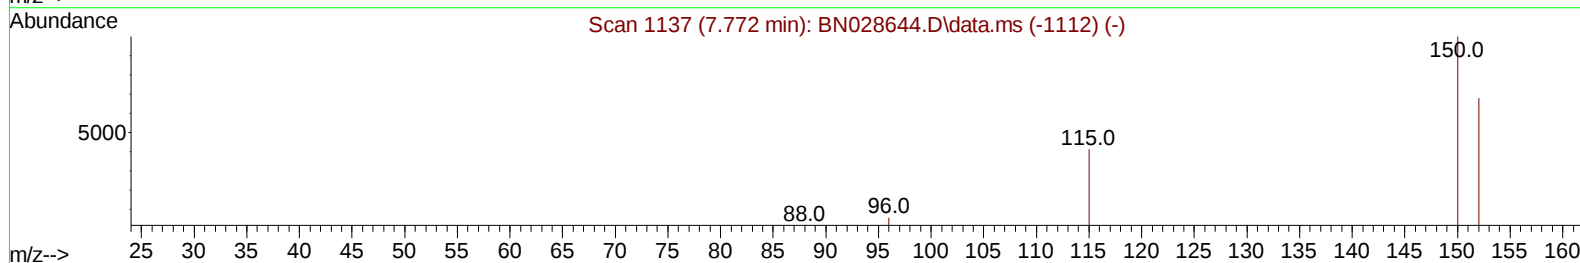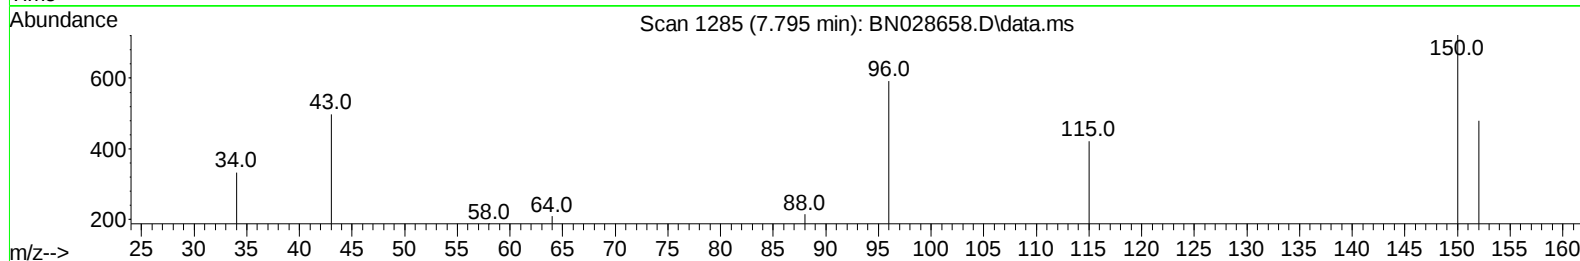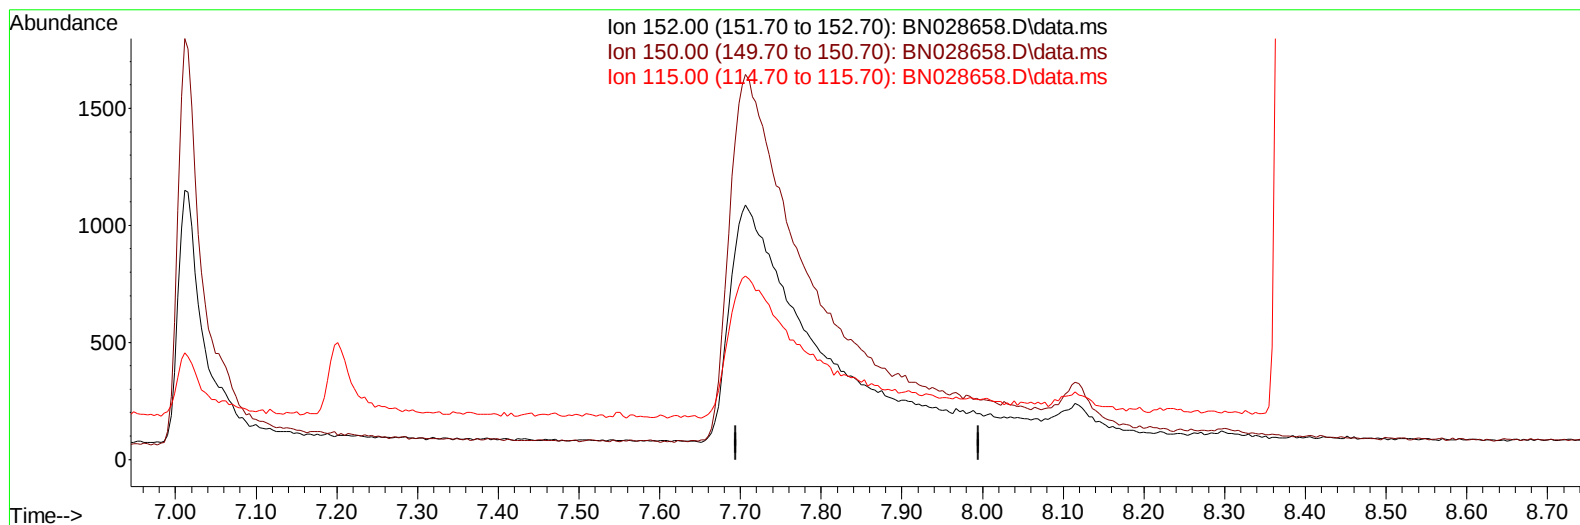

TIC: BN028658.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028658.D
Acq On : 16 Nov 2023 11:36
Operator : MA/JU
Sample : PB157172BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK172

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 16 22:45:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

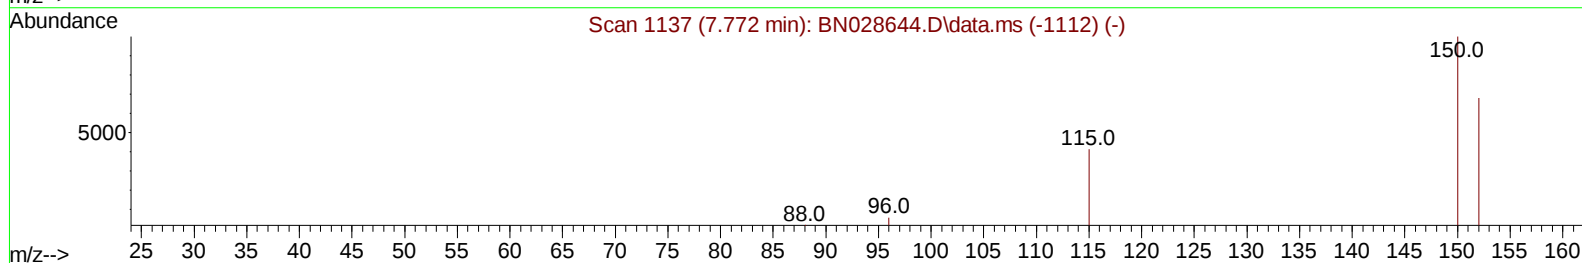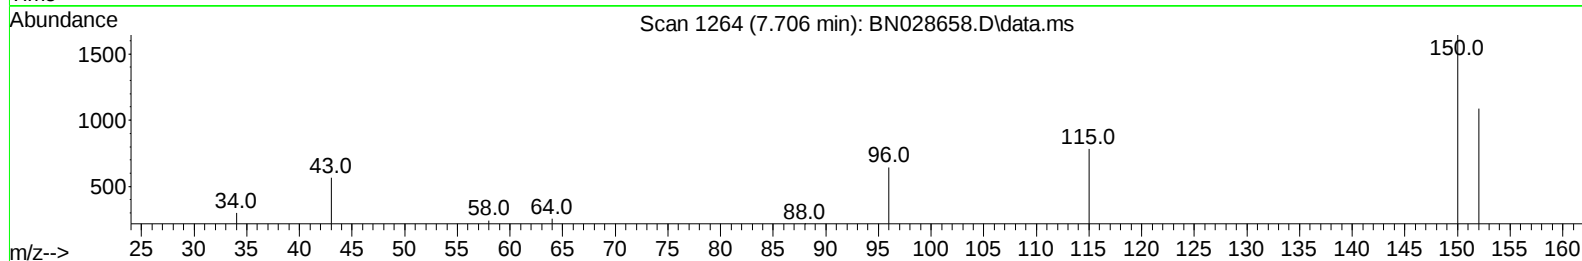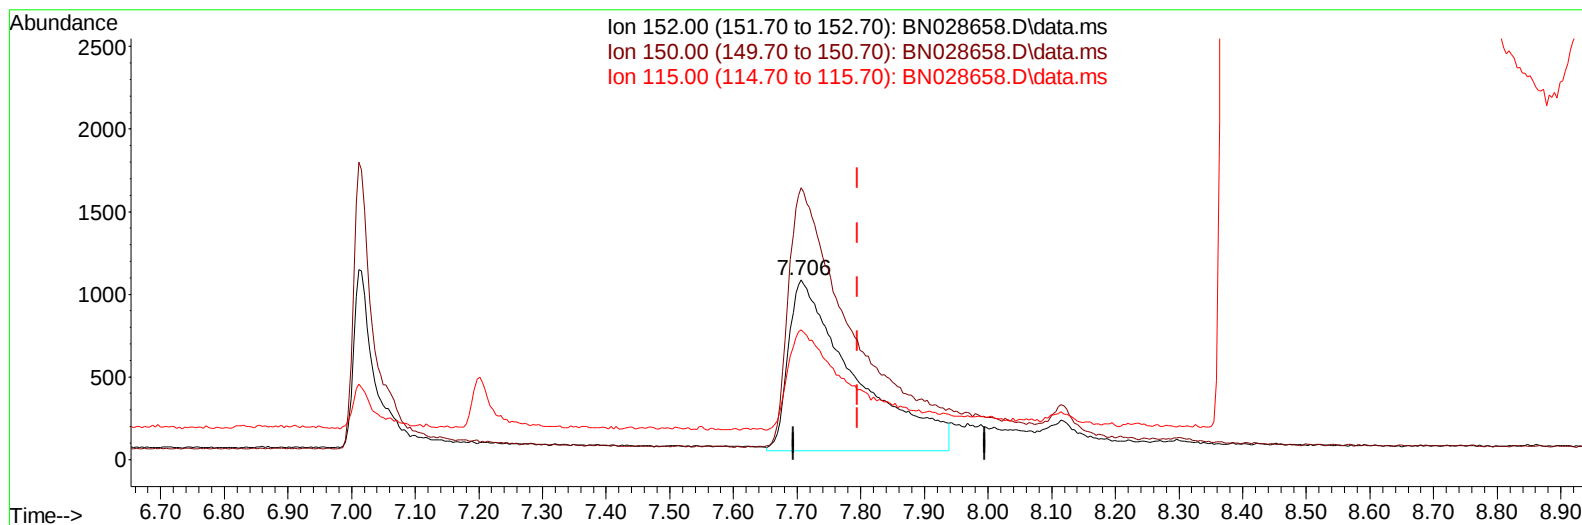

TIC: BN028658.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.706min (-0.089) 0.40 ng/ul m

response 7479

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	151.24
115.00	62.20	72.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028658.D
 Acq On : 16 Nov 2023 11:36
 Operator : MA/JU
 Sample : PB157172BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK172

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 16 22:45:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.706	152	7479m	0.400	ng/ul	-0.09
4) Naphthalene-d8	10.473	136	29329	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.325	164	17225	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.085	188	34920	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240	21621	0.400	ng/ul	# 0.00
23) Perylene-d12	23.581	264	27723	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	49261	5.960	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.123	152	4420	0.100	ng/ul	0.01
18) Fluoranthene-d10	19.122	212	22921	0.329	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028658.D
Acq On : 16 Nov 2023 11:36
Operator : MA/JU
Sample : PB157172BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK172

Manual IntegrationsAPPROVED

Quant Time: Nov 16 22:45:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

