

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028679.D
Acq On : 17 Nov 2023 00:45
Operator : MA/JU
Sample : 05338-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL0




Manual IntegrationsAPPROVED

Quant Time: Nov 17 01:37:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

11/17/2023
Supervised By :mohammad
ahmed

Ion 152.00 (151.70 to 152.70): BN028679.D\data.ms
Ion 150.00 (149.70 to 150.70): BN028679.D\data.ms
Ion 115.00 (114.70 to 115.70): BN028679.D\data.ms

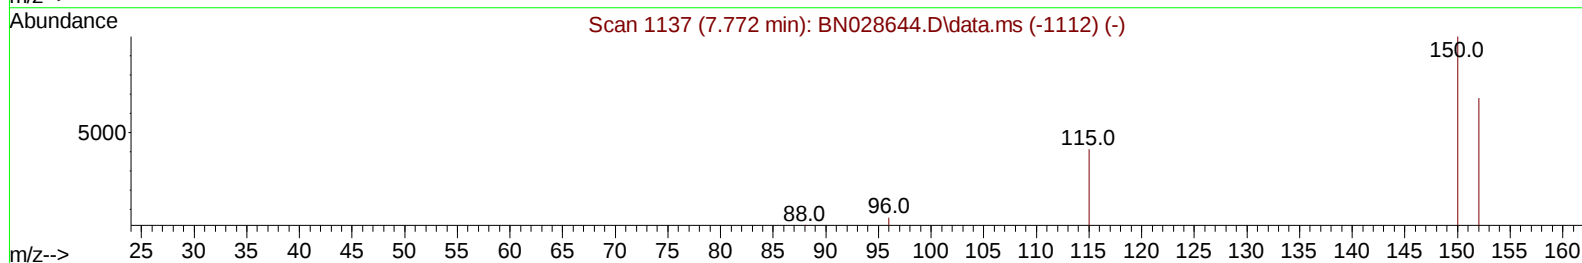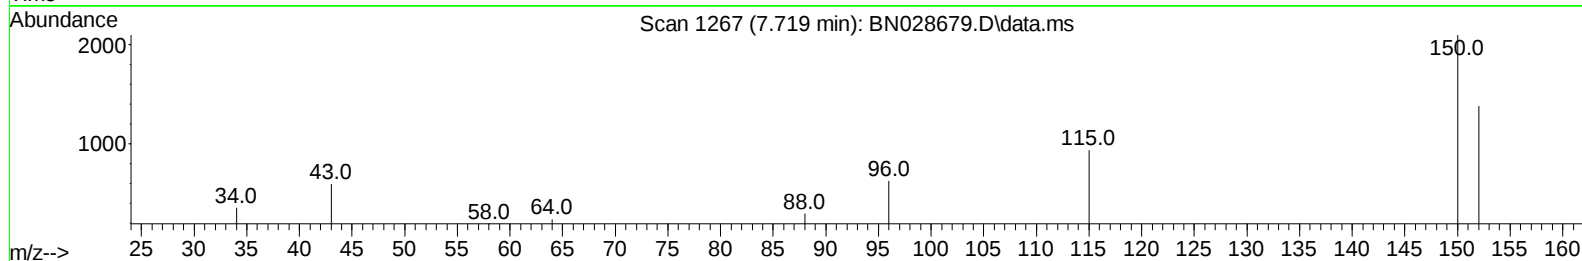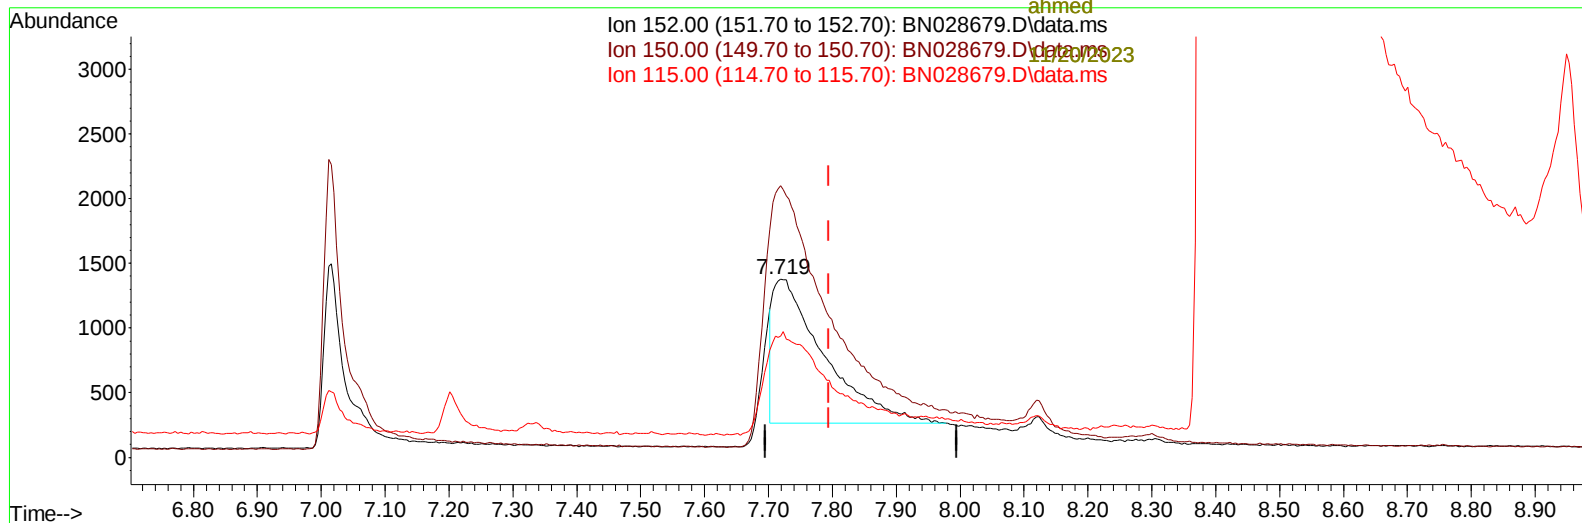

TIC: BN028679.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/u1

response 6228

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	152.14
115.00	62.20	68.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028679.D
Acq On : 17 Nov 2023 00:45
Operator : MA/JU
Sample : 05338-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL0




Manual IntegrationsAPPROVED

Quant Time: Nov 17 01:37:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

11/17/2023
Supervised By :mohammad
ahmed

Ion 152.00 (151.70 to 152.70): BN028679.D\data.ms
Ion 150.00 (149.70 to 150.70): BN028679.D\data.ms
Ion 115.00 (114.70 to 115.70): BN028679.D\data.ms

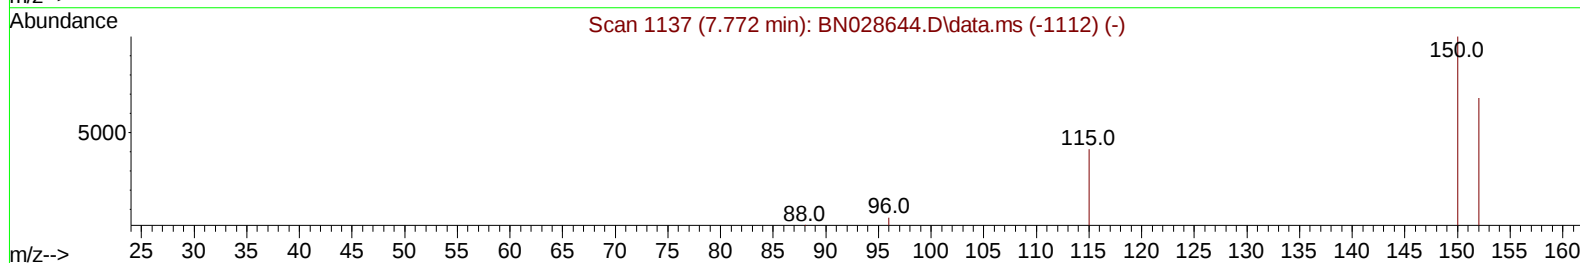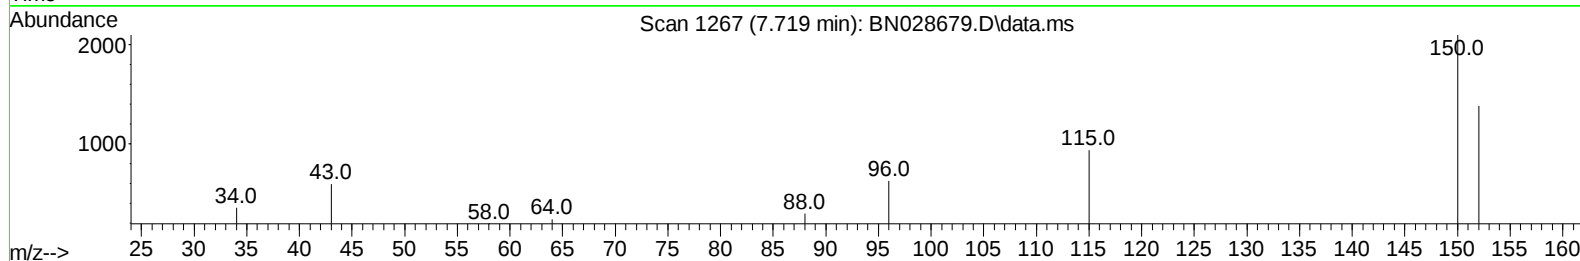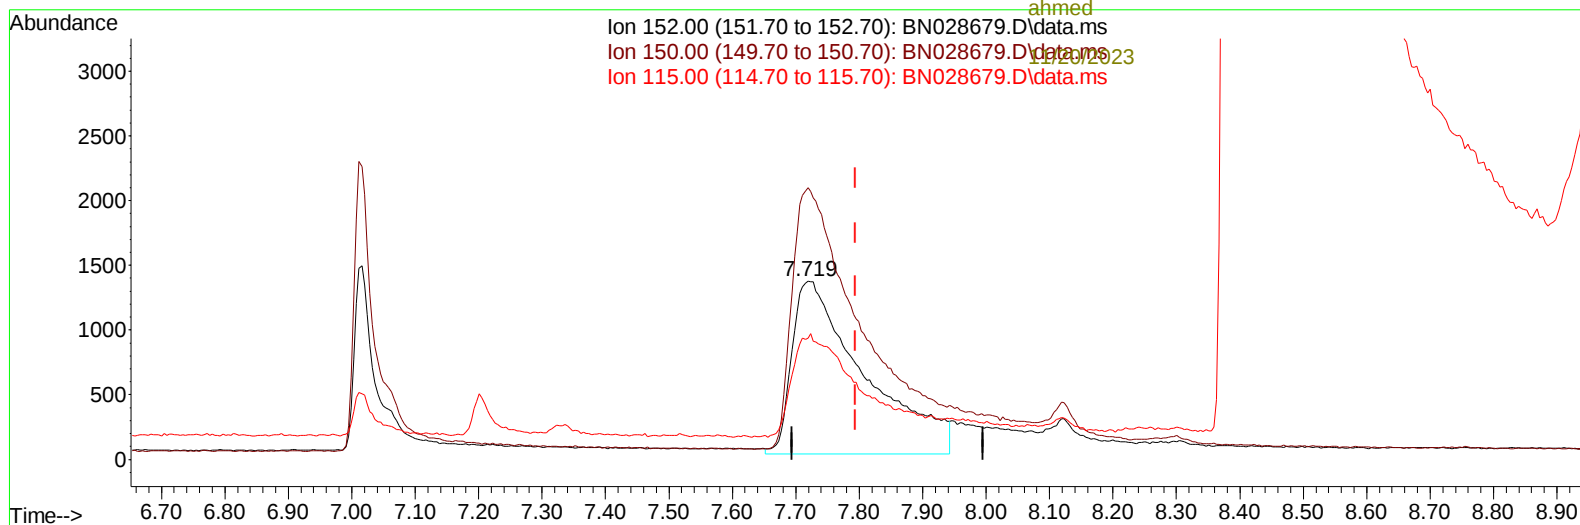

TIC: BN028679.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/ul m

response 10531

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	152.14
115.00	62.20	68.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028679.D
 Acq On : 17 Nov 2023 00:45
 Operator : MA/JU
 Sample : 05338-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 01:37:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----11/20/2023							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.719	152		10531m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.473	136		41184	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164		23584	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.081	188		48363	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.289	240		33636	0.400	ng/ul	# 0.00
23) Perylene-d12	23.569	264		37996	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.116	96		44797	3.849	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.112	152		6780	0.109	ng/ul	0.00
18) Fluoranthene-d10	19.117	212		37422	0.346	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.154	88		1573	0.122	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028679.D
Acq On : 17 Nov 2023 00:45
Operator : MA/JU
Sample : 05338-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL0

Manual IntegrationsAPPROVED

Quant Time: Nov 17 01:37:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

11/17/2023
Supervised By :mohammad
ahmed

11/20/2023

