




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028685.D
Acq On : 17 Nov 2023 04:19
Operator : MA/JU
Sample : 05338-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL6

Manual IntegrationsAPPROVED

Quant Time: Nov 17 04:47:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

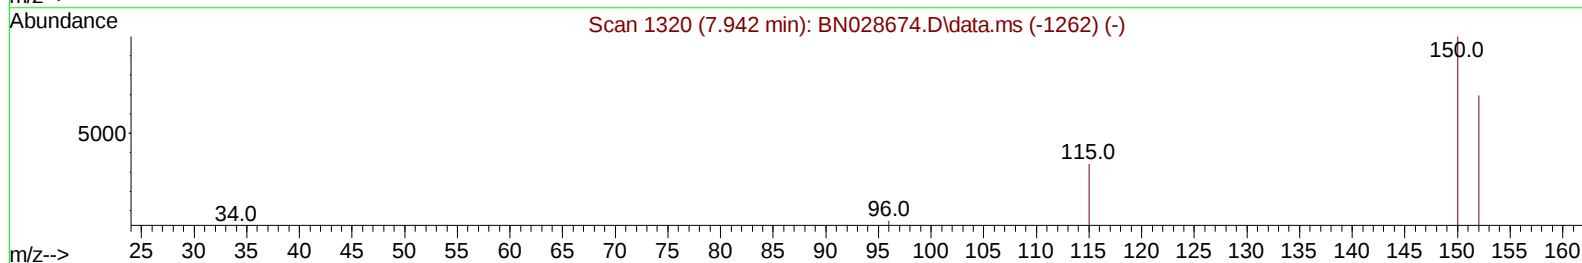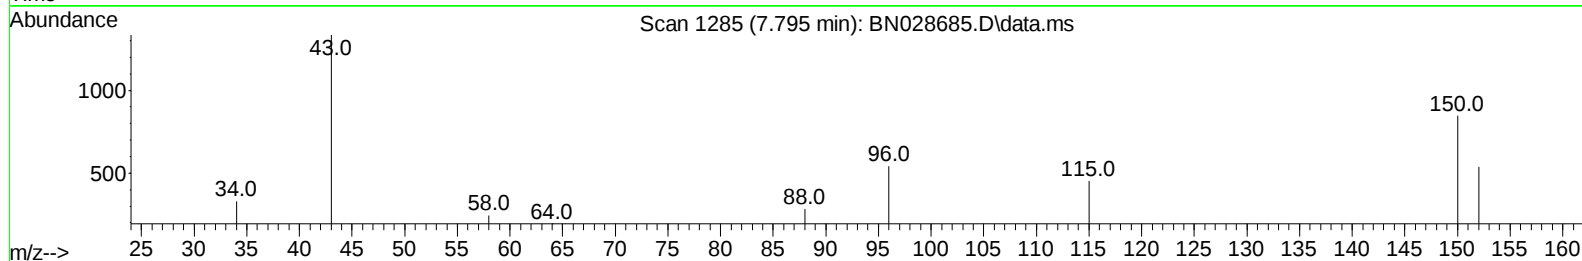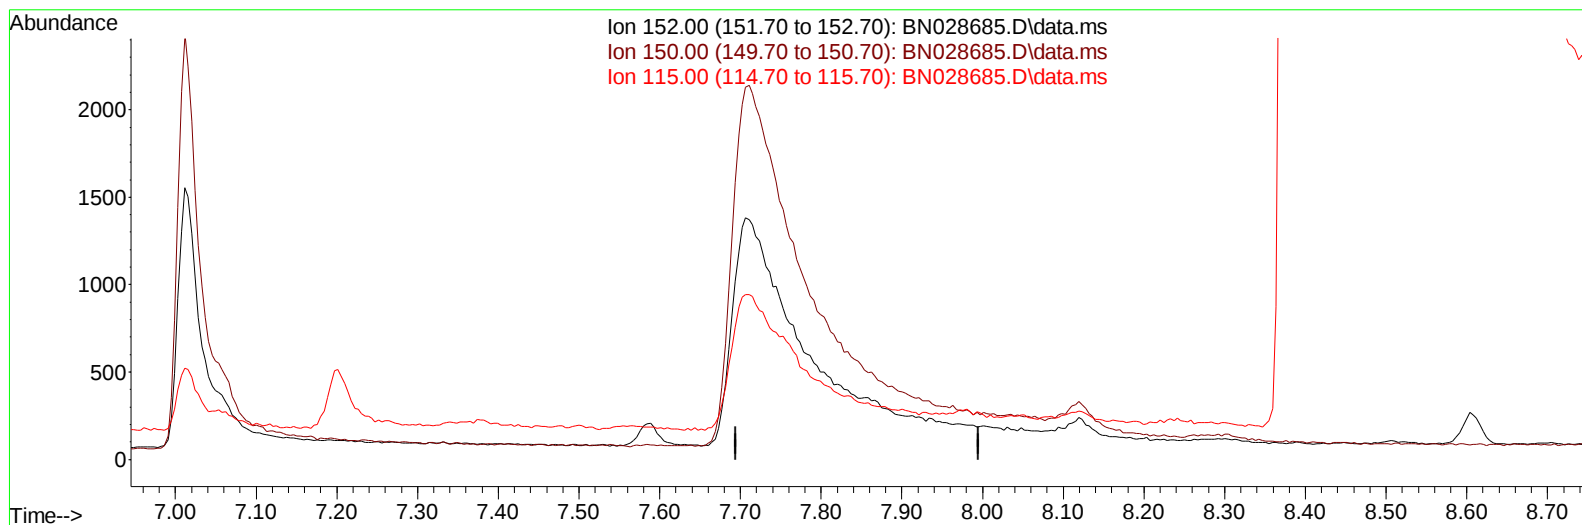

TIC: BN028685.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028685.D
Acq On : 17 Nov 2023 04:19
Operator : MA/JU
Sample : 05338-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL6

Manual IntegrationsAPPROVED

Quant Time: Nov 17 04:47:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

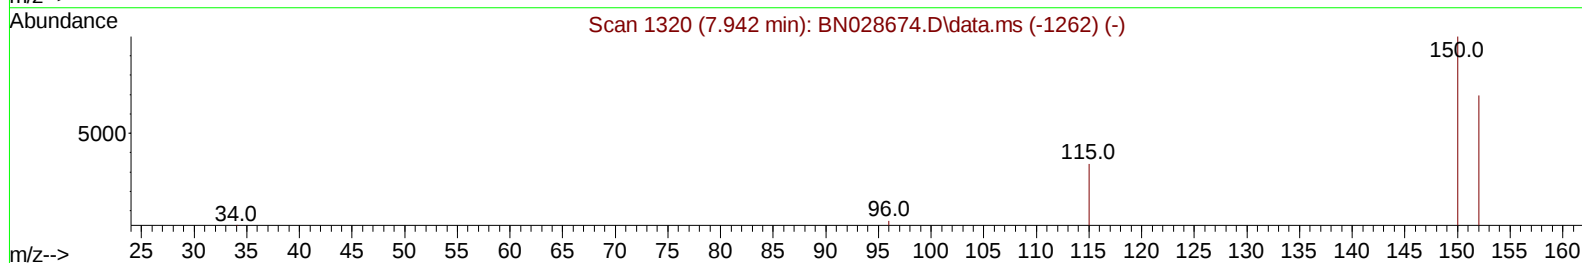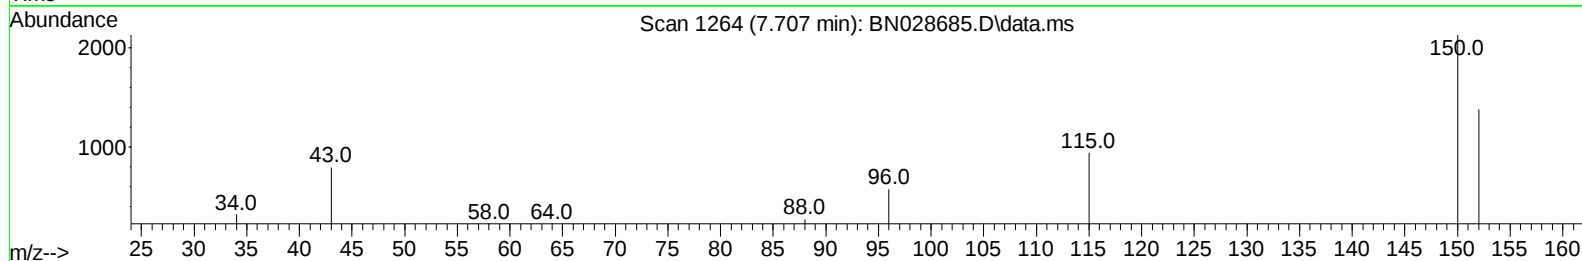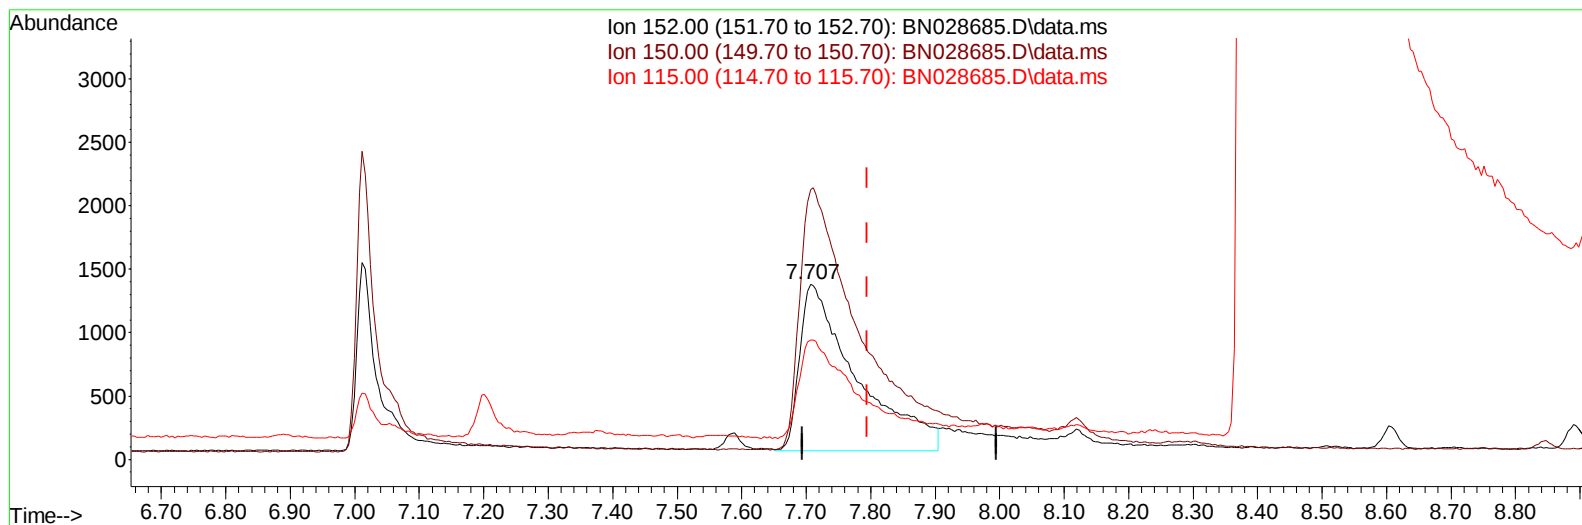

TIC: BN028685.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.707min (-0.088) 0.40 ng/ul m

response 8029

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	154.12
115.00	62.20	68.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028685.D
 Acq On : 17 Nov 2023 04:19
 Operator : MA/JU
 Sample : 05338-11
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 04:47:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.707	152		8029m	0.400	ng/ul	-0.09
4) Naphthalene-d8	10.473	136		33169	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164		19303	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.073	188		39329	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.287	240		26349	0.400	ng/ul	# 0.00
23) Perylene-d12	23.569	264		28027	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.116	96		36112	4.070	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.085	152		9111	0.182	ng/ul	-0.03
18) Fluoranthene-d10	19.113	212		33580	0.396	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.150	88		3091	0.315	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028685.D
Acq On : 17 Nov 2023 04:19
Operator : MA/JU
Sample : 05338-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL6

Manual IntegrationsAPPROVED

Quant Time: Nov 17 04:47:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

