




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028686.D
Acq On : 17 Nov 2023 04:55
Operator : MA/JU
Sample : 05338-12
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL7

Manual IntegrationsAPPROVED

Quant Time: Nov 17 05:24:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

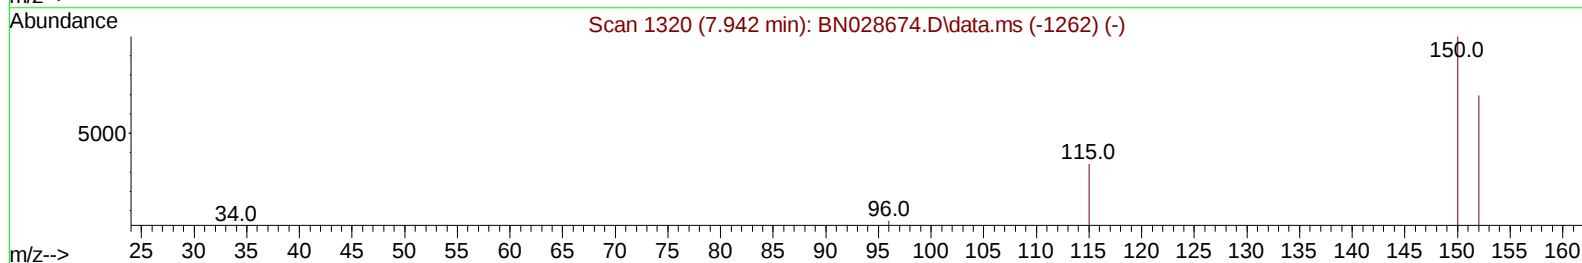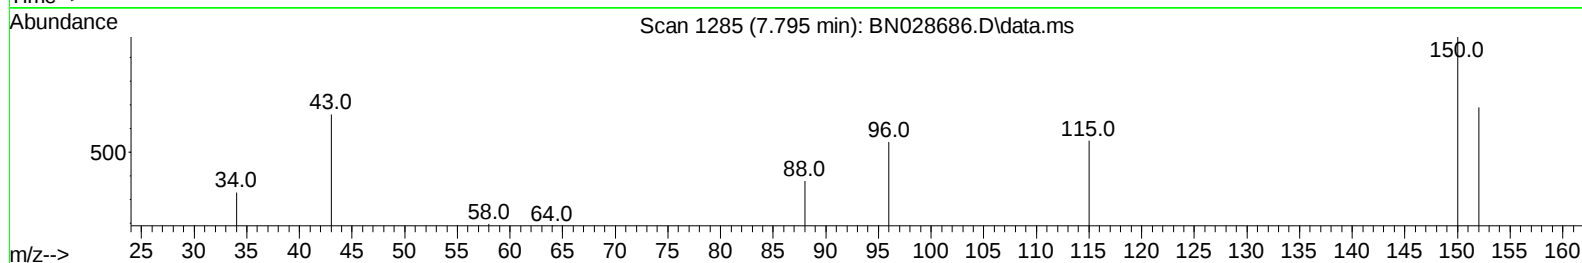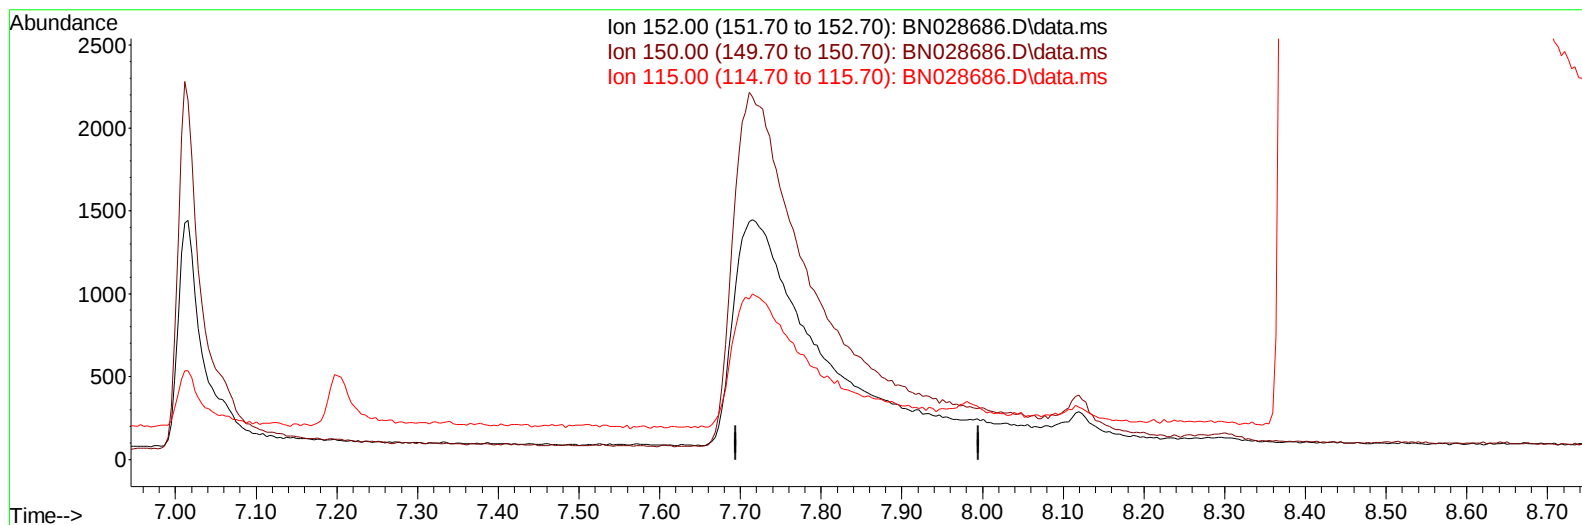

TIC: BN028686.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028686.D
 Acq On : 17 Nov 2023 04:55
 Operator : MA/JU
 Sample : 05338-12
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL7

Manual IntegrationsAPPROVED

Quant Time: Nov 17 05:24:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

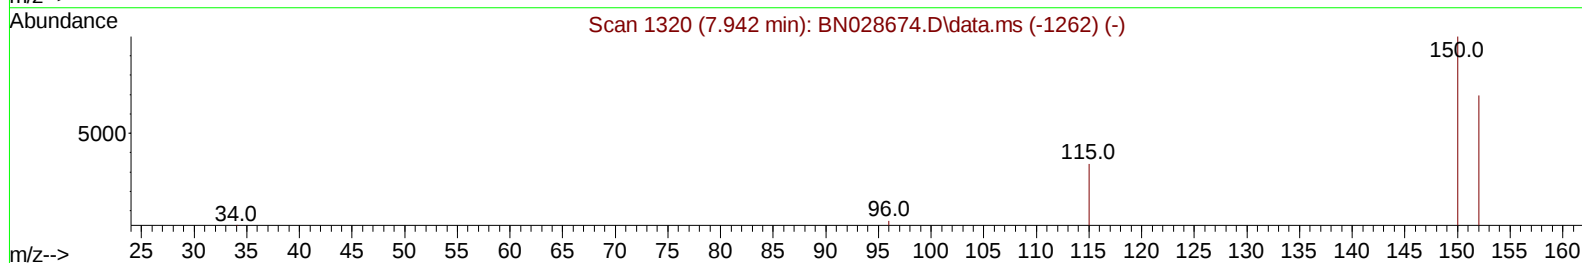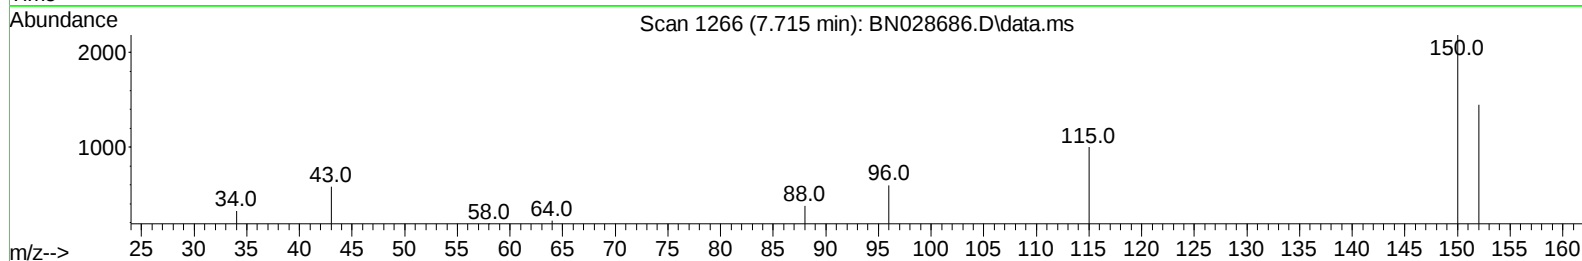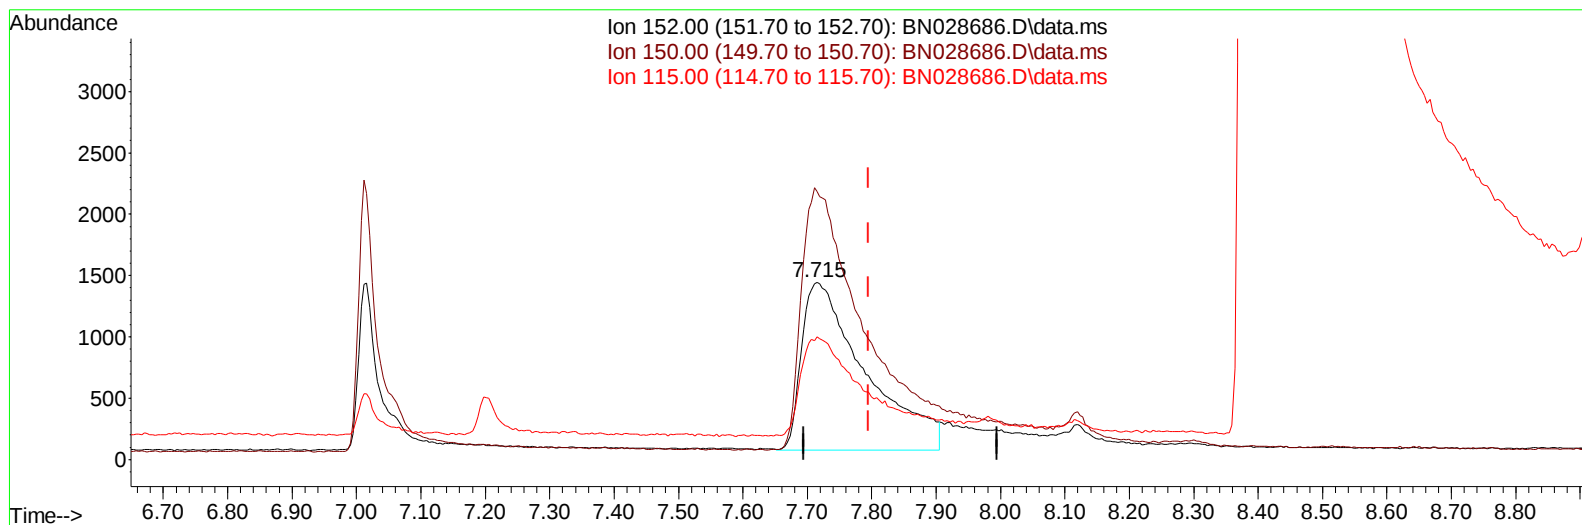

TIC: BN028686.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.715min (-0.080) 0.40 ng/ul m

response 9383

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	151.18
115.00	62.20	69.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028686.D
 Acq On : 17 Nov 2023 04:55
 Operator : MA/JU
 Sample : 05338-12
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 05:24:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.715	152		9383m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.473	136		38630	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.321	164		21801	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.077	188		39831	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.290	240		25854	0.400	ng/ul	# 0.00
23) Perylene-d12	23.569	264		32590	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.116	96		37619	3.628	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.096	152		7414	0.127	ng/ul	-0.02
18) Fluoranthene-d10	19.113	212		29848	0.359	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.154	88		3794	0.331	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028686.D
Acq On : 17 Nov 2023 04:55
Operator : MA/JU
Sample : 05338-12
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL7

Manual IntegrationsAPPROVED

Quant Time: Nov 17 05:24:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

