




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028688.D
 Acq On : 17 Nov 2023 06:06
 Operator : MA/JU
 Sample : 05338-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL9

Manual IntegrationsAPPROVED

Quant Time: Nov 17 06:33:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

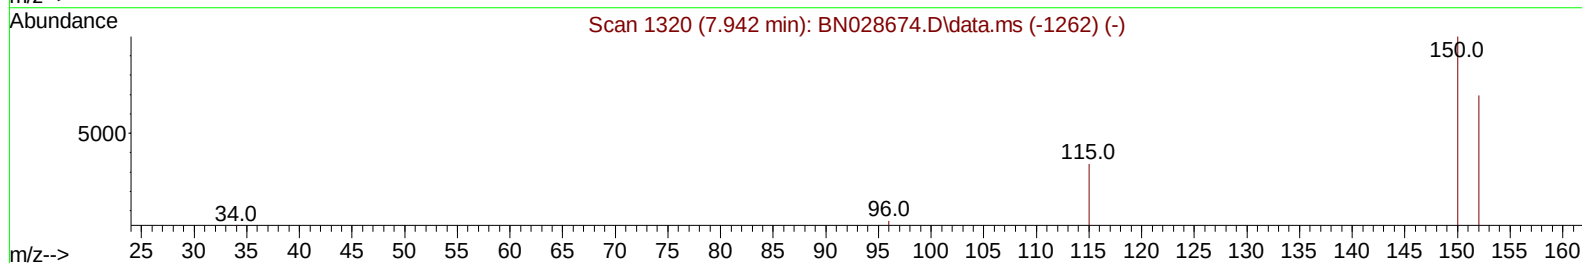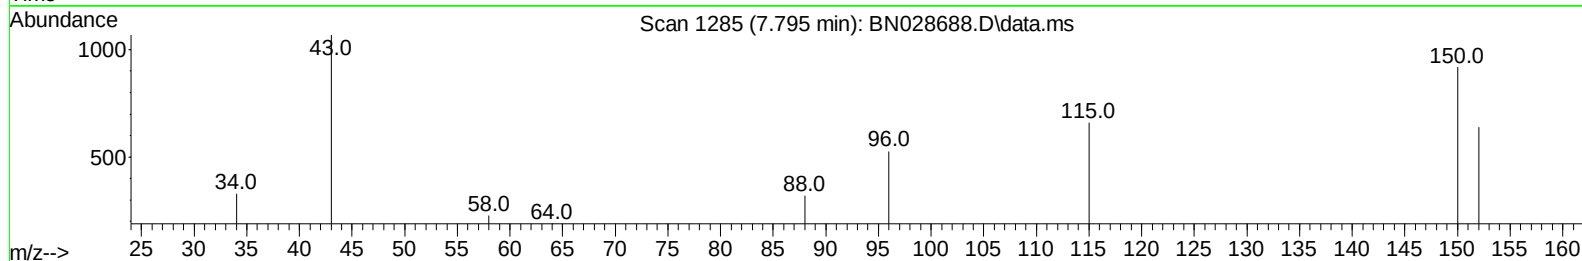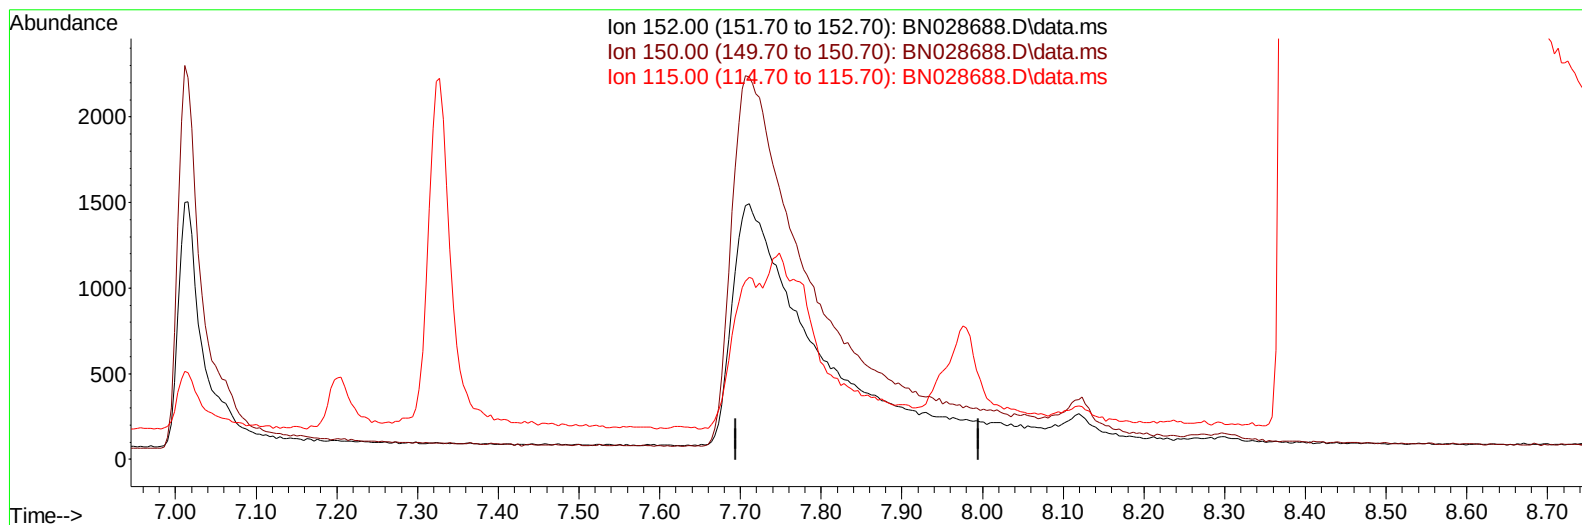

TIC: BN028688.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/ul

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028688.D
 Acq On : 17 Nov 2023 06:06
 Operator : MA/JU
 Sample : 05338-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL9

Manual IntegrationsAPPROVED

Quant Time: Nov 17 06:33:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

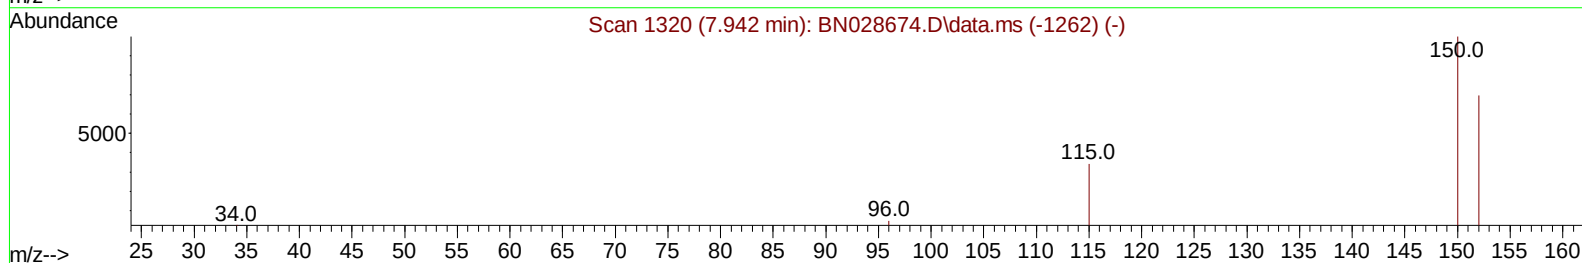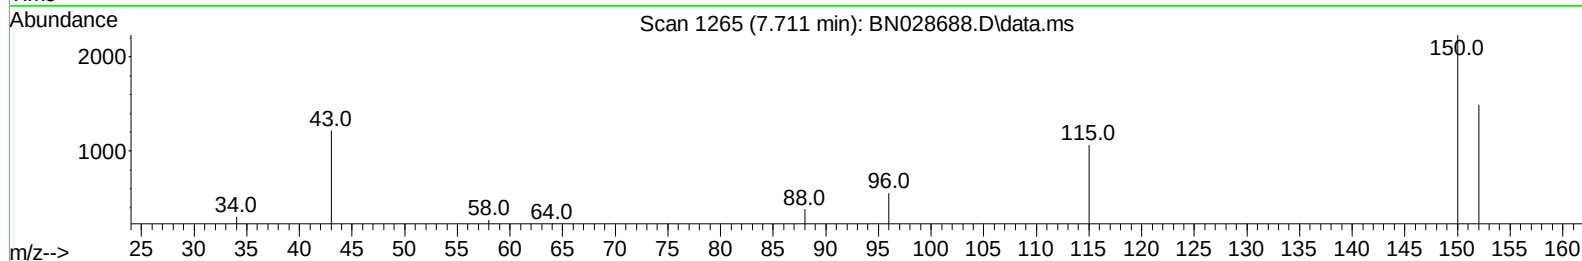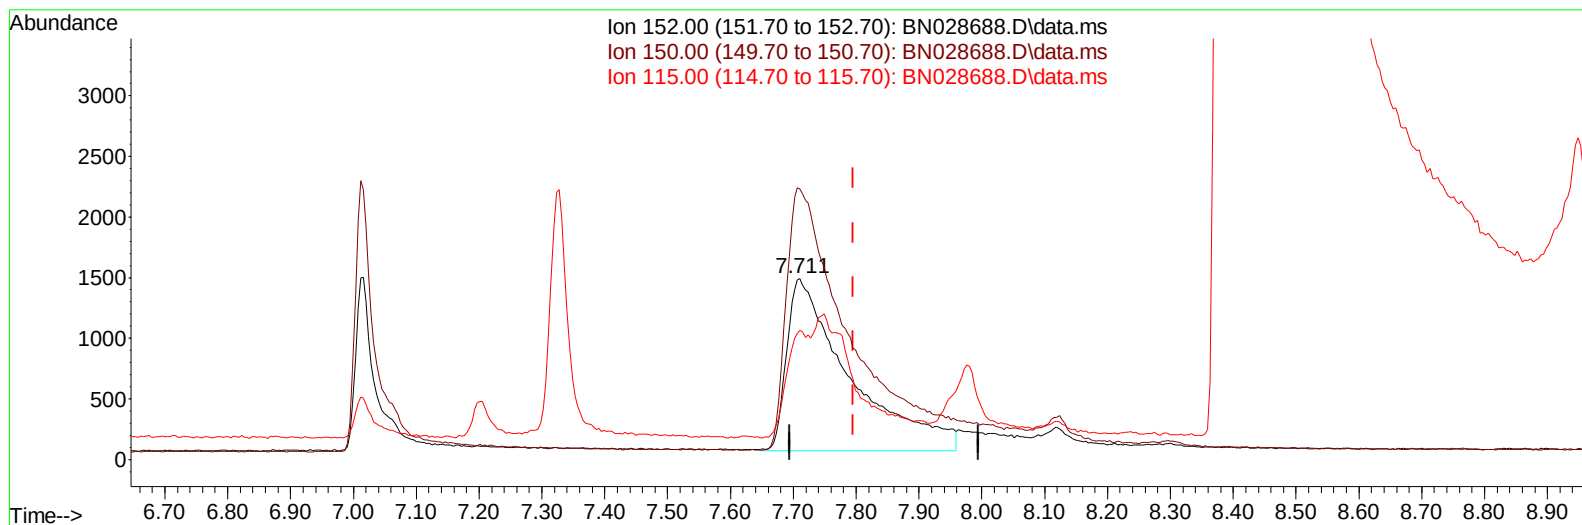

TIC: BN028688.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.711min (-0.084) 0.40 ng/ul m

response 9908

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	149.63
115.00	62.20	71.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028688.D
 Acq On : 17 Nov 2023 06:06
 Operator : MA/JU
 Sample : 05338-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 06:33:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.711	152		9908m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.473	136		36060	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164		19018	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.077	188		35073	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.292	240		23346	0.400	ng/ul	0.00
23) Perylene-d12	23.572	264		30074	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.116	96		37167	3.394	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.101	152		6955	0.128	ng/ul	-0.01
18) Fluoranthene-d10	19.112	212		28204	0.375	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.154	88		1549	0.128	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028688.D
Acq On : 17 Nov 2023 06:06
Operator : MA/JU
Sample : 05338-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDL9

Manual IntegrationsAPPROVED

Quant Time: Nov 17 06:33:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023

