




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028708.D
Acq On : 17 Nov 2023 19:29
Operator : MA/JU
Sample : 05158-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH363

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:23:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023

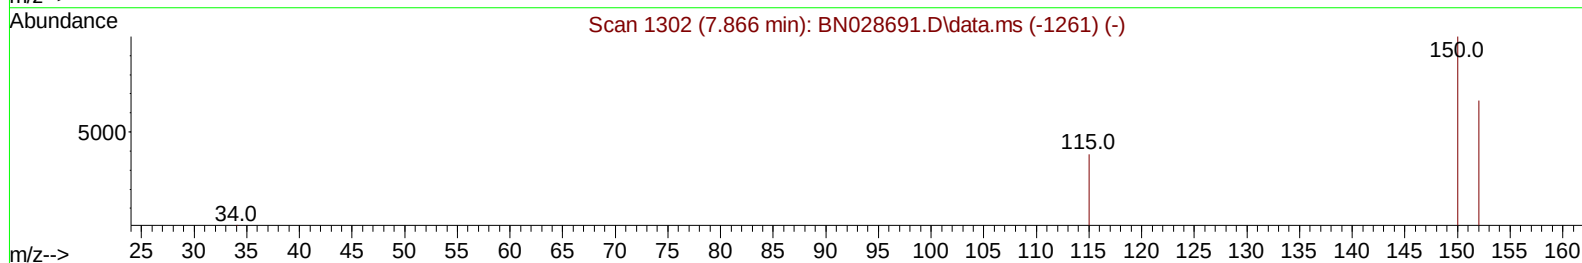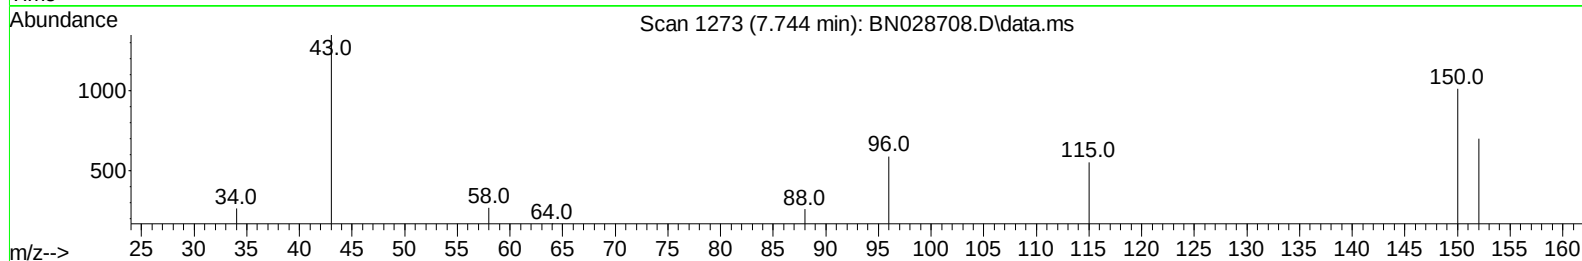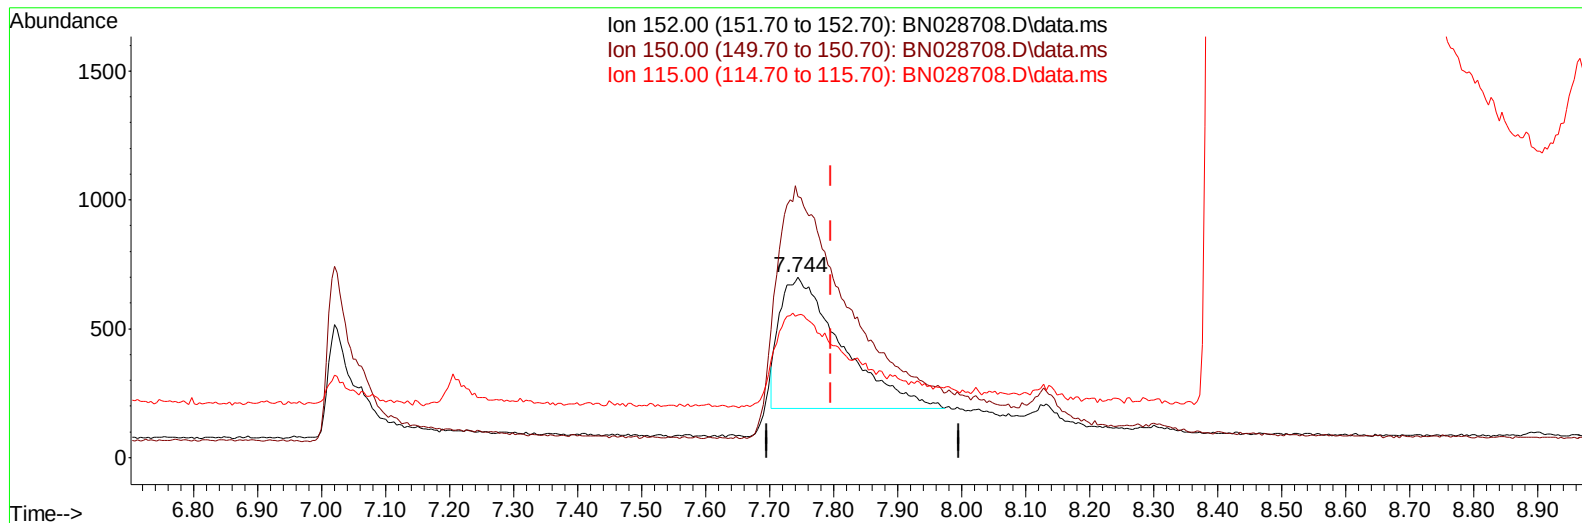

TIC: BN028708.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.744min (-0.051) 0.40 ng/u1

response 3446

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	144.37
115.00	62.20	78.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028708.D
Acq On : 17 Nov 2023 19:29
Operator : MA/JU
Sample : 05158-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH363

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:23:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023

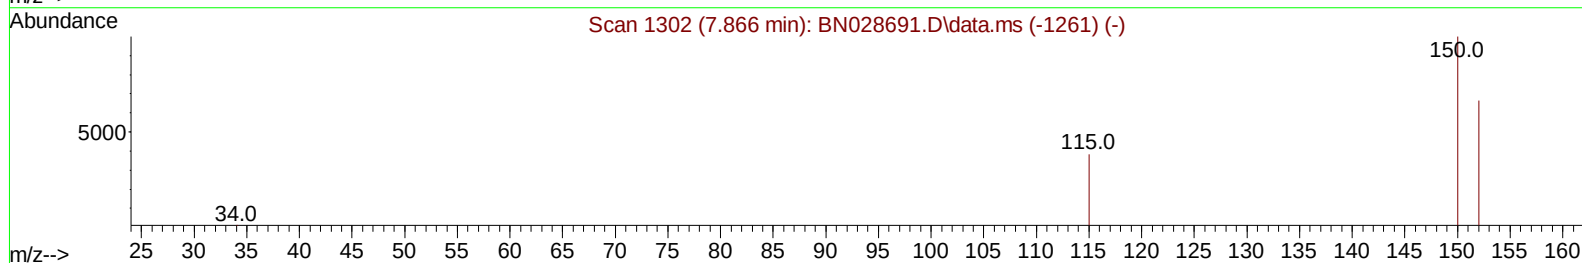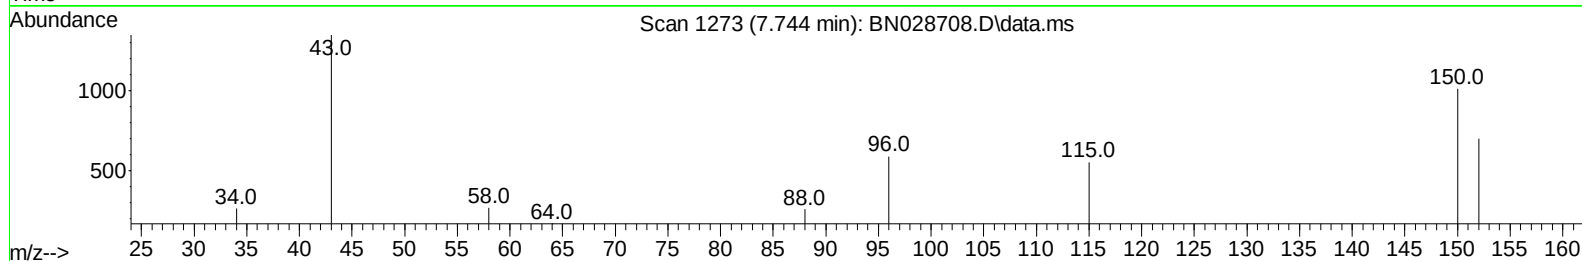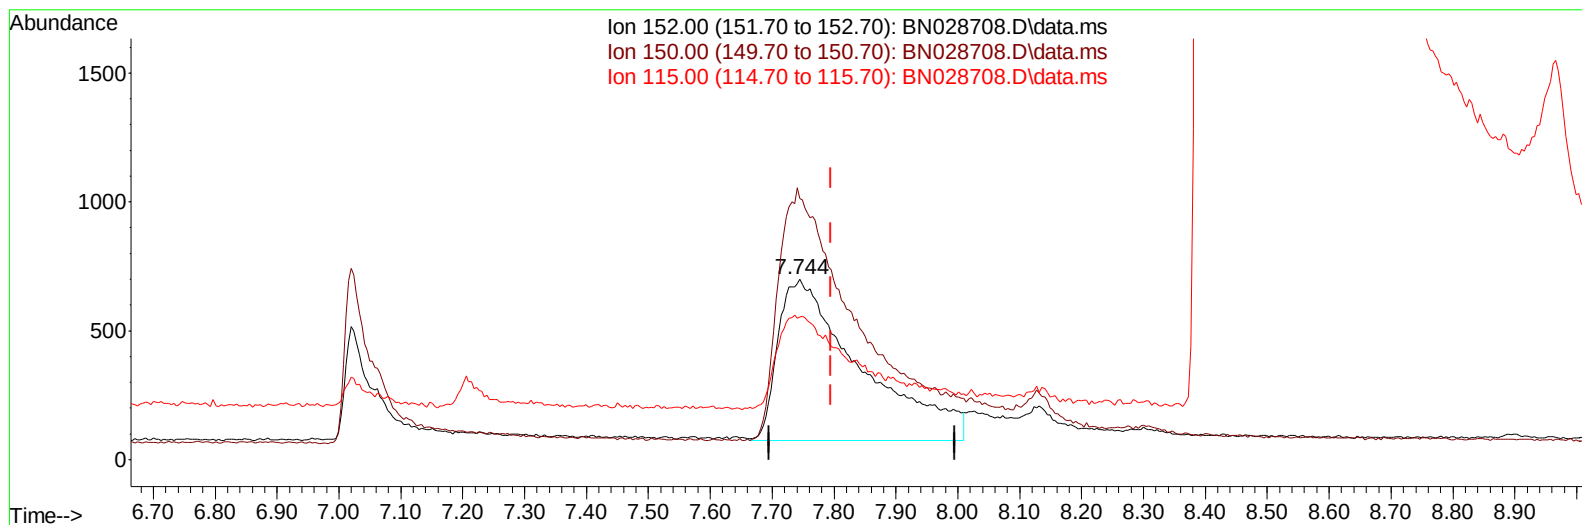

TIC: BN028708.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.744min (-0.051) 0.40 ng/ul m

response 5836

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	144.37
115.00	62.20	78.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028708.D
 Acq On : 17 Nov 2023 19:29
 Operator : MA/JU
 Sample : 05158-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH363

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 23:23:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.744	152		5836m	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.477	136		18071	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.325	164		12994	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.085	188		25239	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.300	240		17229	0.400	ng/ul	# 0.00
23) Perylene-d12	23.577	264		21187	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.116	96		20612	3.196	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.127	152		3088	0.114	ng/ul	0.02
18) Fluoranthene-d10	19.116	212		18244	0.329	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.154	88		755	0.106	ng/ul#	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028708.D
Acq On : 17 Nov 2023 19:29
Operator : MA/JU
Sample : 05158-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH363

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:23:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023

