




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028712.D
Acq On : 17 Nov 2023 21:53
Operator : MA/JU
Sample : 05158-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH369

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:32:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023

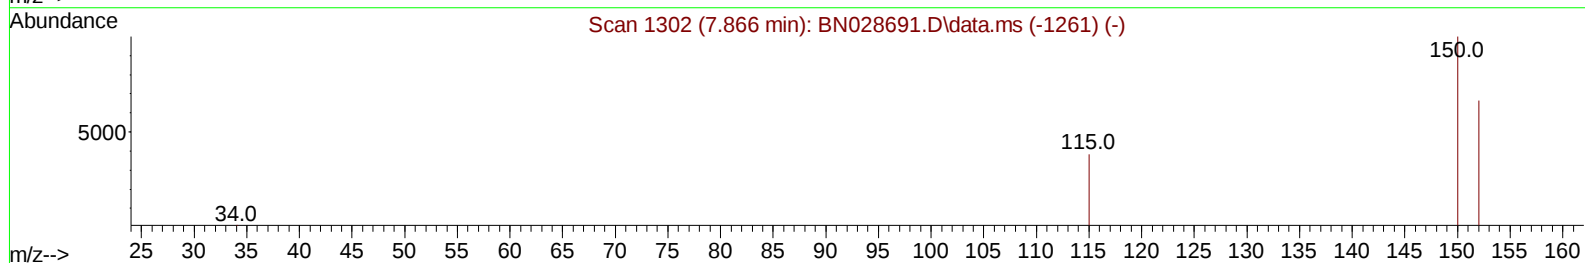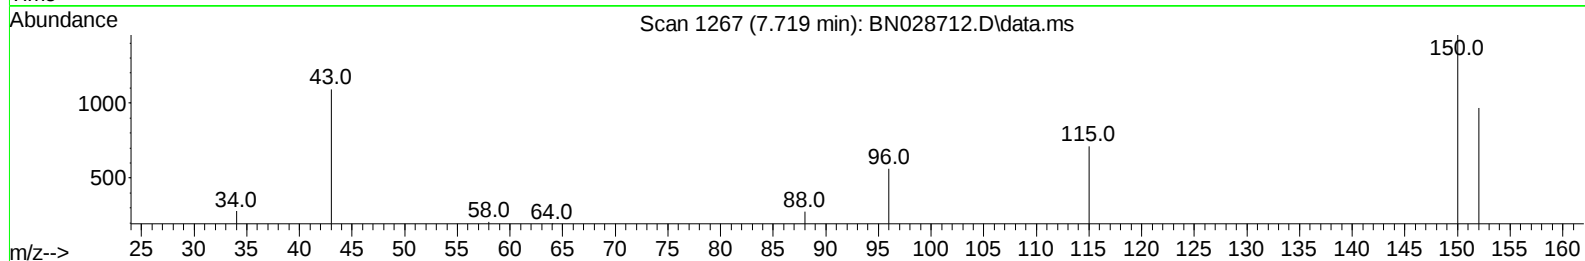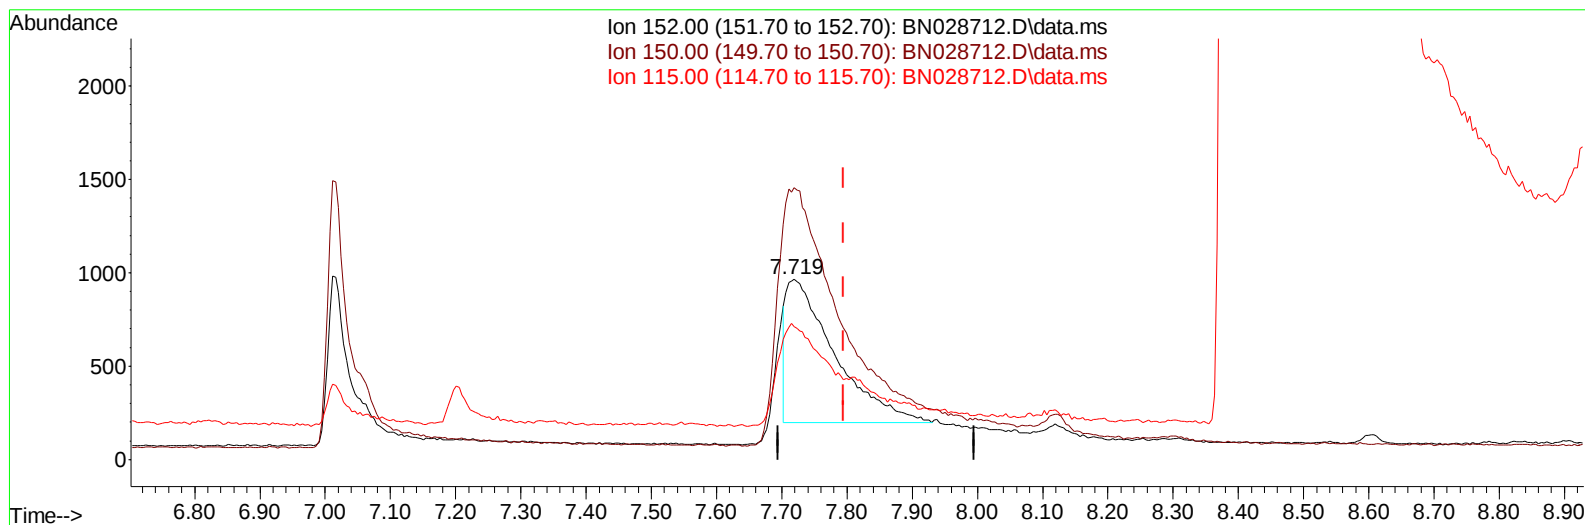

TIC: BN028712.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/u1

response 3954

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	150.52
115.00	62.20	73.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028712.D
 Acq On : 17 Nov 2023 21:53
 Operator : MA/JU
 Sample : 05158-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH369

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:32:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

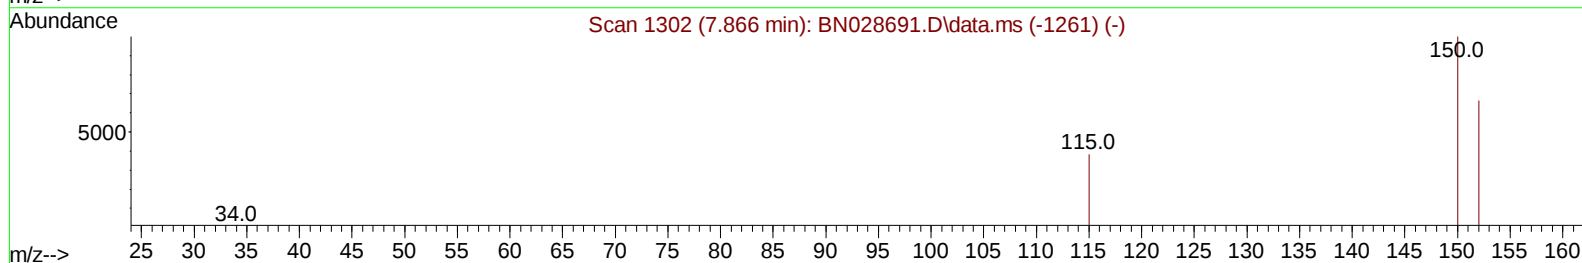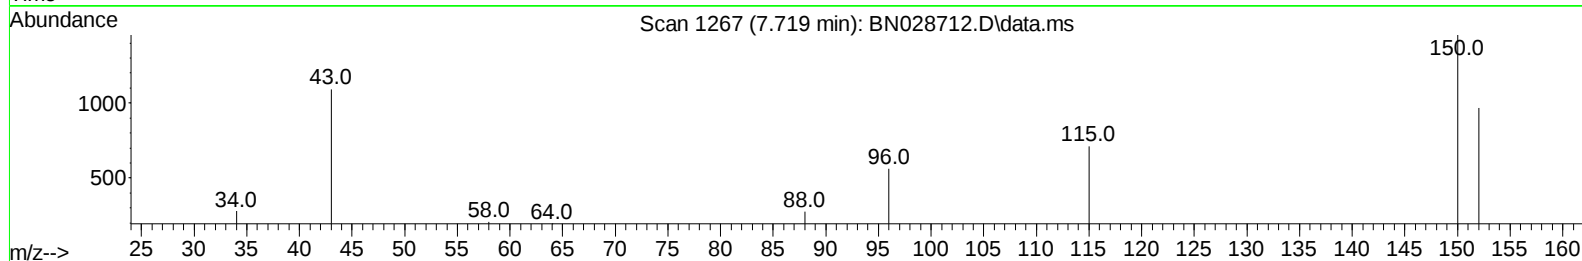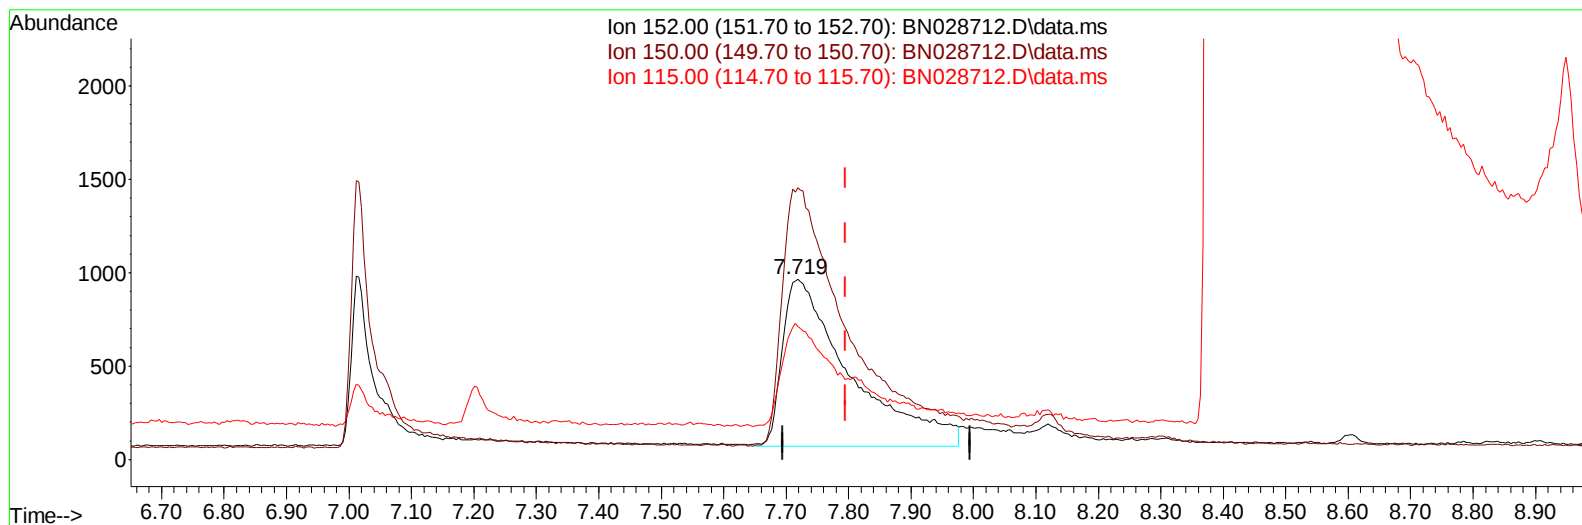

TIC: BN028712.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/ul m

response 6790

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	150.52
115.00	62.20	73.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028713.D
Acq On : 17 Nov 2023 22:29
Operator : MA/JU
Sample : 05158-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH369

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:35:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023

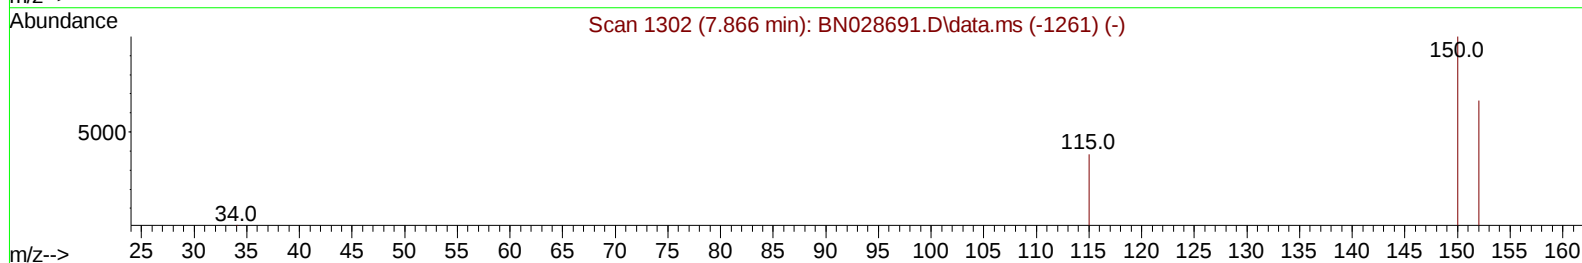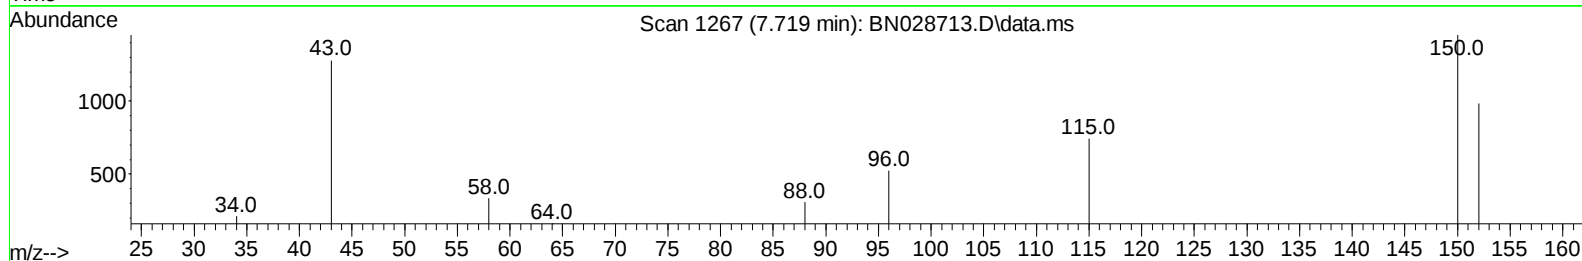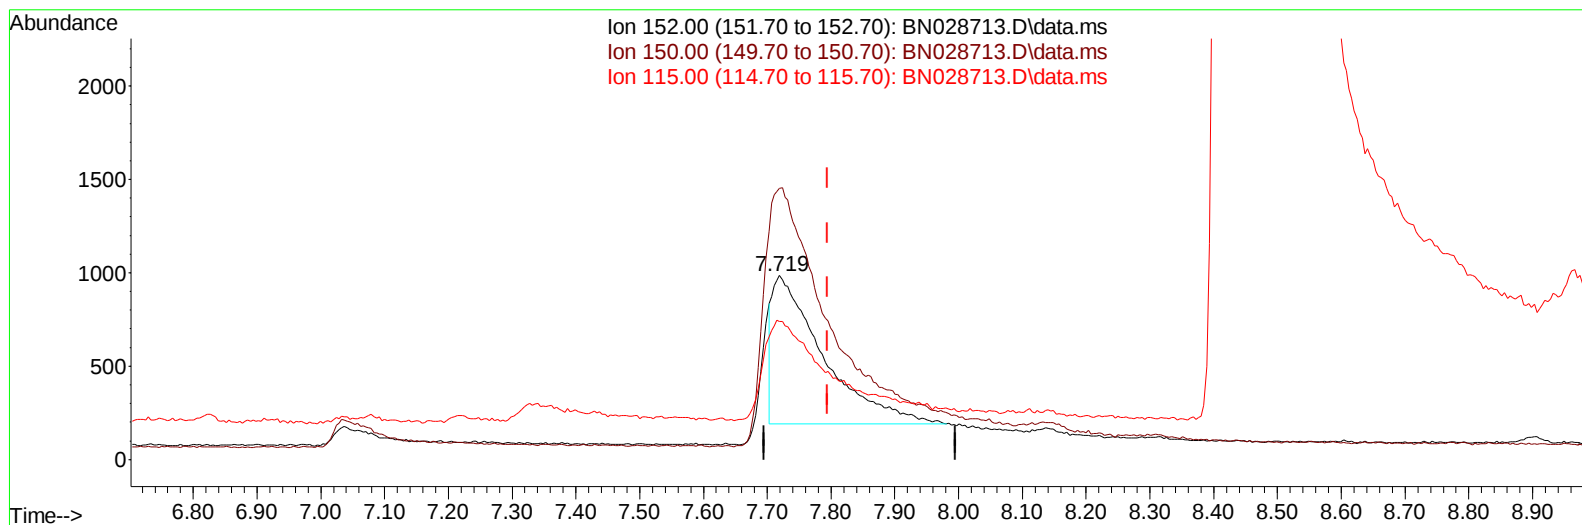

TIC: BN028713.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/u1

response 4388

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	147.51
115.00	62.20	75.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028713.D
 Acq On : 17 Nov 2023 22:29
 Operator : MA/JU
 Sample : 05158-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH369

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:35:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

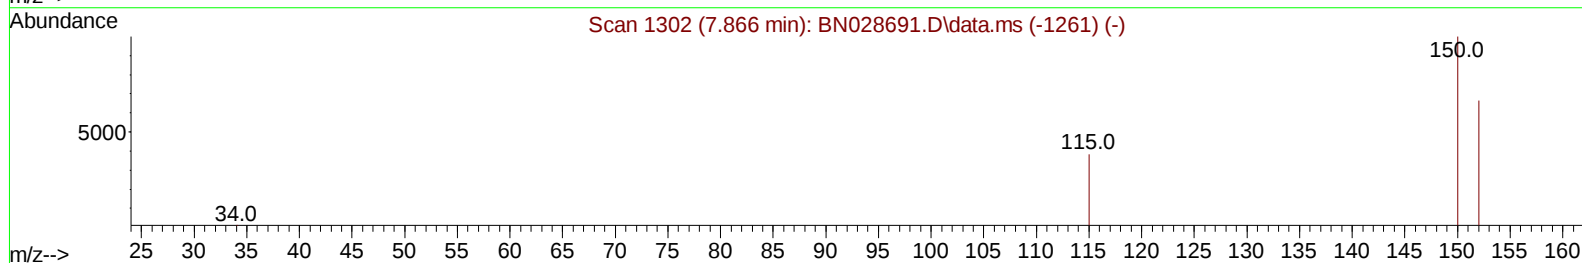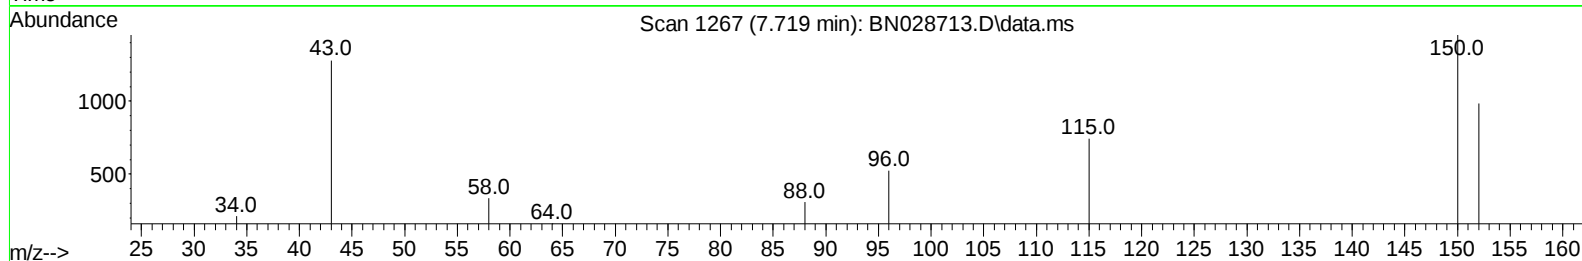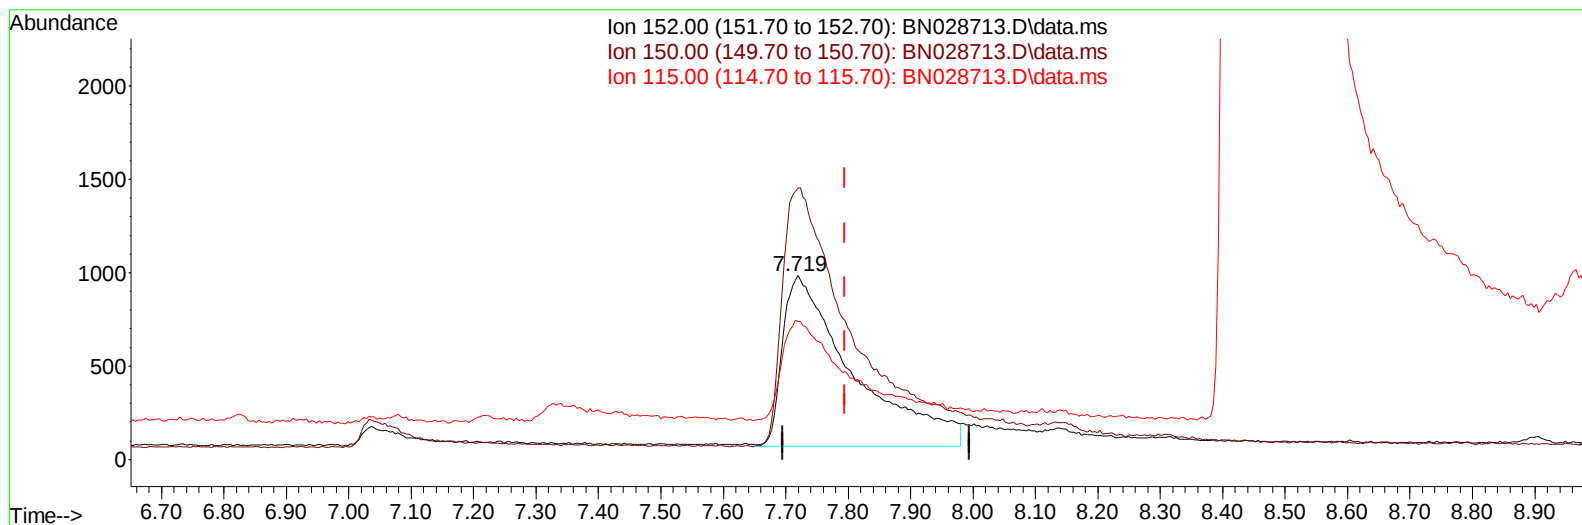

TIC: BN028713.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/ul m

response 7158

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	147.51
115.00	62.20	75.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028713.D
 Acq On : 17 Nov 2023 22:29
 Operator : MA/JU
 Sample : 05158-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH369

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 23:35:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.719	152		7158m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.473	136		28607	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164		16327	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.077	188		33566	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.290	240		27300	0.400	ng/ul	0.00
23) Perylene-d12	23.572	264		25650	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.116	96		17219	2.177	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.096	152		1431	0.033	ng/ul	-0.02
18) Fluoranthene-d10	19.117	212		8542	0.097	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.154	88		624	0.071	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual IntegrationsAPPROVED

Quant Time: Nov 17 23:35:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

