




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028715.D
Acq On : 17 Nov 2023 23:41
Operator : MA/JU
Sample : 05158-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH365

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 18 00:22:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

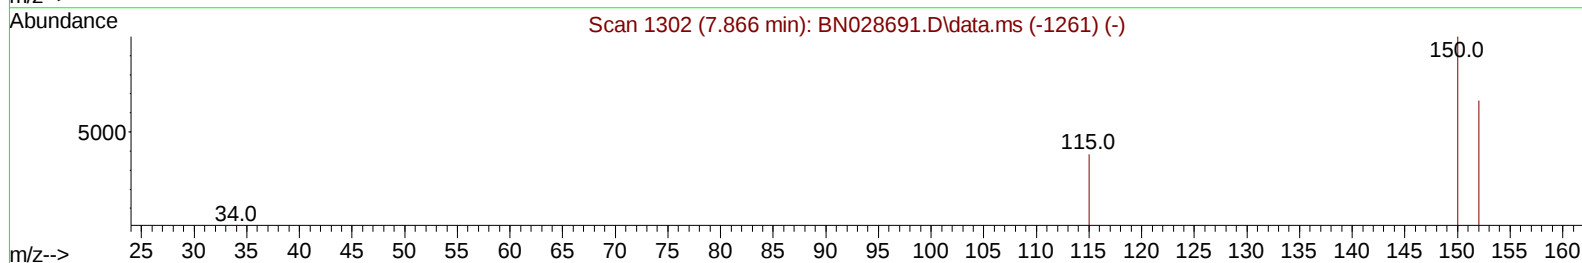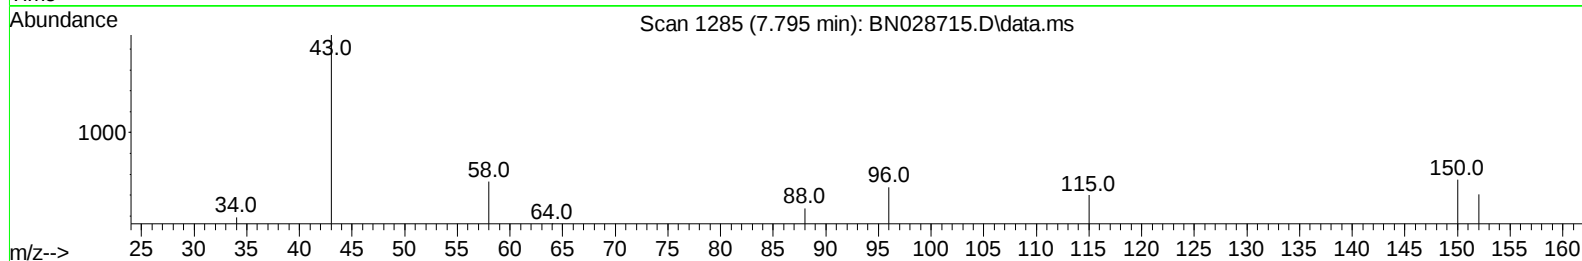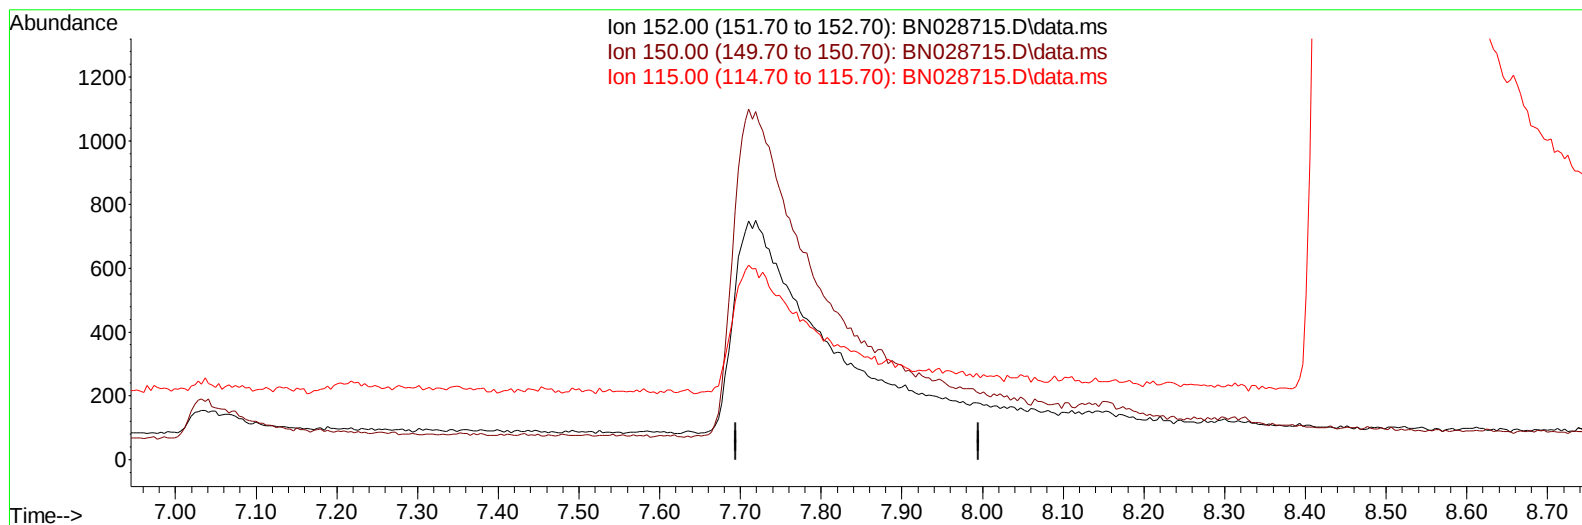

TIC: BN028715.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028715.D
 Acq On : 17 Nov 2023 23:41
 Operator : MA/JU
 Sample : 05158-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH365

Manual IntegrationsAPPROVED

Quant Time: Nov 18 00:22:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

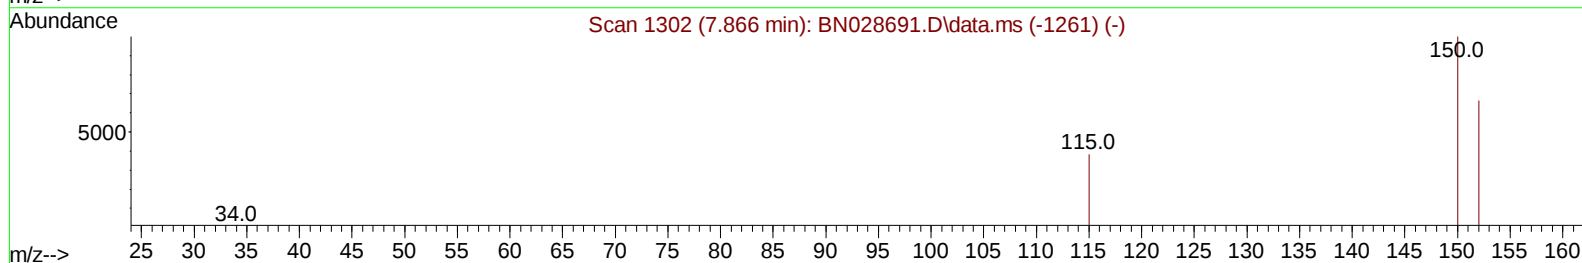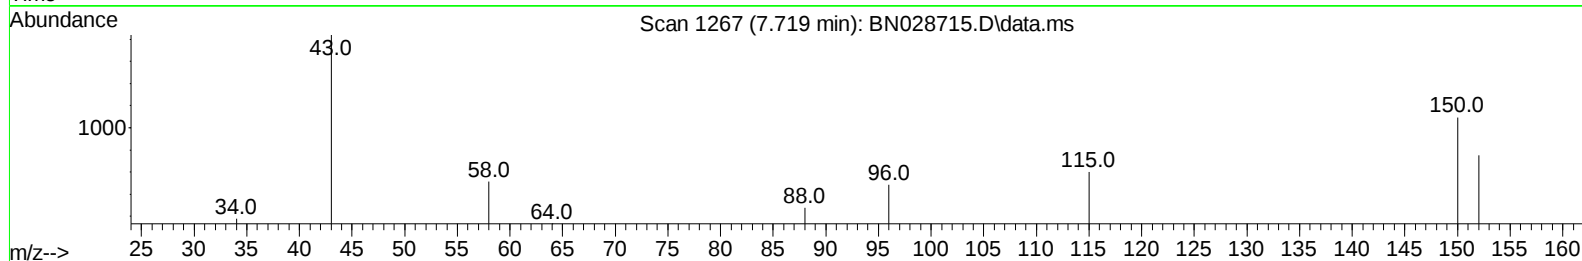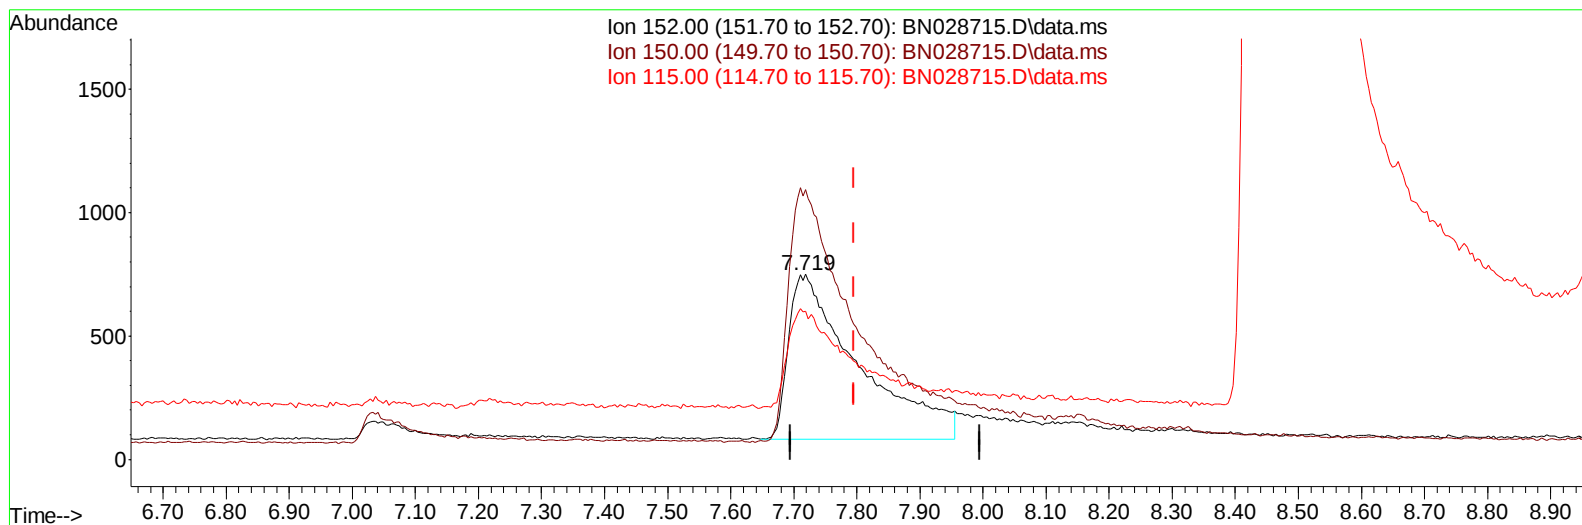

TIC: BN028715.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/ul m

response 5145

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	145.73
115.00	62.20	80.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028715.D
 Acq On : 17 Nov 2023 23:41
 Operator : MA/JU
 Sample : 05158-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH365

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 18 00:22:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.719	152		5145m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.473	136		20964	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164		11421	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.081	188		20467	0.400	ng/ul	0.00
17) Chrysene-d12	21.295	240		15831	0.400	ng/ul	# 0.00
23) Perylene-d12	23.572	264		19856	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.116	96		14842	2.610	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.112	152		1065	0.034	ng/ul	0.00
18) Fluoranthene-d10	19.122	212		4440	0.087	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.154	88		1417	0.225	ng/ul#	16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028715.D
Acq On : 17 Nov 2023 23:41
Operator : MA/JU
Sample : 05158-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH365

Manual IntegrationsAPPROVED

Quant Time: Nov 18 00:22:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023

