




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028747.D
Acq On : 18 Nov 2023 20:05
Operator : MA/JU
Sample : PB157222BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK222

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:37:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

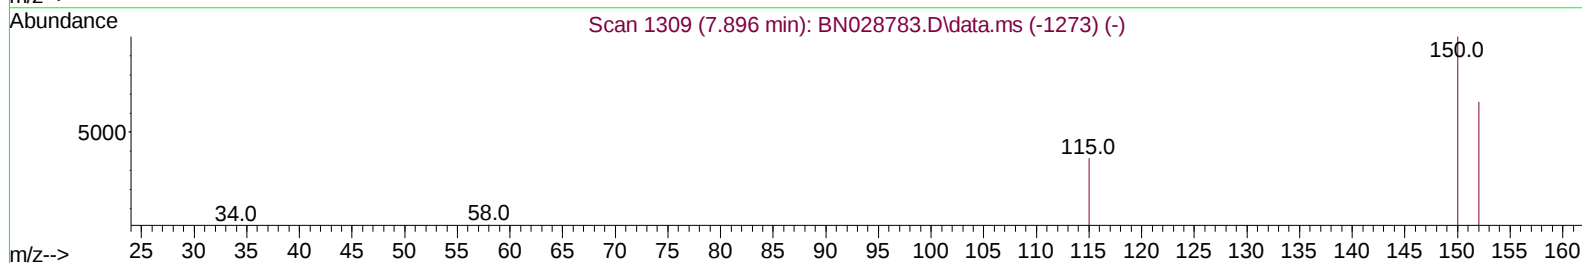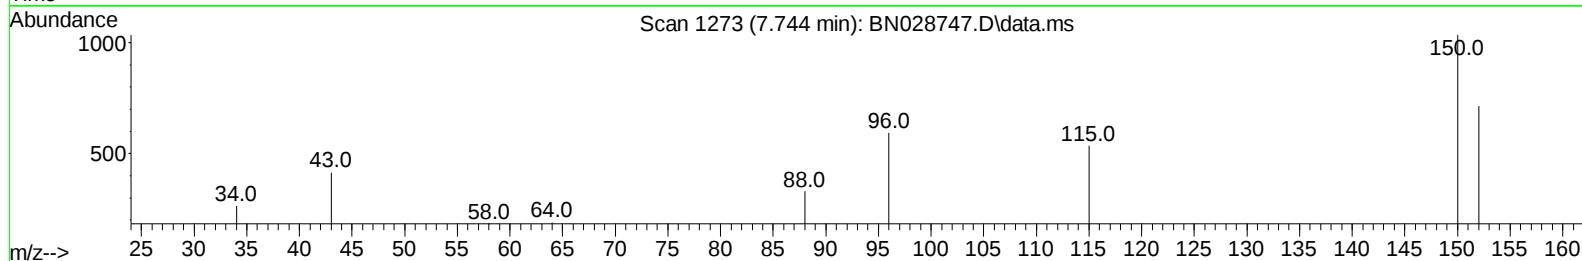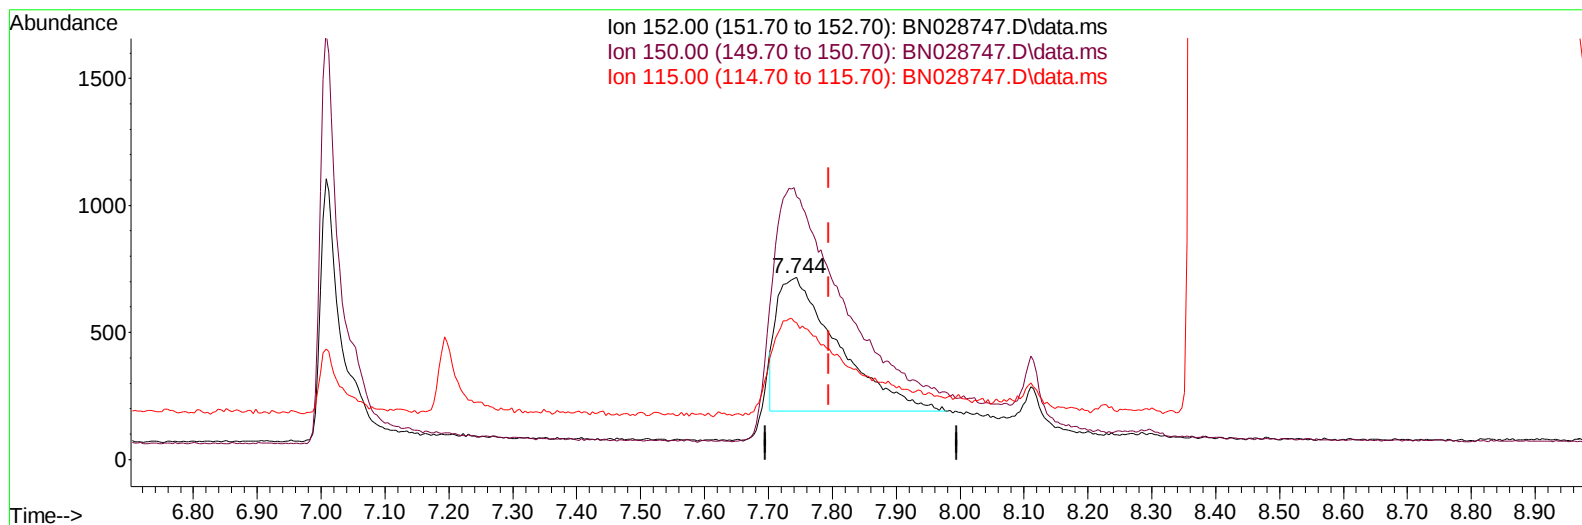

TIC: BN028747.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.744min (-0.051) 0.40 ng/u1

response 3551

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	144.55
115.00	62.20	75.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028747.D
Acq On : 18 Nov 2023 20:05
Operator : MA/JU
Sample : PB157222BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK222

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:37:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

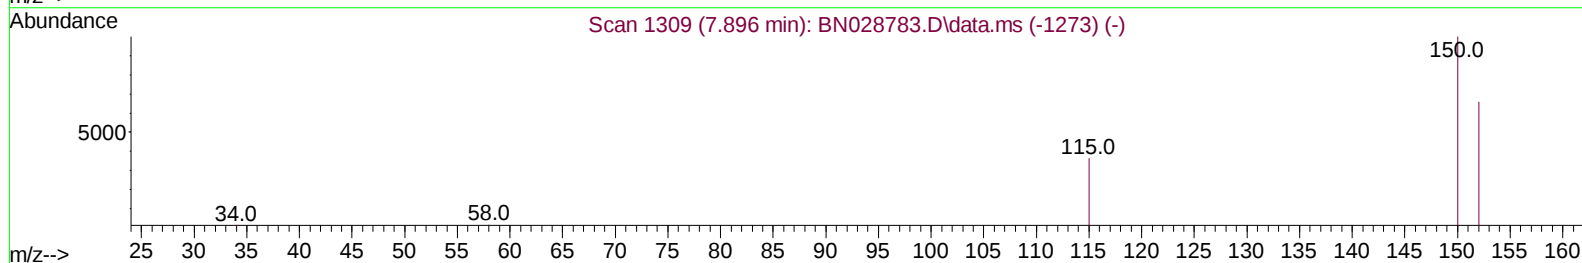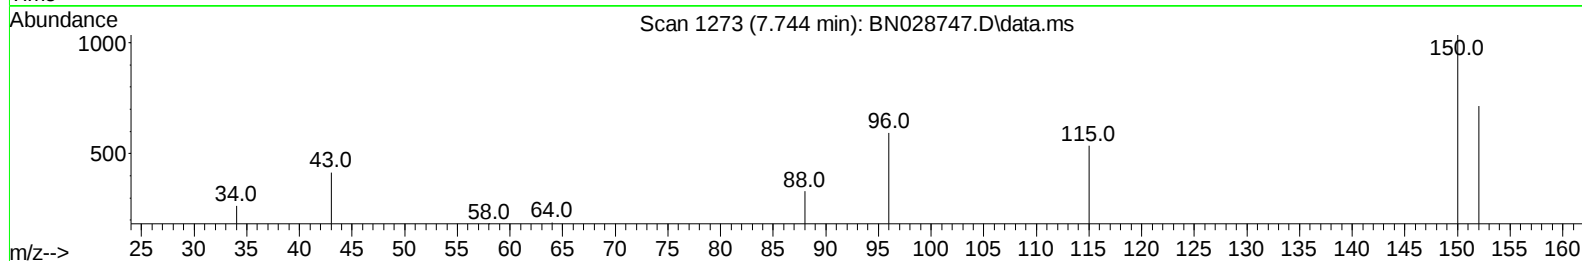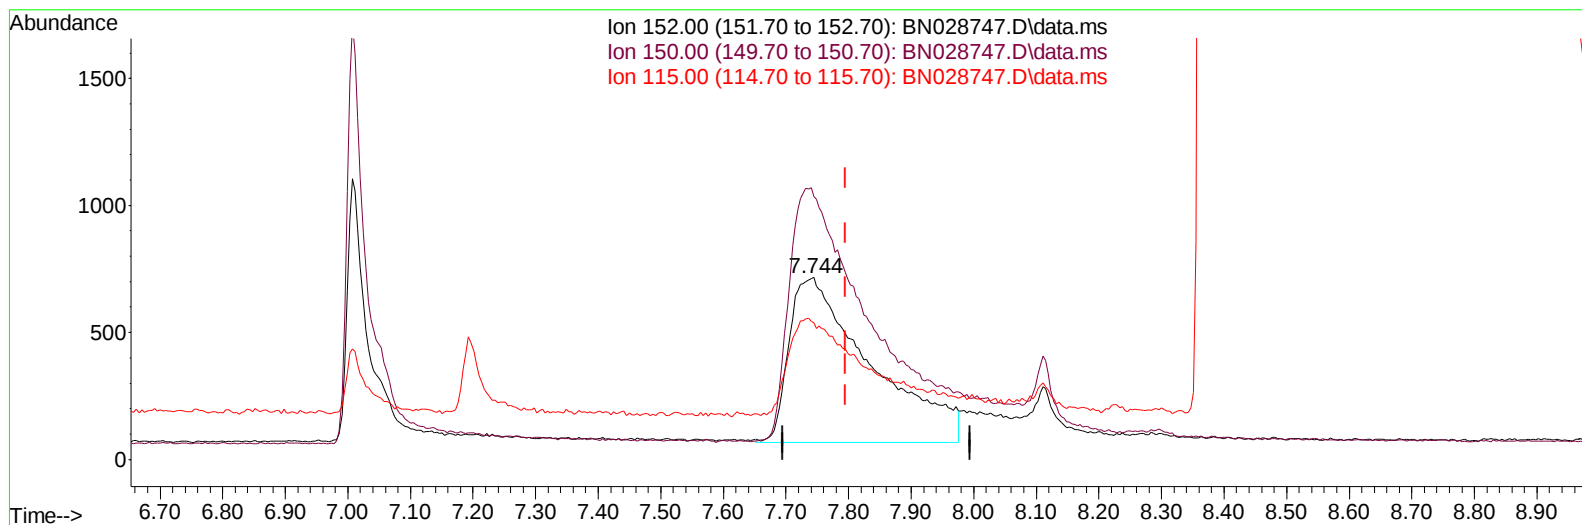

TIC: BN028747.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.744min (-0.051) 0.40 ng/ul m

response 5873

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	144.55
115.00	62.20	75.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028747.D
 Acq On : 18 Nov 2023 20:05
 Operator : MA/JU
 Sample : PB157222BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK222

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:37:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

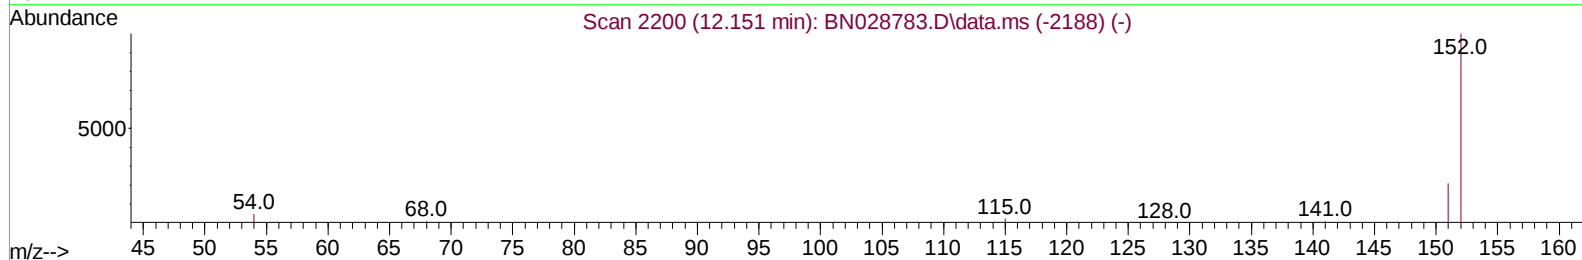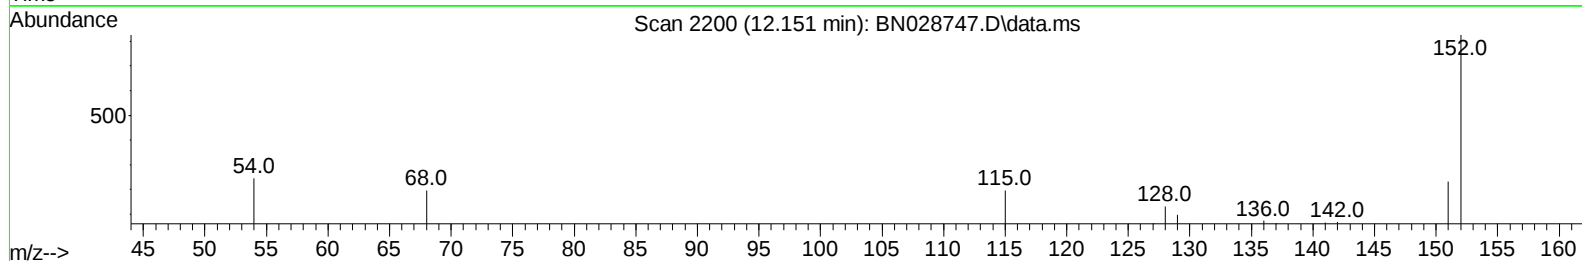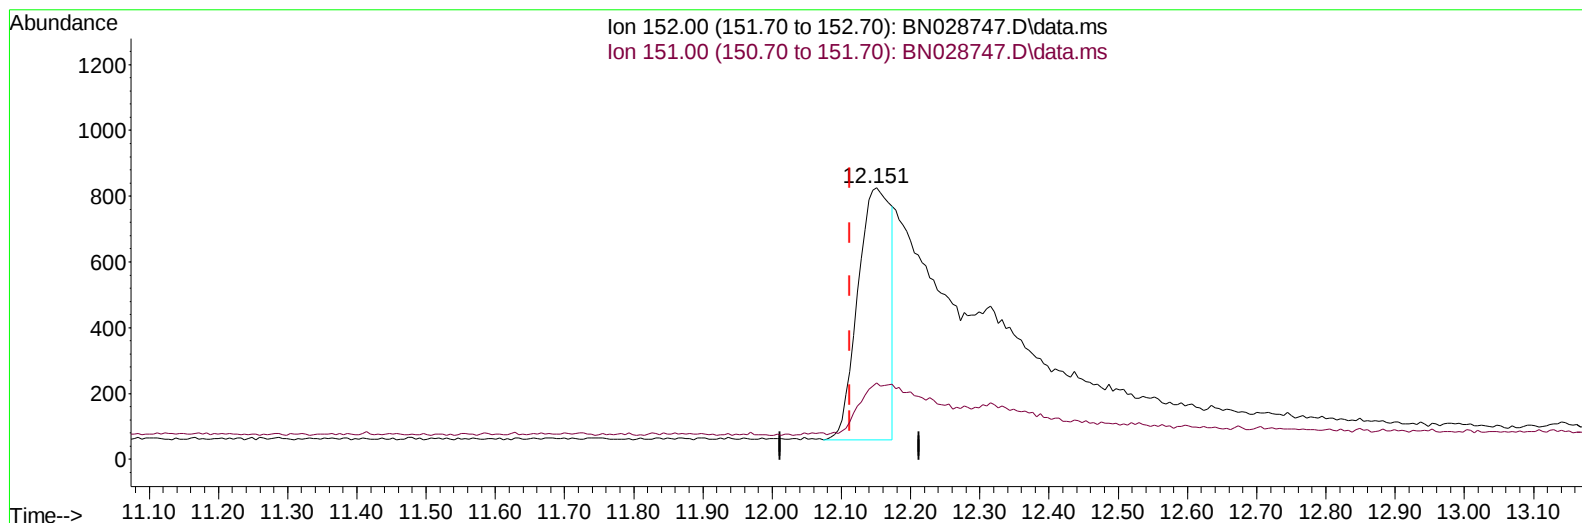

TIC: BN028747.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.151min (+ 0.039) 0.09 ng/u1

response 2500

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	17.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028747.D
Acq On : 18 Nov 2023 20:05
Operator : MA/JU
Sample : PB157222BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK222

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:37:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

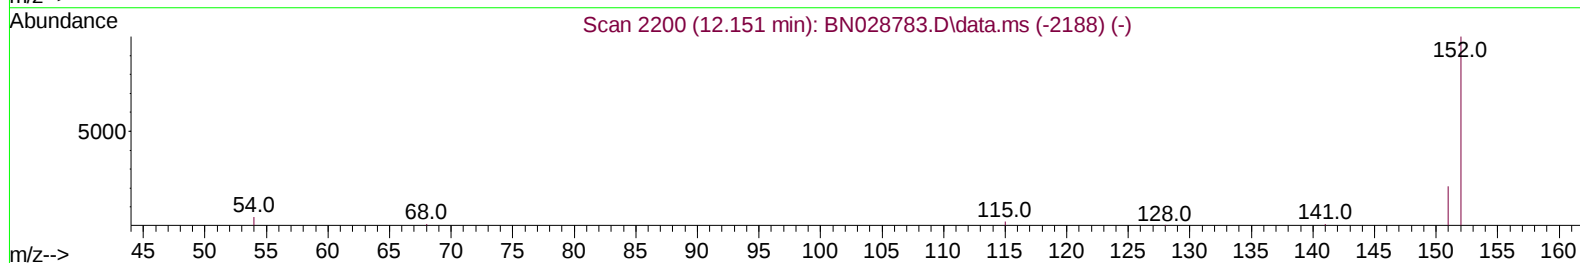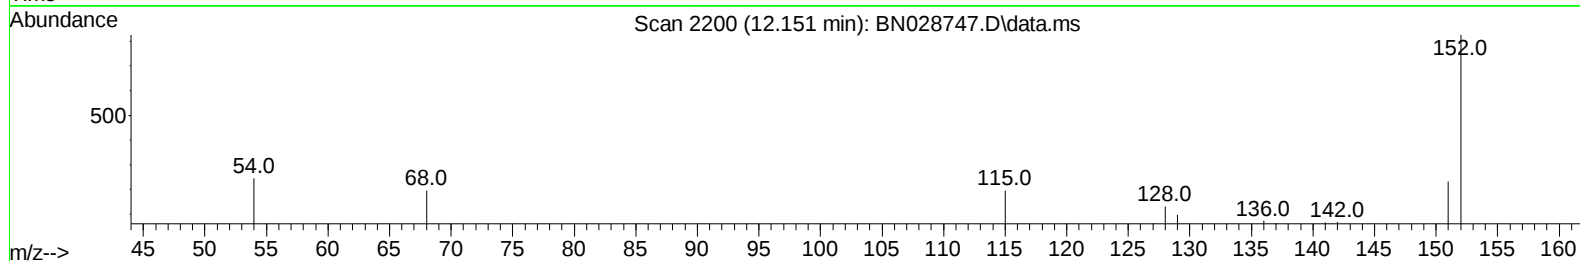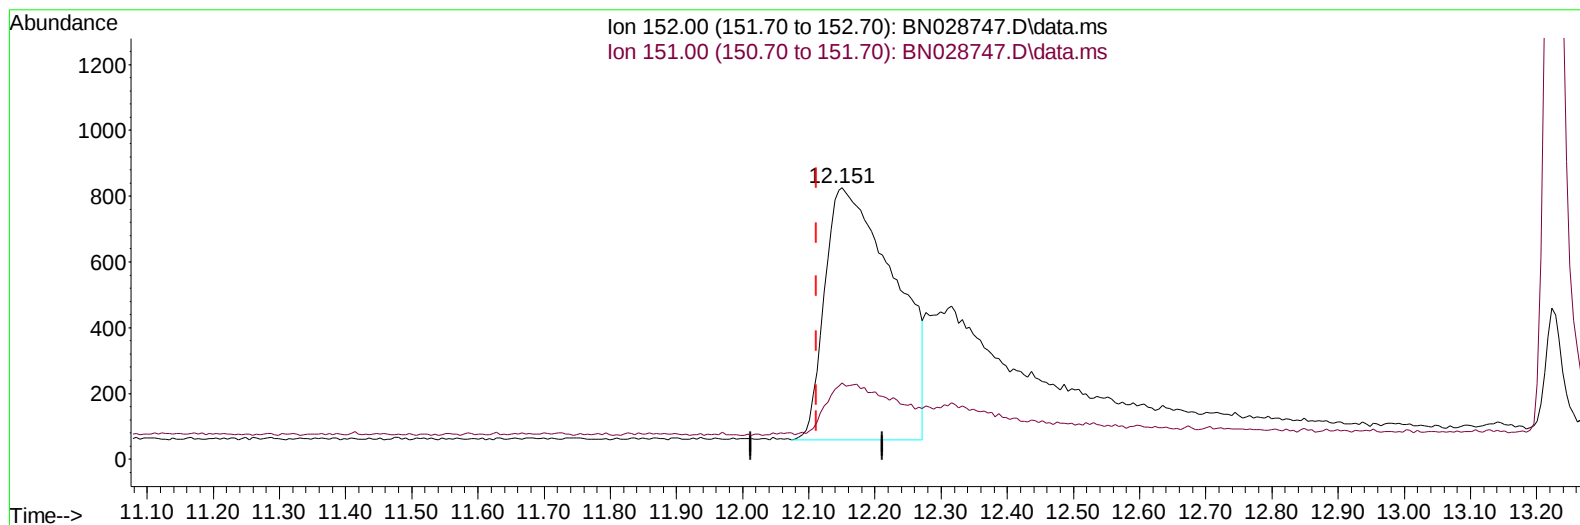

TIC: BN028747.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.151min (+ 0.039) 0.21 ng/ul m

response 5603

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	7.91#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028747.D
 Acq On : 18 Nov 2023 20:05
 Operator : MA/JU
 Sample : PB157222BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK222

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 05:37:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.744	152	5873m	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.473	136	18075	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164	13163	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.085	188	25711	0.400	ng/ul	0.00
17) Chrysene-d12	21.310	240	14996	0.400	ng/ul	# 0.01
23) Perylene-d12	23.575	264	20556	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	44495	6.855	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.151	152	5603m	0.206	ng/ul	0.04
18) Fluoranthene-d10	19.117	212	18911	0.392	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028747.D
Acq On : 18 Nov 2023 20:05
Operator : MA/JU
Sample : PB157222BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK222

Manual IntegrationsAPPROVED

Quant Time: Nov 20 05:37:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

