




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028753.D
Acq On : 19 Nov 2023 00:16
Operator : MA/JU
Sample : 05370-03
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDP9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:43:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

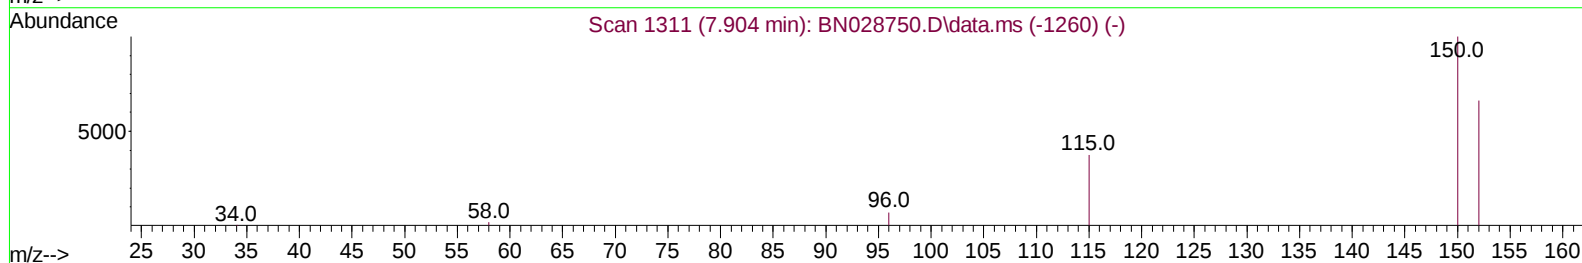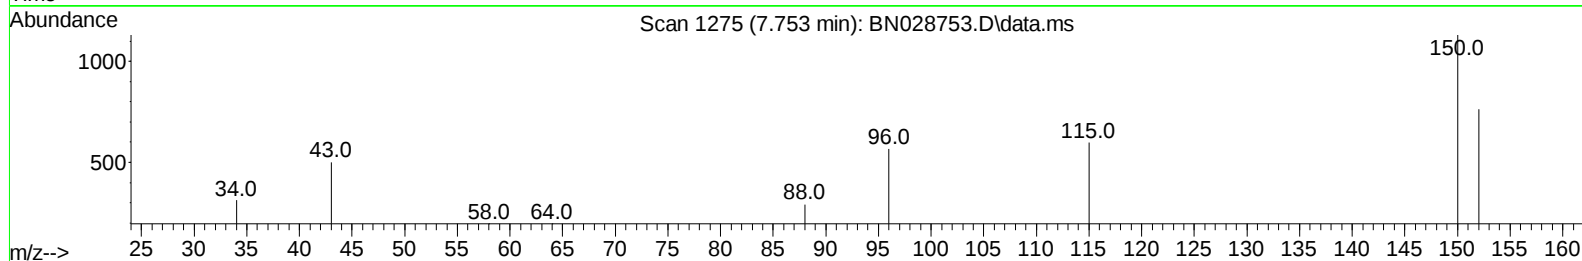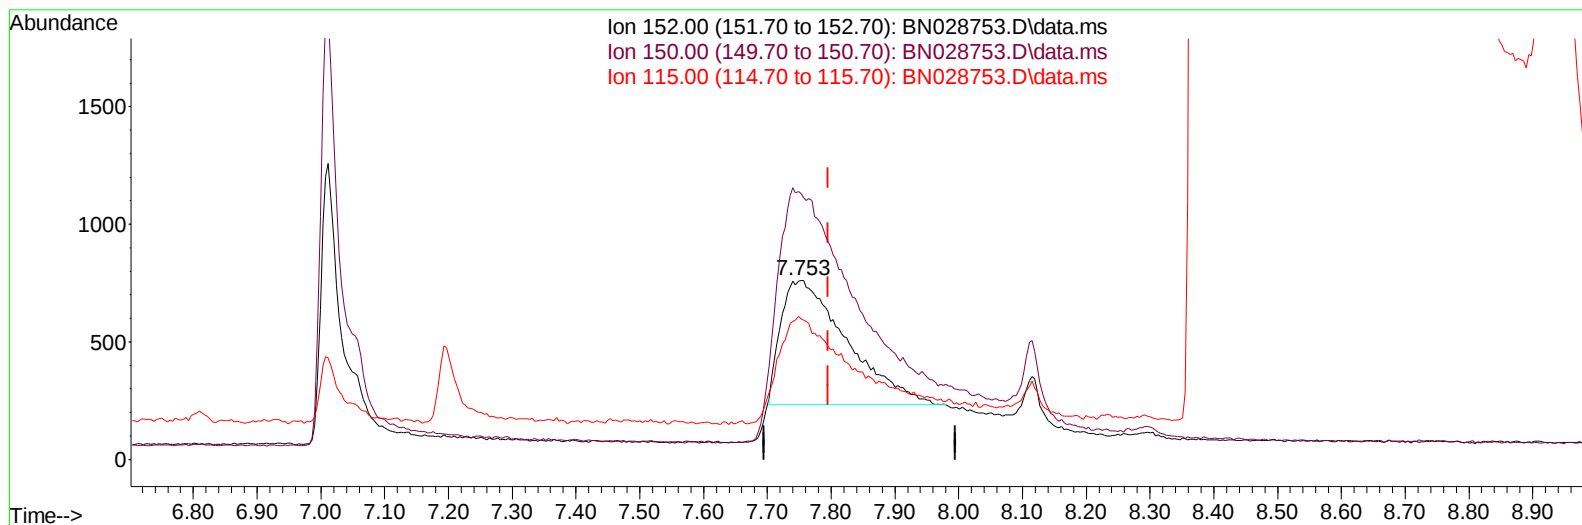

TIC: BN028753.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.753min (-0.042) 0.40 ng/u1

response 3824

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	148.29
115.00	62.20	78.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028753.D
Acq On : 19 Nov 2023 00:16
Operator : MA/JU
Sample : 05370-03
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDP9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:43:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

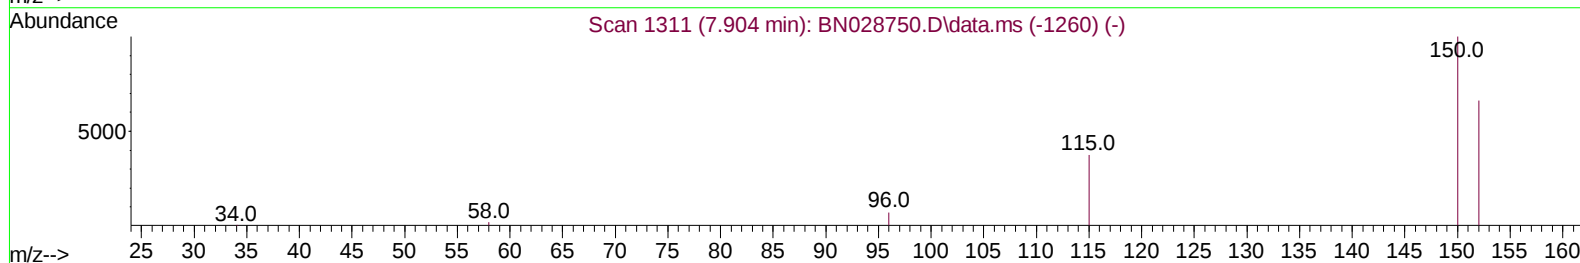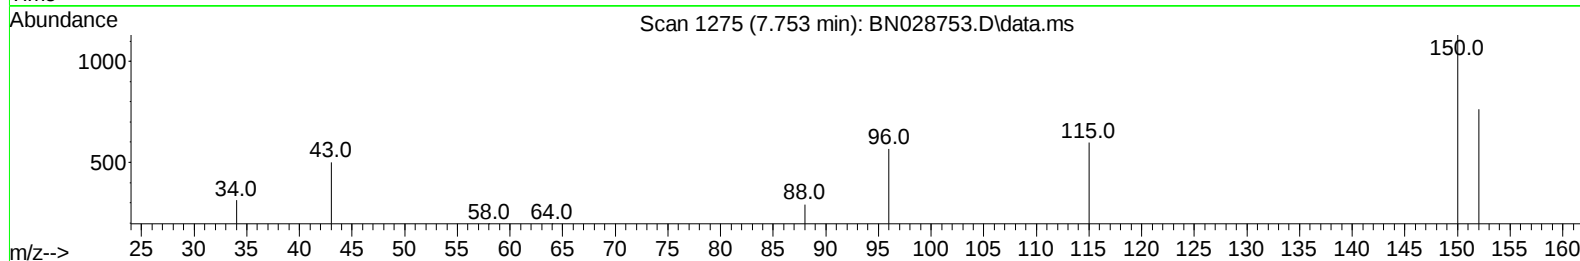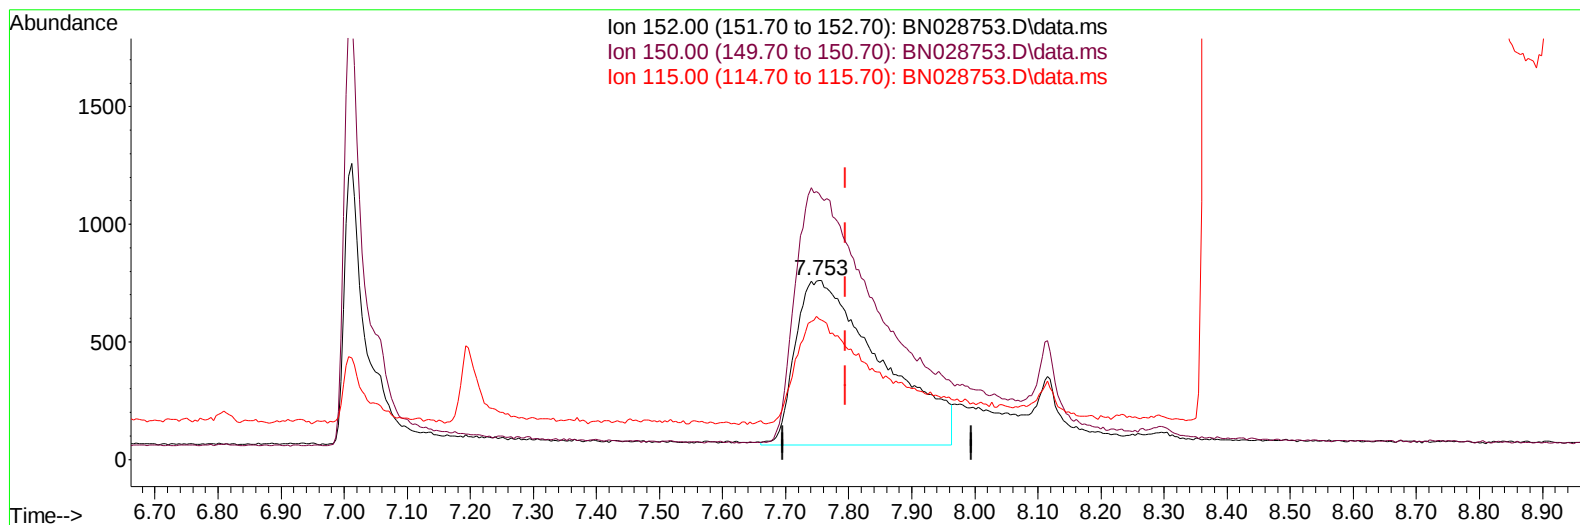

TIC: BN028753.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.753min (-0.042) 0.40 ng/ul m

response 6641

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	148.29
115.00	62.20	78.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028753.D
 Acq On : 19 Nov 2023 00:16
 Operator : MA/JU
 Sample : 05370-03
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDP9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 19 23:43:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.753	152	6641m	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.479	136	25561	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.321	164	15730	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.082	188	31909	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.296	240	20479	0.400	ng/ul	# 0.00
23) Perylene-d12	23.573	264	24714	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	43994	5.994	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.140	152	3972	0.103	ng/ul	0.03
18) Fluoranthene-d10	19.113	212	27537	0.418	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.150	88	5071	0.625	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028753.D
Acq On : 19 Nov 2023 00:16
Operator : MA/JU
Sample : 05370-03
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDP9

Manual IntegrationsAPPROVED

Quant Time: Nov 19 23:43:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

