




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028763.D
Acq On : 19 Nov 2023 06:17
Operator : MA/JU
Sample : 05370-08
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

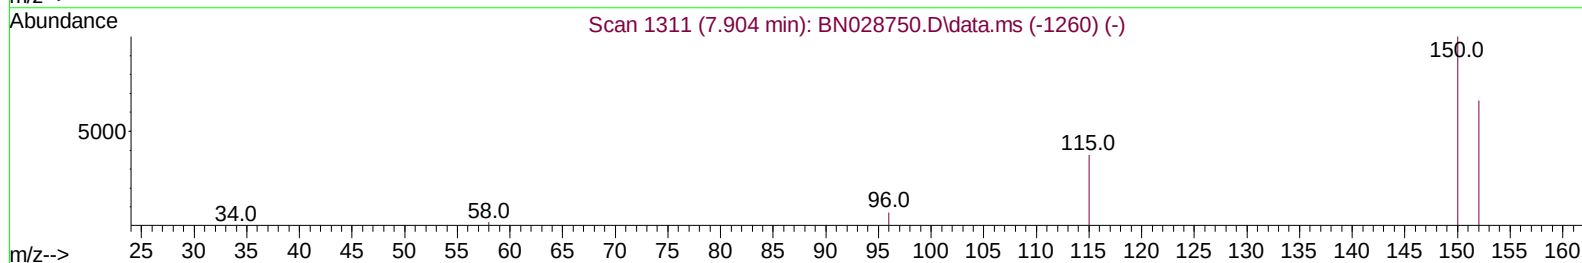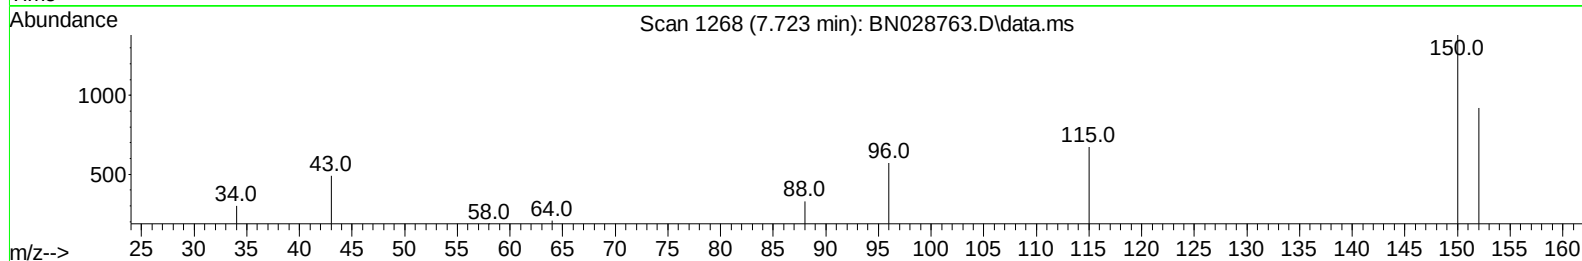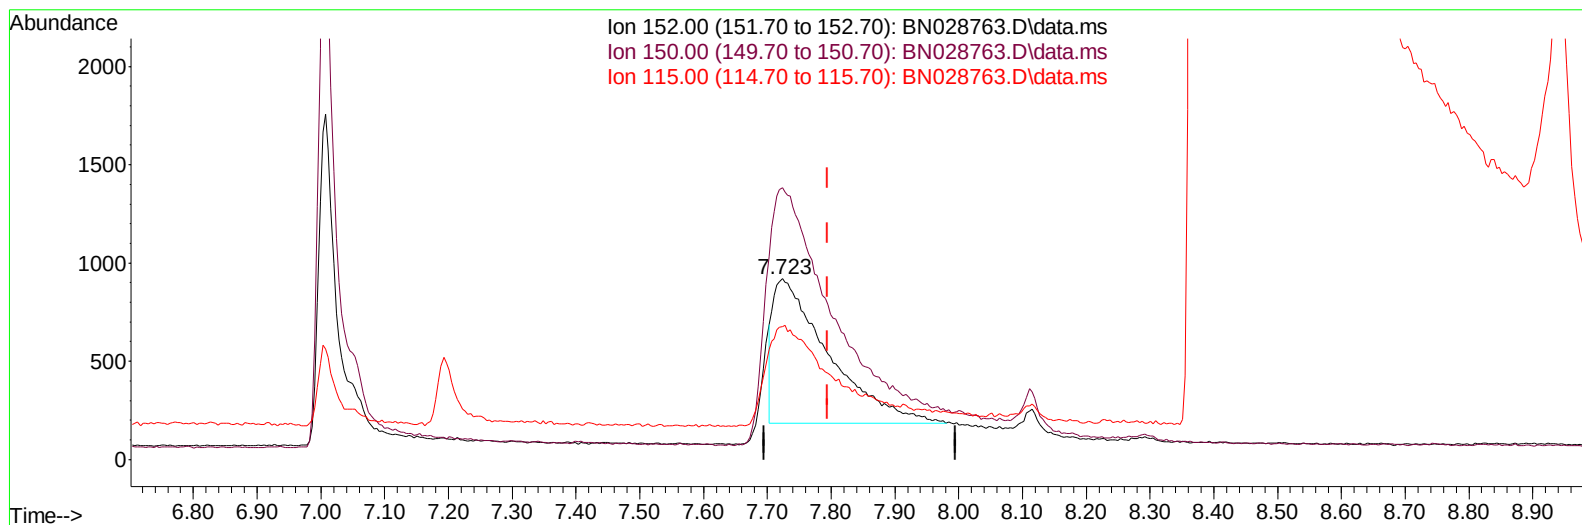

TIC: BN028763.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.723min (-0.072) 0.40 ng/ul

response 4475

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	150.22
115.00	62.20	73.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028763.D
Acq On : 19 Nov 2023 06:17
Operator : MA/JU
Sample : 05370-08
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

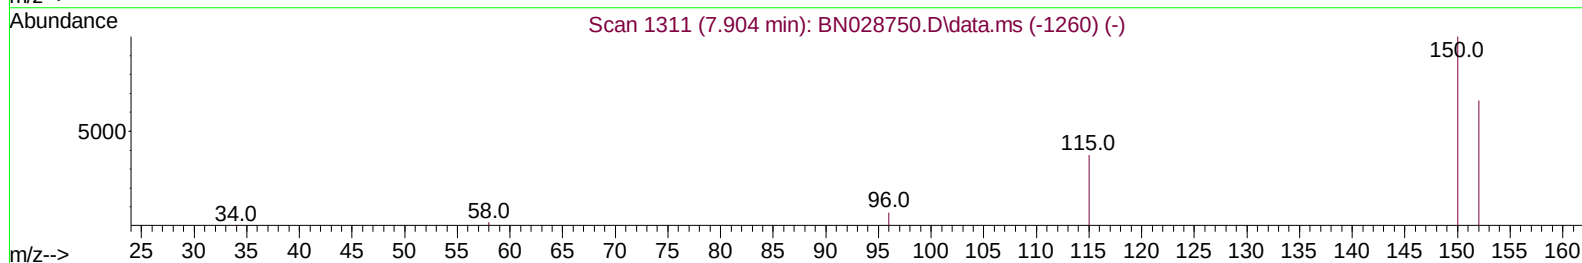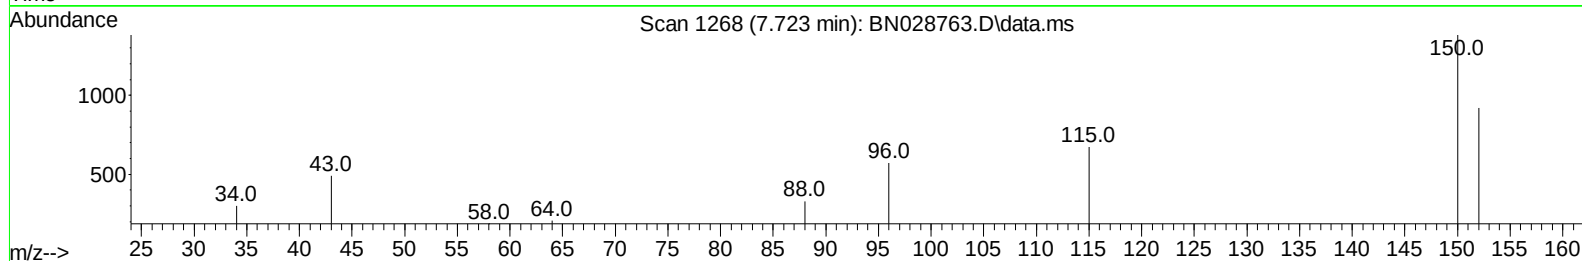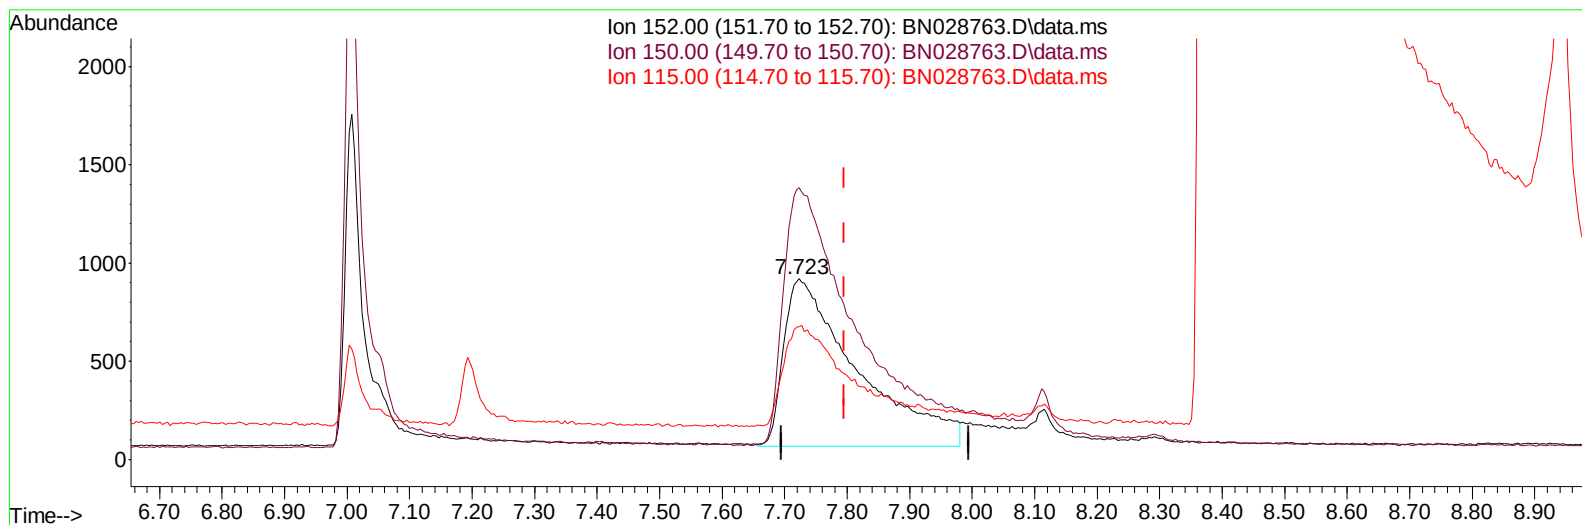

TIC: BN028763.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.723min (-0.072) 0.40 ng/ul m

response 6999

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	150.22
115.00	62.20	73.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028763.D
Acq On : 19 Nov 2023 06:17
Operator : MA/JU
Sample : 05370-08
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

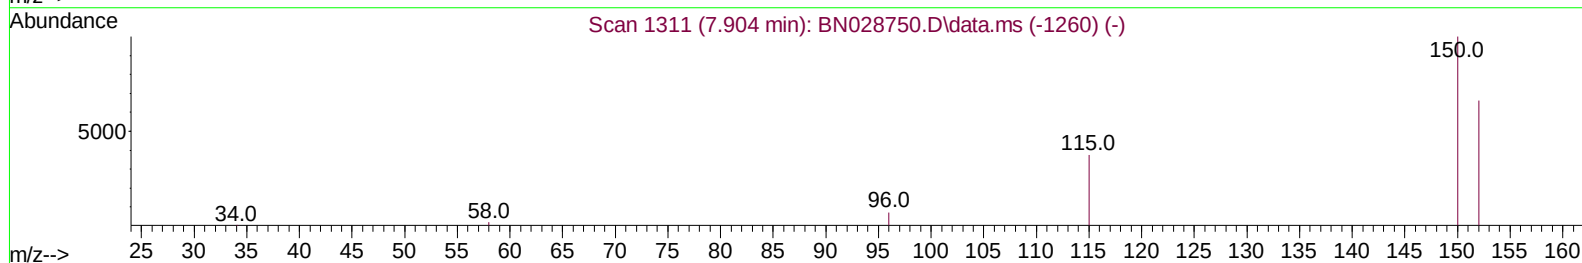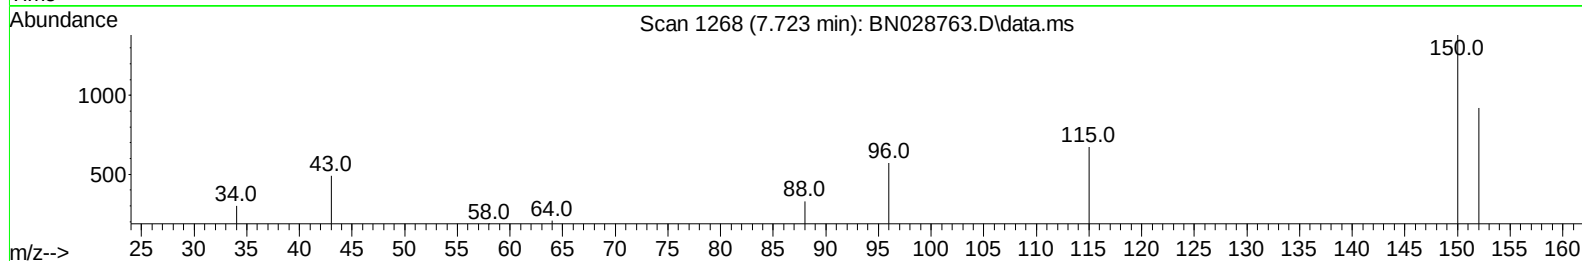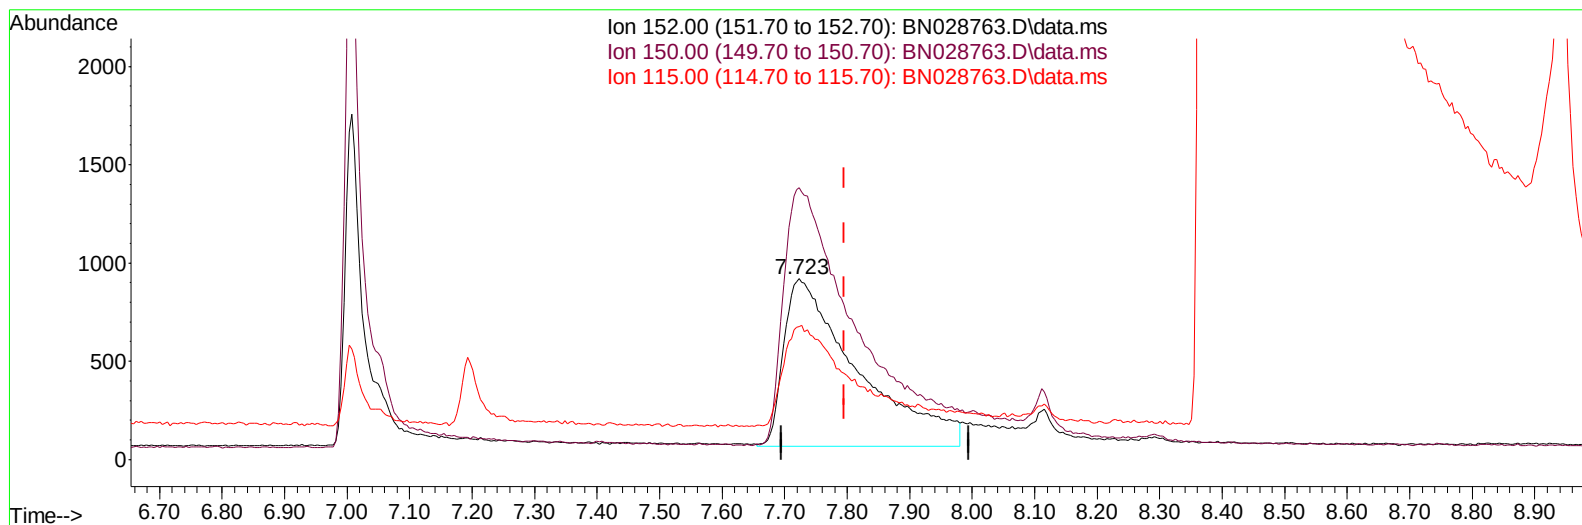

TIC: BN028763.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.723min (-0.072) 0.40 ng/ul m

response 6999

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	150.22
115.00	62.20	73.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028763.D
Acq On : 19 Nov 2023 06:17
Operator : MA/JU
Sample : 05370-08
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

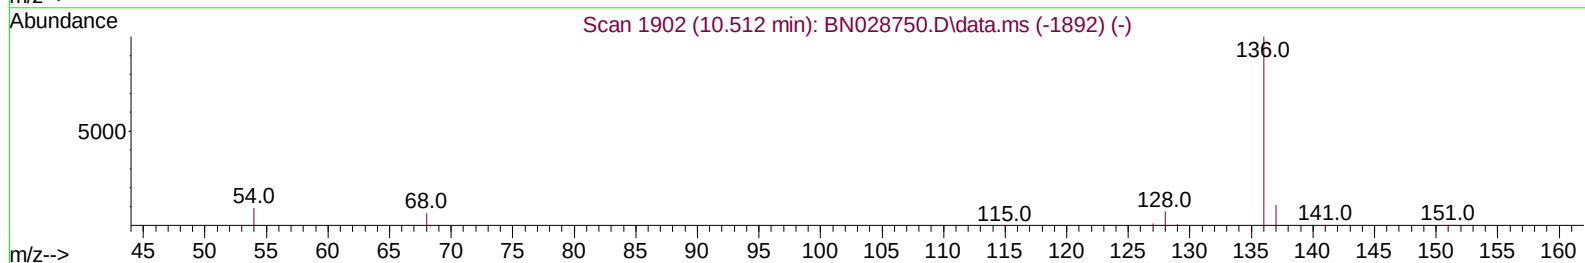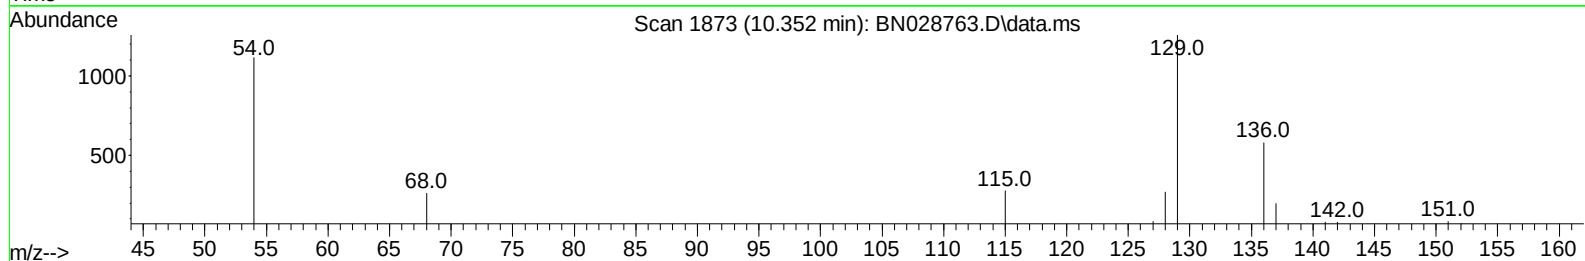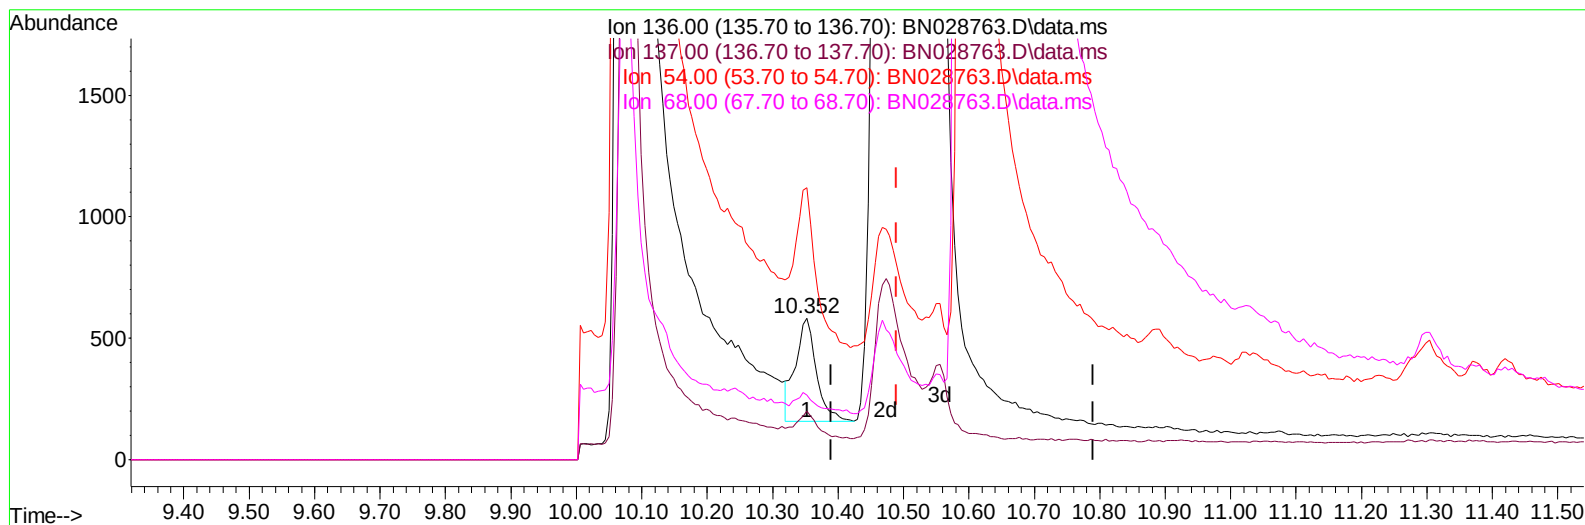

TIC: BN028763.D\data.ms

(4) Naphthalene-d8 (I)

10.352min (-0.138) 0.40 ng/u1

response 949

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.20	34.02#
54.00	9.00	192.27#
68.00	7.10	45.36#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

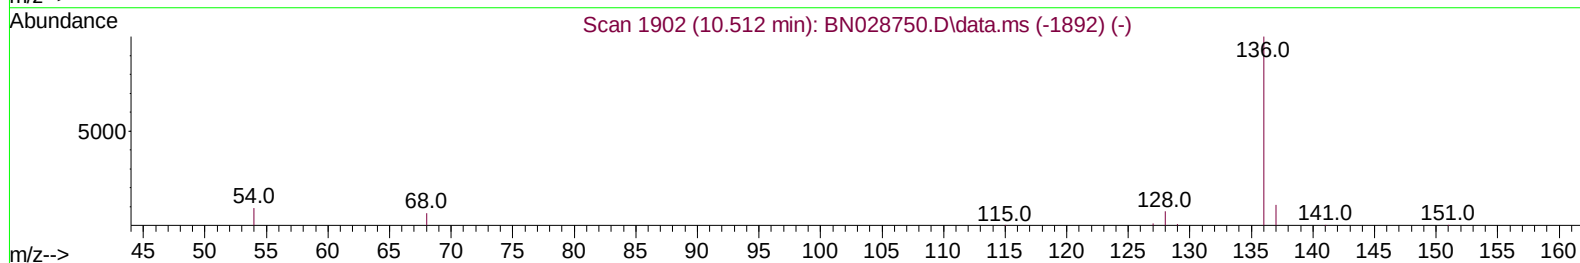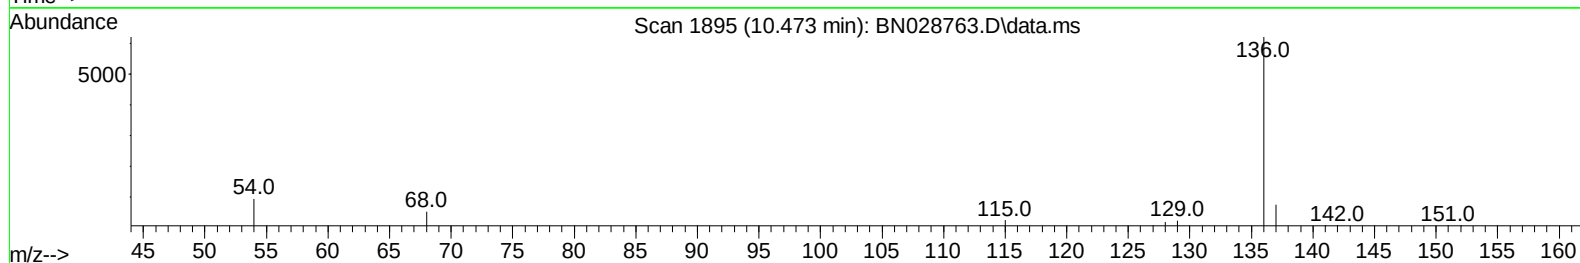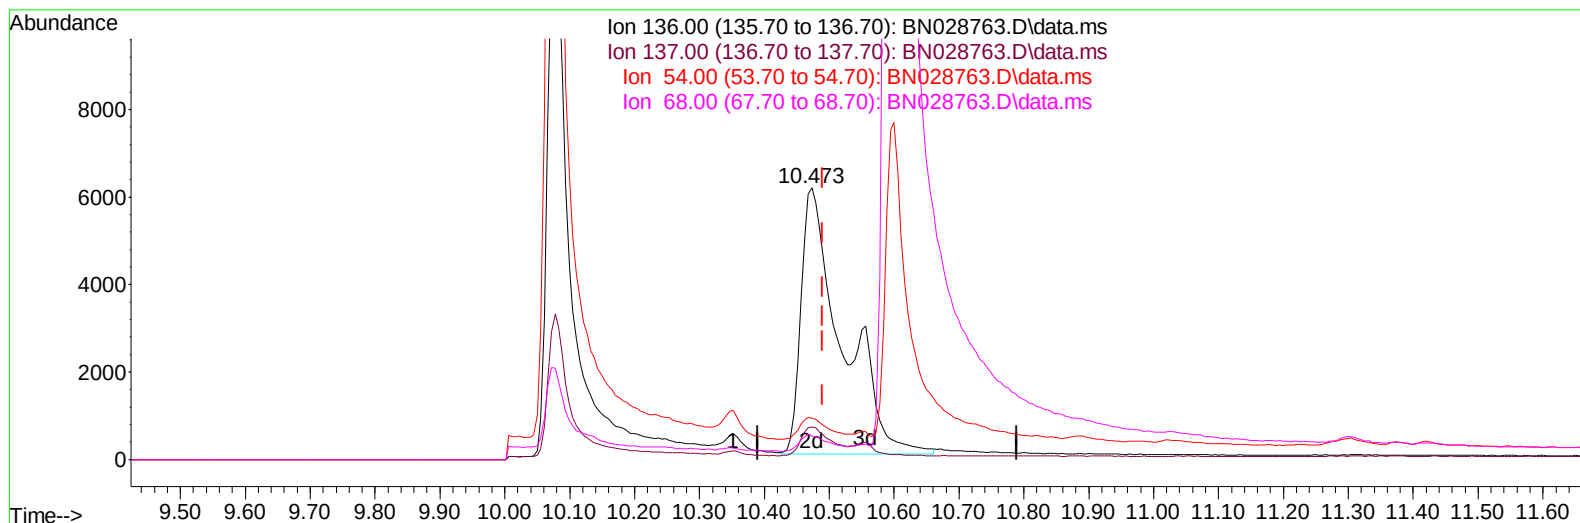

TIC: BN028763.D\data.ms

(4) Naphthalene-d8 (I)

10.473min (-0.017) 0.40 ng/ul m

response 26774

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.20	12.00
54.00	9.00	15.27#
68.00	7.10	8.58#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

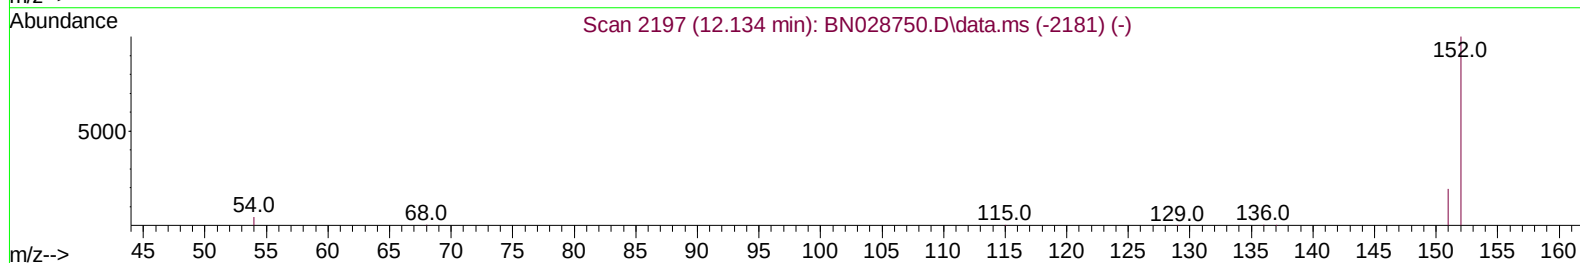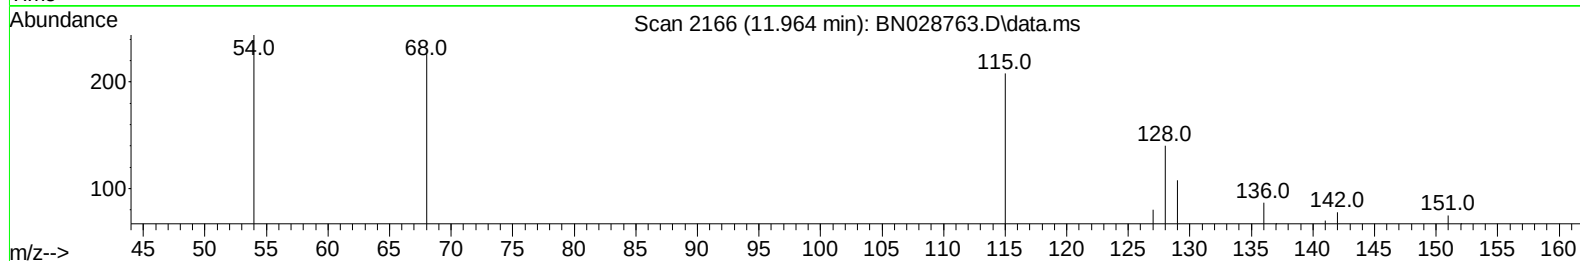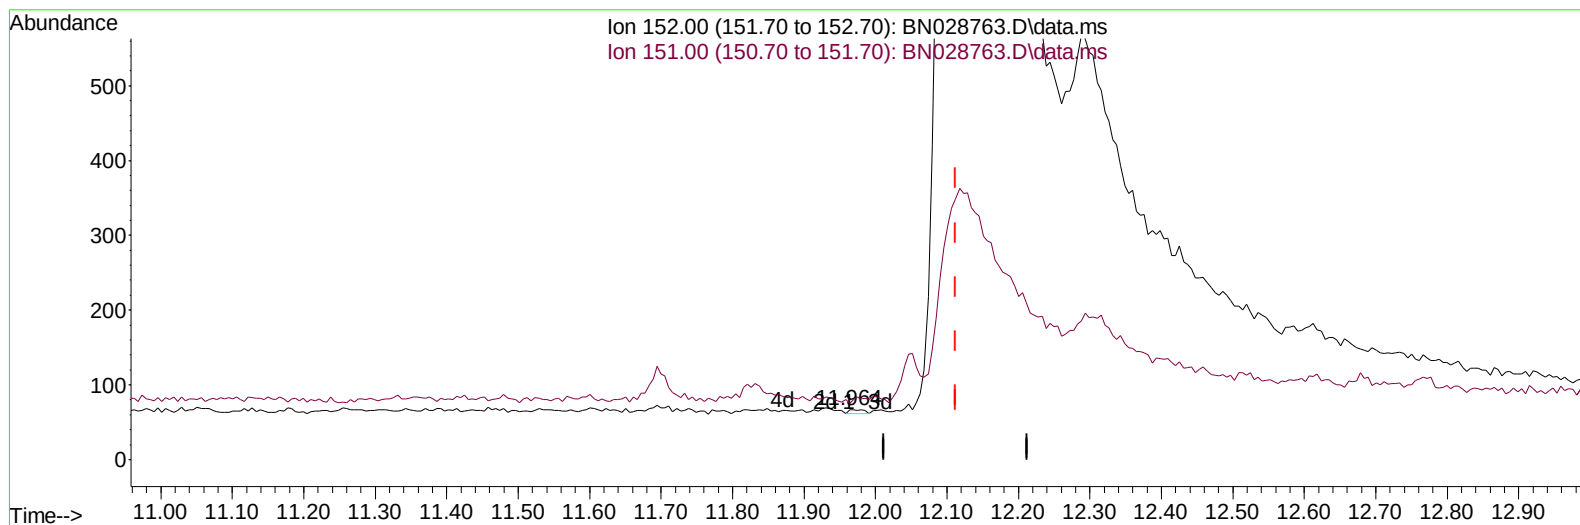

TIC: BN028763.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

11.964min (-0.149) 0.00 ng/u1

response 8

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	137.50#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

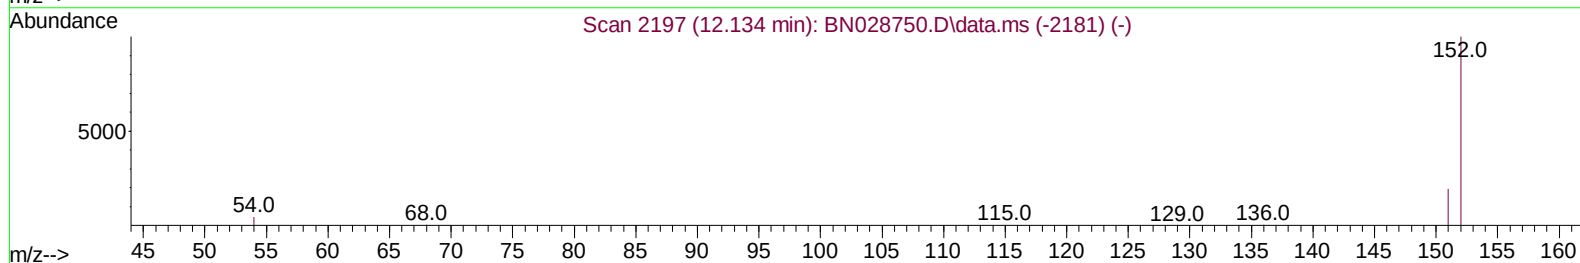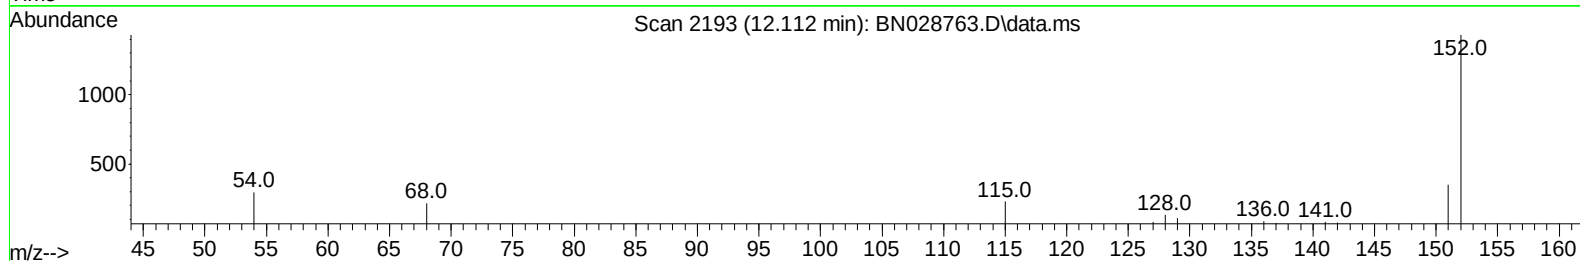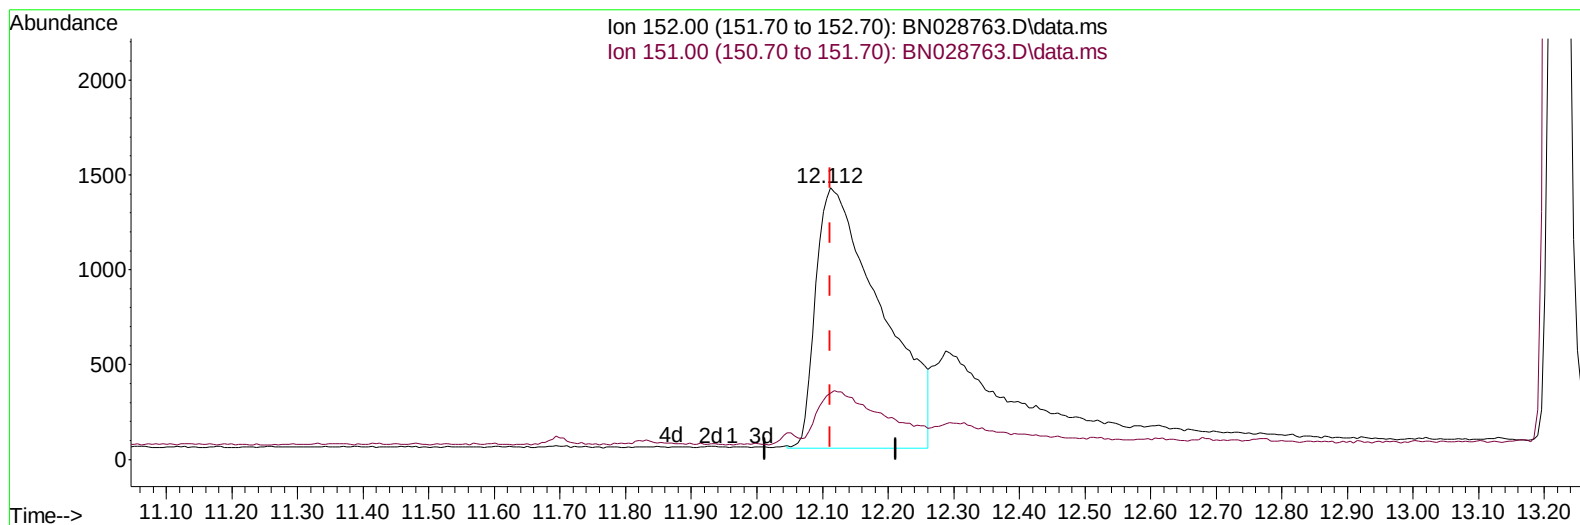

TIC: BN028763.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.112min (-0.000) 0.23 ng/ul m

response 9447

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	0.12#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

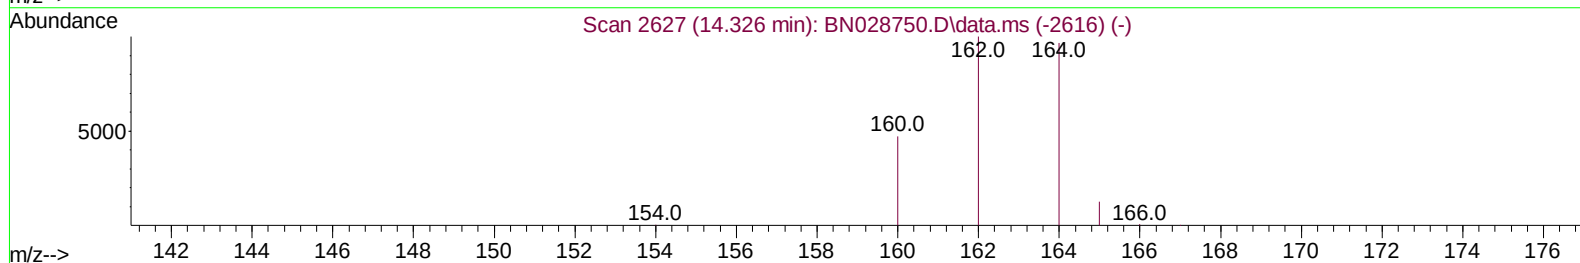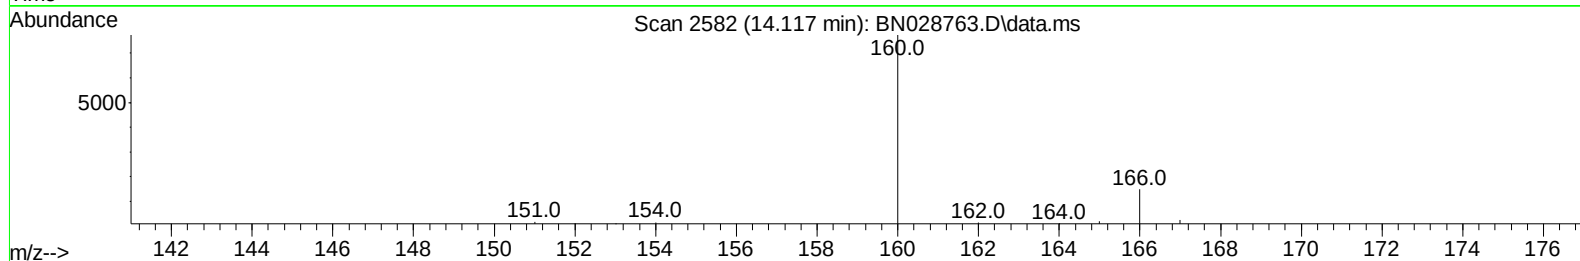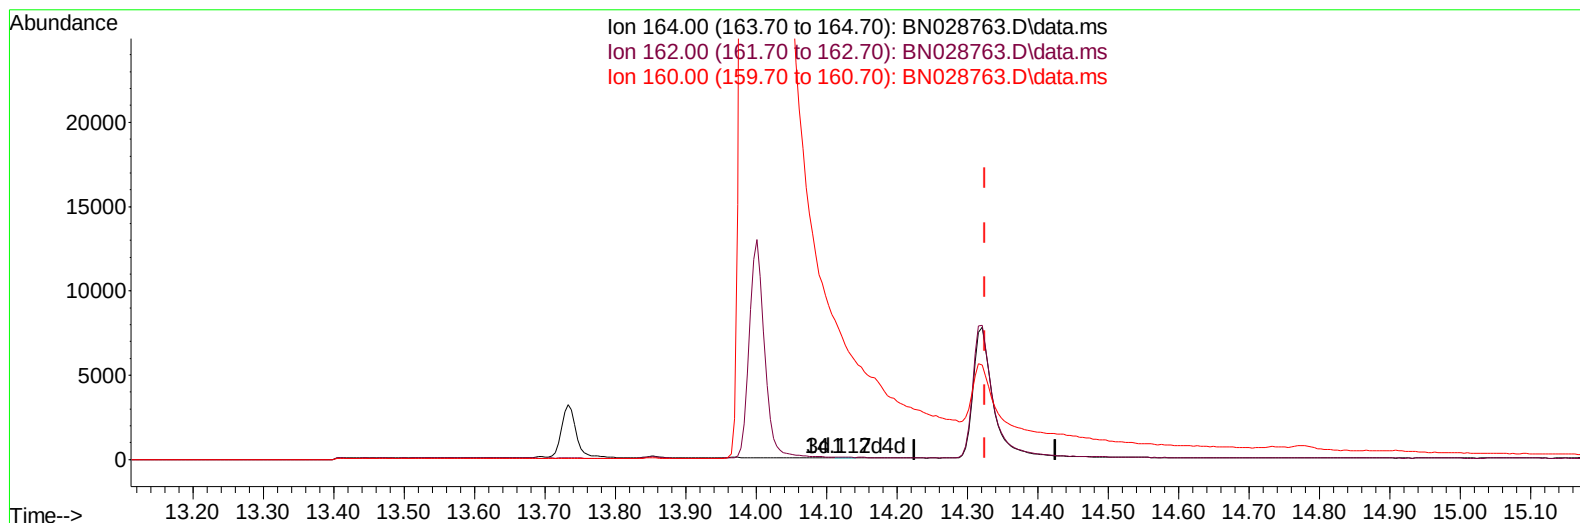

TIC: BN028763.D\data.ms

(9) Acenaphthene-d10 (I)

14.117min (-0.208) 0.40 ng/u1

response 4

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.90	146.59#
160.00	49.20	8793.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

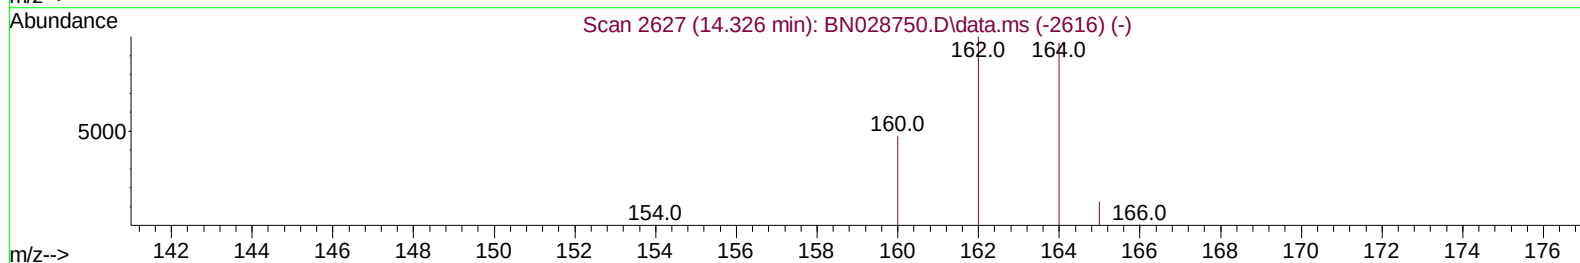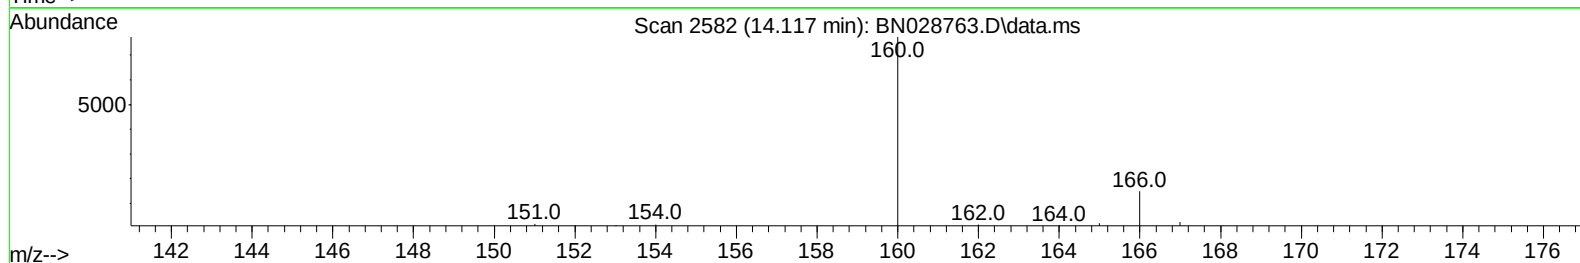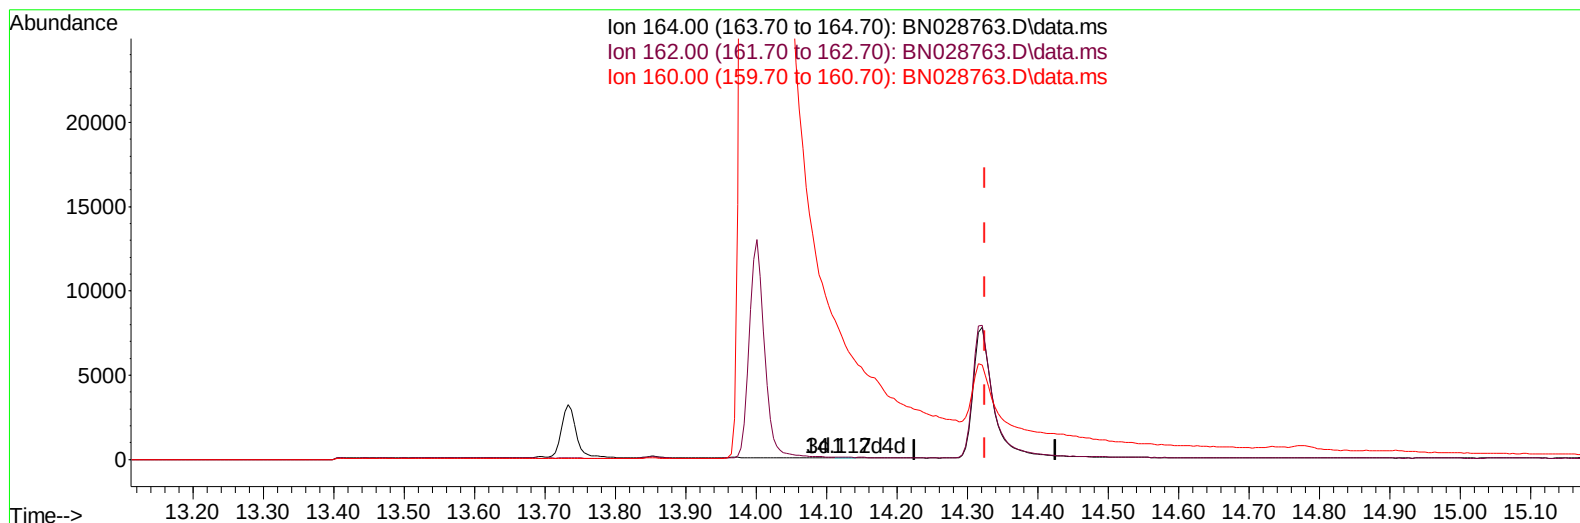

TIC: BN028763.D\data.ms

(9) Acenaphthene-d10 (I)

14.117min (-0.208) 0.40 ng/u1

response 4

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.90	146.59#
160.00	49.20	8793.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

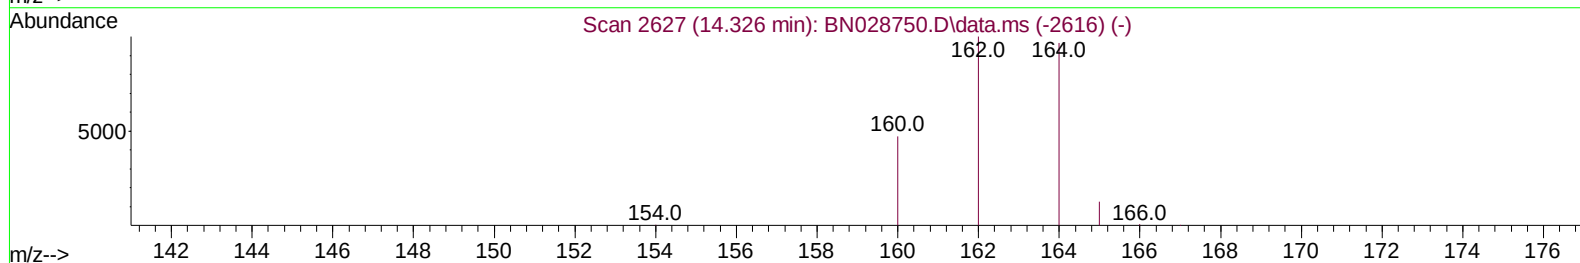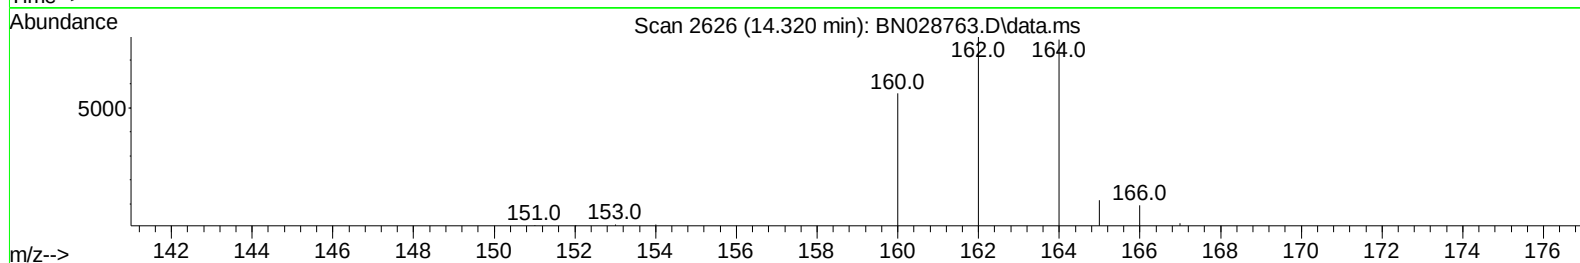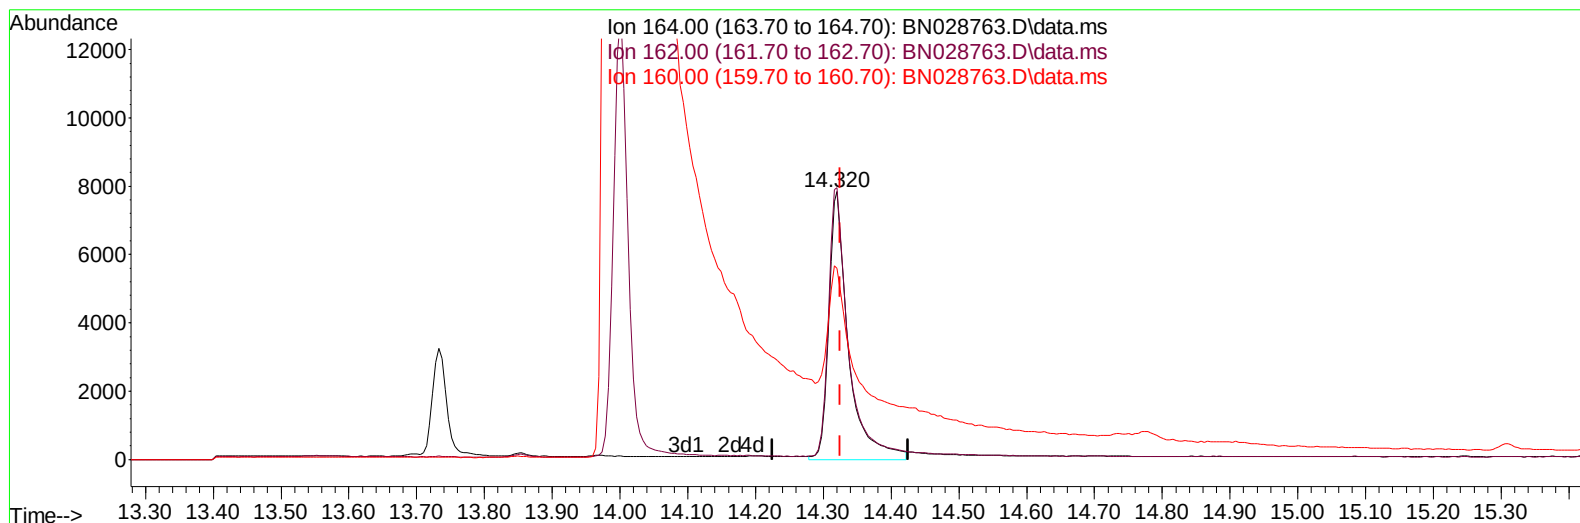

TIC: BN028763.D\data.ms

(9) Acenaphthene-d10 (I)

14.320min (-0.005) 0.40 ng/ul m

response 15906

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.90	101.43
160.00	49.20	71.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

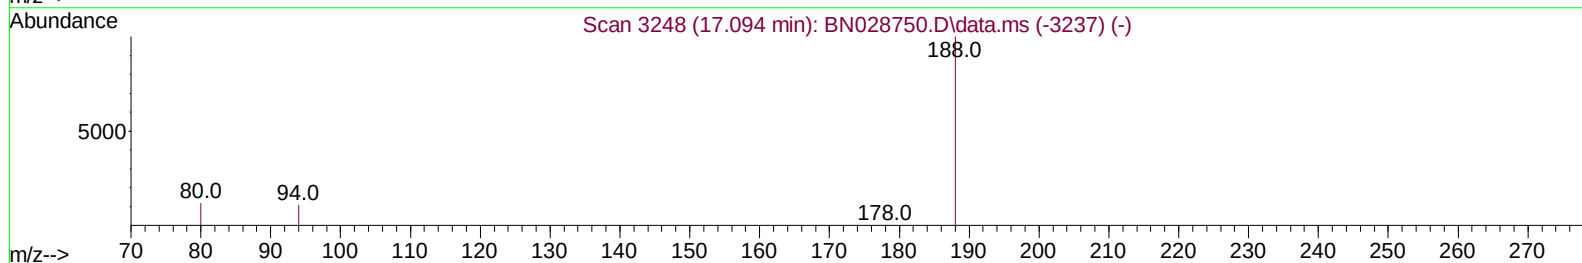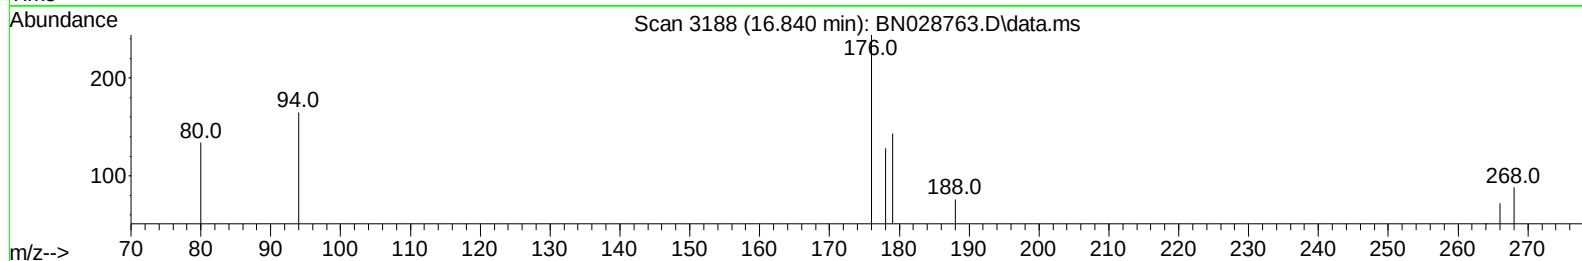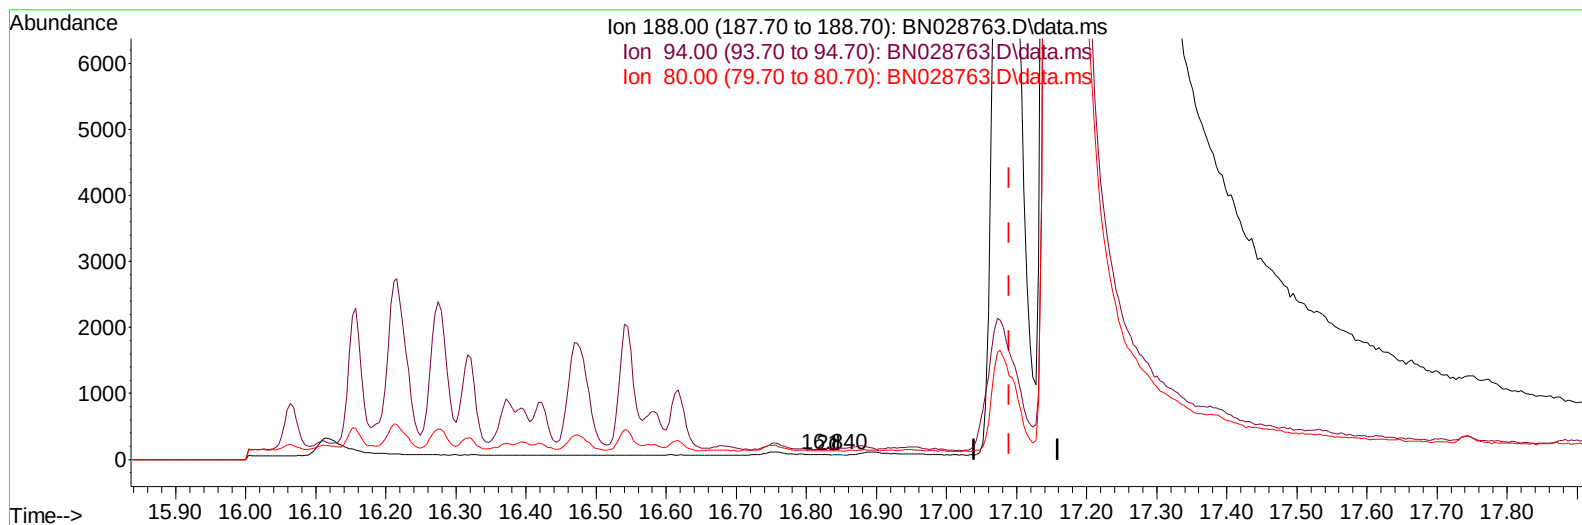

TIC: BN028763.D\data.ms

(13) Phenanthrene-d10 (I)

16.840min (-0.249) 0.40 ng/u1

response 4

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	217.11#
80.00	10.90	176.32#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

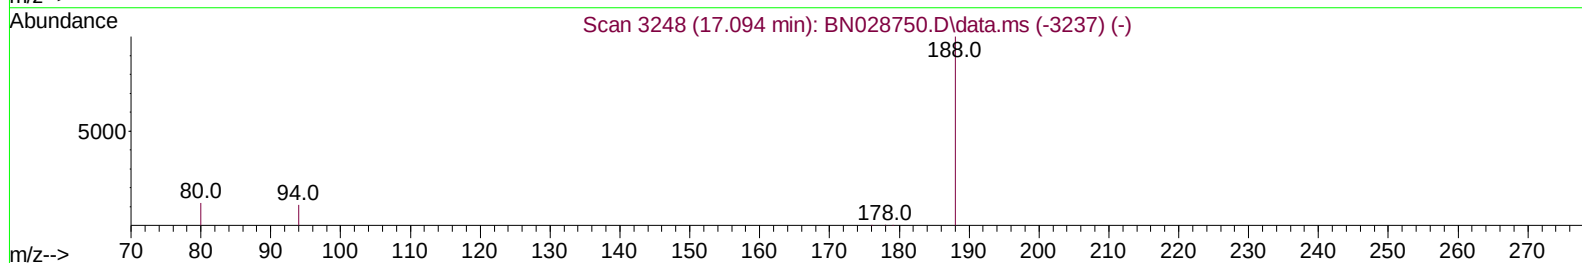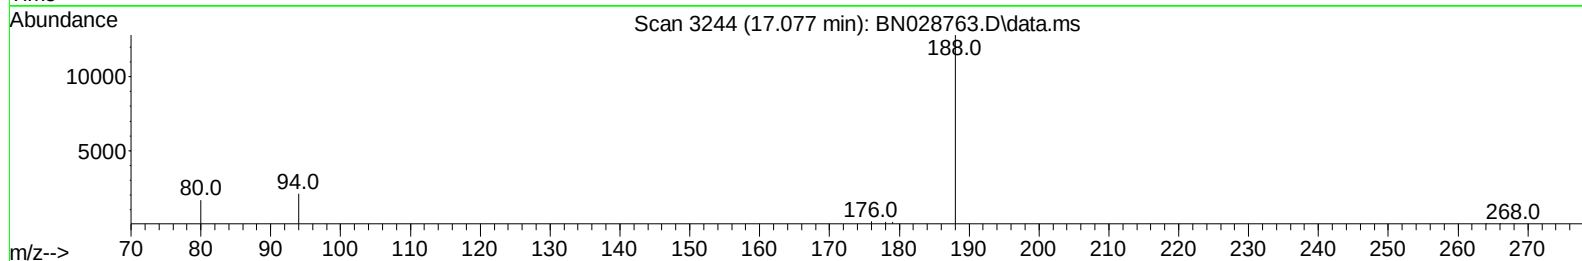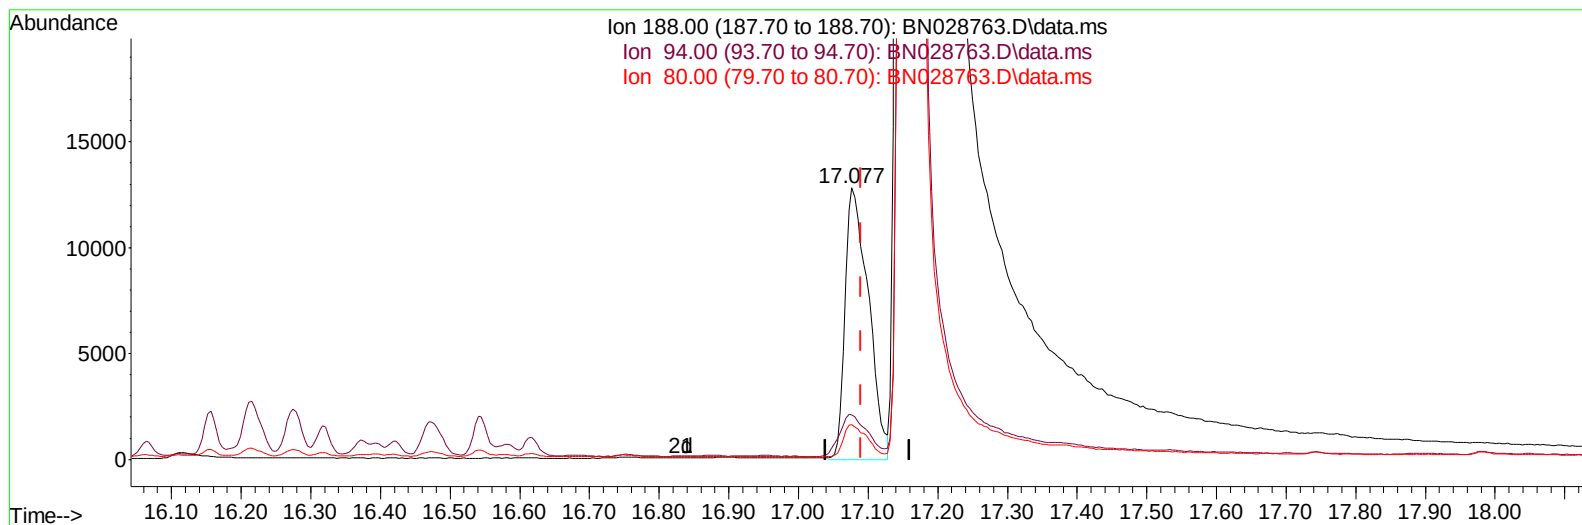

TIC: BN028763.D\data.ms

(13) Phenanthrene-d10 (I)

17.077min (-0.013) 0.40 ng/ul m

response 29790

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	16.45#
80.00	10.90	12.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

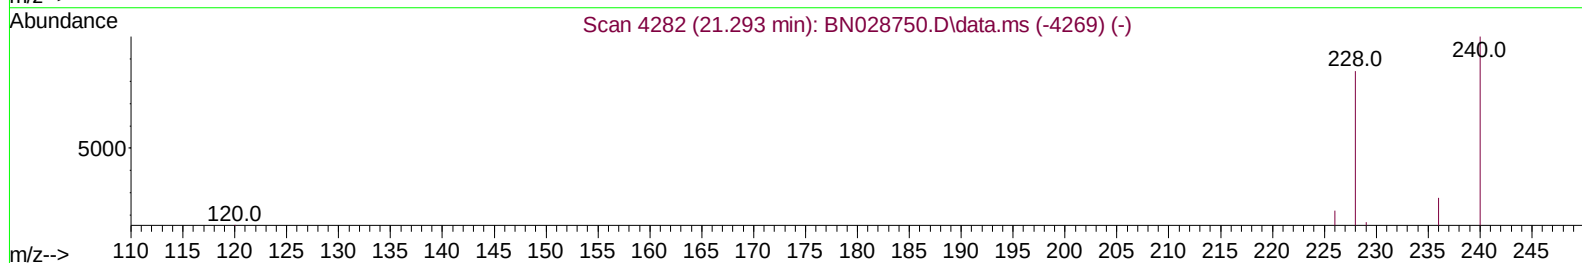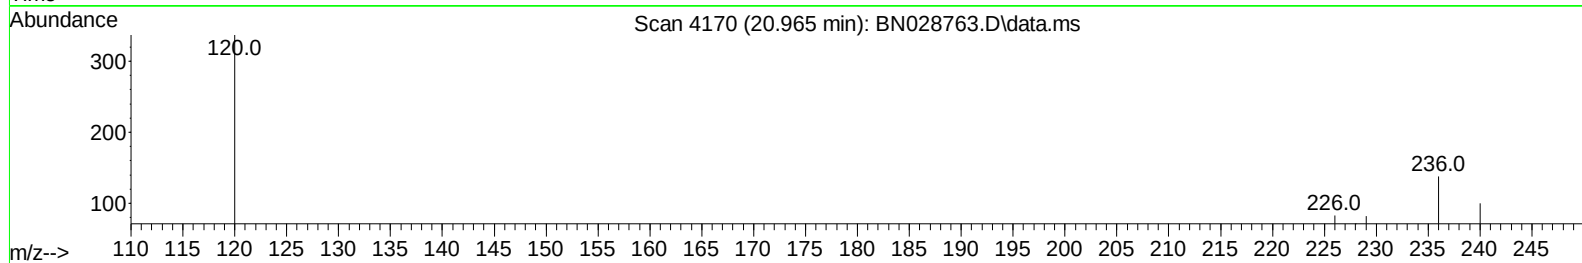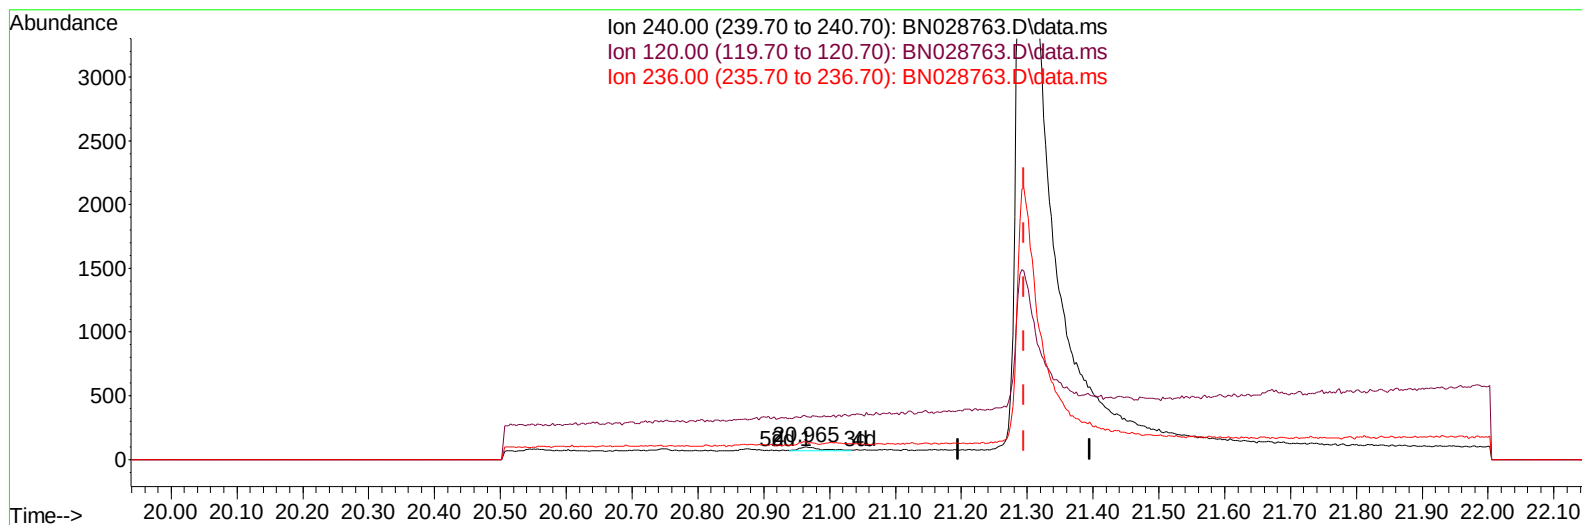

TIC: BN028763.D\data.ms

(17) Chrysene-d12

20.965min (-0.330) 0.40 ng/u1

response 71

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.00	337.00#
236.00	28.00	138.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

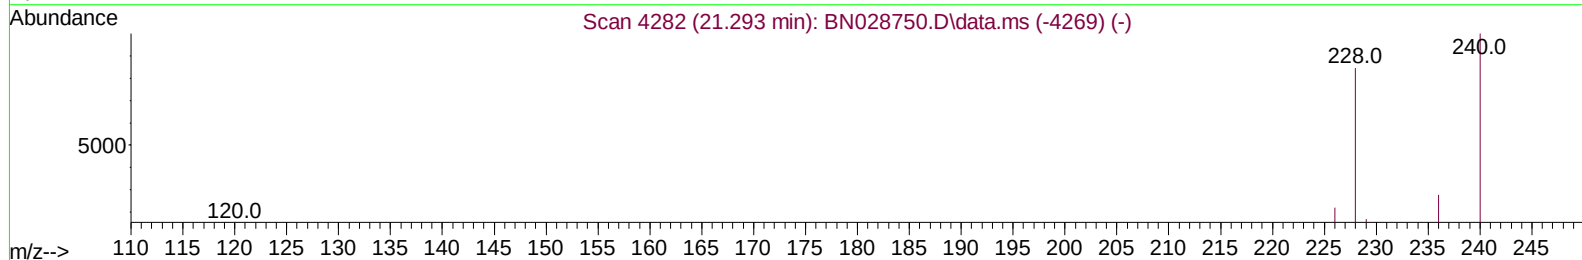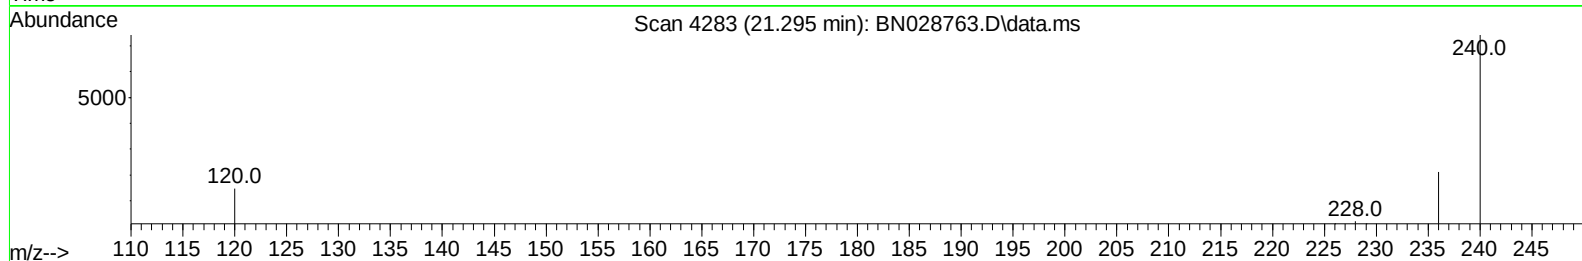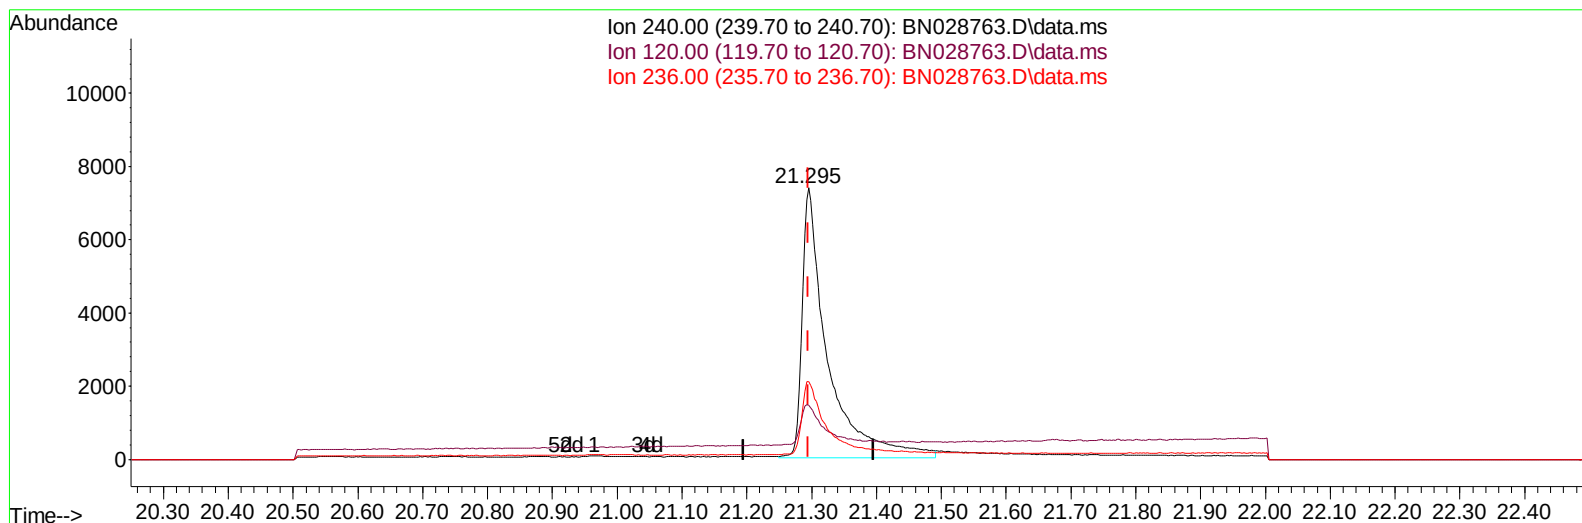

TIC: BN028763.D\data.ms

(17) Chrysene-d12

21.295min (-0.000) 0.40 ng/ul m

response 20067

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.00	19.95#
236.00	28.00	28.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

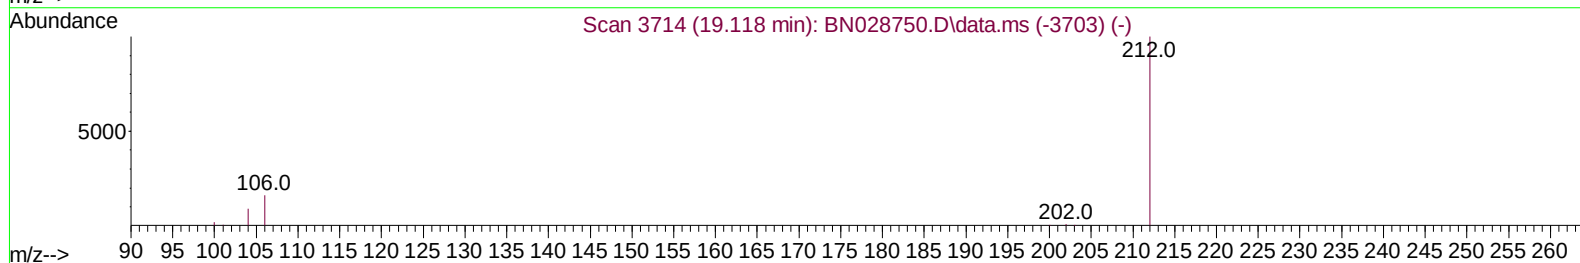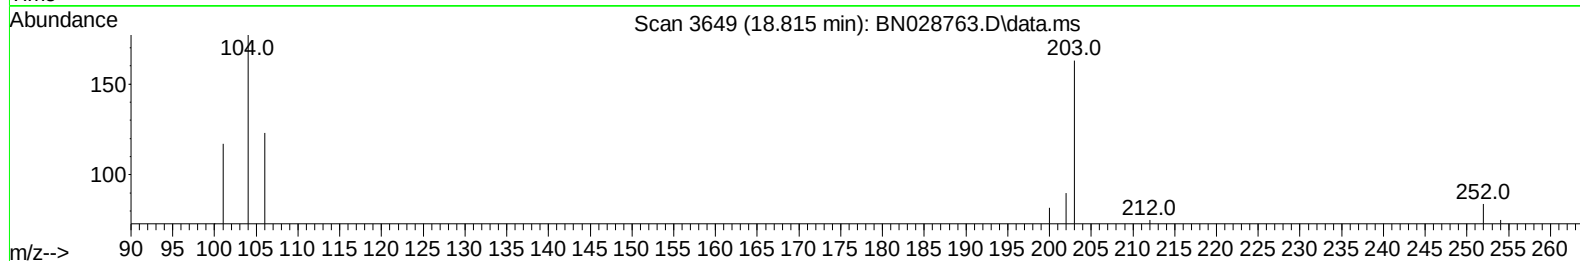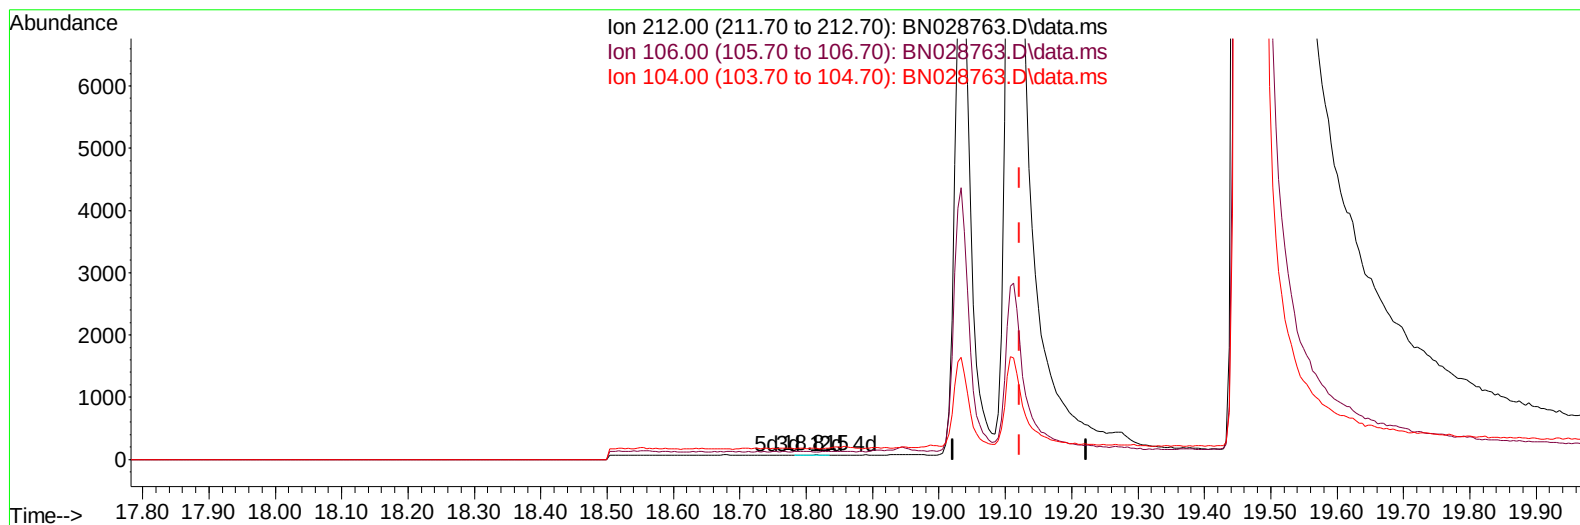

TIC: BN028763.D\data.ms

(18) Fluoranthene-d10 (SURR)

18.815min (-0.307) 0.00 ng/u1

response 11

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	14.80	0.00#
104.00	8.30	81.82#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

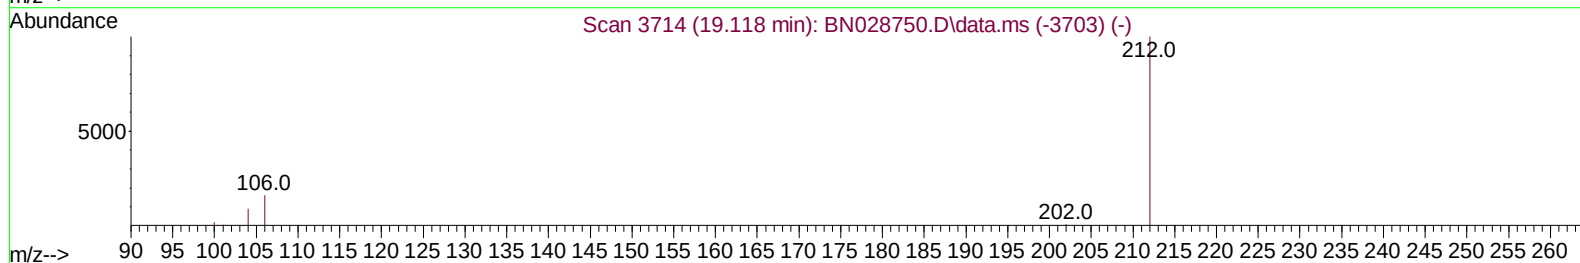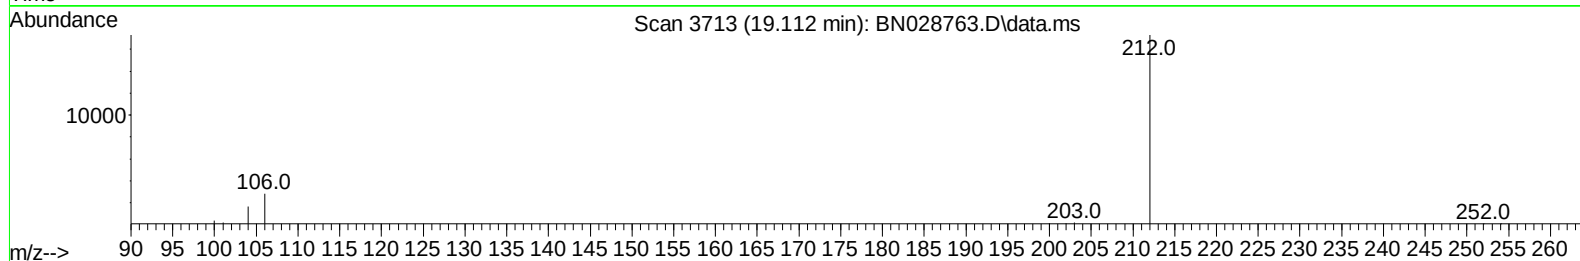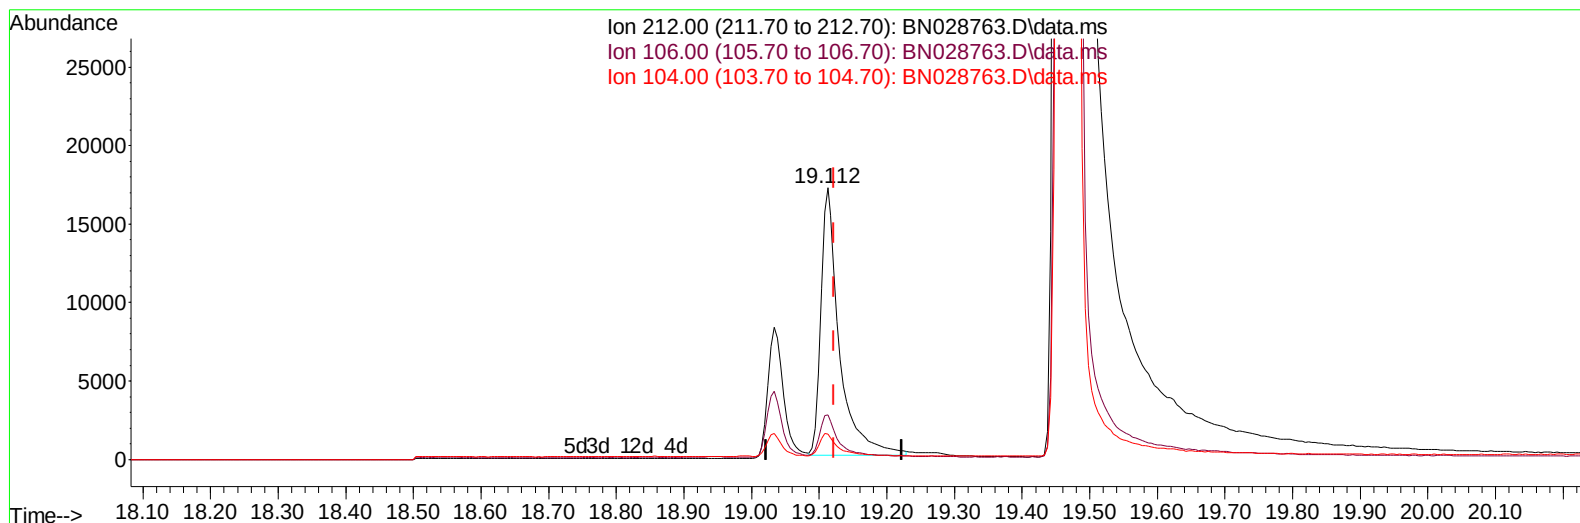

TIC: BN028763.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.112min (-0.009) 0.50 ng/ul m

response 32463

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	14.80	0.00#
104.00	8.30	0.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

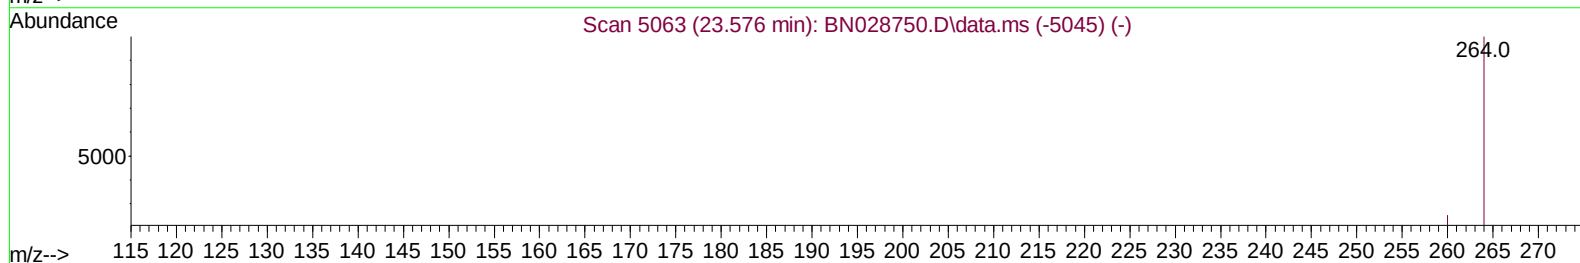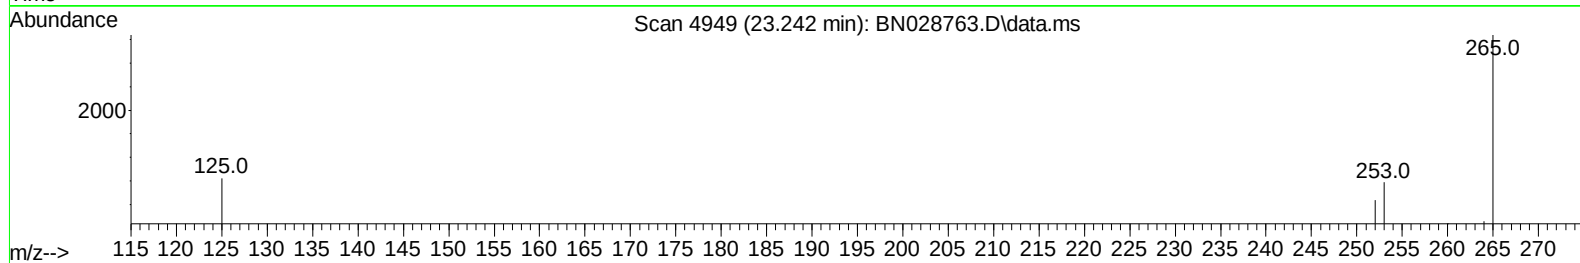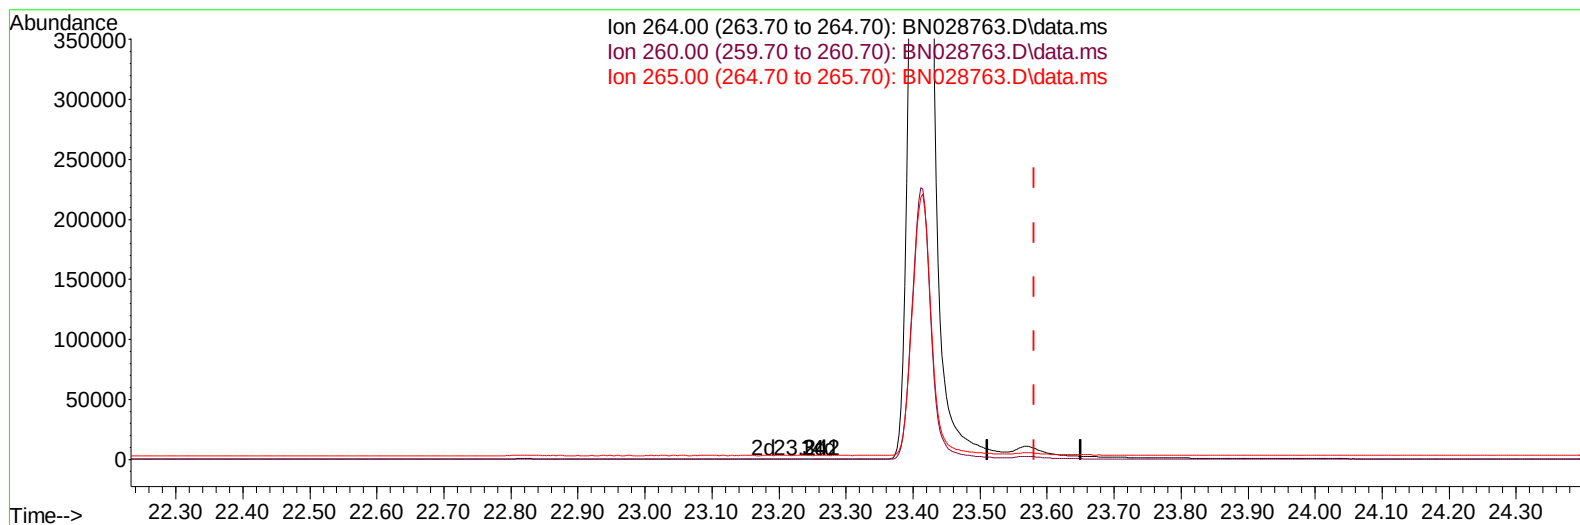

TIC: BN028763.D\data.ms

(23) Perylene-d12 (I)

23.242min (-0.339) 0.40 ng/u1

response 7

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	59.66#
265.00	38.80	2755.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

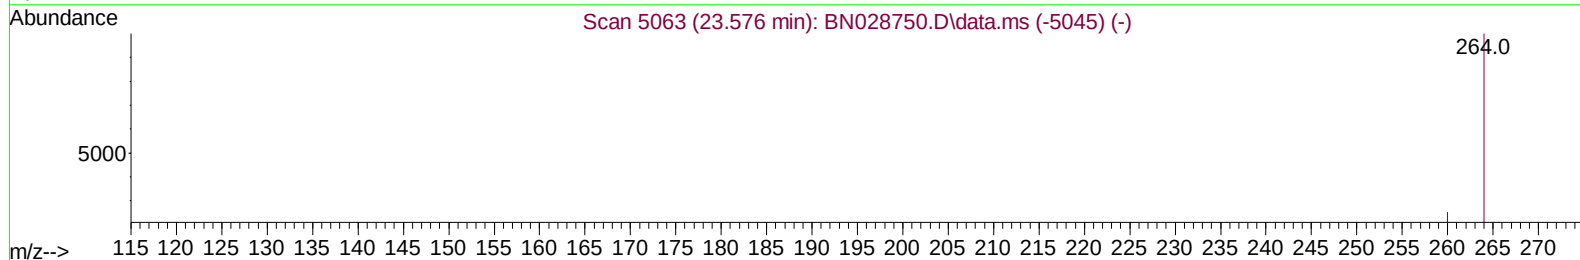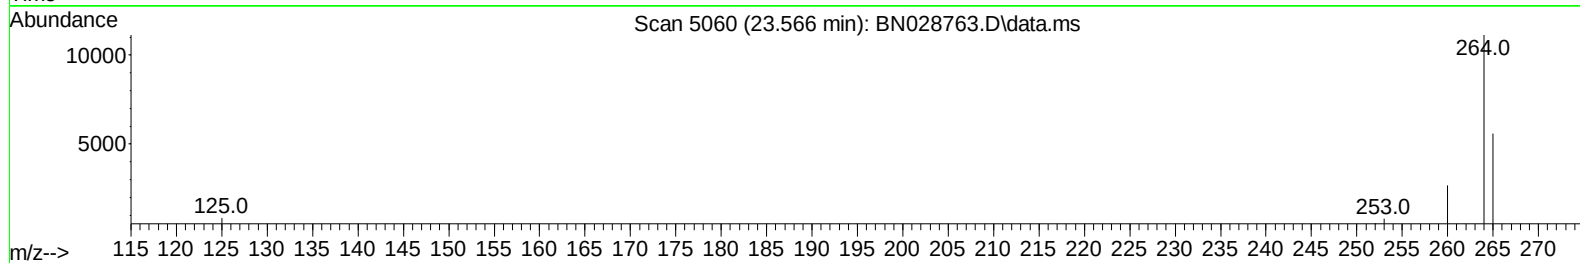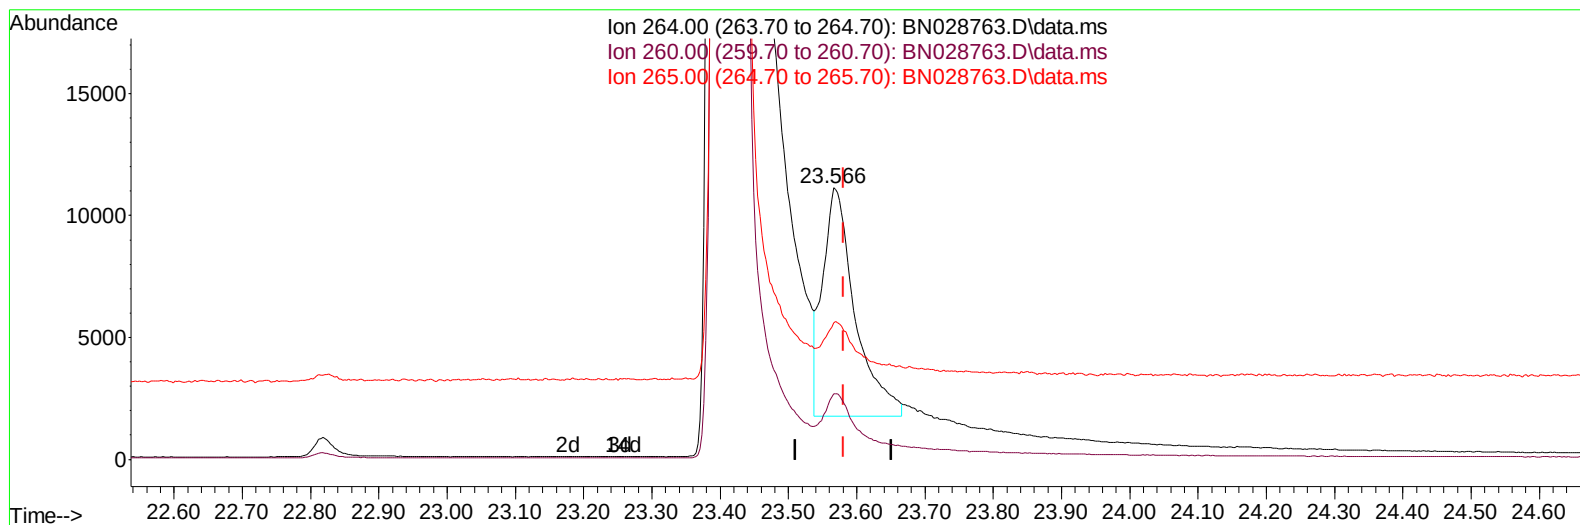

TIC: BN028763.D\data.ms

(23) Perylene-d12 (I)

23.566min (-0.015) 0.40 ng/ul m

response 30853

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.07
265.00	38.80	50.27#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028763.D
 Acq On : 19 Nov 2023 06:17
 Operator : MA/JU
 Sample : 05370-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 00:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.723	152	6999m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.473	136	26774m	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.320	164	15906m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.077	188	29790m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.295	240	20067m	0.400	ng/ul	0.00
23) Perylene-d12	23.566	264	30853m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	38565	4.986	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.112	152	9447m	0.234	ng/ul	0.00
18) Fluoranthene-d10	19.112	212	32463m	0.503	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028763.D
Acq On : 19 Nov 2023 06:17
Operator : MA/JU
Sample : 05370-08
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDQ4

Manual IntegrationsAPPROVED

Quant Time: Nov 20 00:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

