




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028776.D
Acq On : 19 Nov 2023 14:37
Operator : MA/JU
Sample : 05370-16
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDR0

Manual IntegrationsAPPROVED

Quant Time: Nov 20 02:03:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

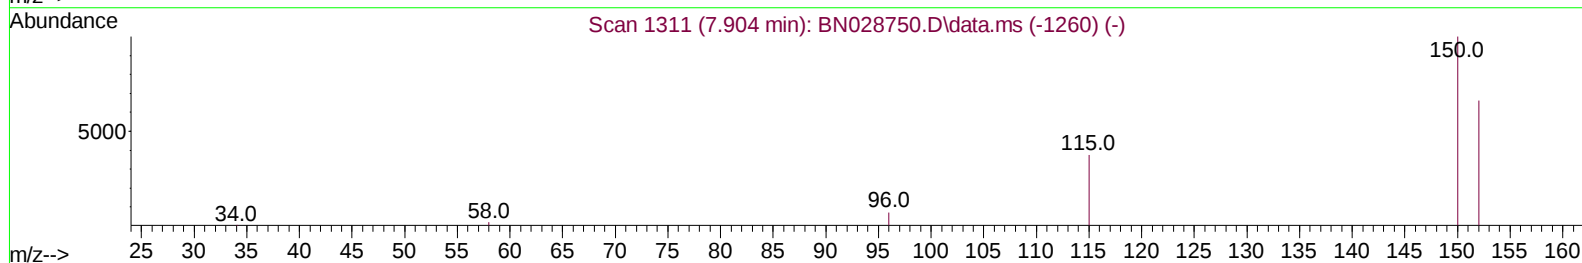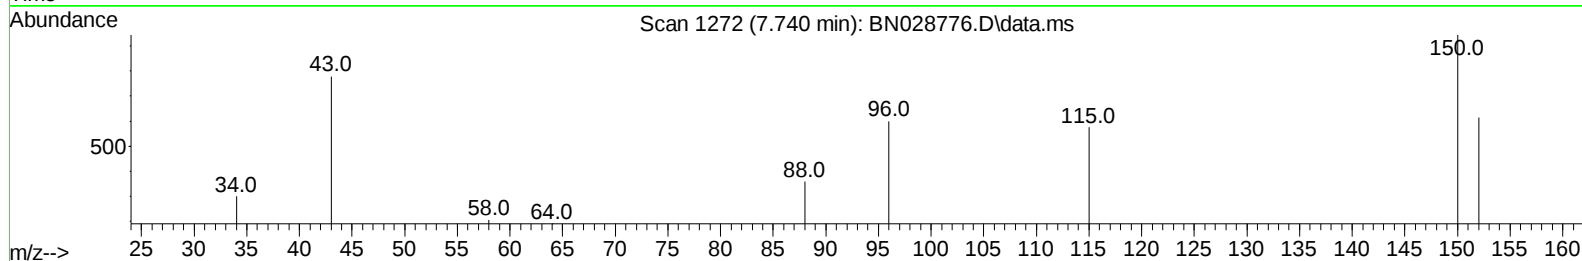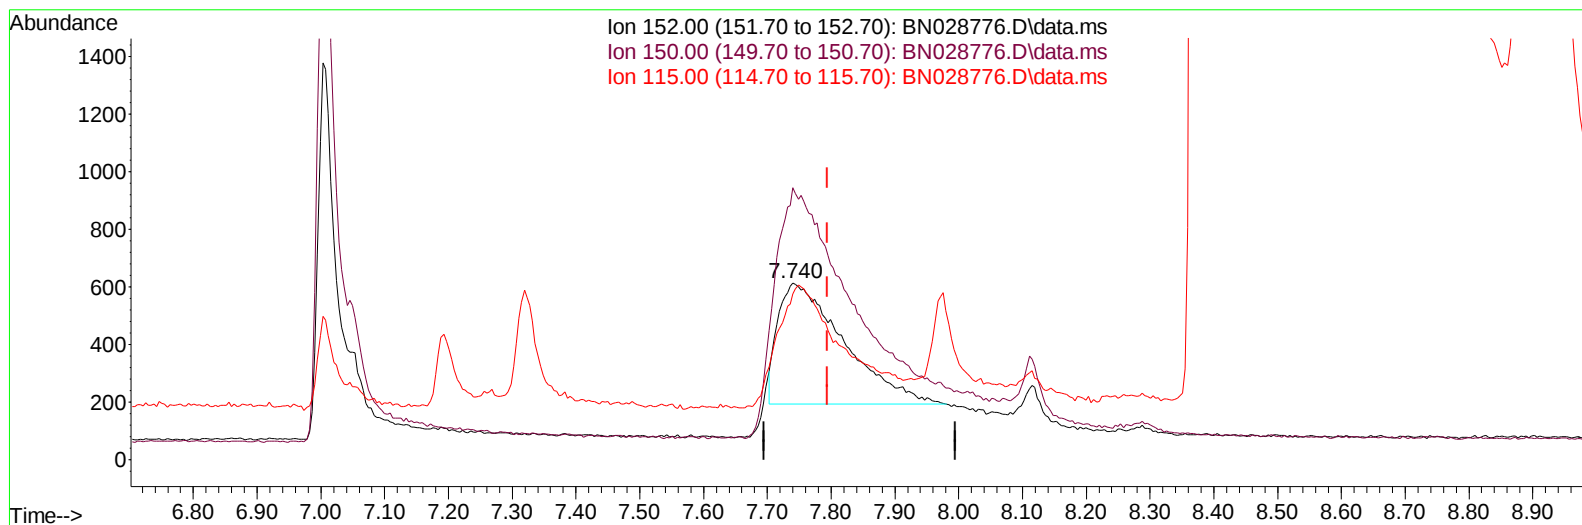

TIC: BN028776.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.740min (-0.055) 0.40 ng/u1

response 3036

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	153.75
115.00	62.20	93.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028776.D
Acq On : 19 Nov 2023 14:37
Operator : MA/JU
Sample : 05370-16
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDR0

Manual IntegrationsAPPROVED

Quant Time: Nov 20 02:03:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

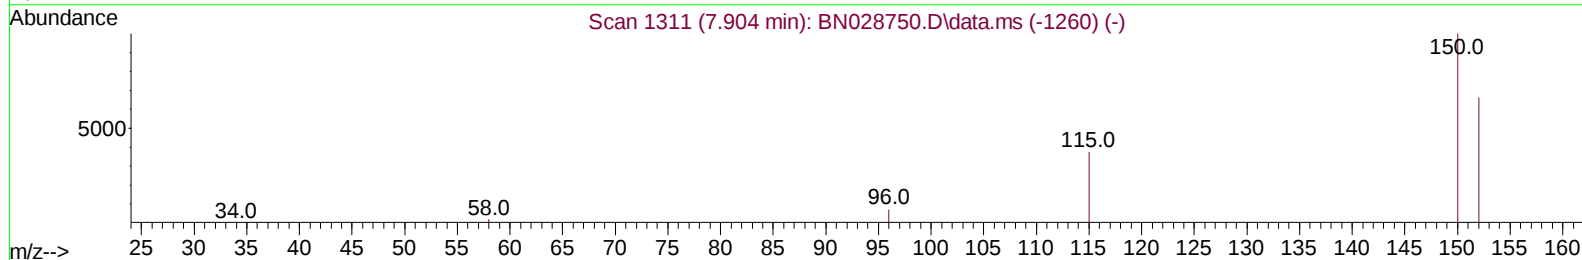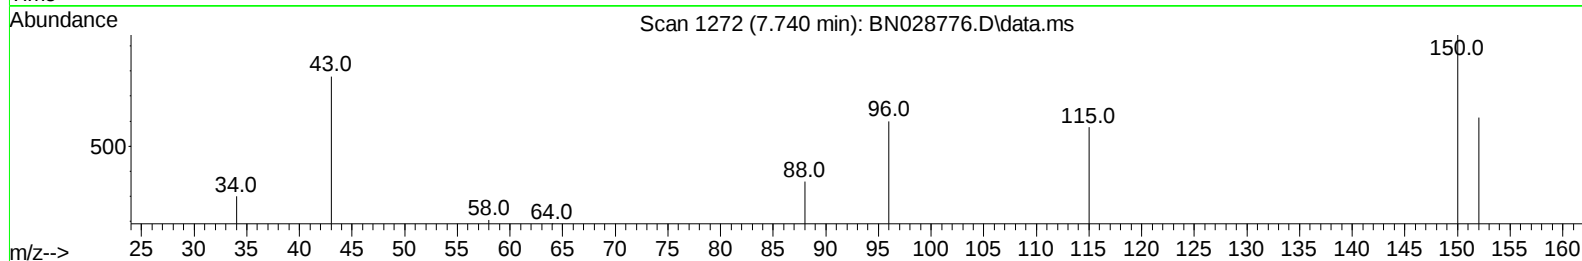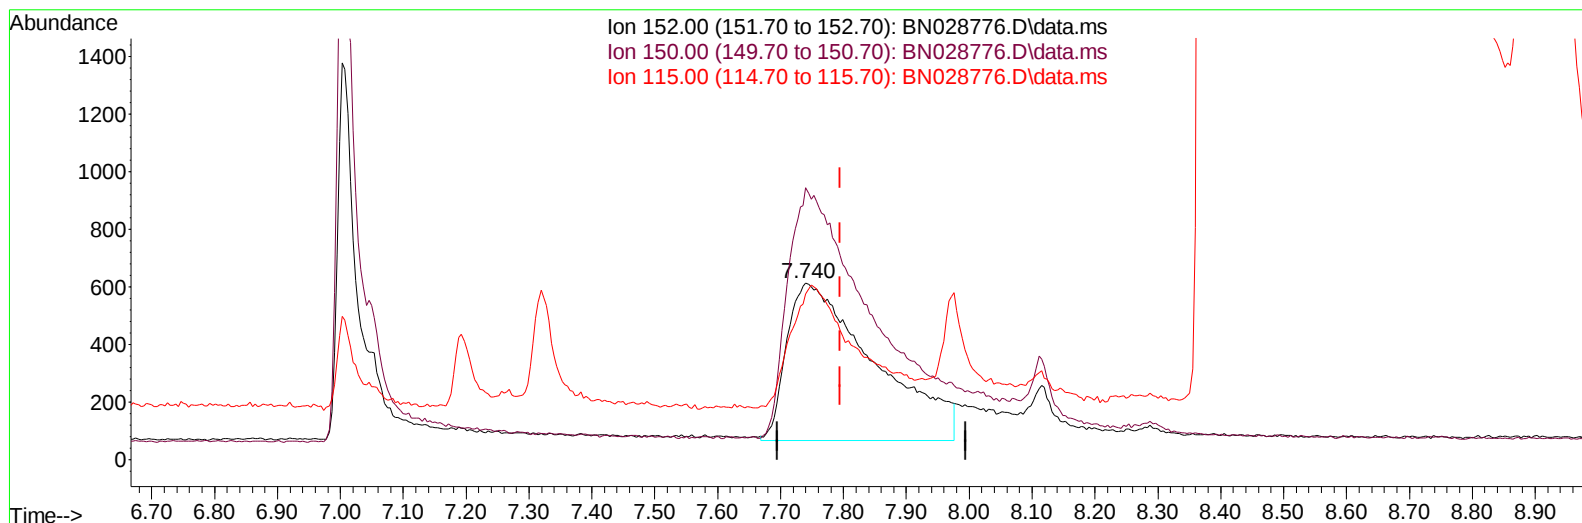

TIC: BN028776.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.740min (-0.055) 0.40 ng/ul m

response 5297

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	153.75
115.00	62.20	93.65#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028776.D
 Acq On : 19 Nov 2023 14:37
 Operator : MA/JU
 Sample : 05370-16
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDR0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 02:03:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.740	152	5297m	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.472	136	15582	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.315	164	12025	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.081	188	23792	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.297	240	14932	0.400	ng/ul	# 0.00
23) Perylene-d12	23.568	264	18218	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	31193	5.328	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.105	152	5548	0.237	ng/ul	0.00
18) Fluoranthene-d10	19.112	212	28582	0.595	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028776.D
Acq On : 19 Nov 2023 14:37
Operator : MA/JU
Sample : 05370-16
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDR0

Manual IntegrationsAPPROVED

Quant Time: Nov 20 02:03:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

