




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

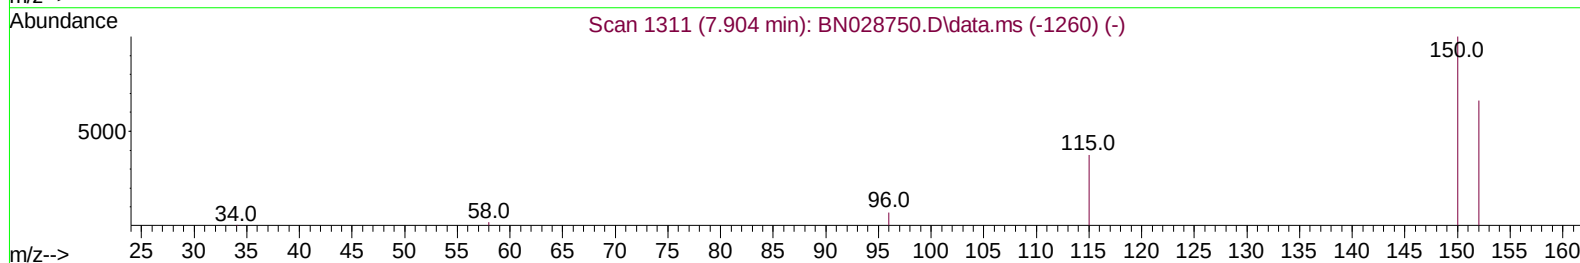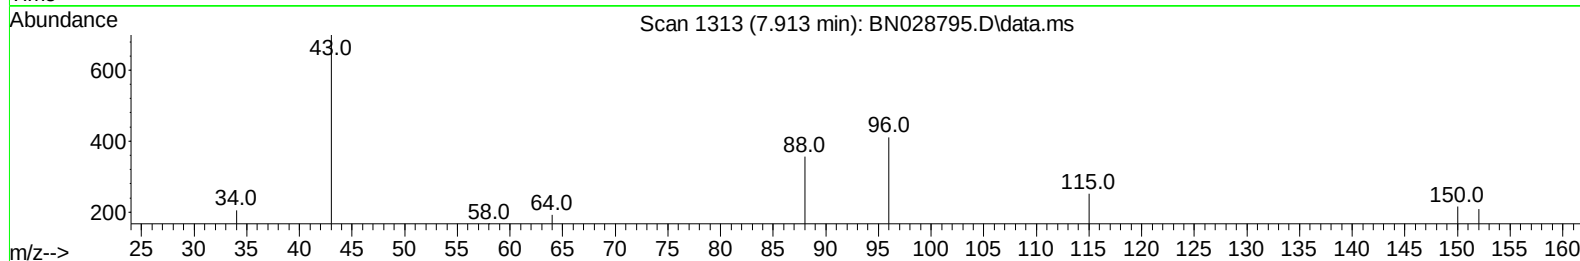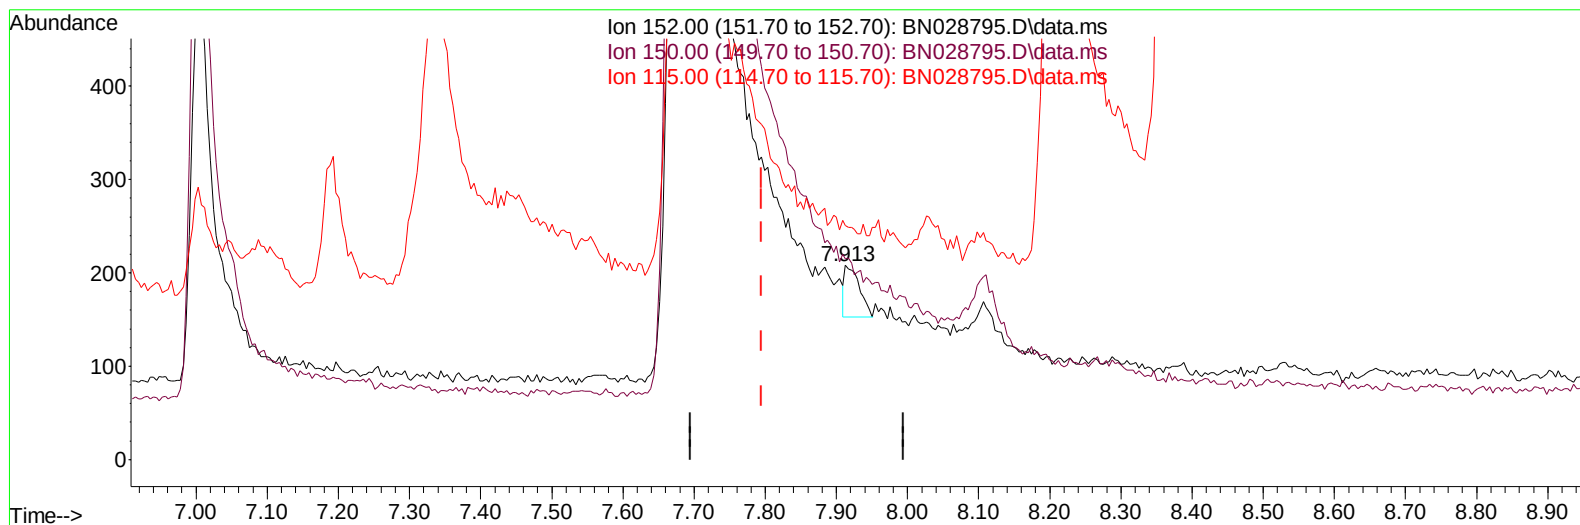

TIC: BN028795.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.913min (+ 0.118) 0.40 ng/ul

response 79

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	103.37#
115.00	62.20	120.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

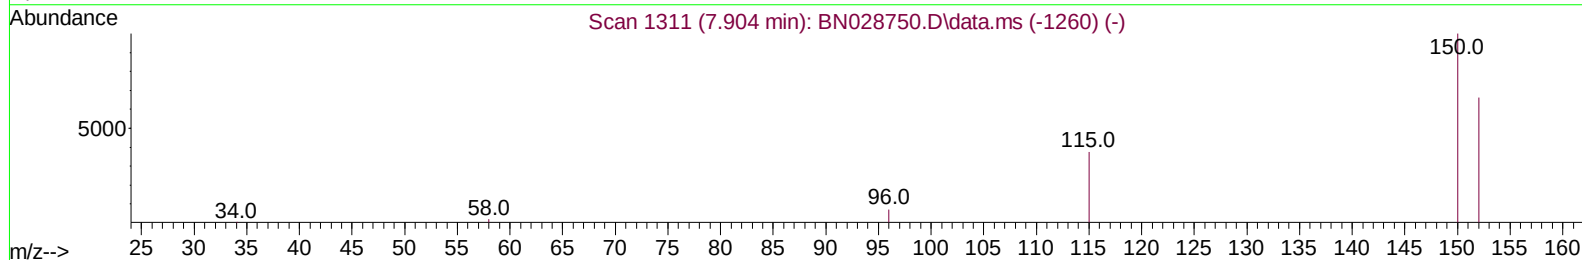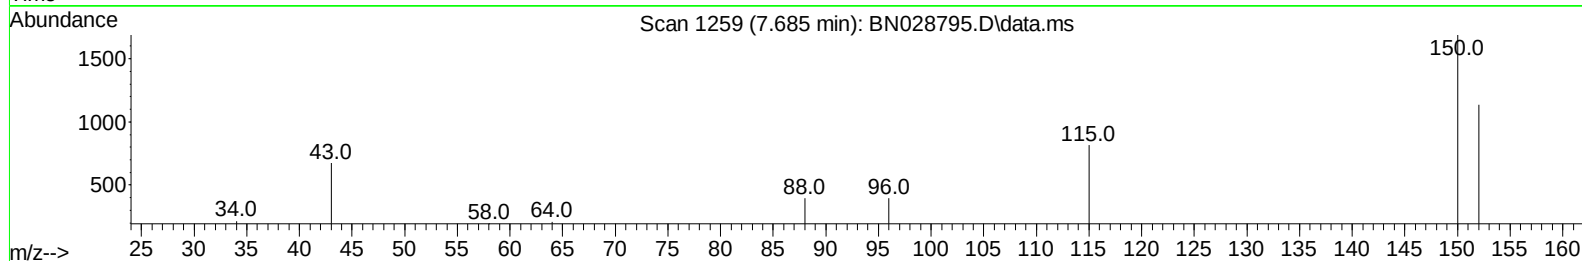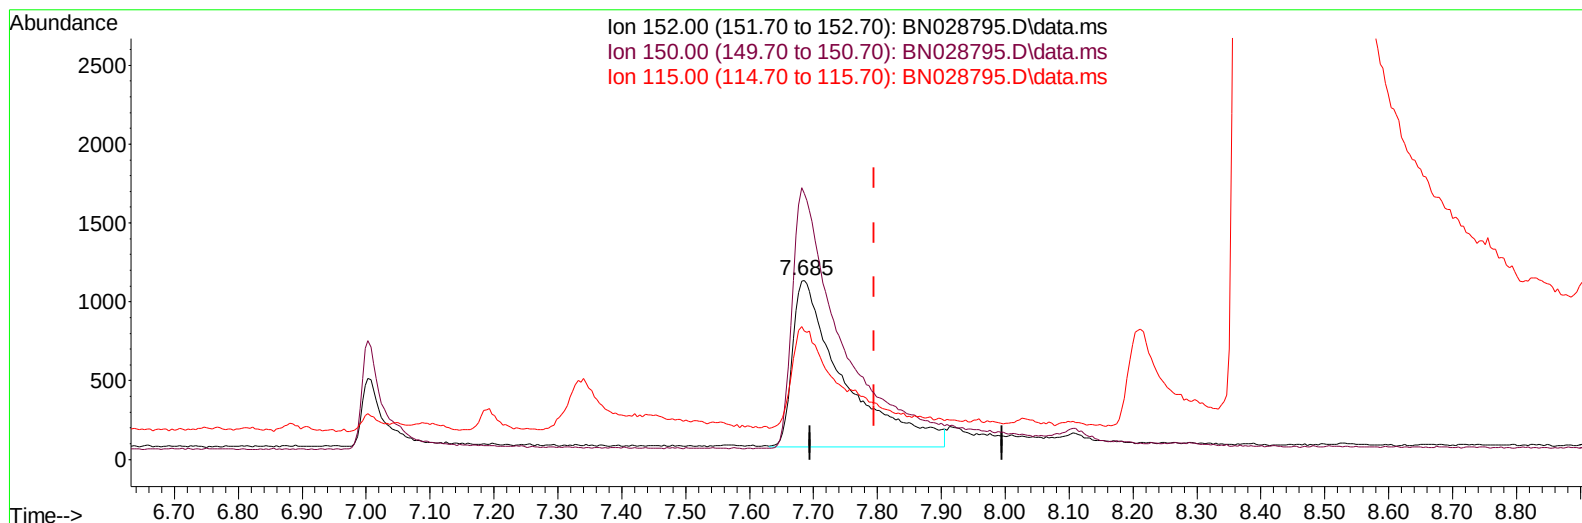

TIC: BN028795.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.685min (-0.110) 0.40 ng/ul m

response 5893

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	148.46
115.00	62.20	71.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

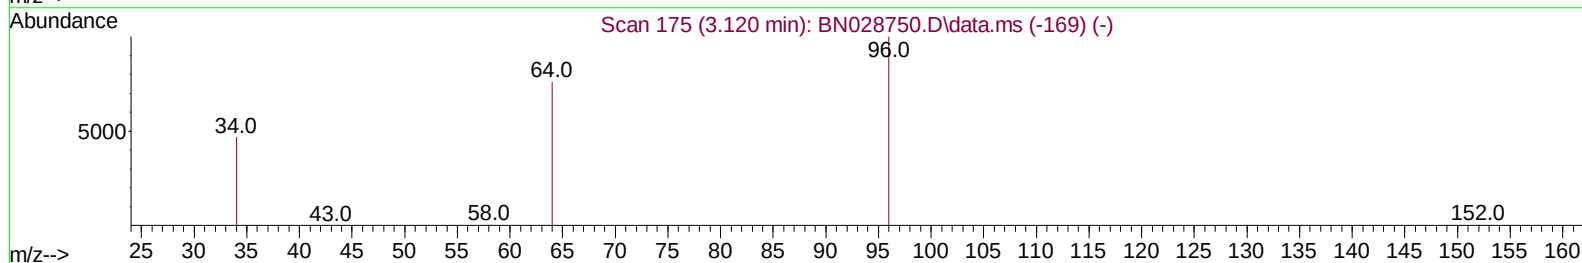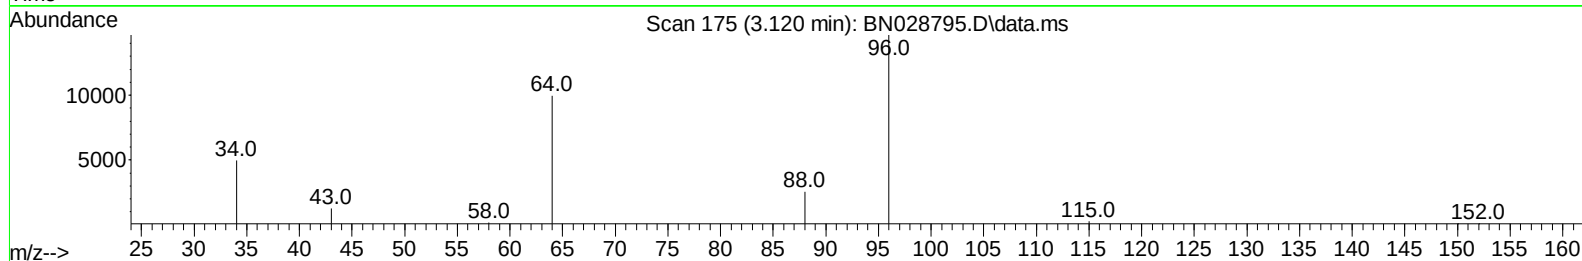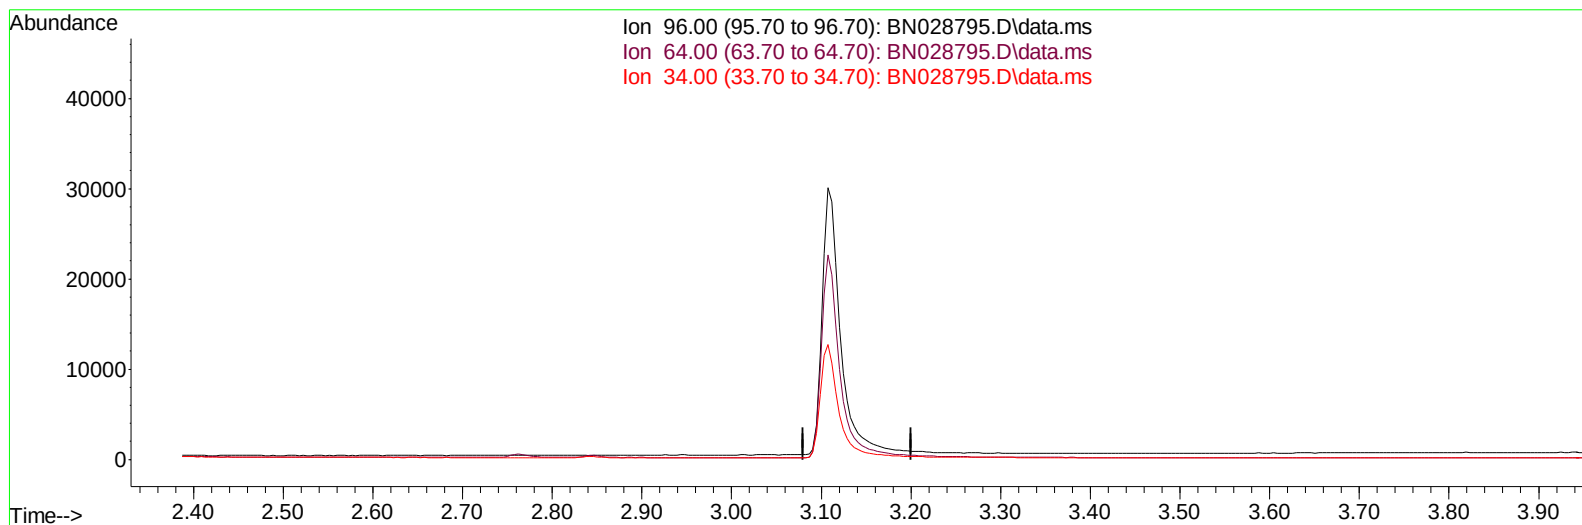

TIC: BN028795.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.120min (-3.120) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	67.40	0.00#
34.00	38.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

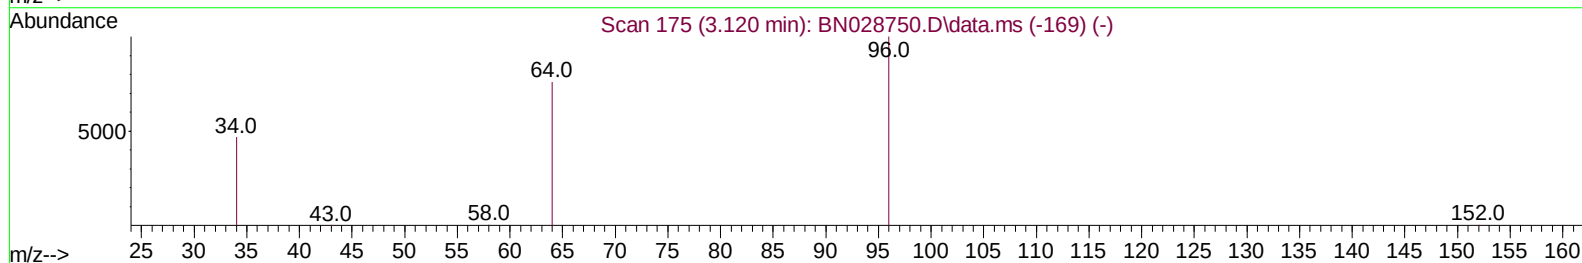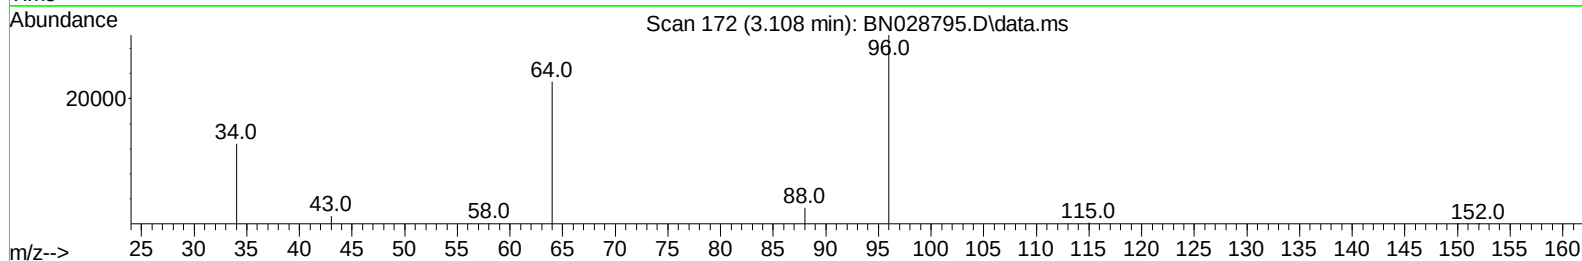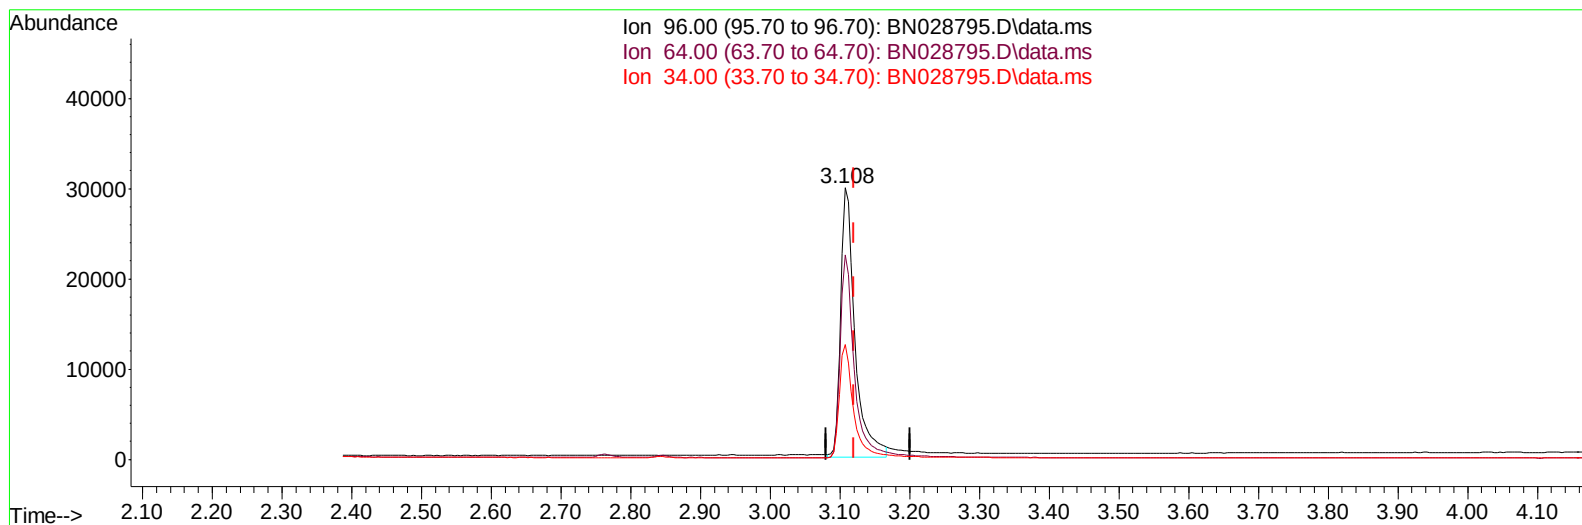

TIC: BN028795.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.108min (-0.013) 6.52 ng/ul m

response 42470

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.40	75.22
34.00	38.60	42.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

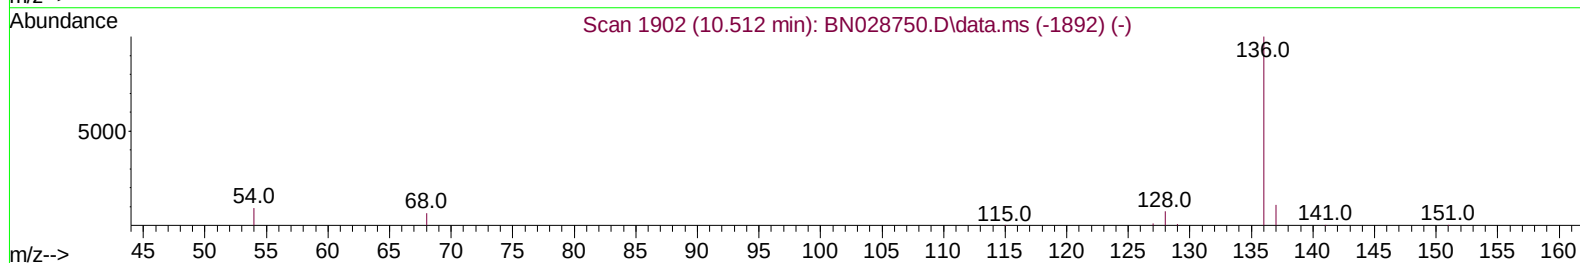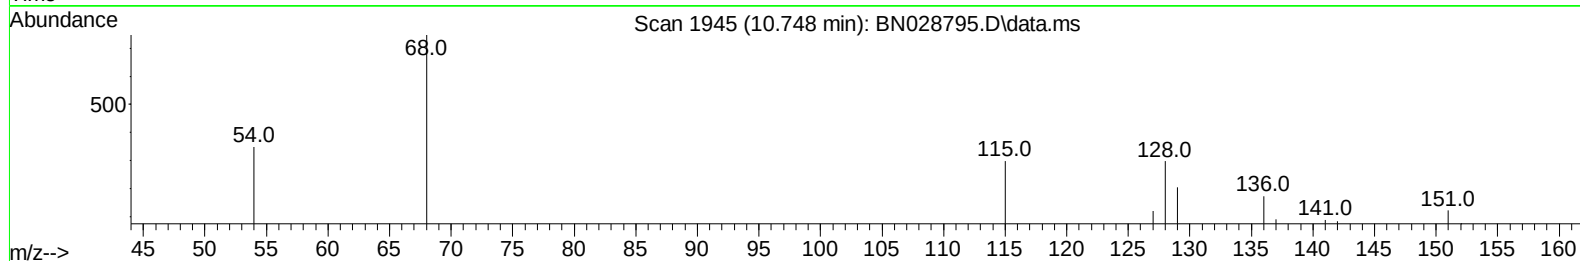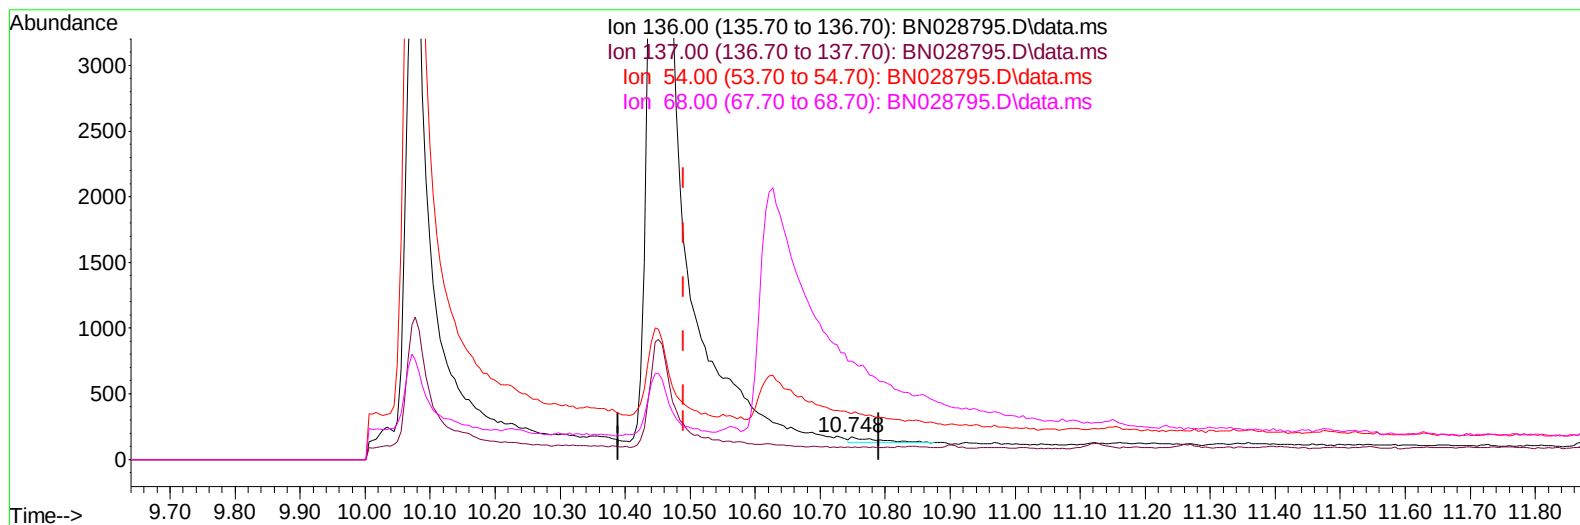

TIC: BN028795.D\data.ms

(4) Naphthalene-d8 (I)

10.748min (+ 0.258) 0.40 ng/ul

response 124

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.20	52.87#
54.00	9.00	200.57#
68.00	7.10	429.31#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

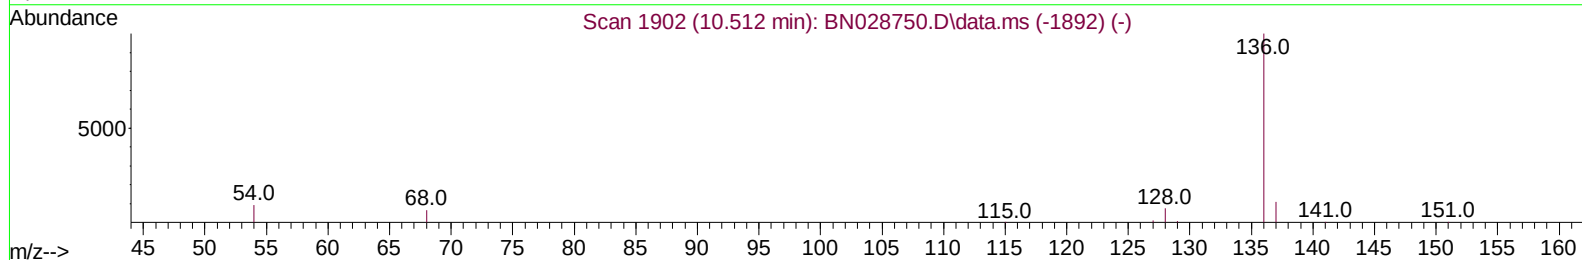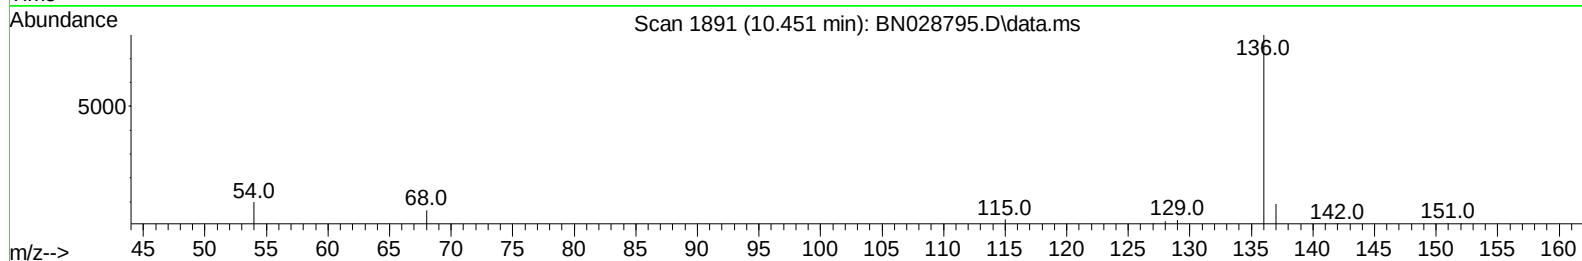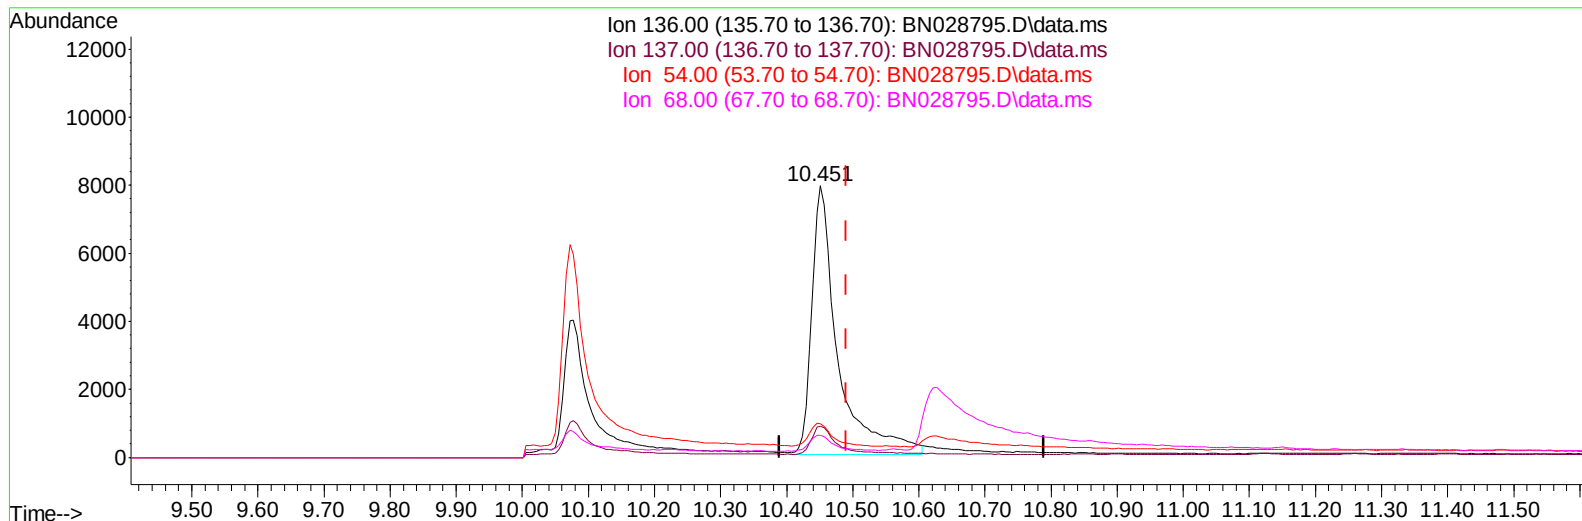

TIC: BN028795.D\data.ms

(4) Naphthalene-d8 (I)

10.451min (-0.039) 0.40 ng/ul m

response 21680

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.20	11.46
54.00	9.00	12.41#
68.00	7.10	8.25




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

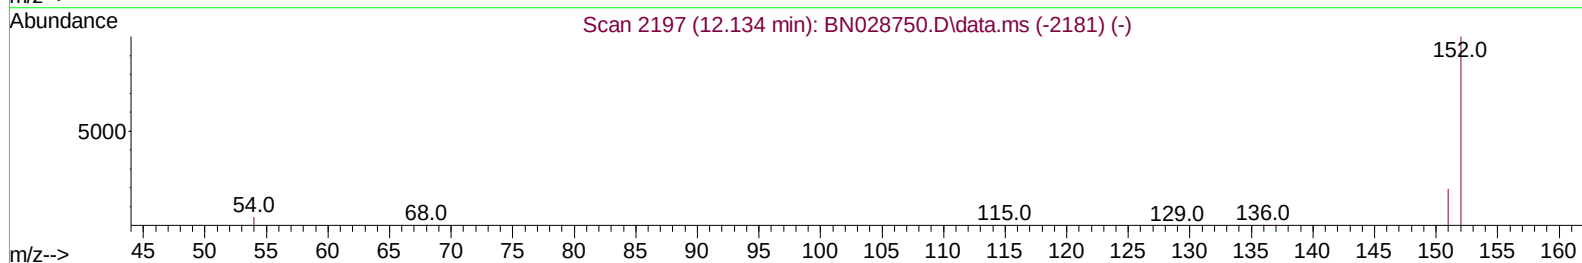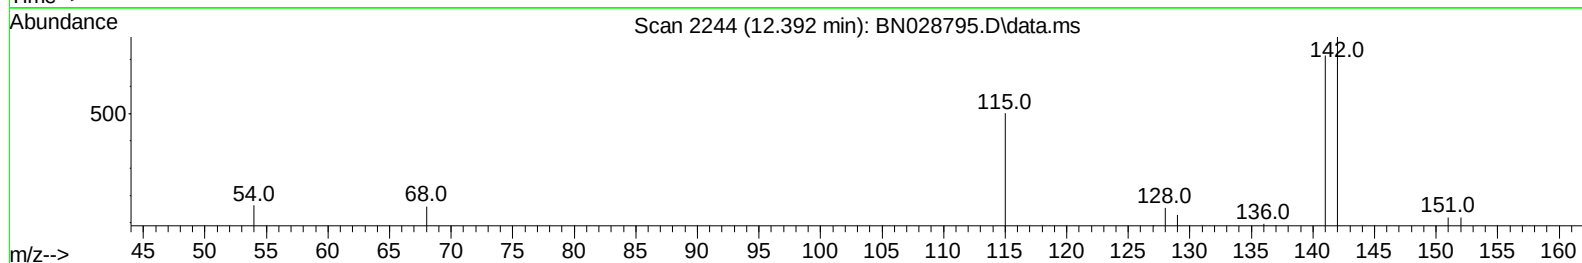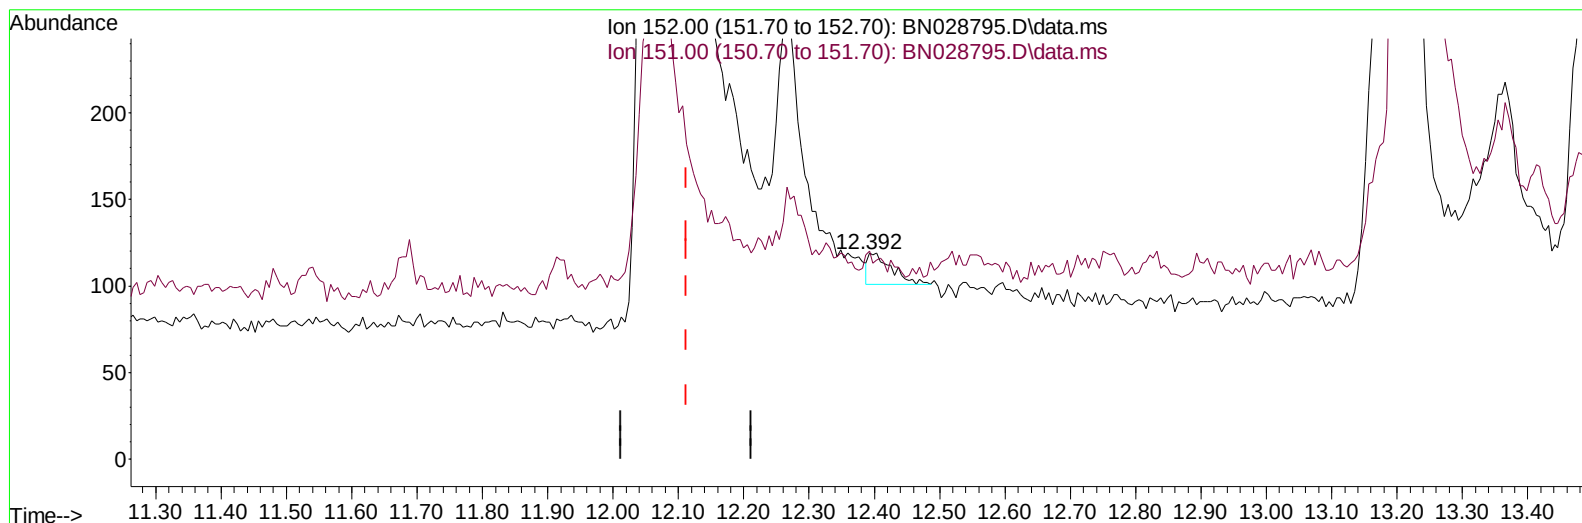

TIC: BN028795.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.392min (+ 0.280) 0.00 ng/u1

response 44

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	40.91#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

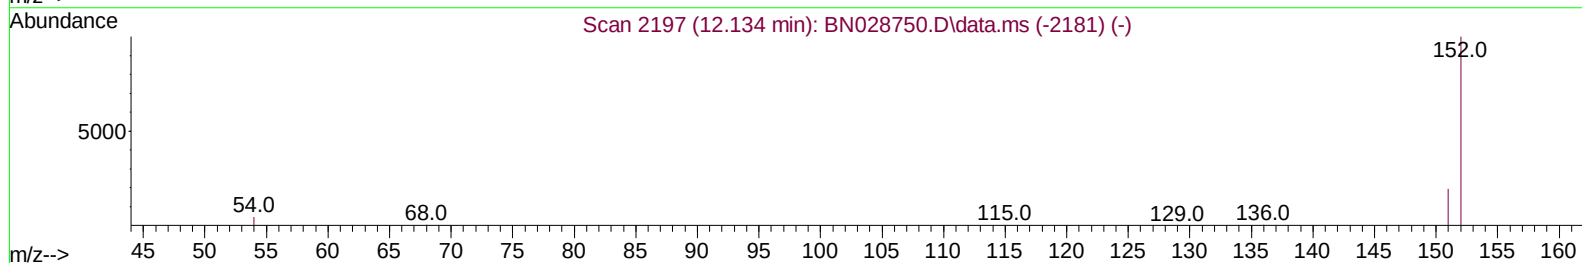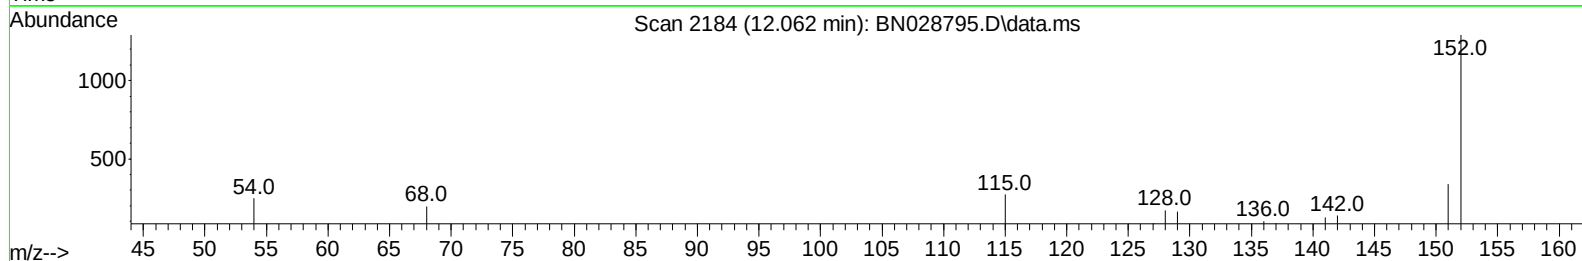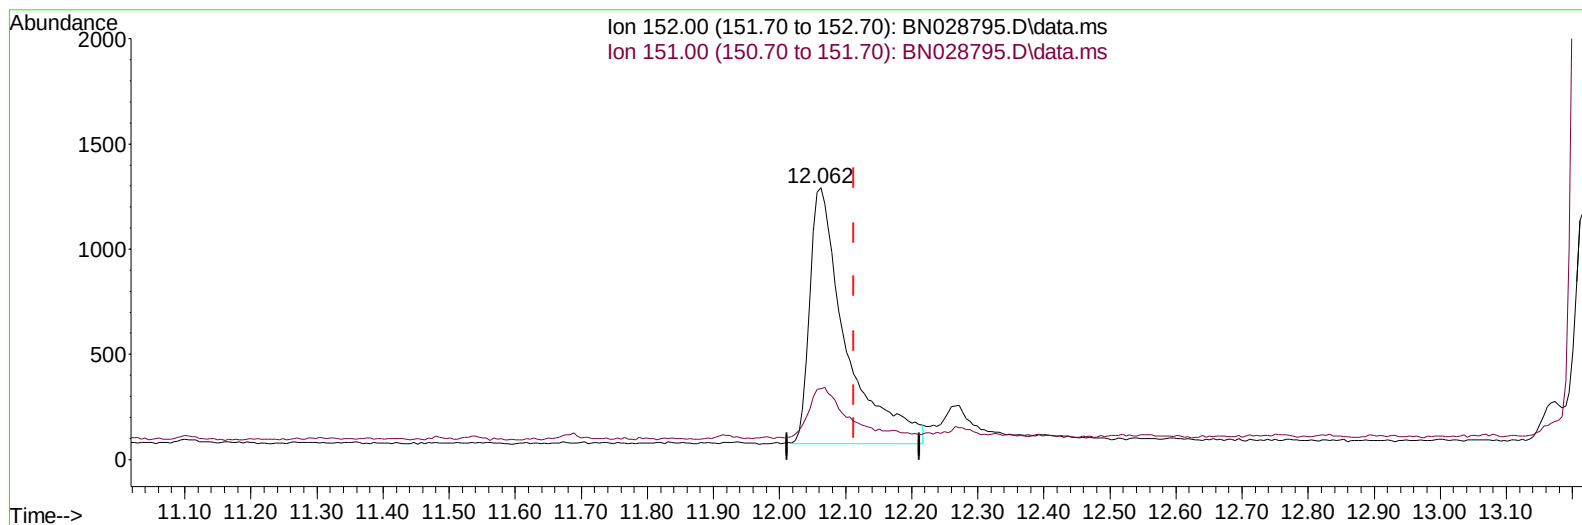

TIC: BN028795.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.062min (-0.050) 0.14 ng/ul m

response 4616

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.50	0.39#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

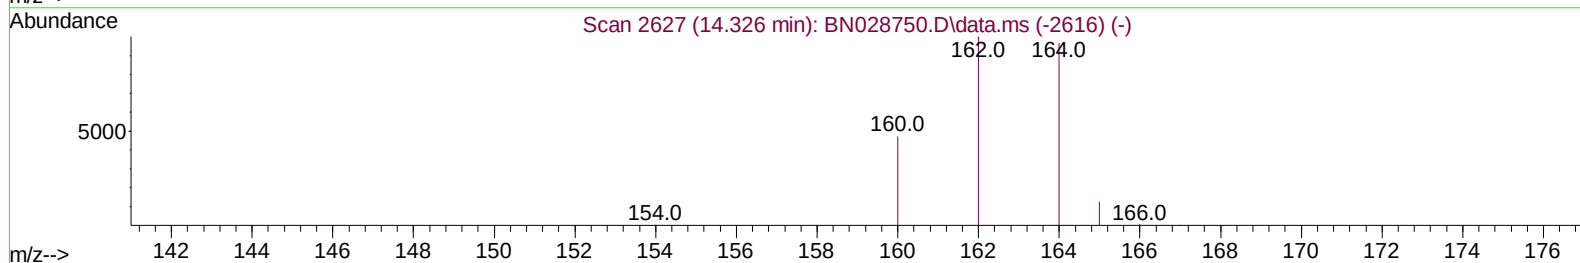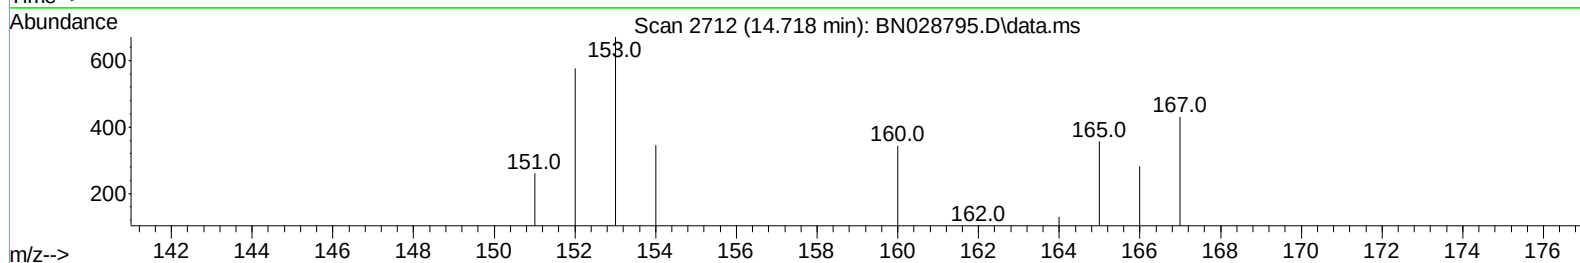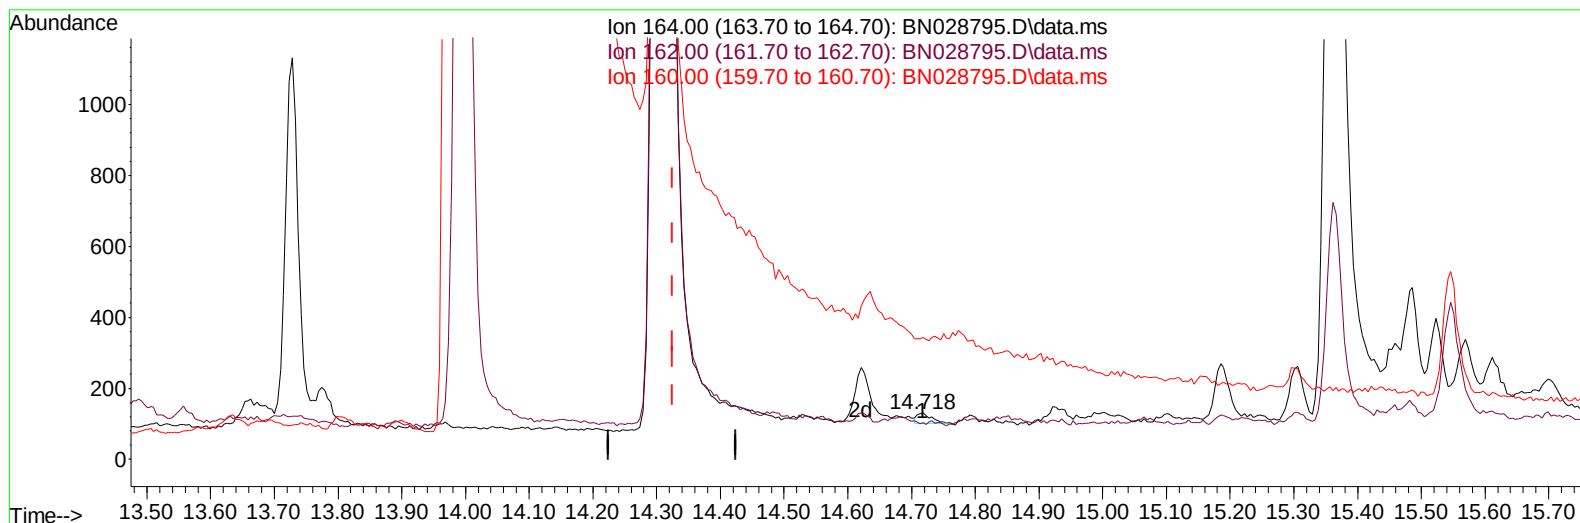

TIC: BN028795.D\data.ms

(9) Acenaphthene-d10 (I)

14.718min (+ 0.393) 0.40 ng/u1

response 43

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.90	79.23#
160.00	49.20	263.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

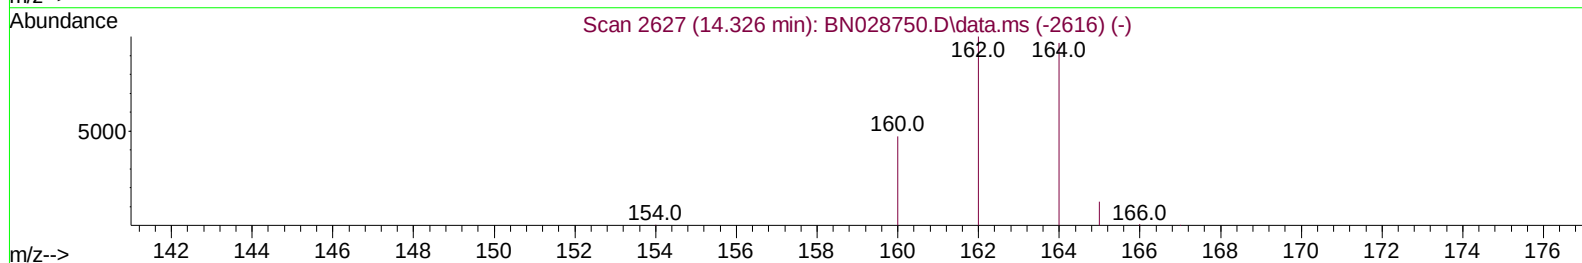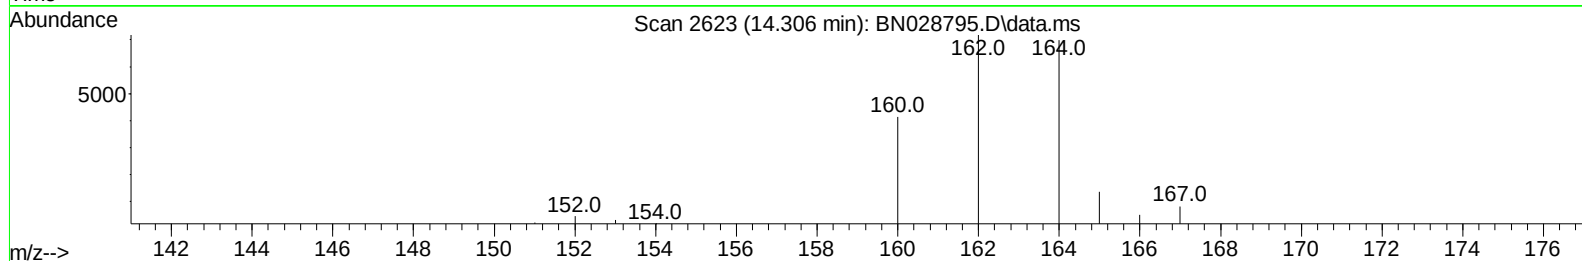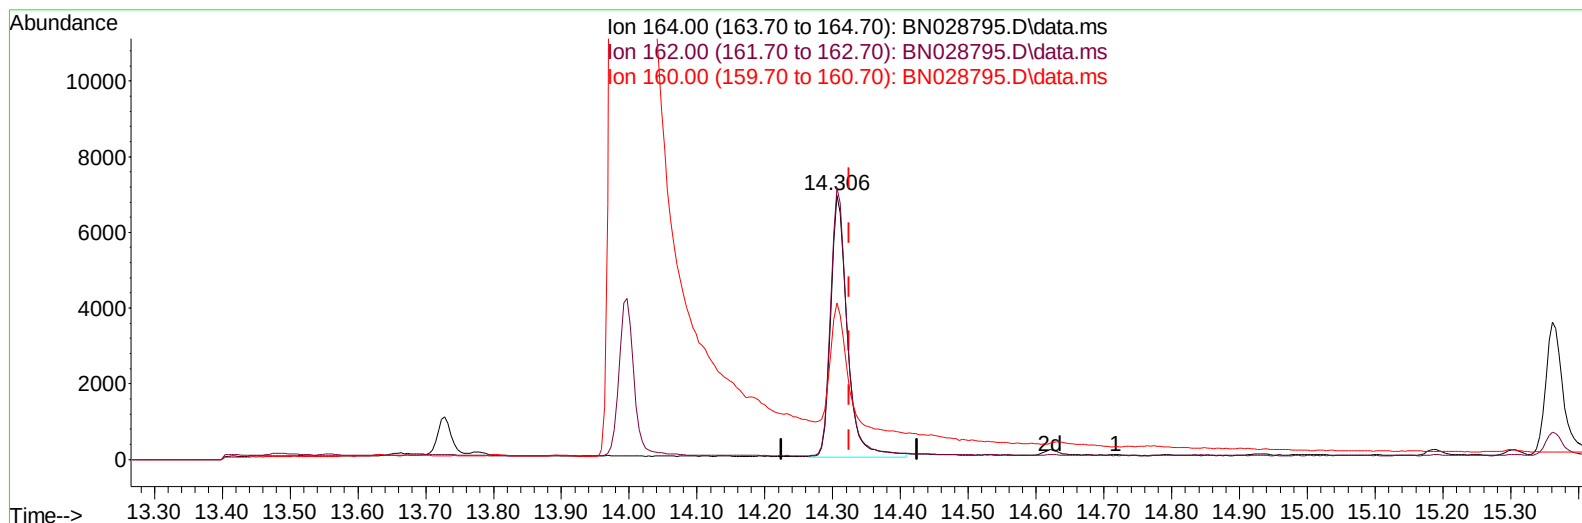

TIC: BN028795.D\data.ms

(9) Acenaphthene-d10 (I)

14.306min (-0.019) 0.40 ng/ul m

response 11689

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.90	102.81
160.00	49.20	59.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

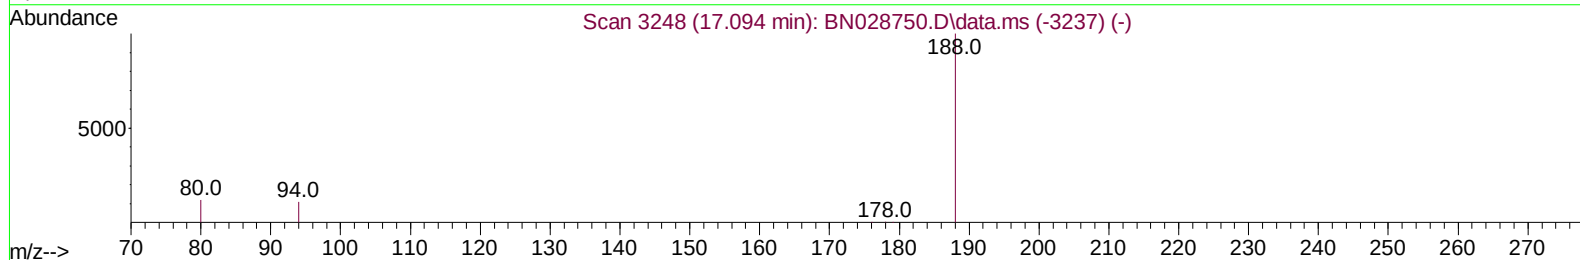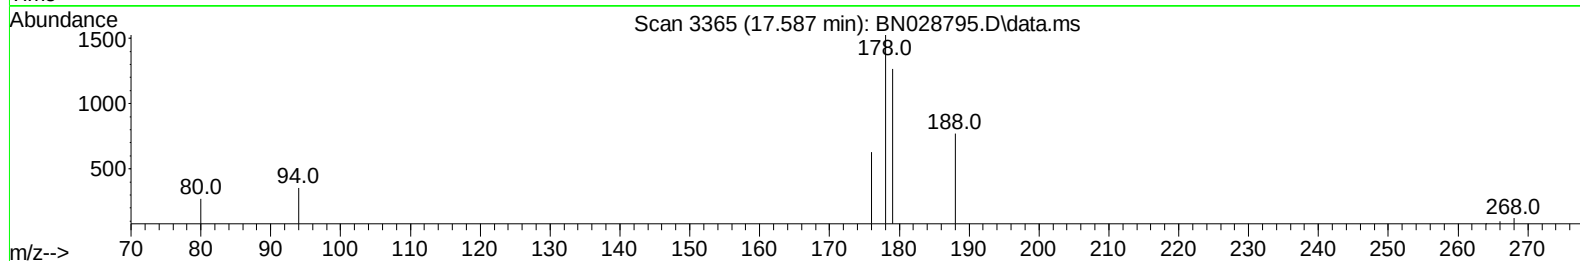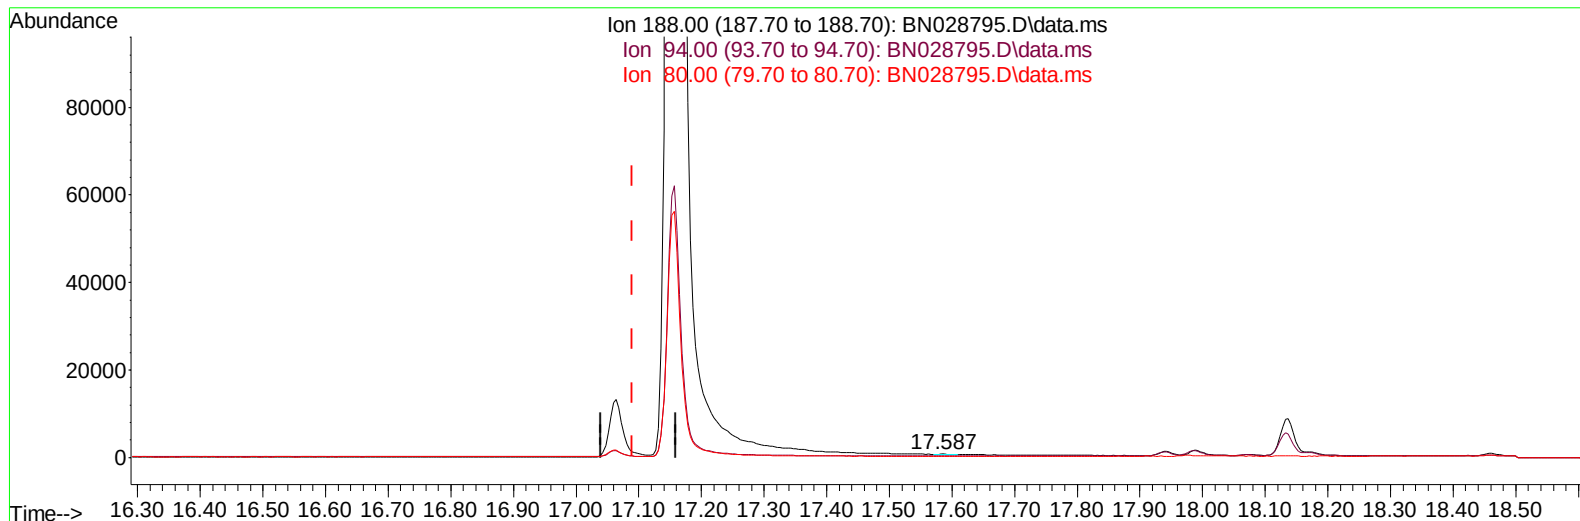

TIC: BN028795.D\data.ms

(13) Phenanthrene-d10 (I)

17.587min (+ 0.498) 0.40 ng/u1

response 94

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	45.90#
80.00	10.90	35.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

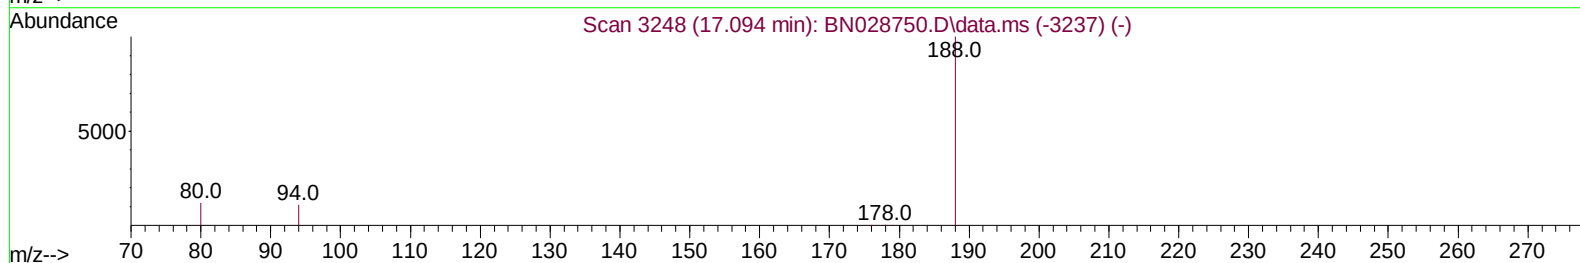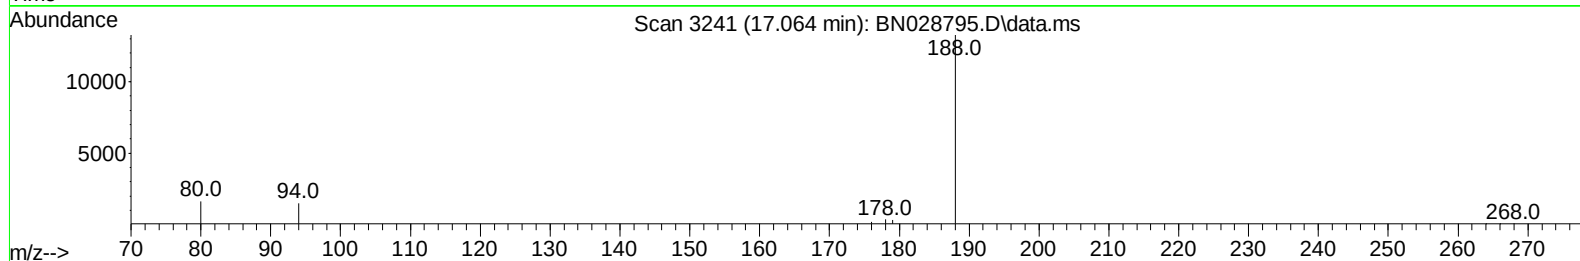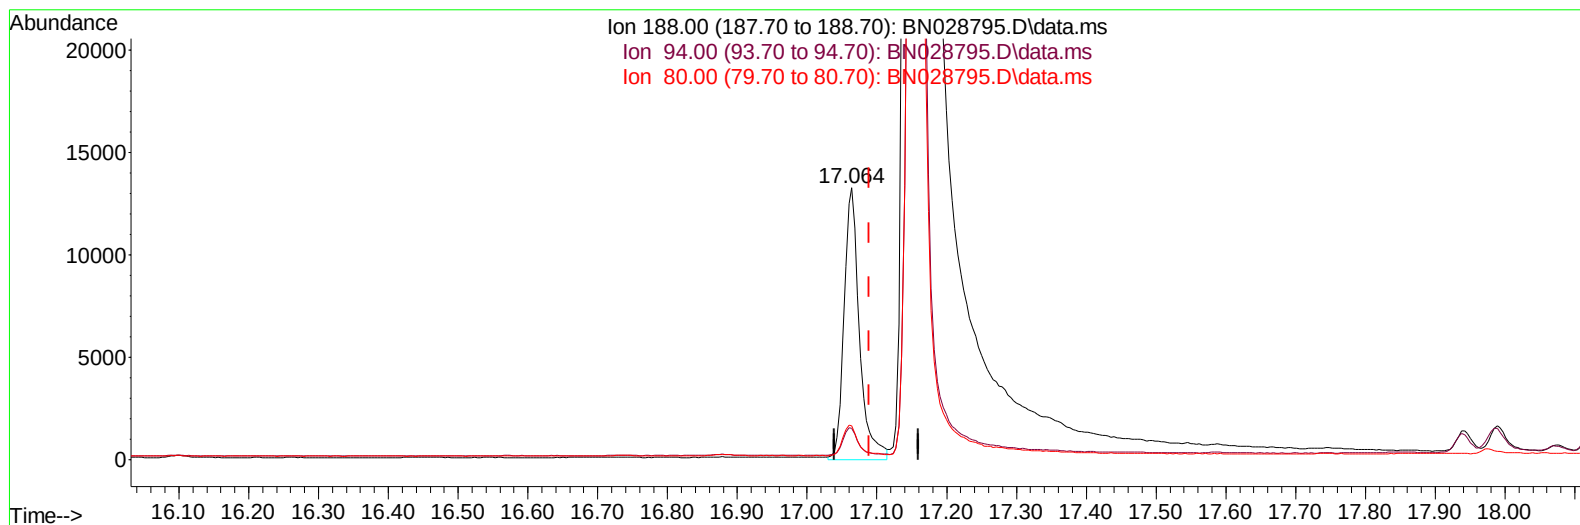

TIC: BN028795.D\data.ms

(13) Phenanthrene-d10 (I)

17.064min (-0.025) 0.40 ng/ul m

response 20306

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	11.35
80.00	10.90	12.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

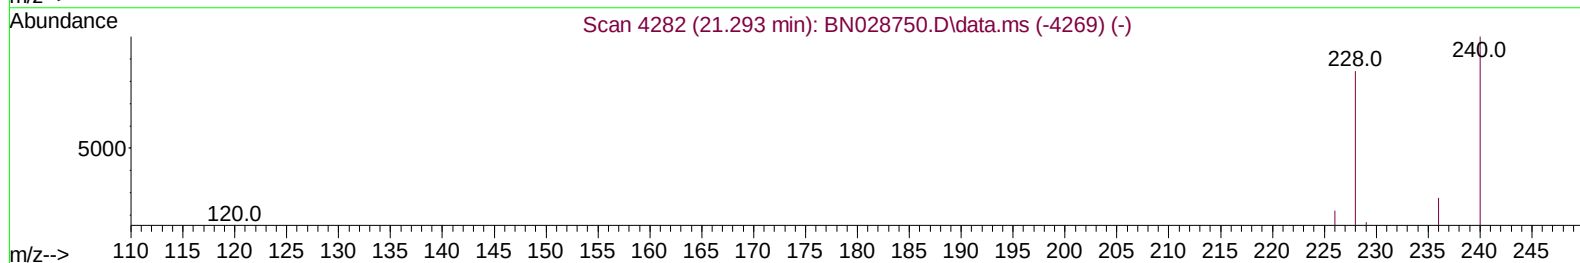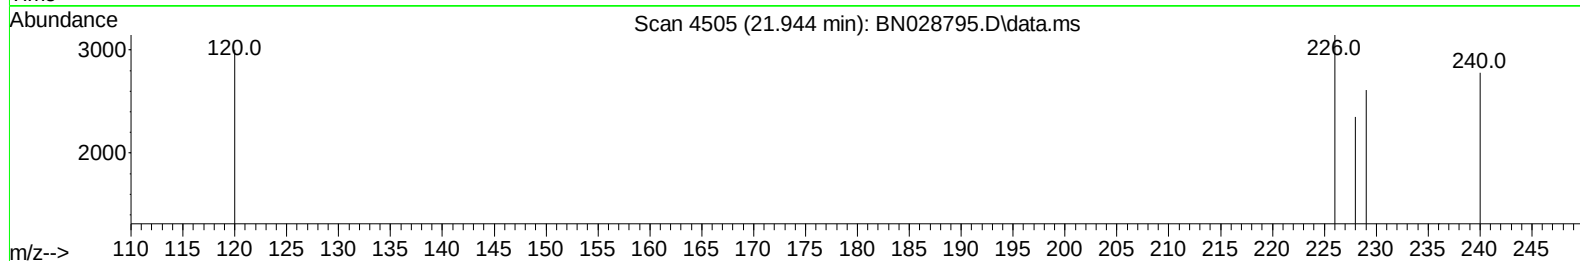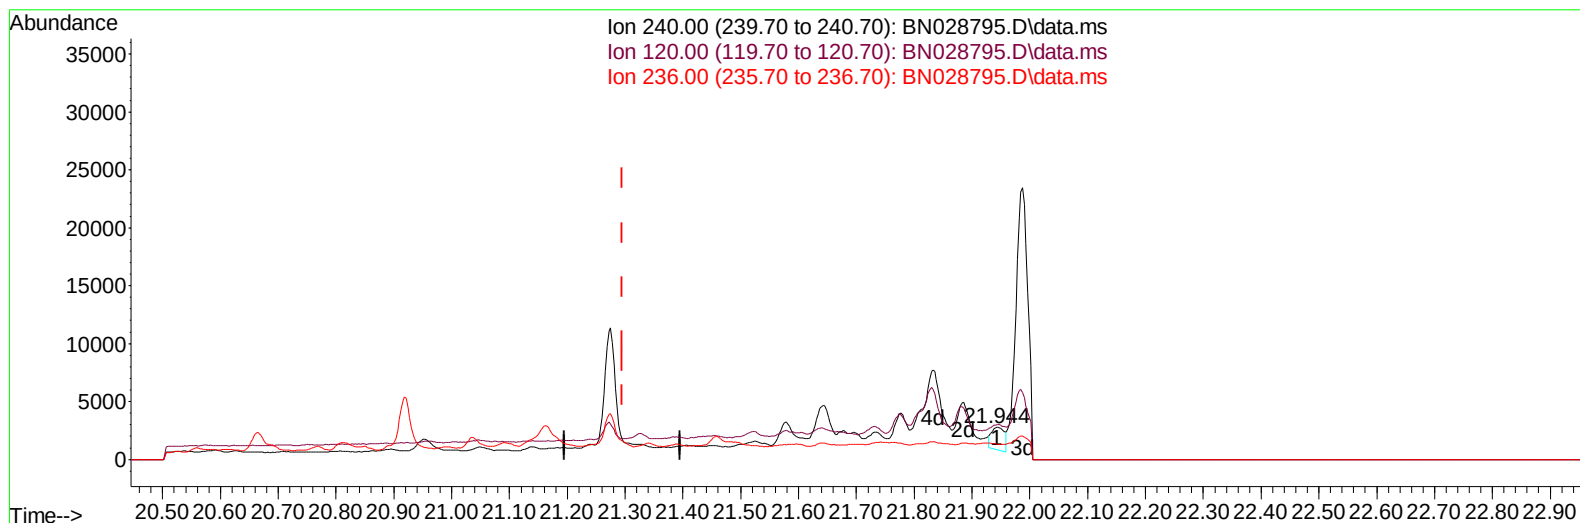

TIC: BN028795.D\data.ms

(17) Chrysene-d12

21.944min (+ 0.648) 0.40 ng/u1

response 3004

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.00	107.95#
236.00	28.00	47.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

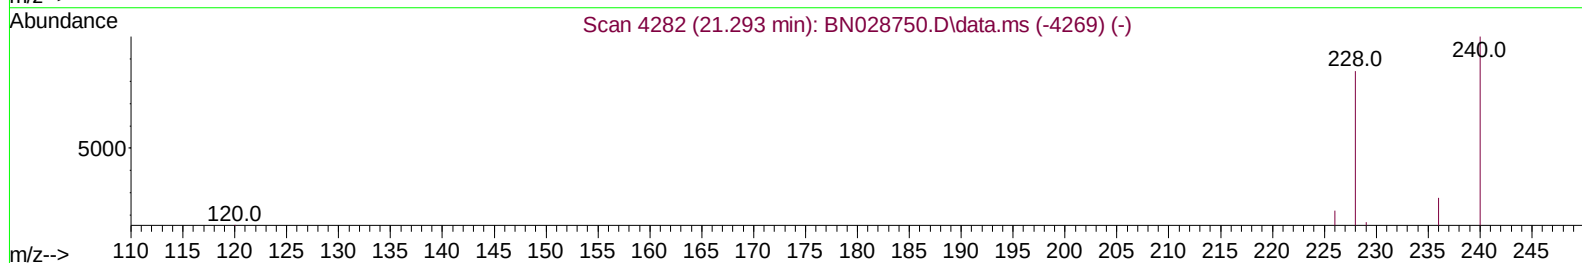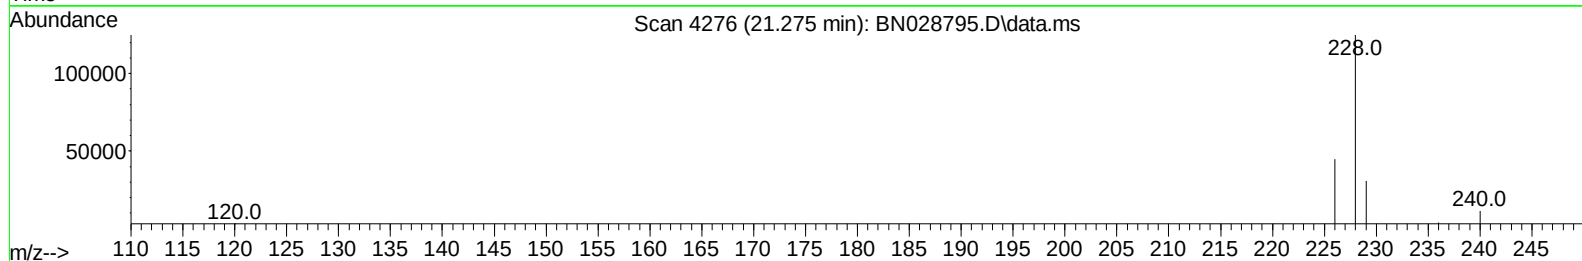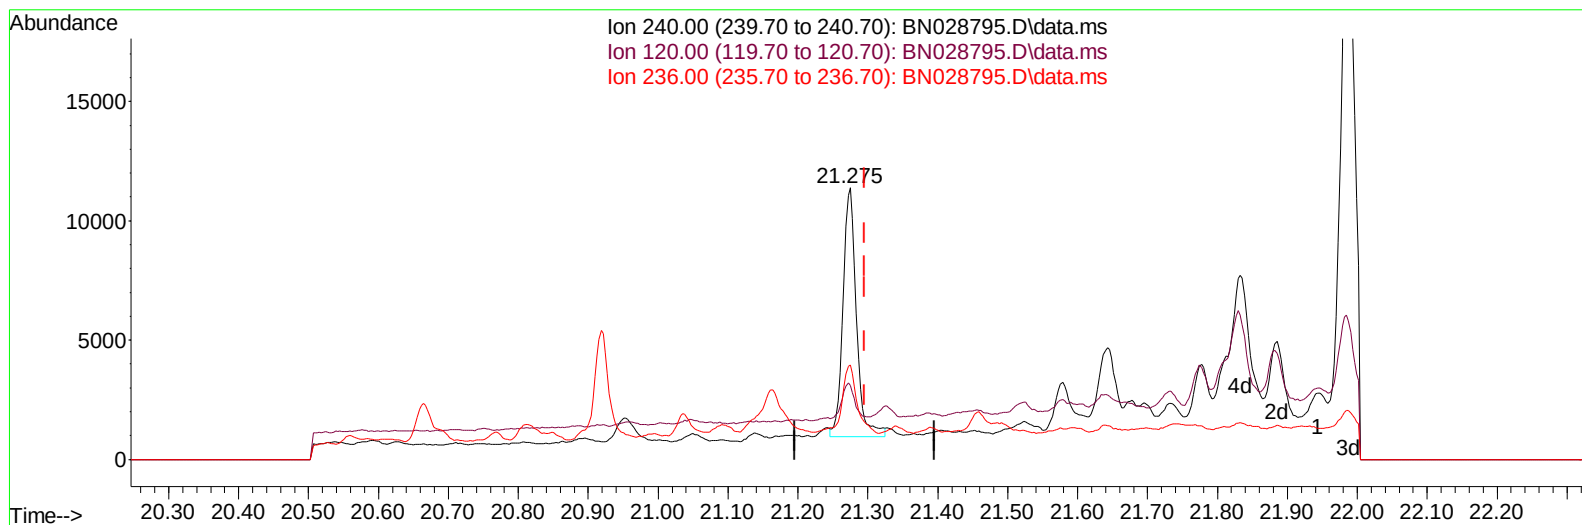

TIC: BN028795.D\data.ms

(17) Chrysene-d12

21.275min (-0.021) 0.40 ng/ul m

response 13845

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.00	27.16#
236.00	28.00	34.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

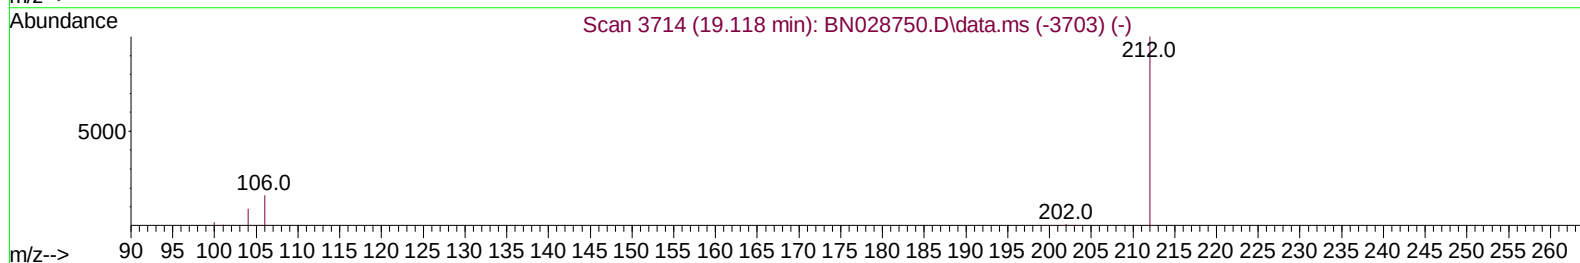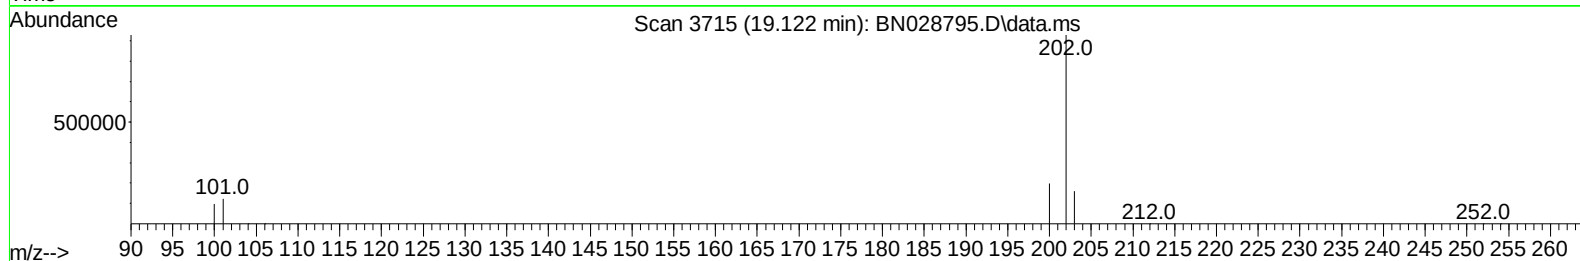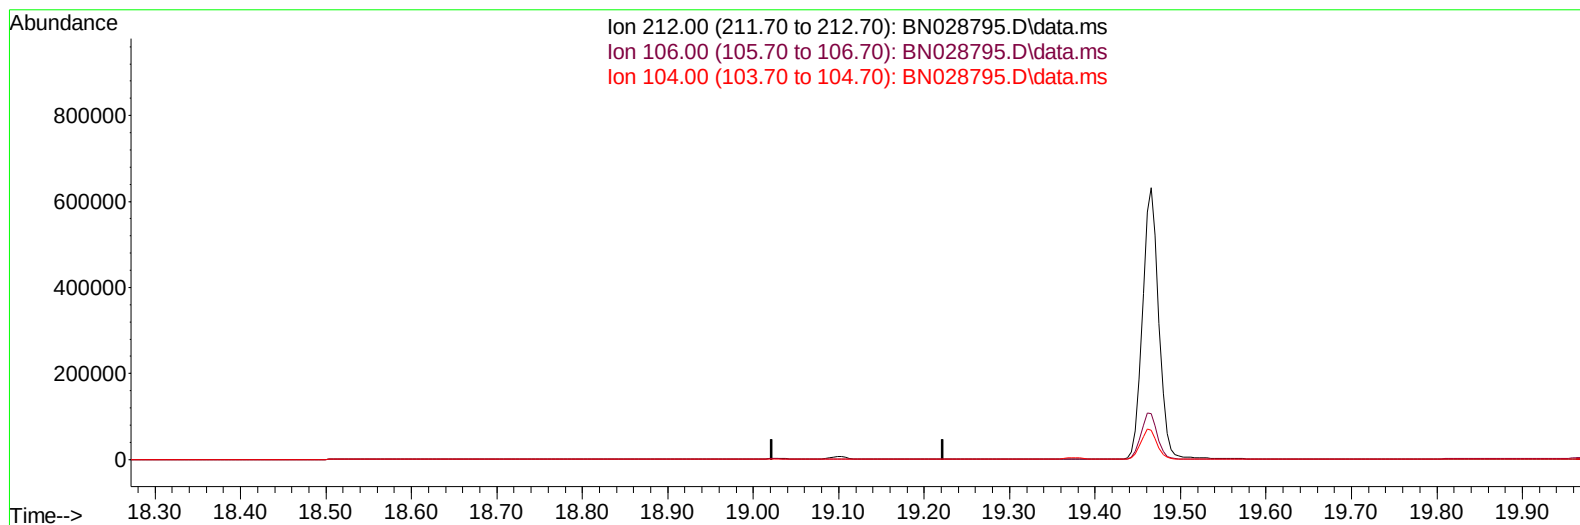

TIC: BN028795.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.122min (-19.122) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	14.80	0.00#
104.00	8.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

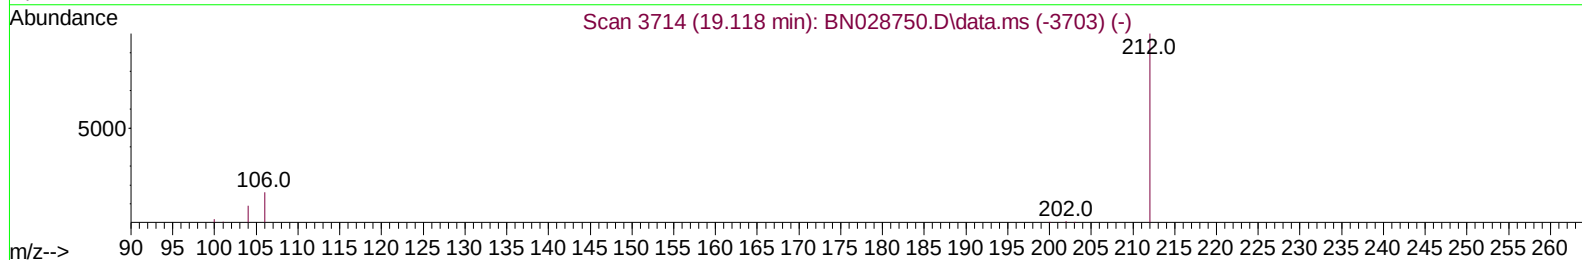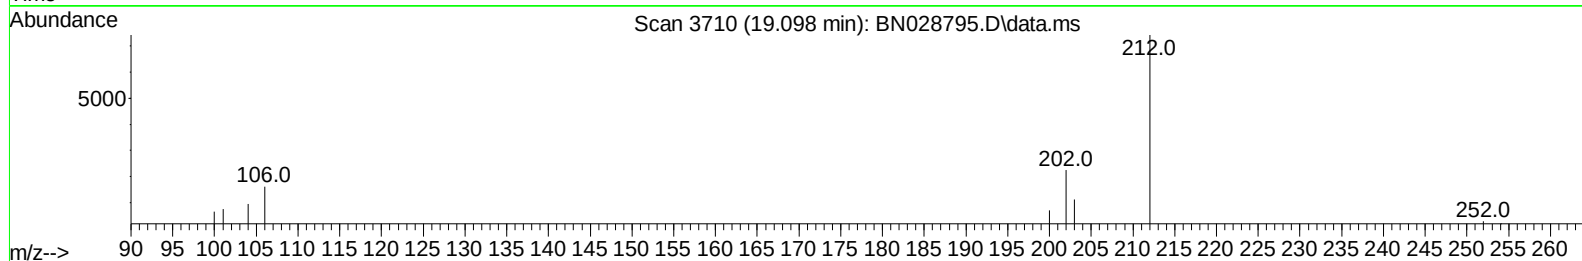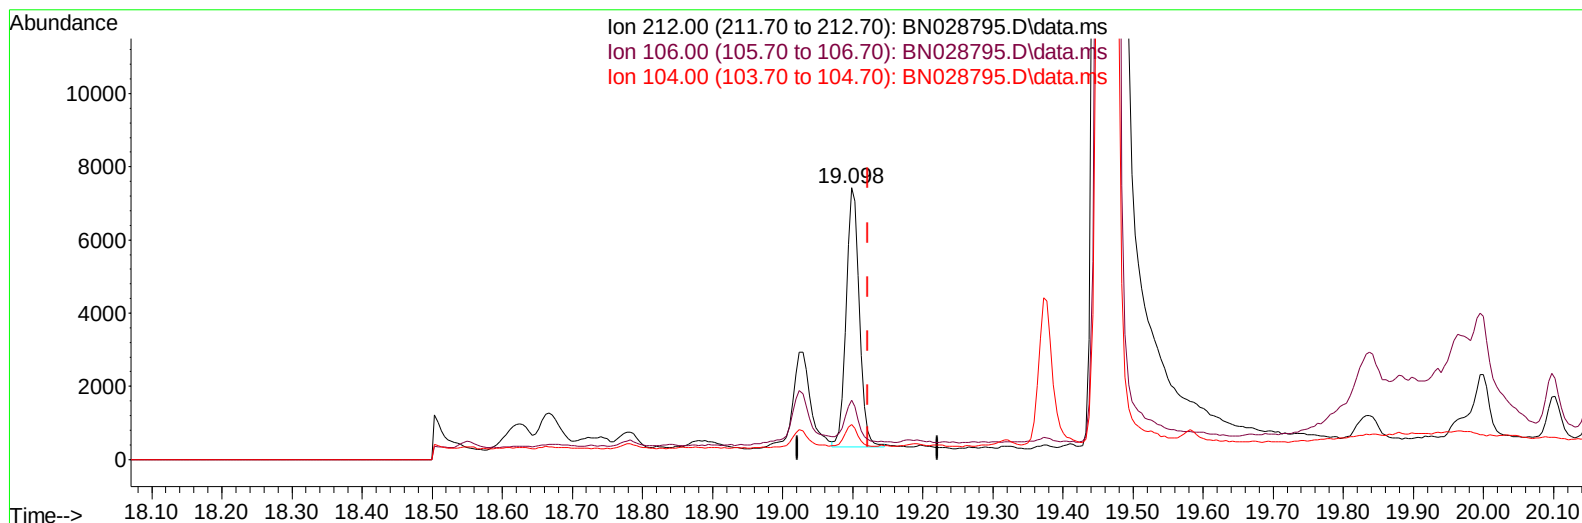

TIC: BN028795.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.098min (-0.023) 0.21 ng/ul m

response 9387

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	14.80	0.00#
104.00	8.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

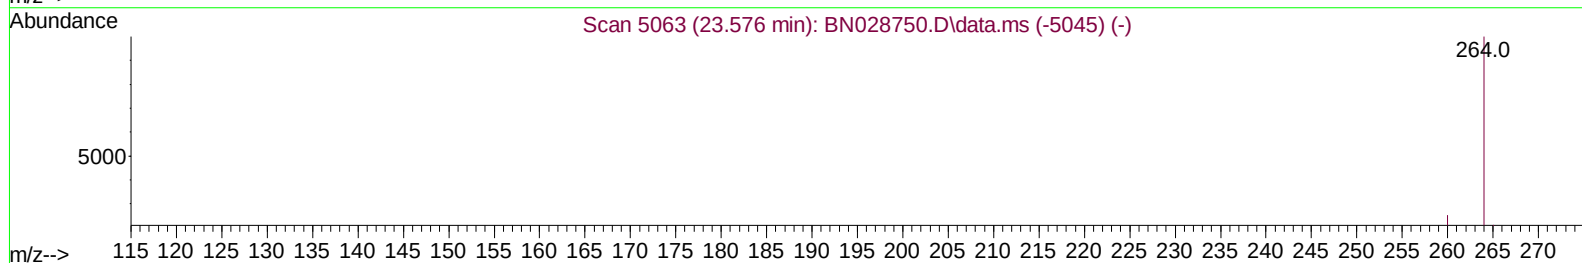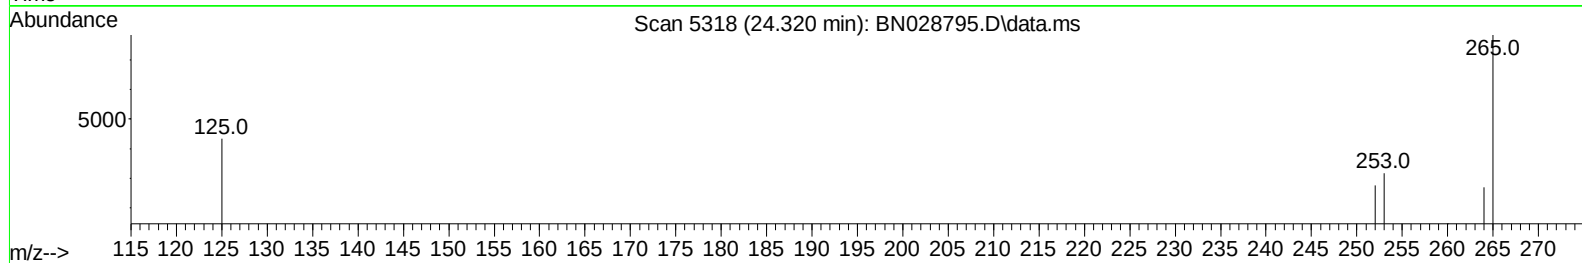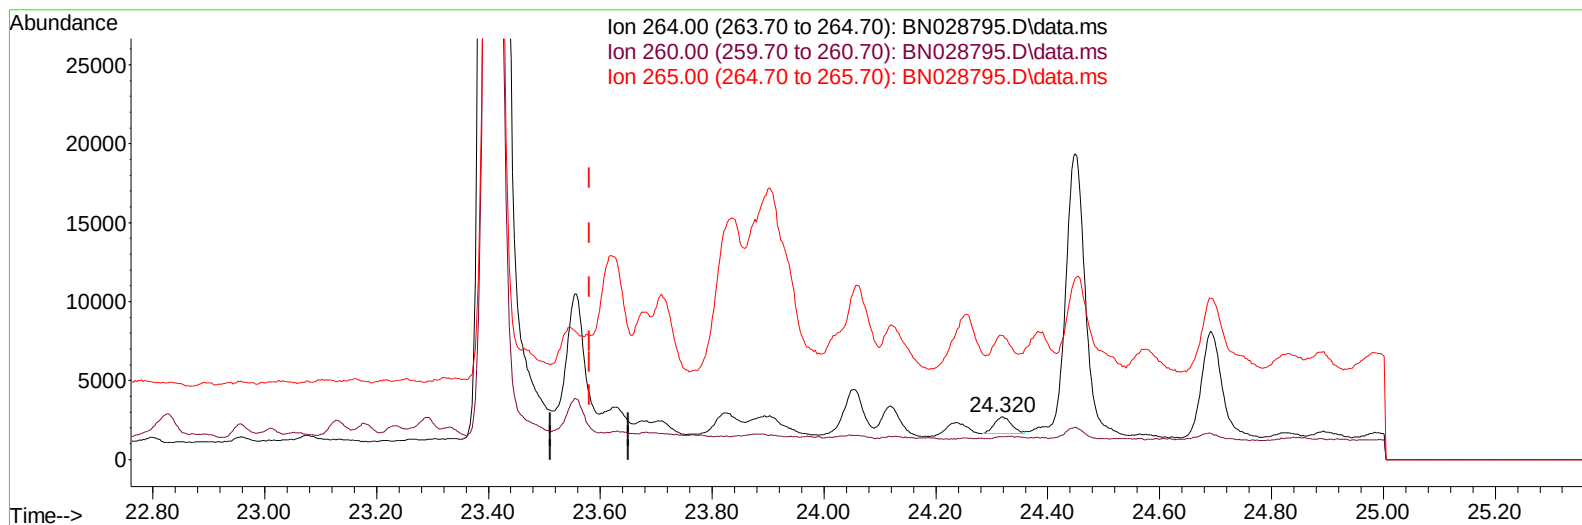

TIC: BN028795.D\data.ms

(23) Perylene-d12 (I)

24.320min (+ 0.740) 0.40 ng/ul

response 2281

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	54.26#
265.00	38.80	291.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

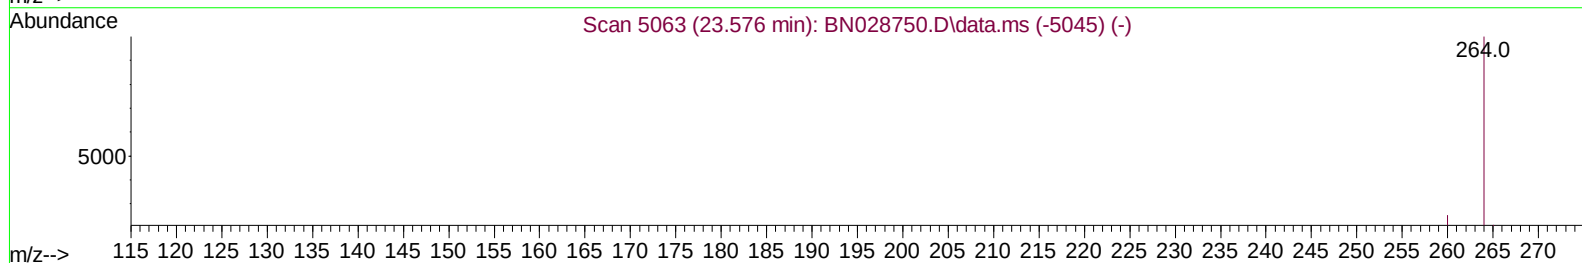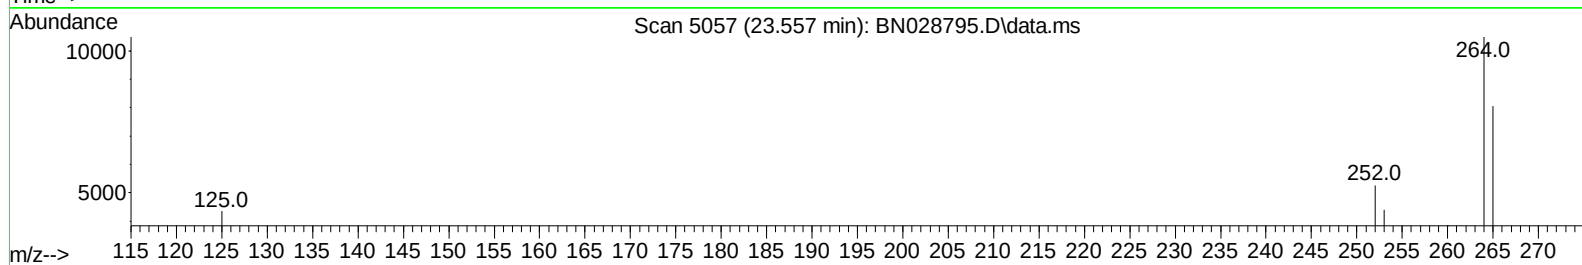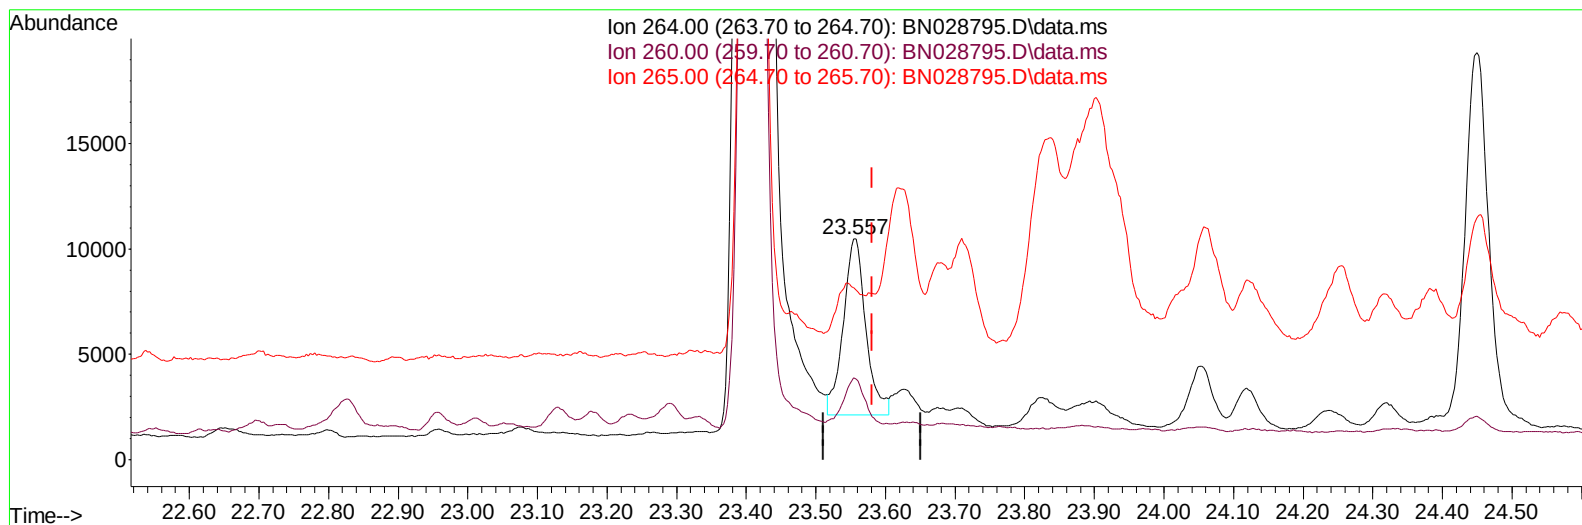

TIC: BN028795.D\data.ms

(23) Perylene-d12 (I)

23.557min (-0.024) 0.40 ng/ul m

response 18781

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	36.51#
265.00	38.80	76.83#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028795.D
 Acq On : 20 Nov 2023 02:35
 Operator : MA/JU
 Sample : 05174-19
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 03:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.685	152	5893m	0.400	ng/ul	-0.11
4) Naphthalene-d8	10.451	136	21680m	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.306	164	11689m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.064	188	20306m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.275	240	13845m	0.400	ng/ul	-0.02
23) Perylene-d12	23.557	264	18781m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.108	96	42470m	6.521	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.062	152	4616m	0.141	ng/ul	-0.05
18) Fluoranthene-d10	19.098	212	9387m	0.211	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028795.D
Acq On : 20 Nov 2023 02:35
Operator : MA/JU
Sample : 05174-19
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN6

Manual IntegrationsAPPROVED

Quant Time: Nov 20 03:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

