




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028797.D
 Acq On : 20 Nov 2023 03:46
 Operator : MA/JU
 Sample : PB156868BL
 Misc :
 ALS Vial : 102 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK868

Manual IntegrationsAPPROVED

Quant Time: Nov 20 04:15:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

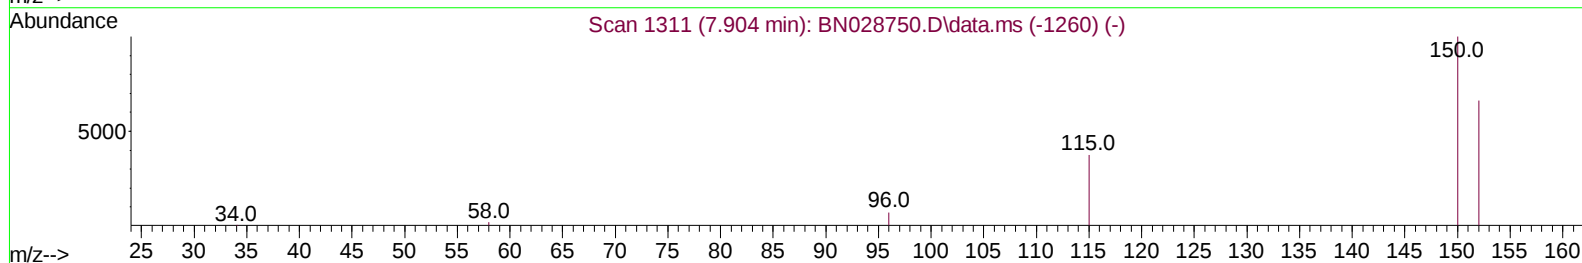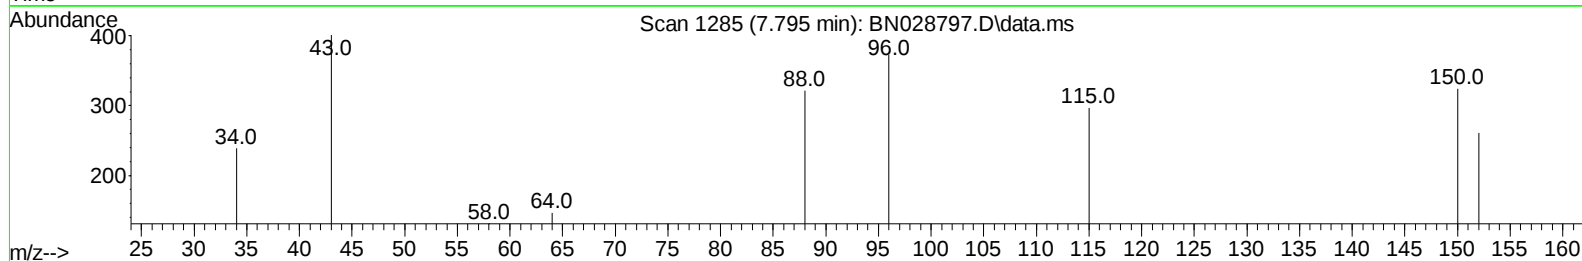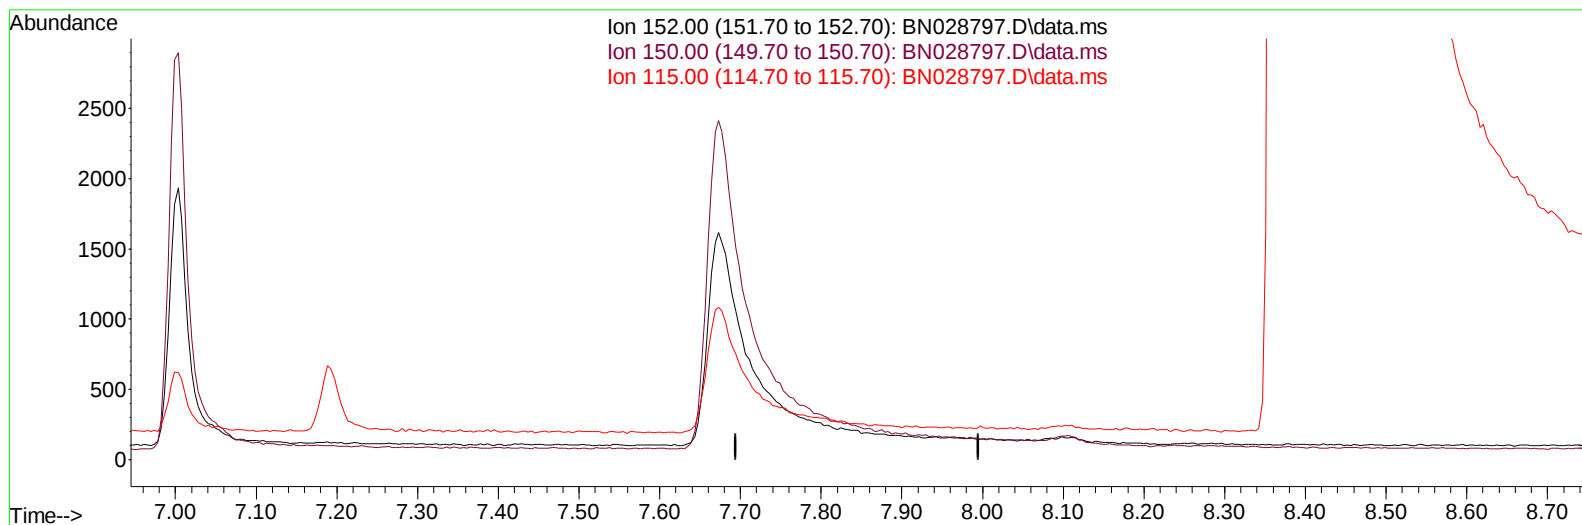

TIC: BN028797.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.795min (-7.795) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
150.00	155.30	0.00#
115.00	62.20	0.00#
0.00	0.00	0.00



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028797.D
Acq On : 20 Nov 2023 03:46
Operator : MA/JU
Sample : PB156868BL
Misc :
ALS Vial : 102 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK868

Manual IntegrationsAPPROVED

Quant Time: Nov 20 04:15:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

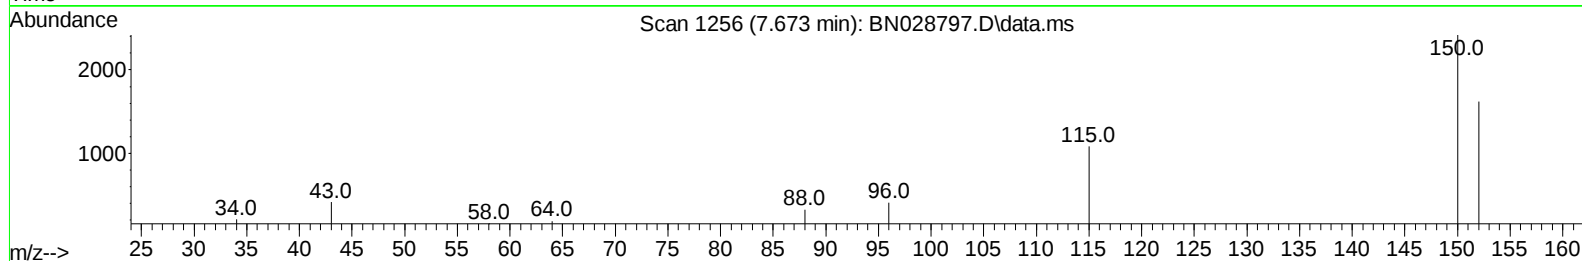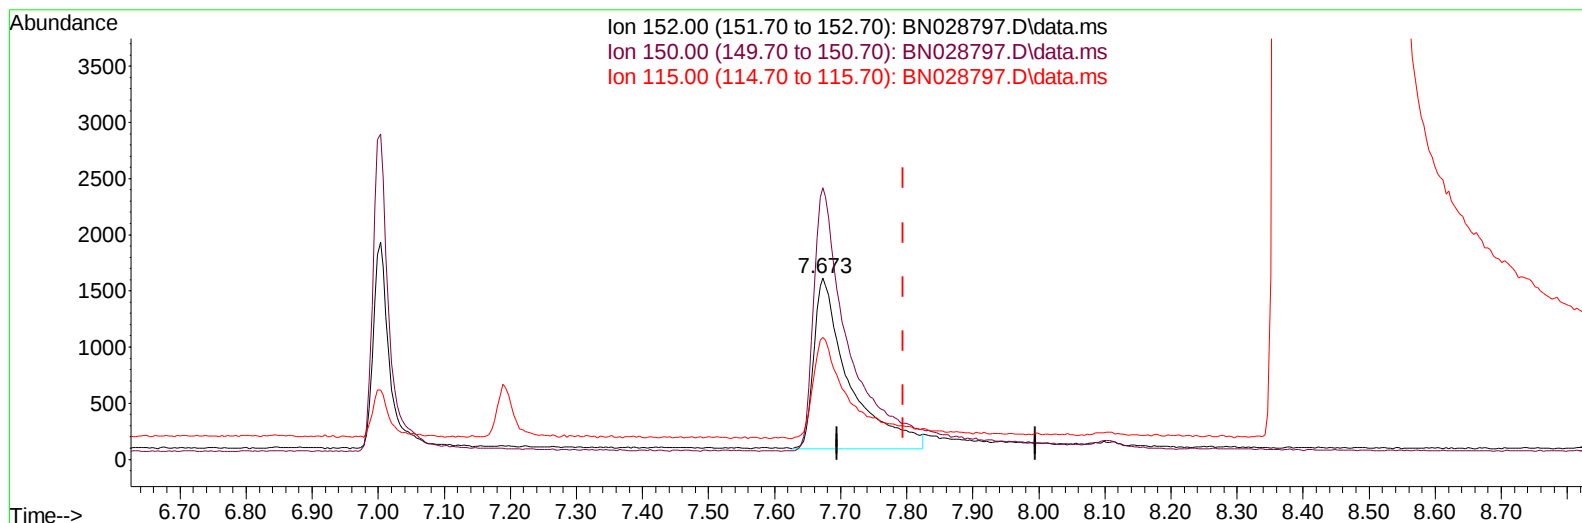

TIC: BN028797.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.673min (-0.122) 0.40 ng/ul m

response 5671

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	149.47
115.00	62.20	66.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028797.D
 Acq On : 20 Nov 2023 03:46
 Operator : MA/JU
 Sample : PB156868BL
 Misc :
 ALS Vial : 102 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK868

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 04:15:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.673	152	5671m	0.400	ng/ul	-0.12
4) Naphthalene-d8	10.450	136	21776	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.315	164	12187	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.068	188	22021	0.400	ng/ul	-0.02
17) Chrysene-d12	21.283	240	12964	0.400	ng/ul	#-0.01
23) Perylene-d12	23.563	264	17637	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.108	96	51416	8.203	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.061	152	9718	0.296	ng/ul	-0.05
18) Fluoranthene-d10	19.107	212	19895	0.477	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028797.D
Acq On : 20 Nov 2023 03:46
Operator : MA/JU
Sample : PB156868BL
Misc :
ALS Vial : 102 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK868

Manual IntegrationsAPPROVED

Quant Time: Nov 20 04:15:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

