

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028640.D
 Acq On : 15 Nov 2023 22:34
 Operator : MA/JU
 Sample : 05337-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ5

Quant Time: Nov 15 23:09:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 15 18:38:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.696	152	7292	0.400	ng/ul	0.02
4) Naphthalene-d8	10.469	136	30867	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.326	164	20662	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.078	188	43562	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.294	240	32905	0.400	ng/ul	# 0.00
23) Perylene-d12	23.577	264	38748	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.114	96	31263	3.879	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.085	152	7653	0.165	ng/ul	0.02
18) Fluoranthene-d10	19.113	212	41521	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.152	88	2525	0.283	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028640.D
Acq On : 15 Nov 2023 22:34
Operator : MA/JU
Sample : 05337-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDJ5

Quant Time: Nov 15 23:09:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 18:38:25 2023
Response via : Initial Calibration

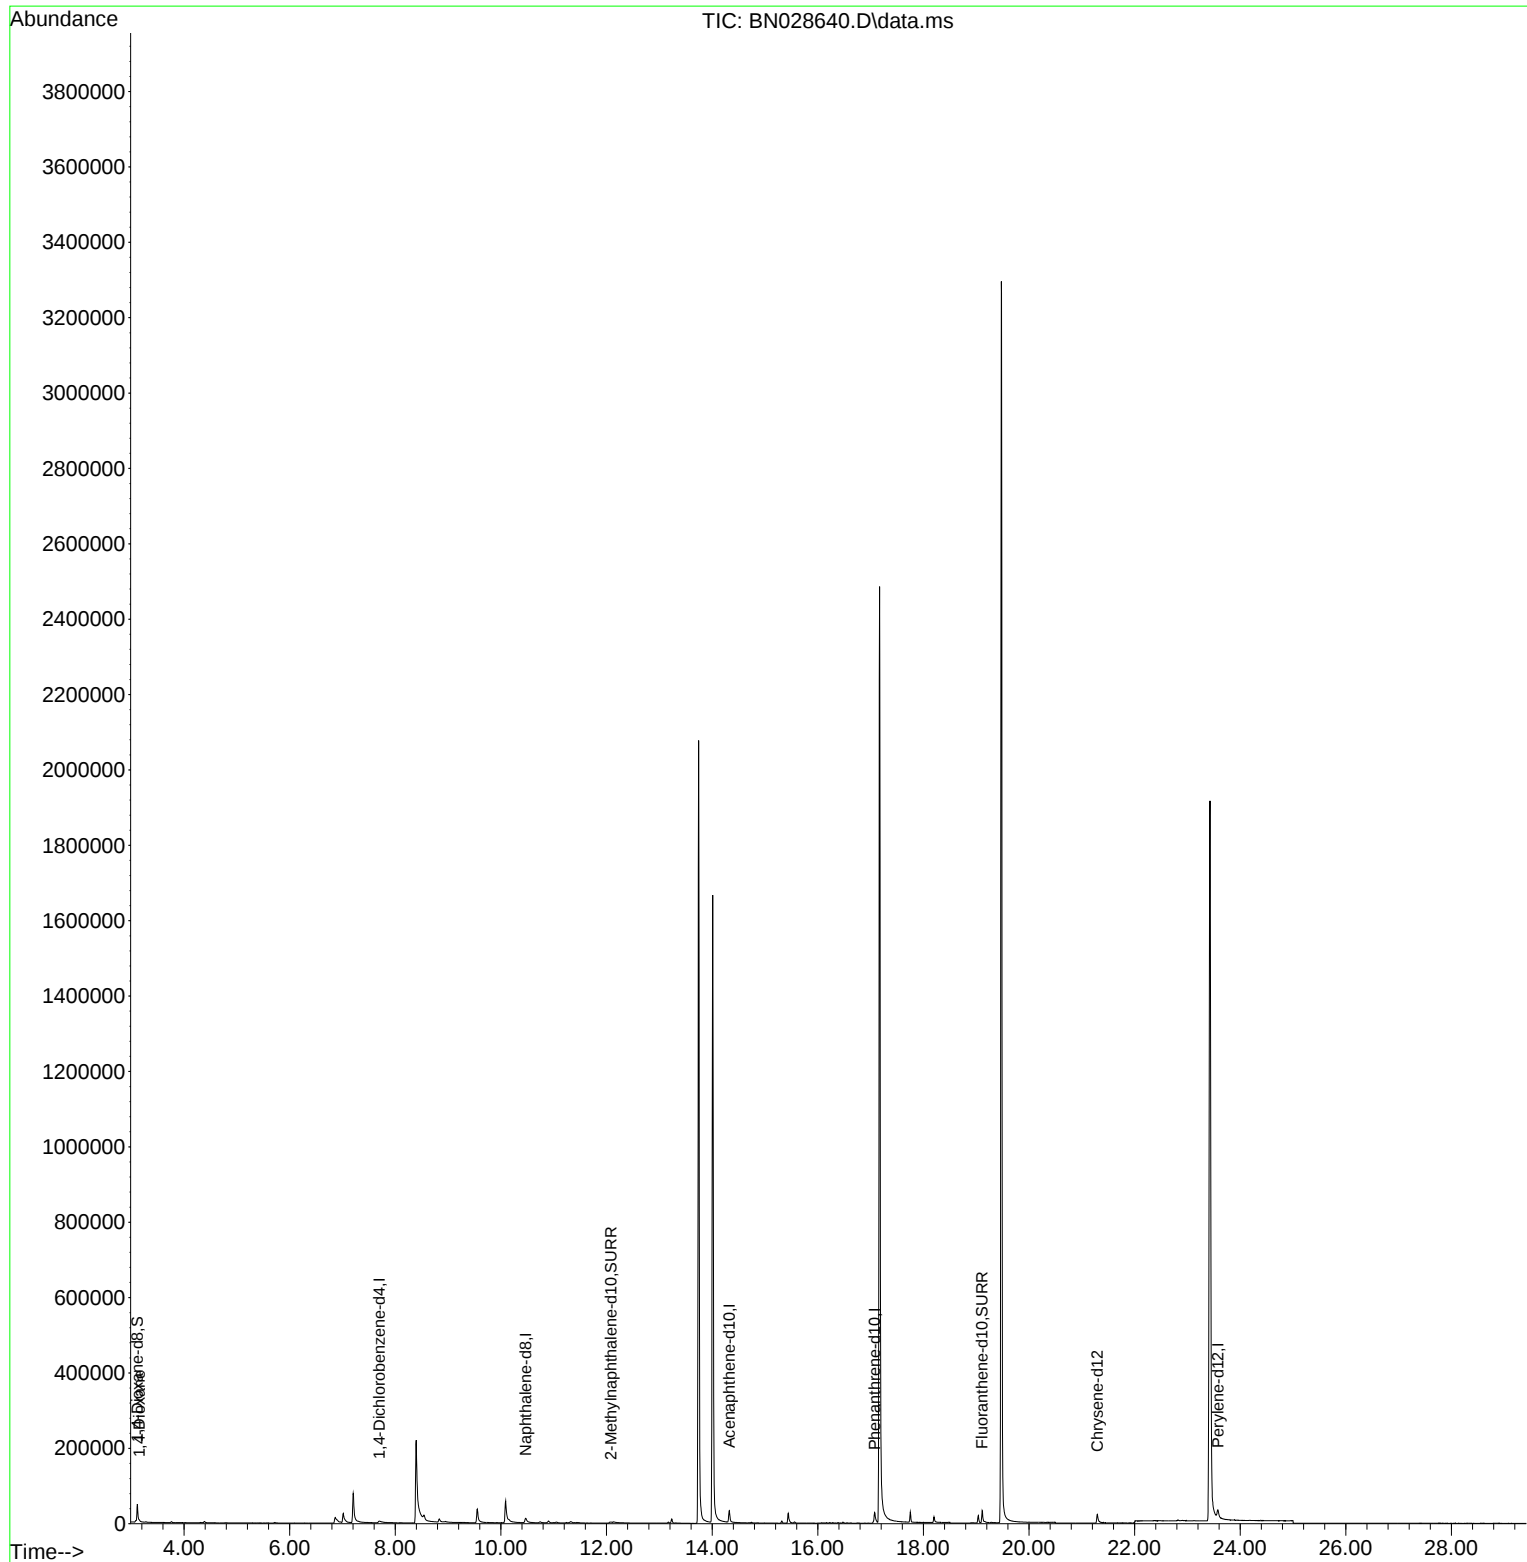

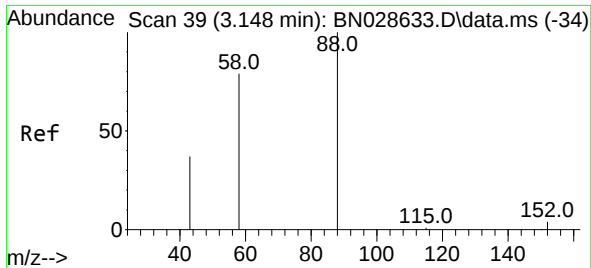

#2
 1,4-Dioxane
 Concen: 0.283 ng/ul
 RT: 3.152 min Scan# 40
 Delta R.T. 0.004 min
 Lab File: BN028640.D
 Acq: 15 Nov 2023 22:34

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ5

Tgt Ion: 88 Resp: 2525

Ion	Ratio	Lower	Upper
88	100		
43	49.9	32.9	49.3#
58	40.7	41.8	62.8#

