

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028642.D
 Acq On : 15 Nov 2023 23:46
 Operator : MA/JU
 Sample : 05337-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ7

Quant Time: Nov 16 00:23:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 15 18:38:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.709	152	4873	0.400	ng/ul	0.03
4) Naphthalene-d8	10.470	136	23041	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.322	164	14882	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.079	188	30430	0.400	ng/ul	0.00
17) Chrysene-d12	21.296	240	23953	0.400	ng/ul	0.00
23) Perylene-d12	23.575	264	30729	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.114	96	25853	4.800	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.092	152	5027	0.145	ng/ul	0.03
18) Fluoranthene-d10	19.119	212	33002	0.428	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.152	88	1930	0.324	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028642.D
Acq On : 15 Nov 2023 23:46
Operator : MA/JU
Sample : 05337-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDJ7

Quant Time: Nov 16 00:23:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 18:38:25 2023
Response via : Initial Calibration

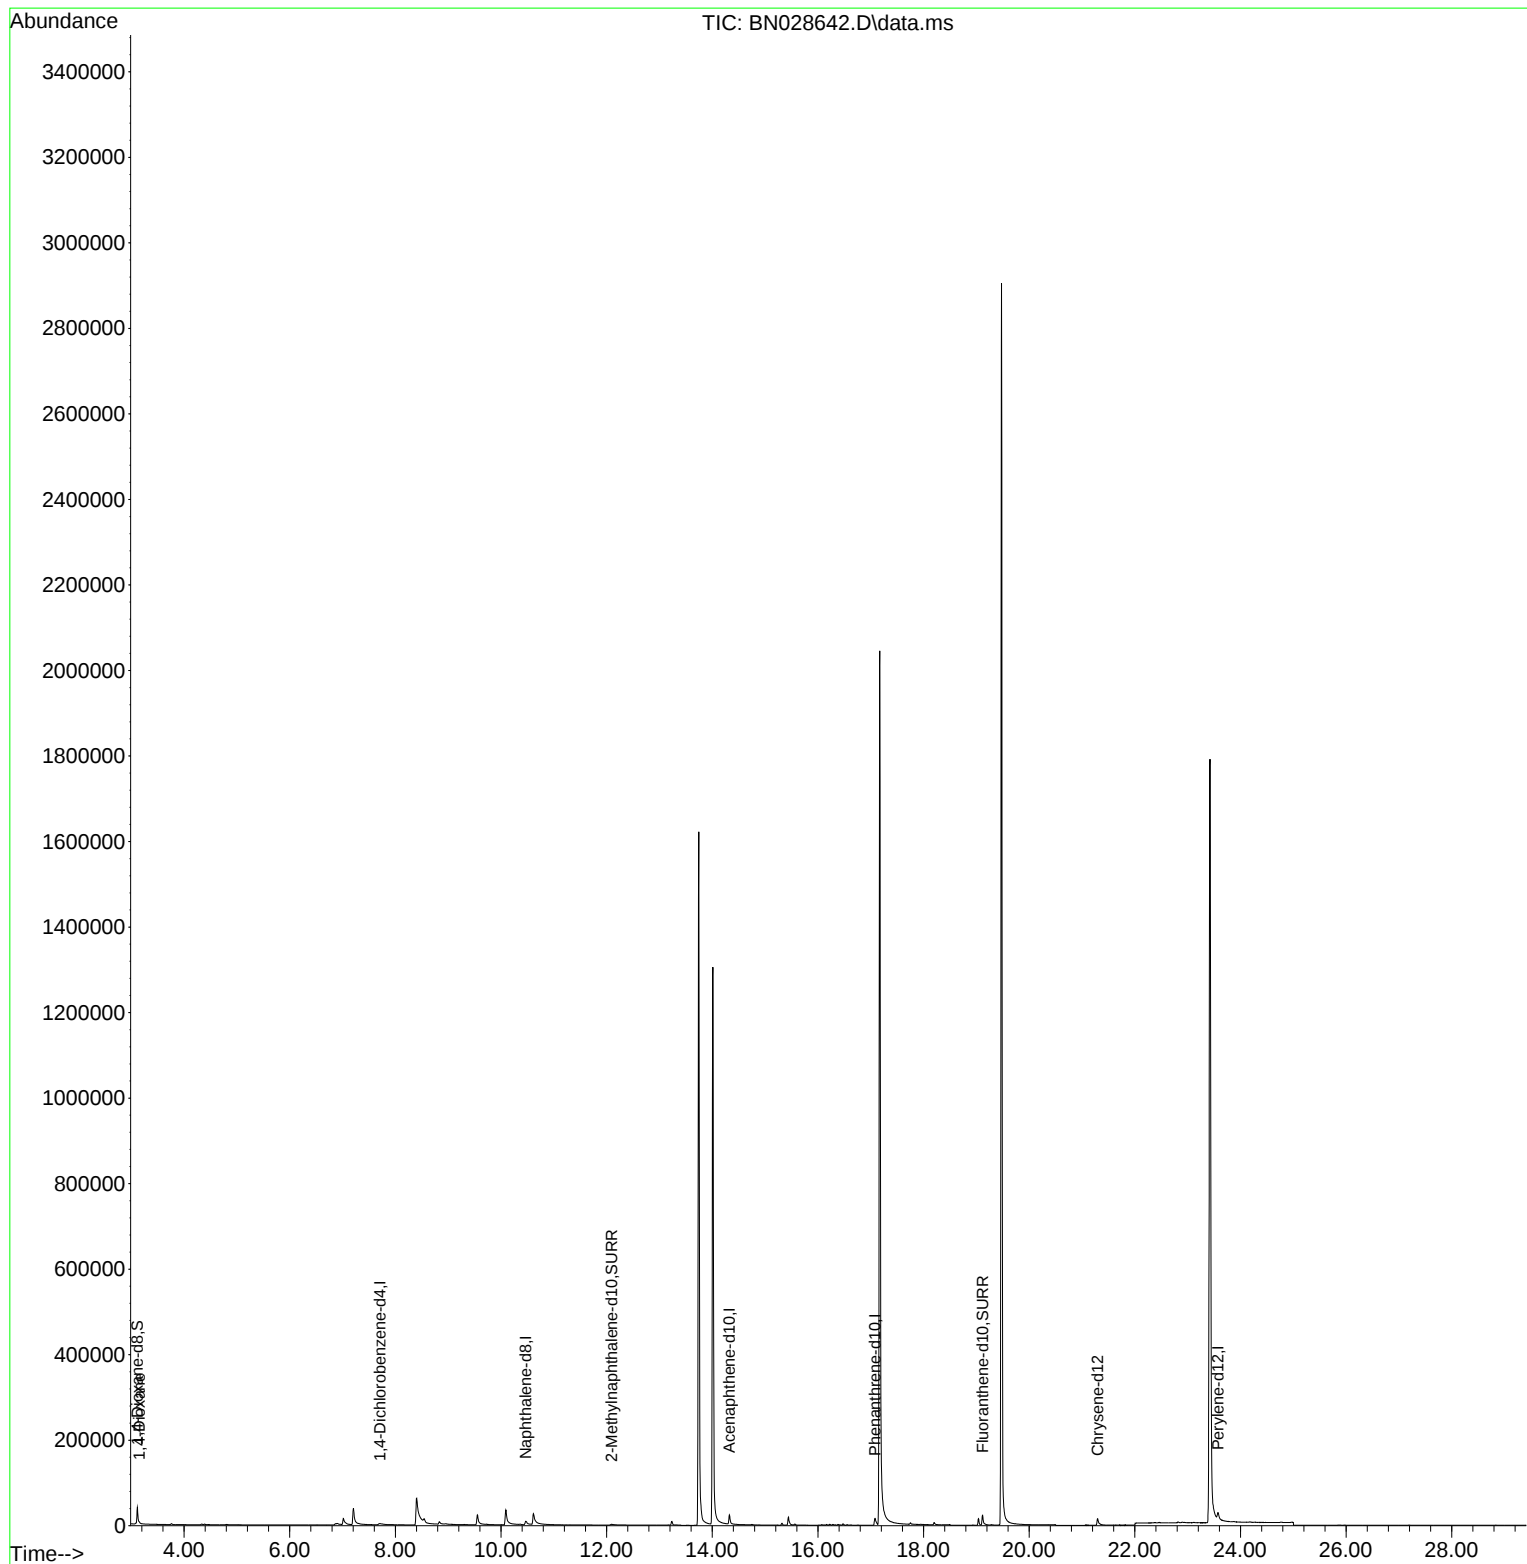

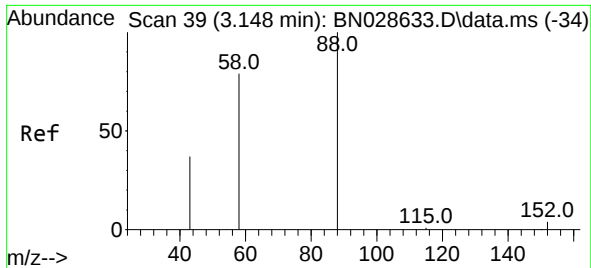

#2
 1,4-Dioxane
 Concen: 0.324 ng/ul
 RT: 3.152 min Scan# 40
 Delta R.T. 0.004 min
 Lab File: BN028642.D
 Acq: 15 Nov 2023 23:46

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ7

Tgt Ion: 88 Resp: 1930
 Ion Ratio Lower Upper
 88 100
 43 41.1 32.9 49.3
 58 33.1 41.8 62.8#

