

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028643.D
 Acq On : 16 Nov 2023 00:21
 Operator : MA/JU
 Sample : 05337-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ8

Quant Time: Nov 16 00:52:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 15 18:38:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	6303	0.400	ng/ul	0.03
4) Naphthalene-d8	10.470	136	29756	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.327	164	18946	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.079	188	38656	0.400	ng/ul	0.00
17) Chrysene-d12	21.293	240	28540	0.400	ng/ul	0.00
23) Perylene-d12	23.575	264	33700	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.118	96	26997	3.875	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.086	152	5448	0.122	ng/ul	0.02
18) Fluoranthene-d10	19.114	212	35268	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.152	88	2134	0.277	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028643.D
Acq On : 16 Nov 2023 00:21
Operator : MA/JU
Sample : 05337-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDJ8

Quant Time: Nov 16 00:52:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 18:38:25 2023
Response via : Initial Calibration

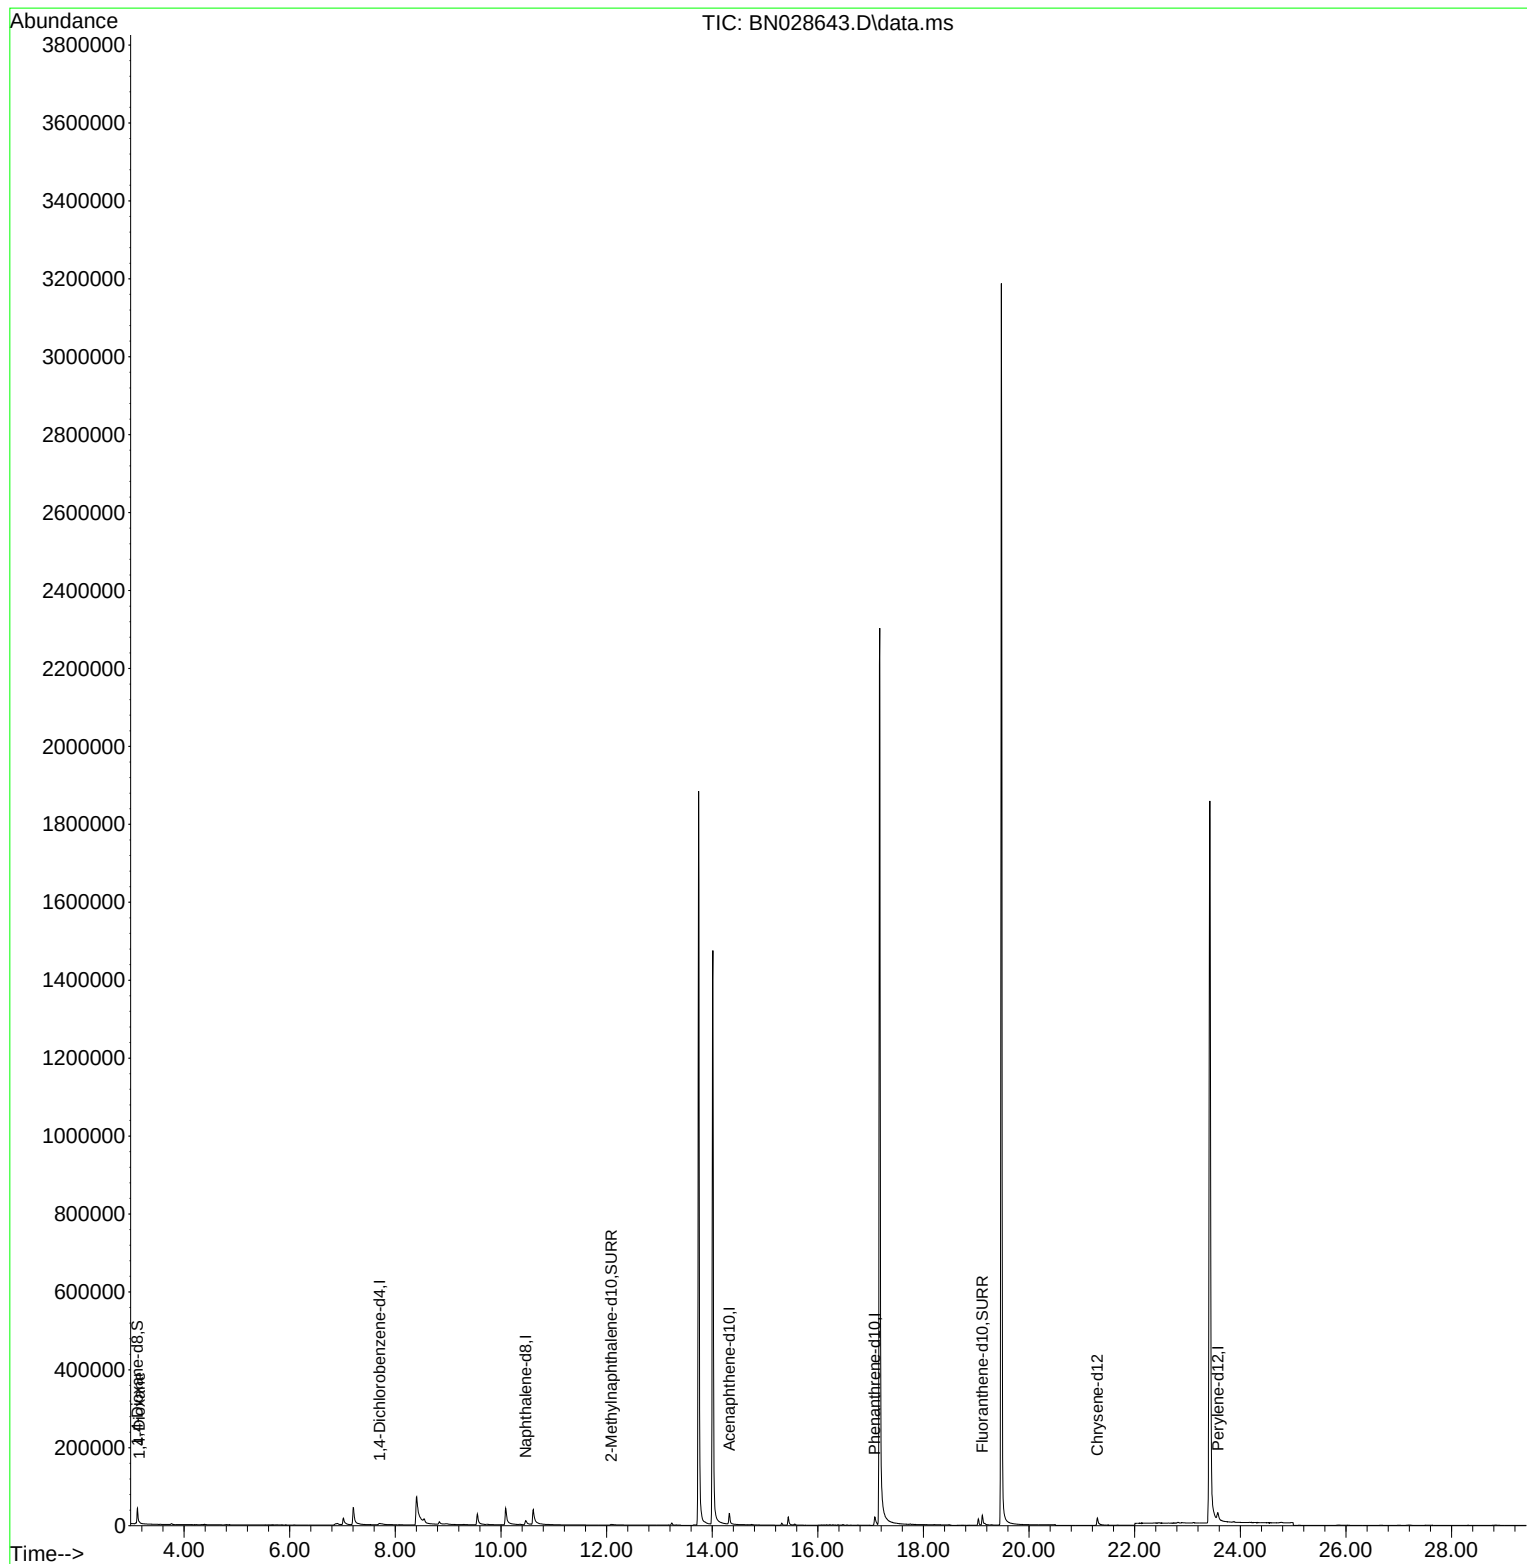

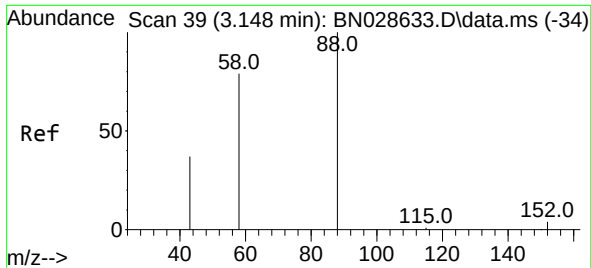

#2
 1,4-Dioxane
 Concen: 0.277 ng/ul
 RT: 3.152 min Scan# 40
 Delta R.T. 0.004 min
 Lab File: BN028643.D
 Acq: 16 Nov 2023 00:21

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ8

Tgt Ion: 88 Resp: 2134
 Ion Ratio Lower Upper
 88 100
 43 33.8 32.9 49.3
 58 26.7 41.8 62.8#

