

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028648.D
 Acq On : 16 Nov 2023 03:56
 Operator : MA/JU
 Sample : 05337-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDH9

Quant Time: Nov 16 04:40:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 04:34:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.713	152	5524	0.400	ng/ul	0.03
4) Naphthalene-d8	10.470	136	26827	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.322	164	17129	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.083	188	35401	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.293	240	27699	0.400	ng/ul	# 0.00
23) Perylene-d12	23.575	264	32974	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.118	96	23303	3.817	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.098	152	4558	0.113	ng/ul	0.03
18) Fluoranthene-d10	19.115	212	30540	0.343	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.152	88	1640	0.243	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028648.D
Acq On : 16 Nov 2023 03:56
Operator : MA/JU
Sample : 05337-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDH9

Quant Time: Nov 16 04:40:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 04:34:21 2023
Response via : Initial Calibration

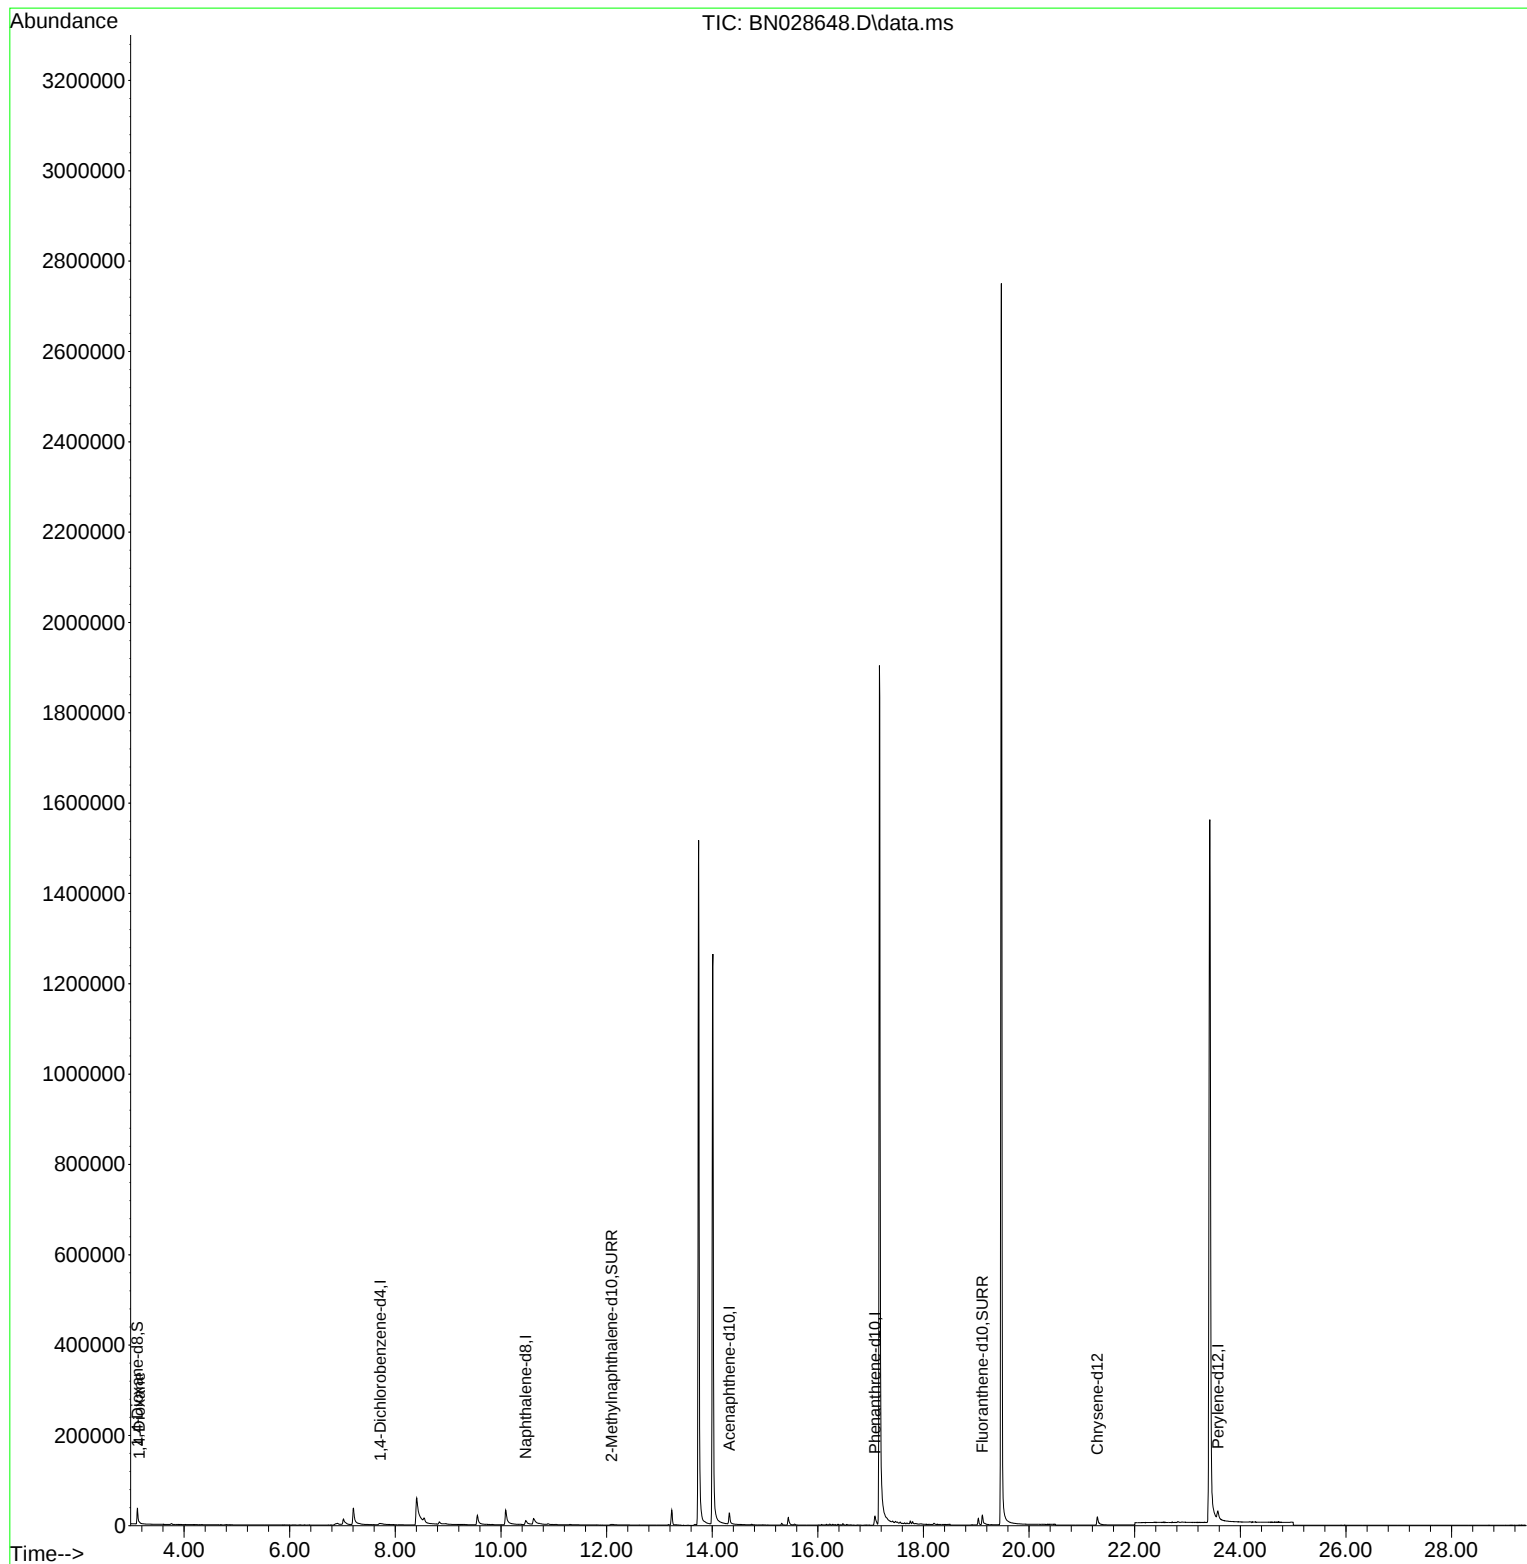

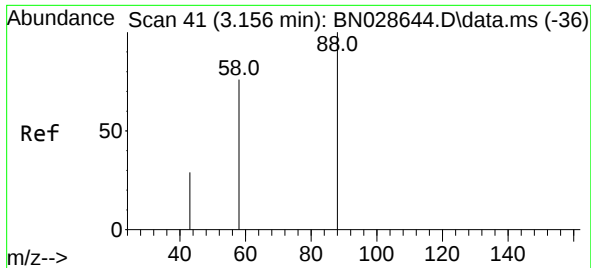

#2
 1,4-Dioxane
 Concen: 0.243 ng/ul
 RT: 3.152 min Scan# 40
 Delta R.T. 0.004 min
 Lab File: BN028648.D
 Acq: 16 Nov 2023 03:56

Instrument :
 BNA_N
 ClientSampleId :
 GCDH9

Tgt Ion: 88 Resp: 1640
 Ion Ratio Lower Upper
 88 100
 43 36.2 32.9 49.3
 58 29.9 41.8 62.8#

