

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028650.D
 Acq On : 16 Nov 2023 05:07
 Operator : MA/JU
 Sample : 05337-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ9

Quant Time: Nov 16 05:52:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 04:48:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.709	152	5002	0.400	ng/ul	# 0.03
4) Naphthalene-d8	10.470	136	25456	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.323	164	15807	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.079	188	32729	0.400	ng/ul	0.00
17) Chrysene-d12	21.293	240	24489	0.400	ng/ul	# 0.00
23) Perylene-d12	23.573	264	28506	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.114	96	29135	5.270	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.076	152	8642	0.226	ng/ul	0.01
18) Fluoranthene-d10	19.115	212	35813	0.454	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.152	88	1676	0.274	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028650.D
Acq On : 16 Nov 2023 05:07
Operator : MA/JU
Sample : 05337-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDJ9


Quant Time: Nov 16 05:52:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 04:48:33 2023
Response via : Initial Calibration

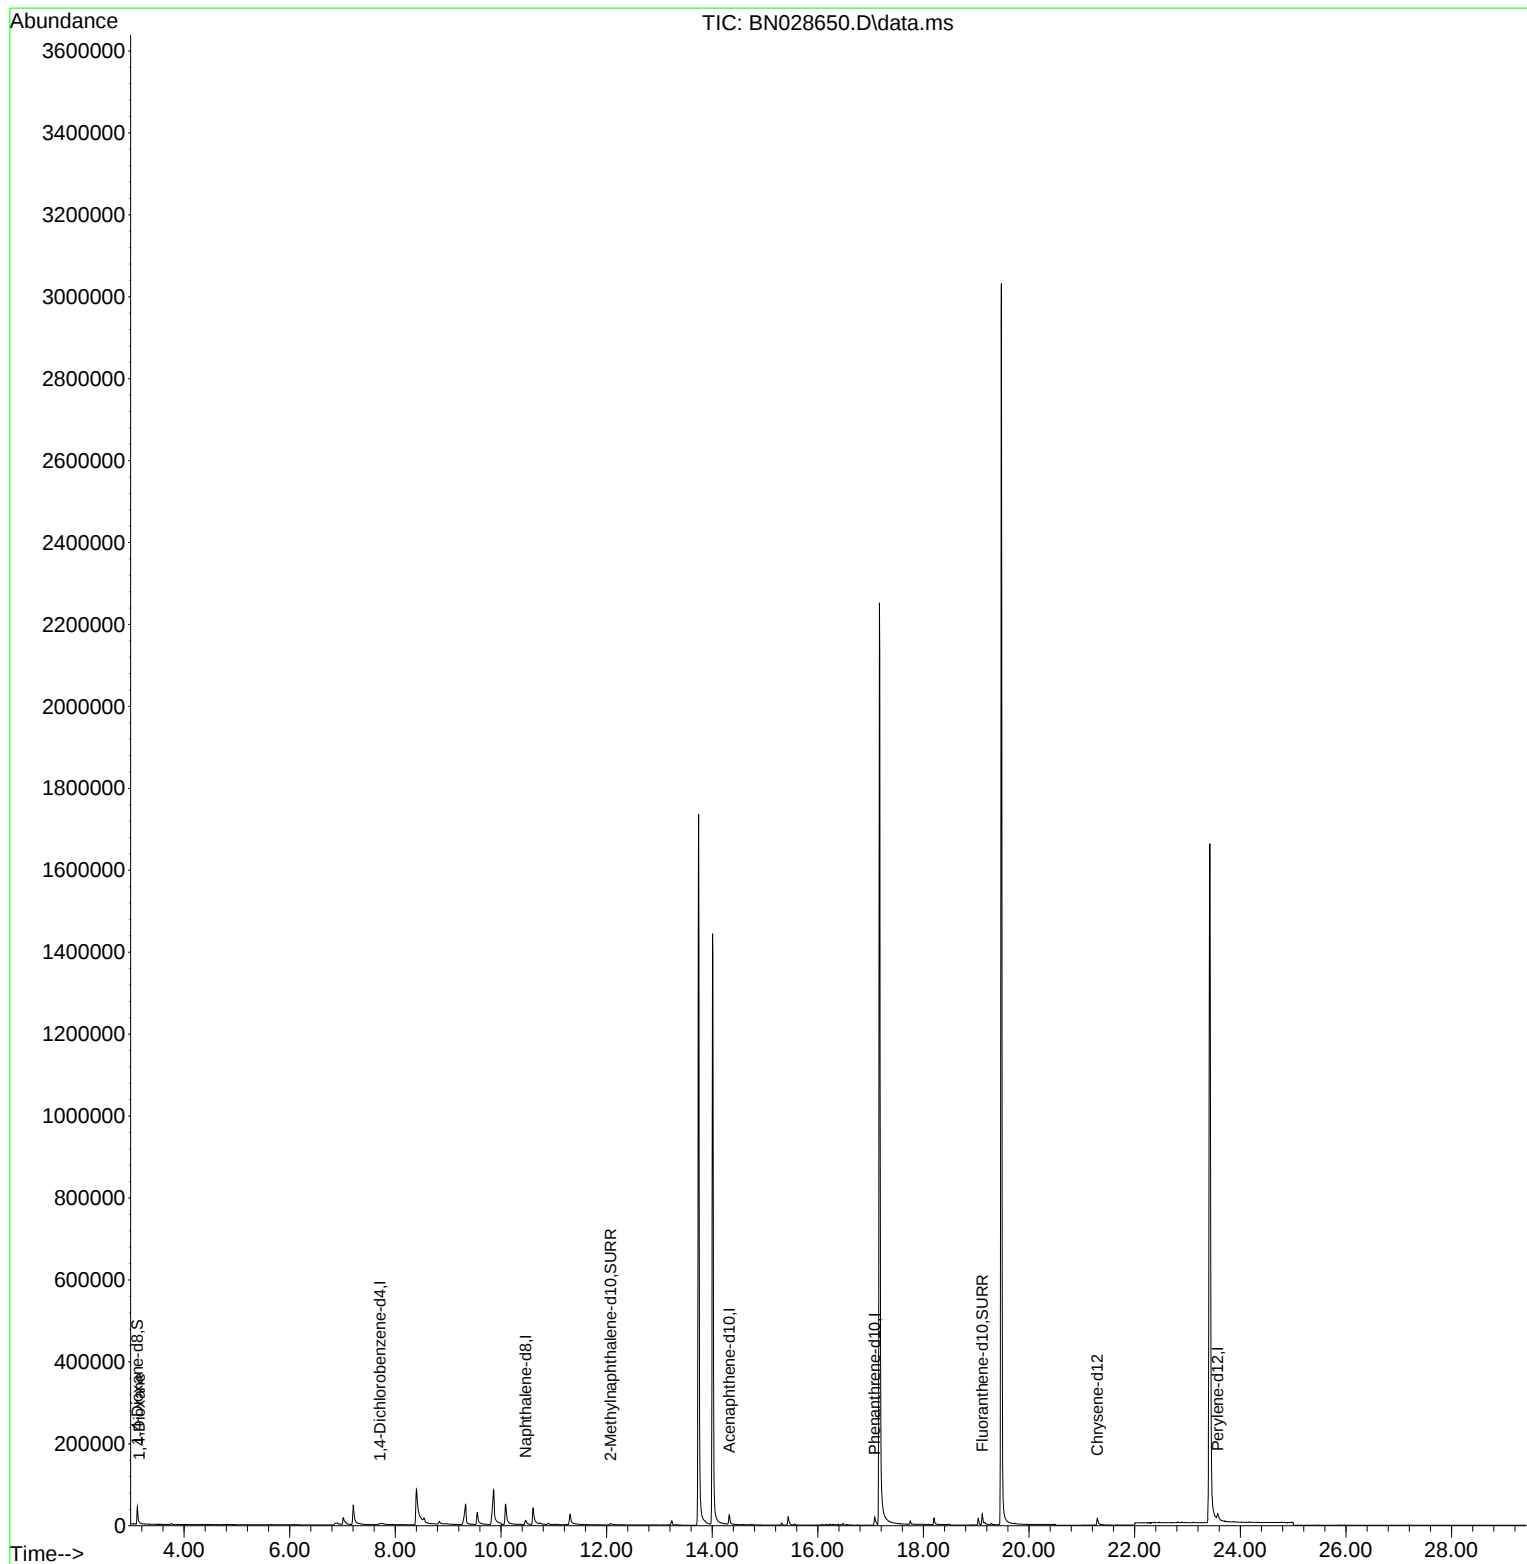

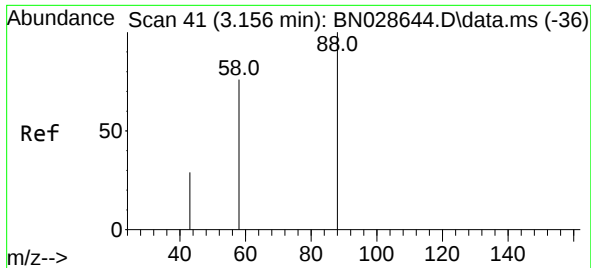

#2
 1,4-Dioxane
 Concen: 0.274 ng/ul
 RT: 3.152 min Scan# 40
 Delta R.T. 0.004 min
 Lab File: BN028650.D
 Acq: 16 Nov 2023 05:07

Instrument :
 BNA_N
 ClientSampleId :
 GCDJ9

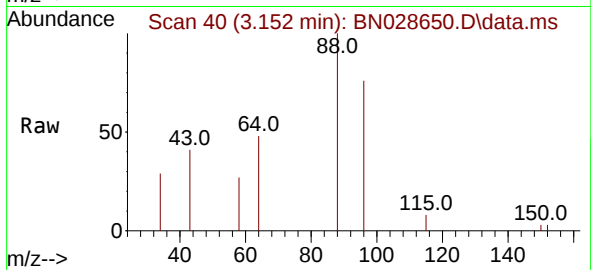

Tgt Ion:	88	Resp:	1676
Ion	Ratio	Lower	Upper
88	100		
43	40.5	32.9	49.3
58	26.6	41.8	62.8

