

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028679.D
 Acq On : 17 Nov 2023 00:45
 Operator : MA/JU
 Sample : 05338-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 01:37:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.719	152	10531m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.473	136	41184	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164	23584	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.081	188	48363	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.289	240	33636	0.400	ng/ul	# 0.00
23) Perylene-d12	23.569	264	37996	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	44797	3.849	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.112	152	6780	0.109	ng/ul	0.00
18) Fluoranthene-d10	19.117	212	37422	0.346	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.154	88	1573	0.122	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028679.D
Acq On : 17 Nov 2023 00:45
Operator : MA/JU
Sample : 05338-05
Misc :
ALS Vial : 47 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDL0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023


Quant Time: Nov 17 01:37:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

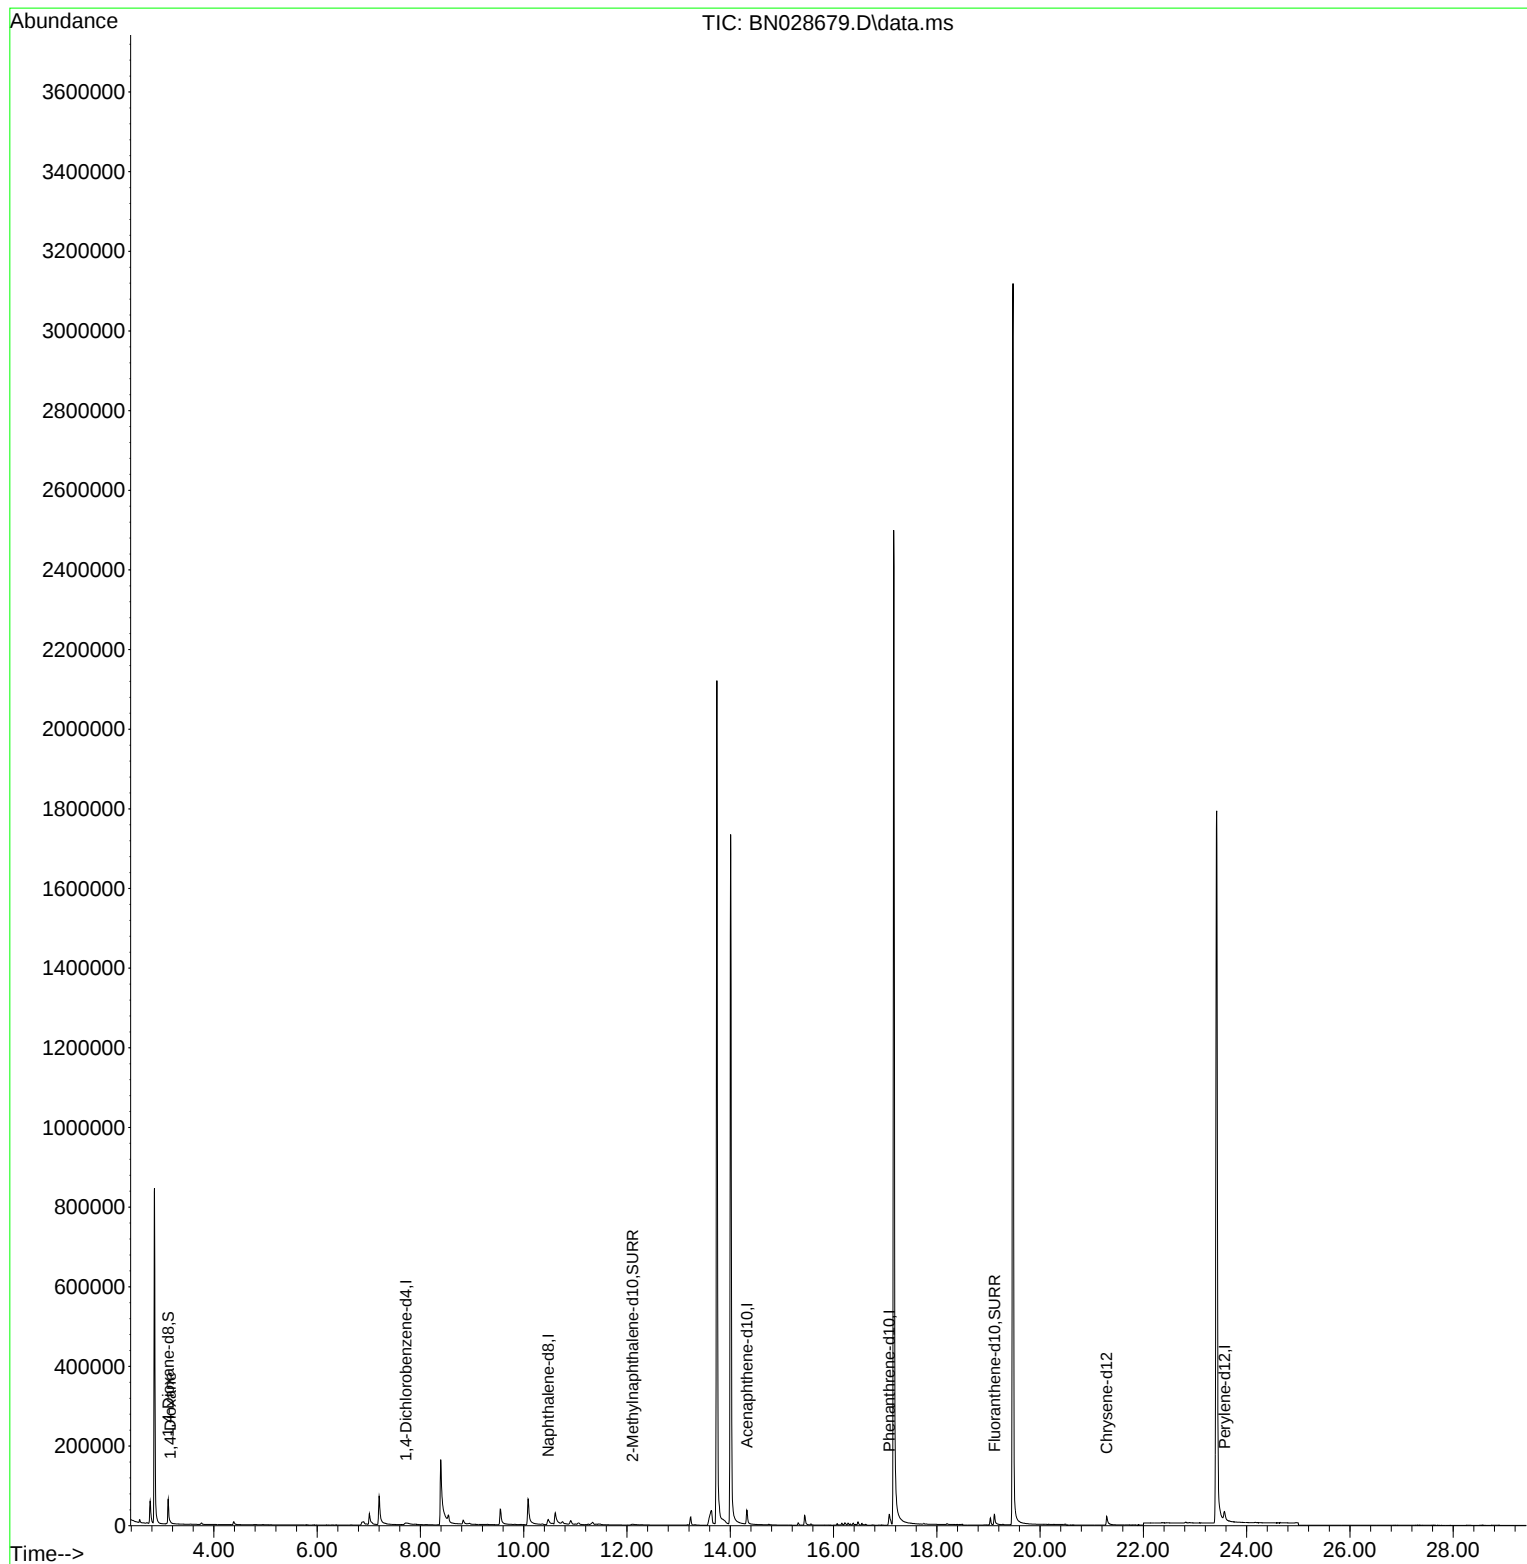

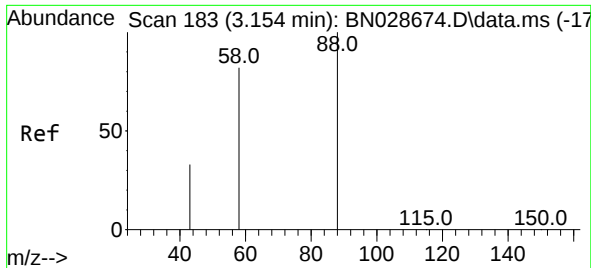

#2
 1,4-Dioxane
 Concen: 0.122 ng/ul
 RT: 3.154 min Scan# 183
 Delta R.T. -0.000 min
 Lab File: BN028679.D
 Acq: 17 Nov 2023 00:45

Instrument :
 BNA_N
 ClientSampleId :
 GCDL0

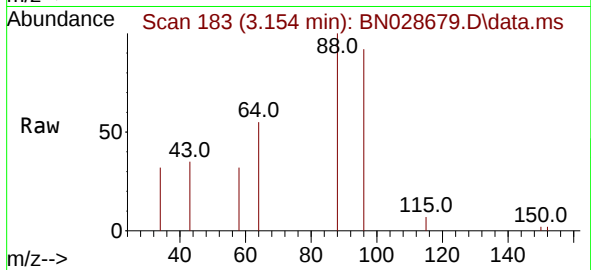

Tgt Ion: 88 Resp: 1573
 Ion Ratio Lower Upper
 88 100
 43 34.7 32.9 49.3
 58 31.6 41.8 62.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

