

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028680.D
 Acq On : 17 Nov 2023 01:21
 Operator : MA/JU
 Sample : 05338-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDL1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 03:10:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 22:38:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.715	152	9182m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.473	136	37735	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164	20851	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.081	188	41547	0.400	ng/ul	0.00
17) Chrysene-d12	21.292	240	29286	0.400	ng/ul	0.00
23) Perylene-d12	23.566	264	40471	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	40762	4.017	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.112	152	6563	0.116	ng/ul	0.00
18) Fluoranthene-d10	19.117	212	33130	0.352	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.154	88	1770	0.158	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028680.D
Acq On : 17 Nov 2023 01:21
Operator : MA/JU
Sample : 05338-06
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDL1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/20/2023


Quant Time: Nov 17 03:10:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 22:38:14 2023
Response via : Initial Calibration

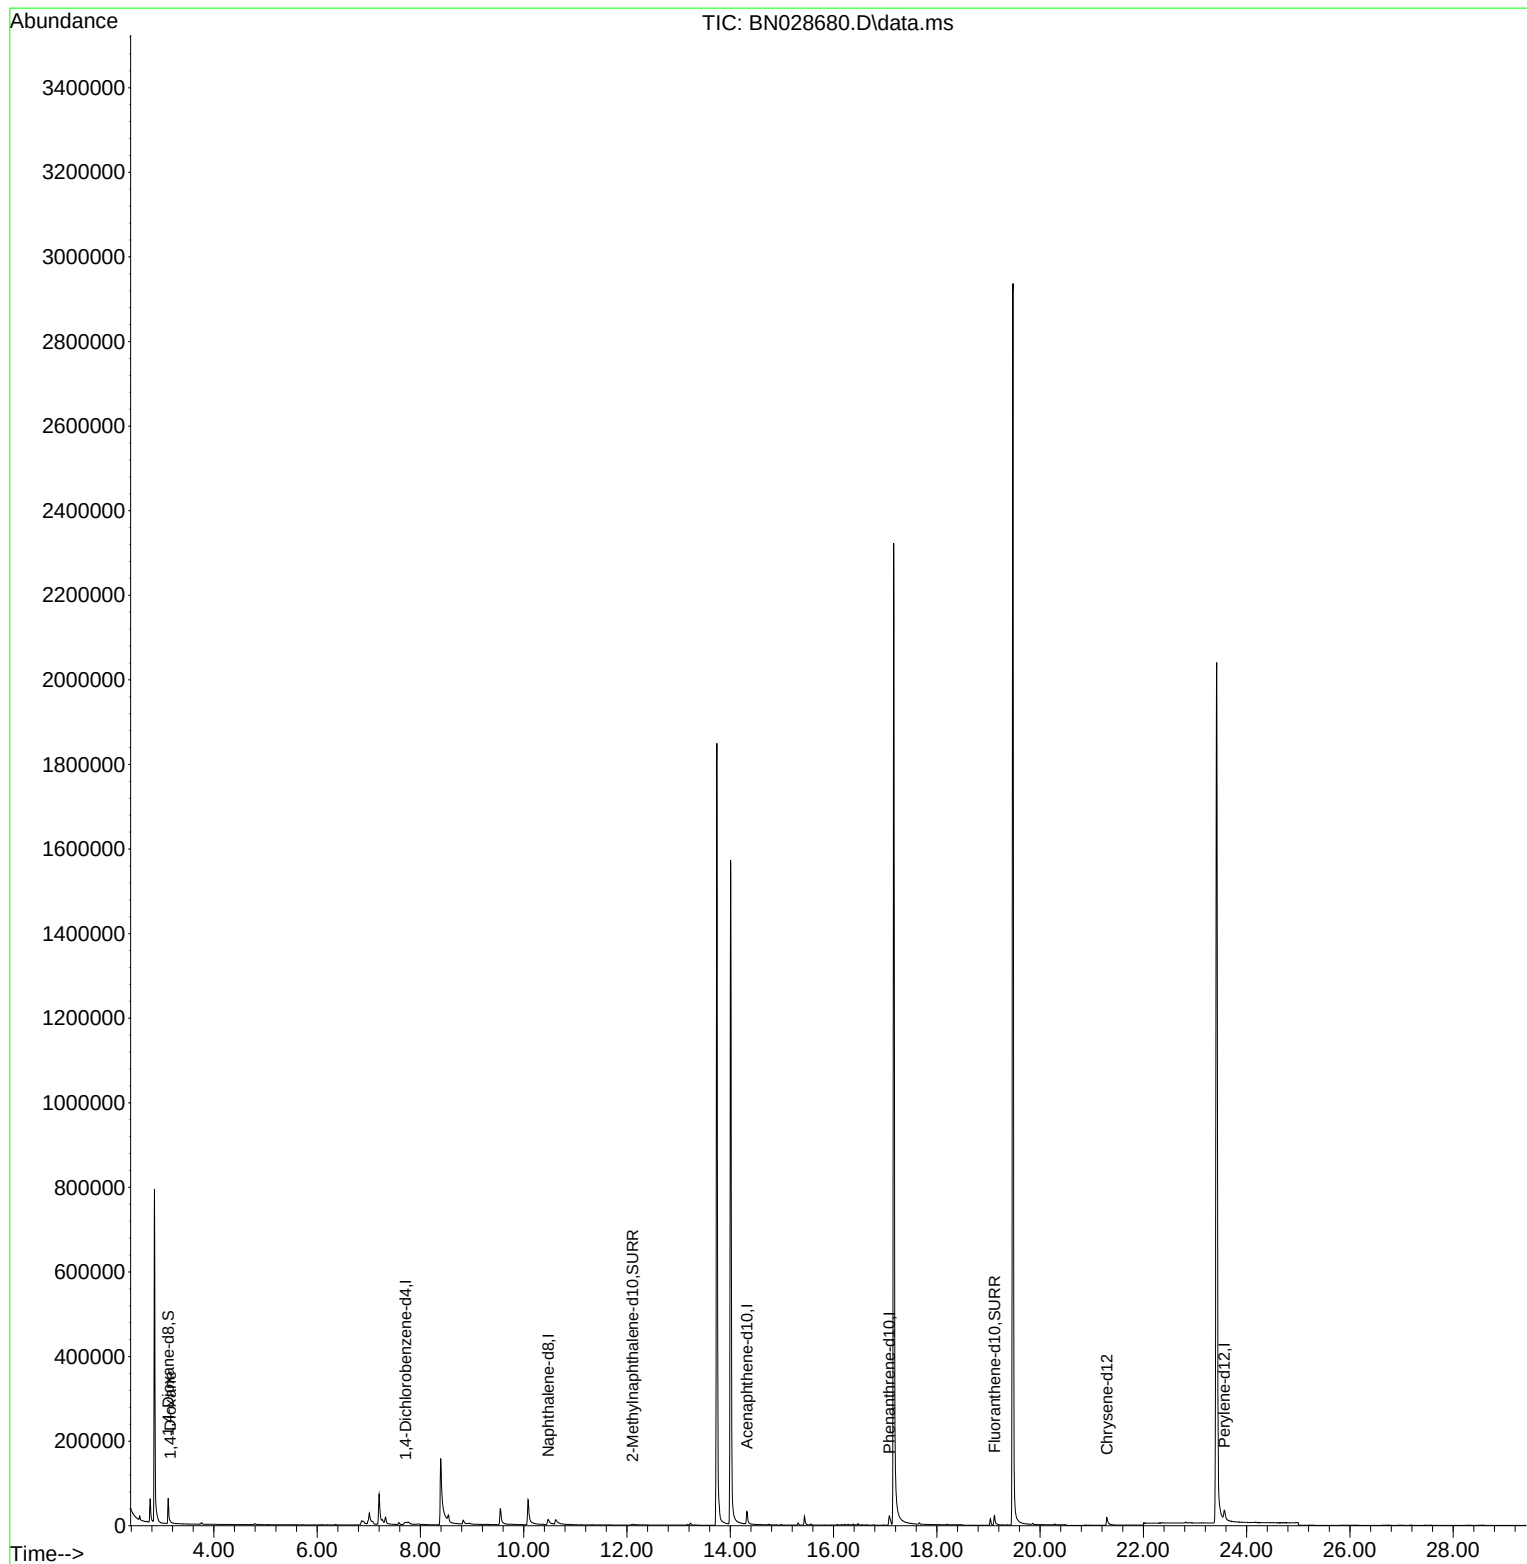

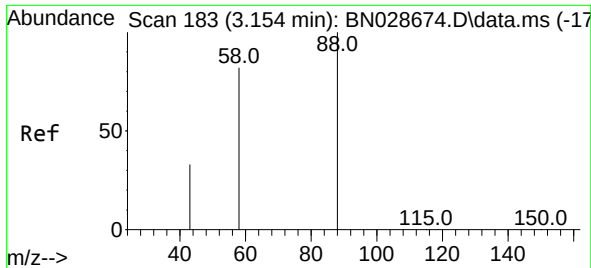

#2
 1,4-Dioxane
 Concen: 0.158 ng/ul
 RT: 3.154 min Scan# 183
 Delta R.T. -0.000 min
 Lab File: BN028680.D
 Acq: 17 Nov 2023 01:21

Instrument :
 BNA_N
 ClientSampleId :
 GCDL1

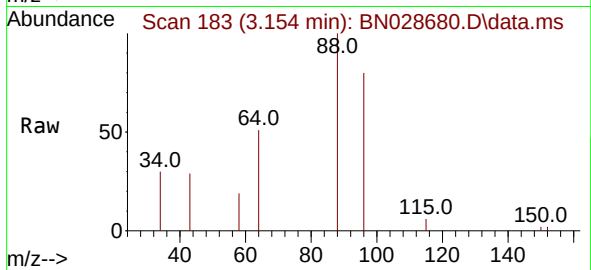

Tgt Ion: 88 Resp: 1770

Ion	Ratio	Lower	Upper
88	100		
43	29.4	32.9	49.3
58	19.1	41.8	62.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/20/2023

