

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028714.D
 Acq On : 17 Nov 2023 23:05
 Operator : MA/JU
 Sample : 05158-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH370

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 17 23:37:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.702	152	6182m	0.400	ng/ul	-0.09
4) Naphthalene-d8	10.467	136	27525	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.320	164	13825	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.072	188	26911	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.286	240	18568	0.400	ng/ul	# 0.00
23) Perylene-d12	23.568	264	22330	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	30438	4.455	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.072	152	10096	0.244	ng/ul	-0.04
18) Fluoranthene-d10	19.112	212	31872	0.533	ng/ul	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.154	88	1784	0.236	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028714.D
Acq On : 17 Nov 2023 23:05
Operator : MA/JU
Sample : 05158-14
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BH370

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2023
Supervised By :mohammad ahmed 11/20/2023


Quant Time: Nov 17 23:37:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

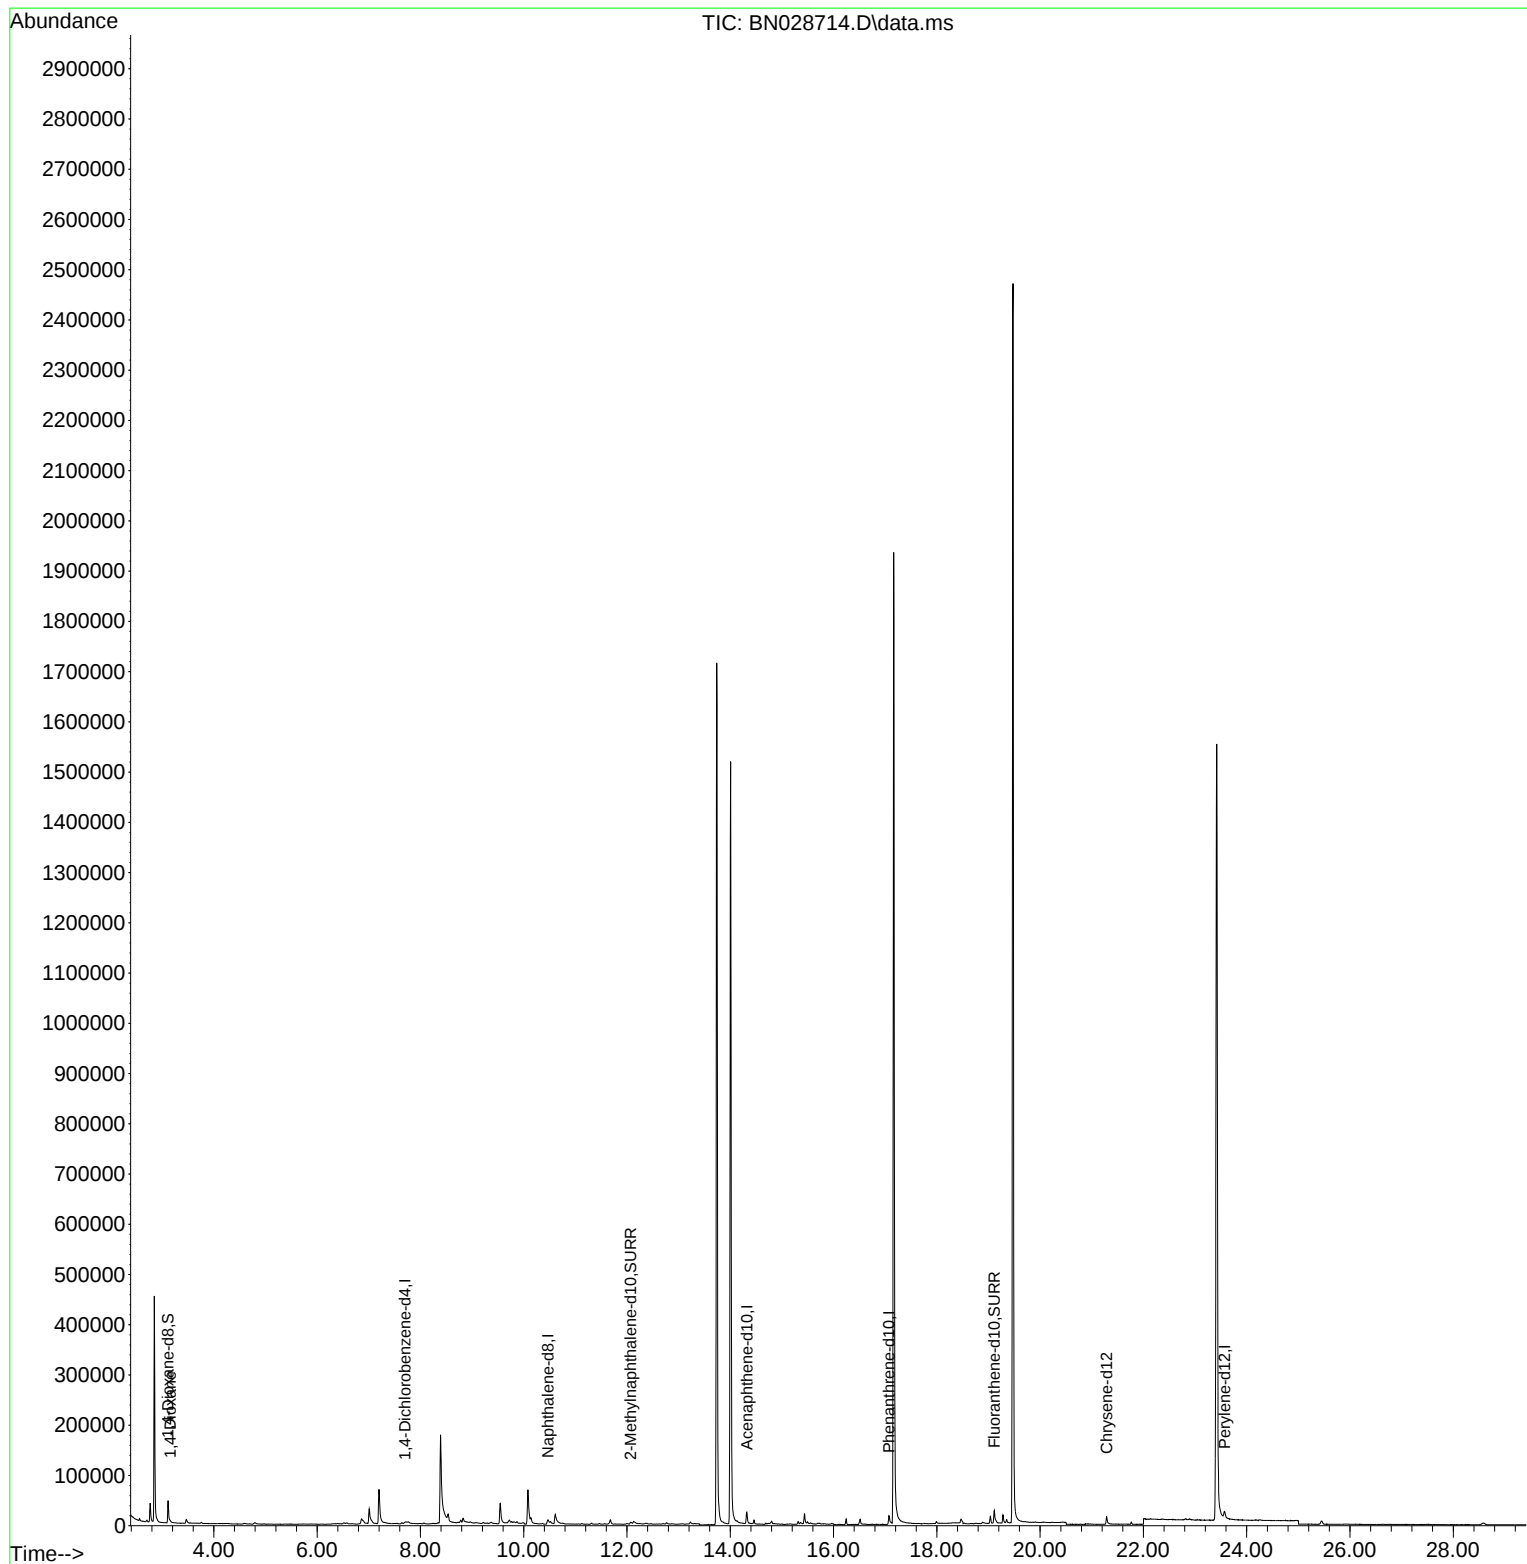

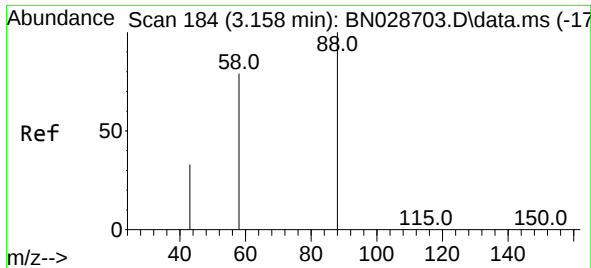

#2
 1,4-Dioxane
 Concen: 0.236 ng/ul
 RT: 3.154 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN028714.D
 Acq: 17 Nov 2023 23:05

Instrument :
 BNA_N
 ClientSampleId :
 BH370

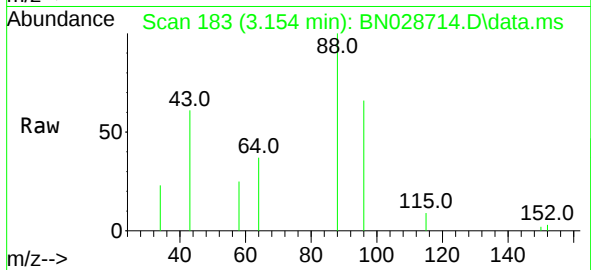

Tgt Ion: 88 Resp: 1784
 Ion Ratio Lower Upper
 88 100
 43 60.7 32.9 49.3
 58 25.3 41.8 62.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2023
 Supervised By :mohammad ahmed 11/20/2023

