

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028746.D
 Acq On : 18 Nov 2023 19:29
 Operator : MA/JU
 Sample : 05370-02
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDP8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 19 23:02:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.736	152	5019m	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.479	136	22206m	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.321	164	11177m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.086	188	20459m	0.400	ng/ul	0.00
17) Chrysene-d12	21.299	240	19479m	0.400	ng/ul	0.00
23) Perylene-d12	23.573	264	18458m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	36743	6.624	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.128	152	5993m	0.179	ng/ul	0.02
18) Fluoranthene-d10	19.113	212	28311m	0.452	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.154	88	1559	0.254	ng/ul#	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028746.D
Acq On : 18 Nov 2023 19:29
Operator : MA/JU
Sample : 05370-02
Misc :
ALS Vial : 46 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDP8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023


Quant Time: Nov 19 23:02:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

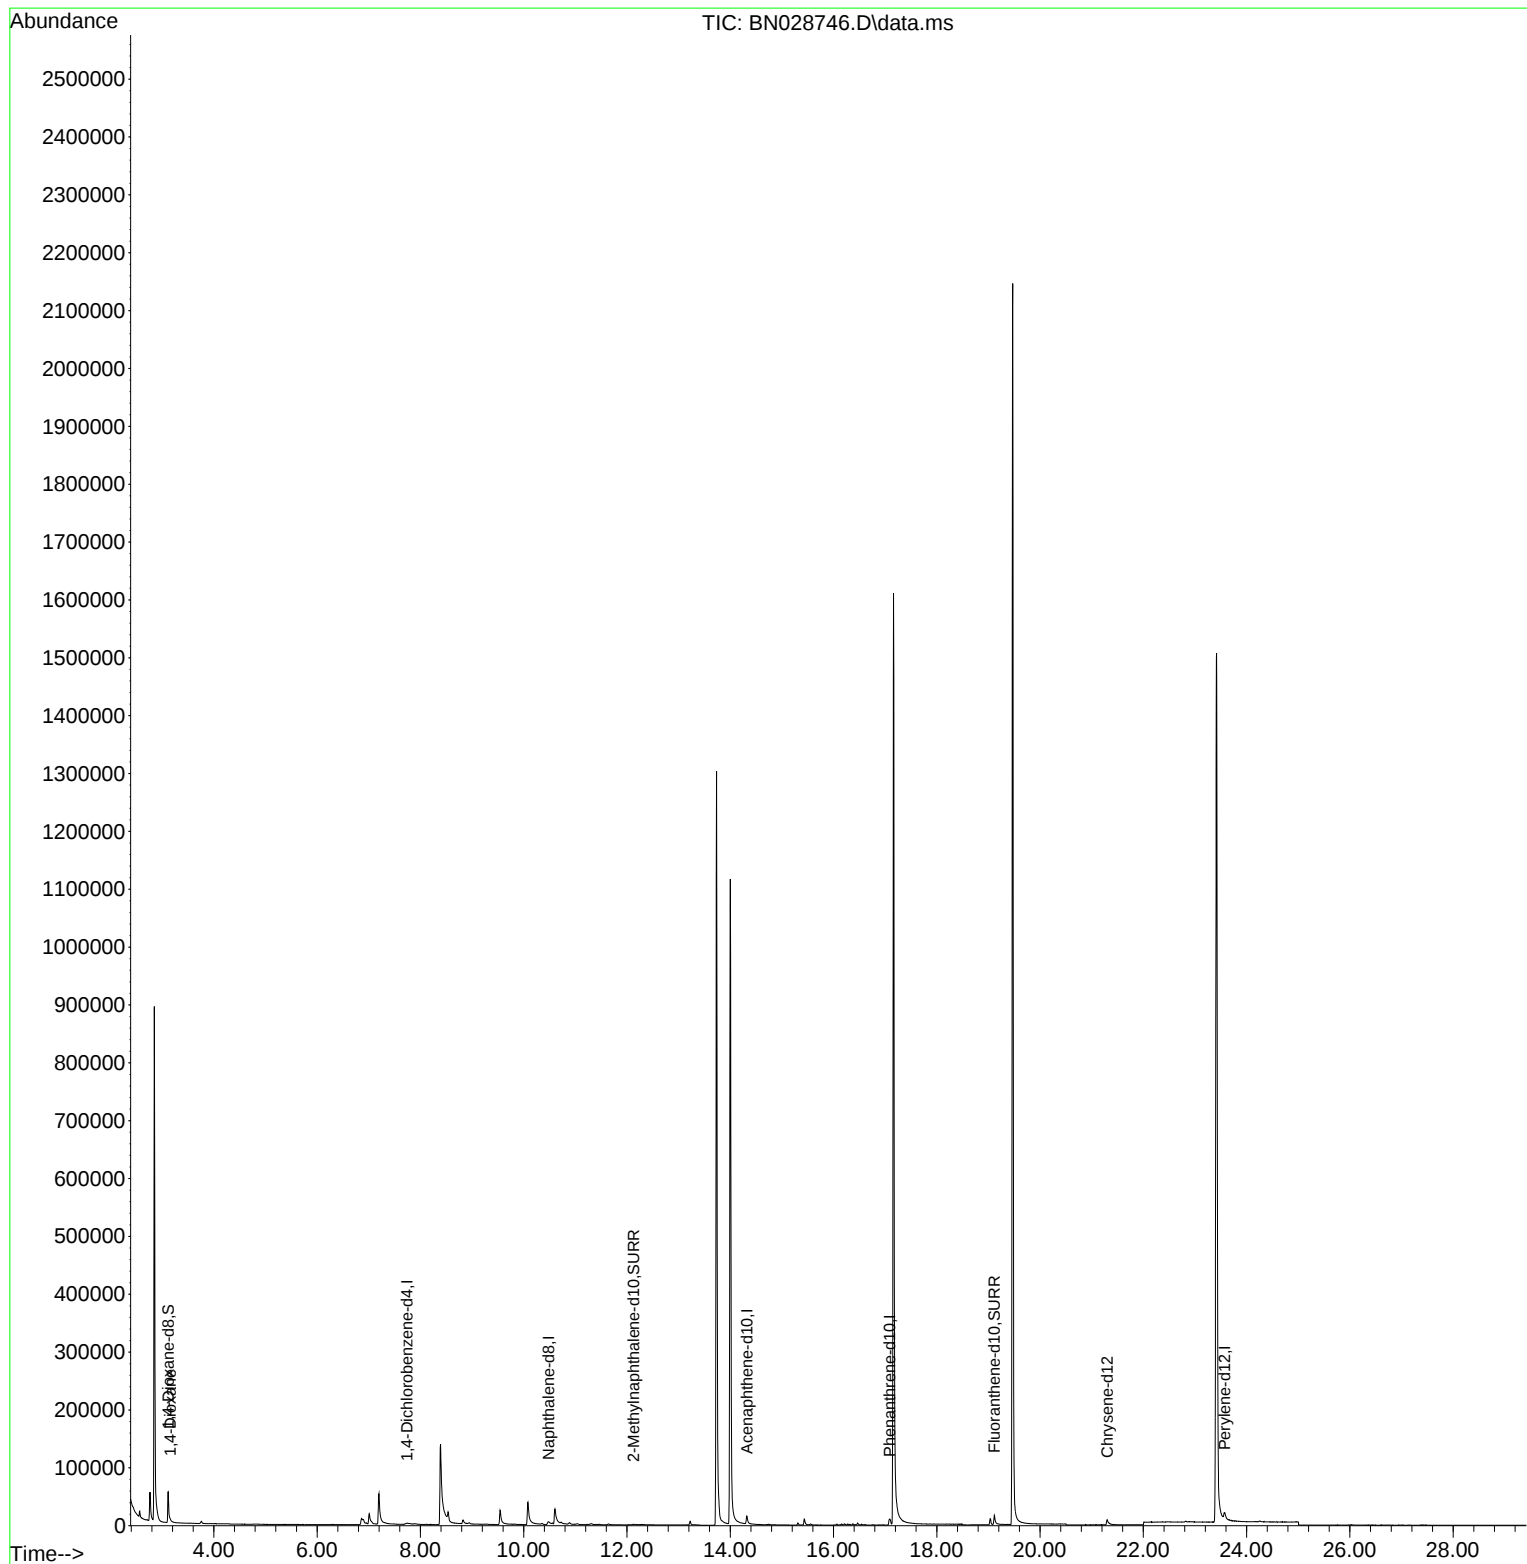

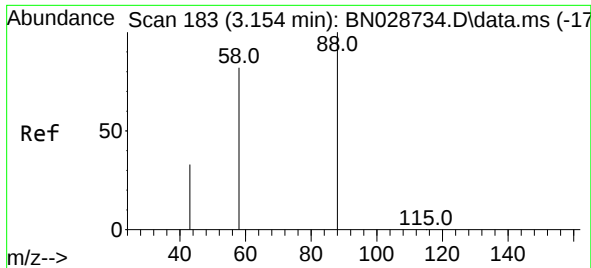

#2
 1,4-Dioxane
 Concen: 0.254 ng/ul
 RT: 3.154 min Scan# 183
 Delta R.T. -0.000 min
 Lab File: BN028746.D
 Acq: 18 Nov 2023 19:29

Instrument :
 BNA_N
 ClientSampleId :
 GCDP8

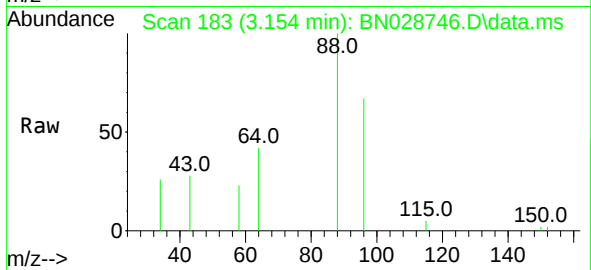

Tgt Ion: 88 Resp: 1559

Ion	Ratio	Lower	Upper
88	100		
43	28.2	32.9	49.3
58	23.4	41.8	62.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

