

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028753.D
 Acq On : 19 Nov 2023 00:16
 Operator : MA/JU
 Sample : 05370-03
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDP9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 19 23:43:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.753	152	6641m	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.479	136	25561	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.321	164	15730	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.082	188	31909	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.296	240	20479	0.400	ng/ul	# 0.00
23) Perylene-d12	23.573	264	24714	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	43994	5.994	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.140	152	3972	0.103	ng/ul	0.03
18) Fluoranthene-d10	19.113	212	27537	0.418	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.150	88	5071	0.625	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028753.D
Acq On : 19 Nov 2023 00:16
Operator : MA/JU
Sample : 05370-03
Misc :
ALS Vial : 54 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDP9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023


Quant Time: Nov 19 23:43:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

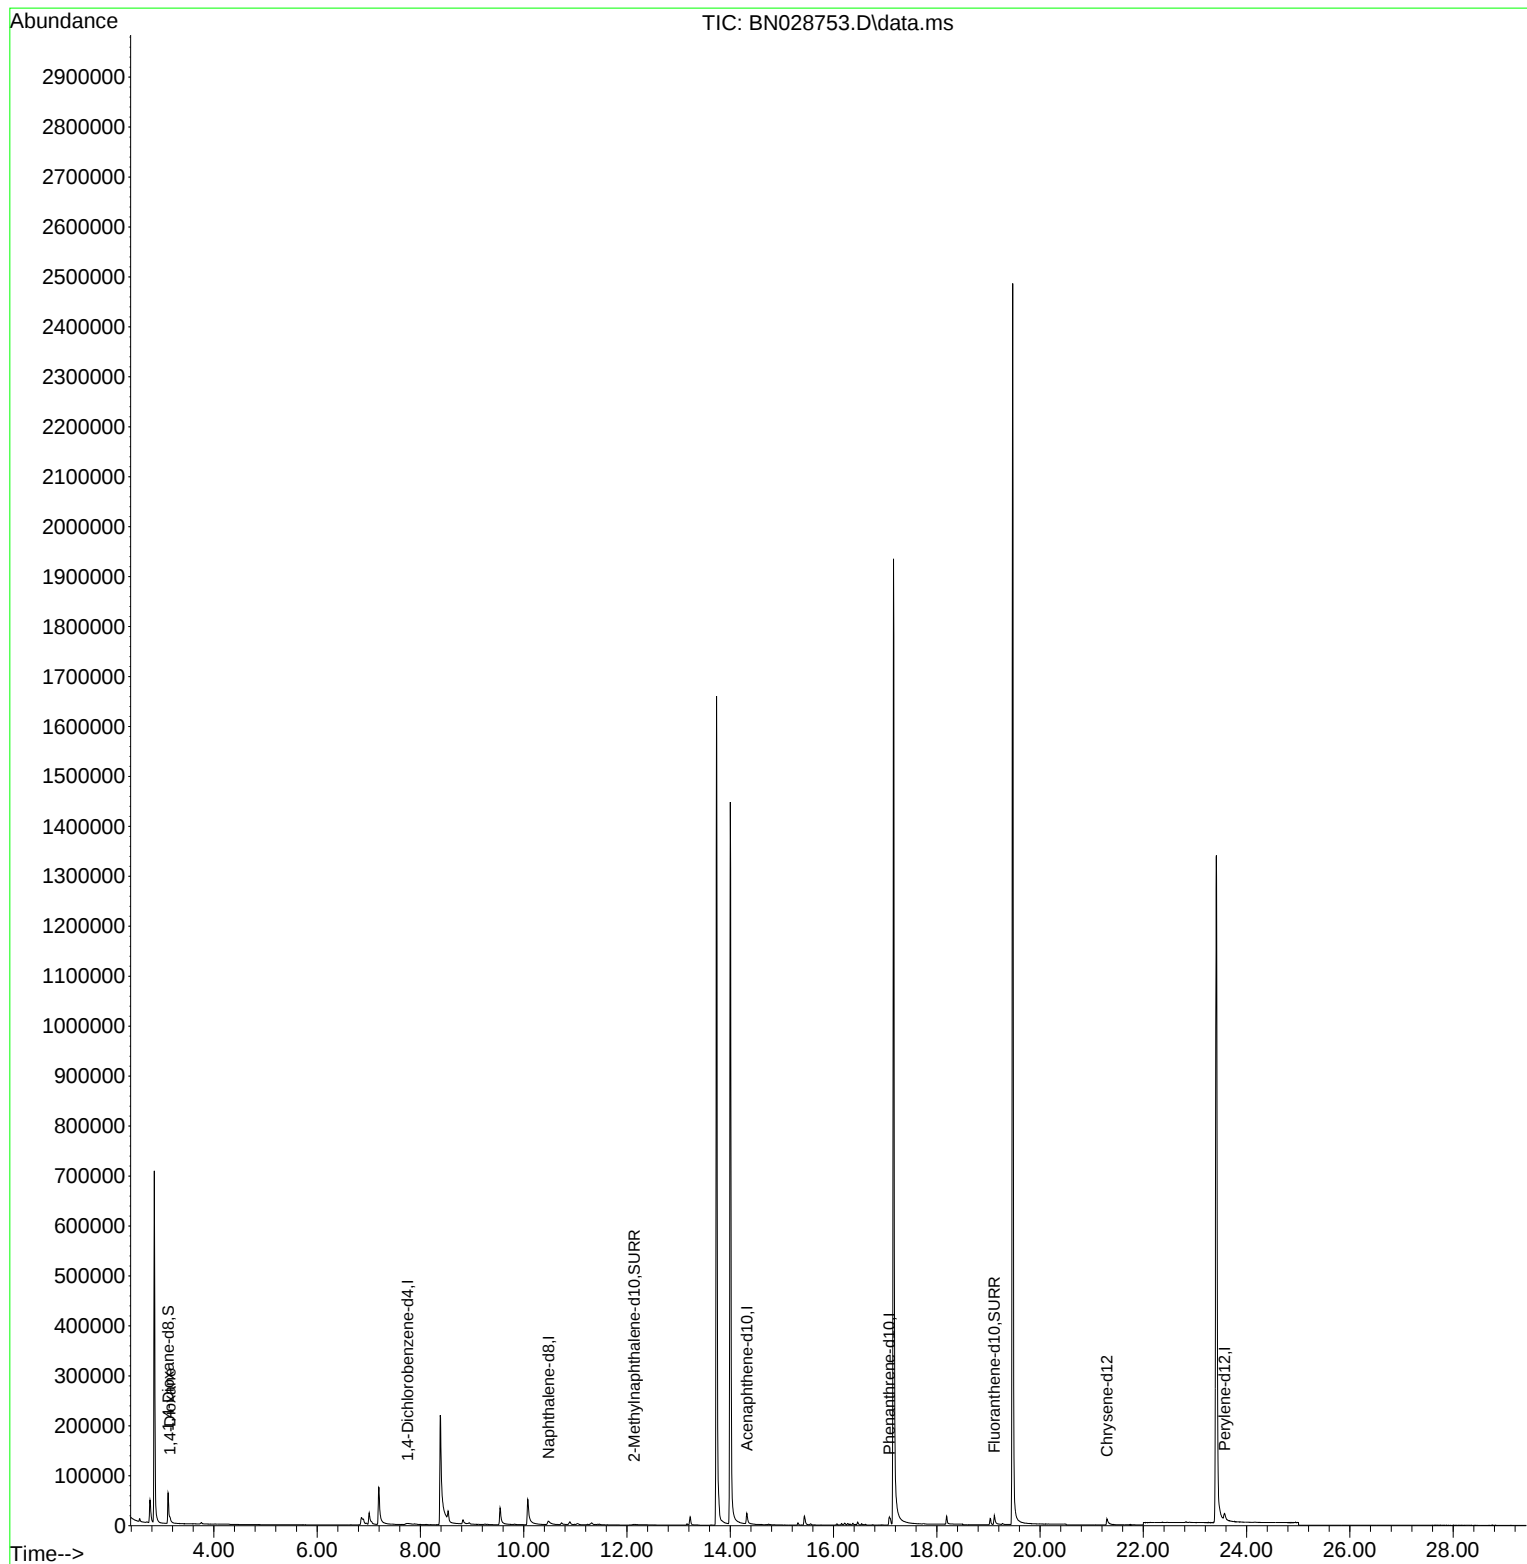

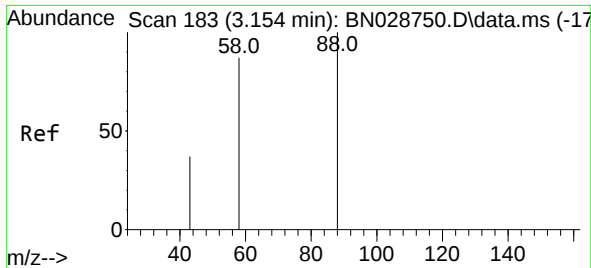

#2
1,4-Dioxane
Concen: 0.625 ng/ul
RT: 3.150 min Scan# 183
Delta R.T. -0.004 min
Lab File: BN028753.D
Acq: 19 Nov 2023 00:16

Instrument :
BNA_N
ClientSampleId :
GCDP9

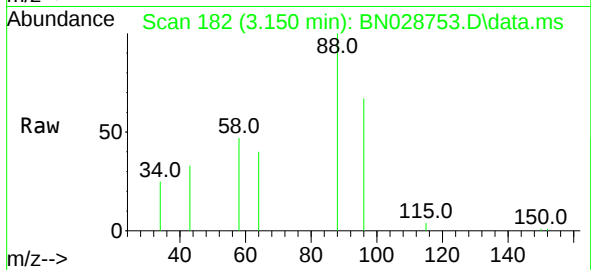

Tgt Ion: 88 Resp: 507
Ion Ratio Lower Upper
88 100
43 33.4 32.9 49.3
58 46.9 41.8 62.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

