

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028754.D
 Acq On : 19 Nov 2023 00:53
 Operator : MA/JU
 Sample : 05370-04
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 19 23:48:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.753	152	5148m	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.468	136	20640	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.321	164	11652	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.081	188	24033m	0.400	ng/ul	0.00
17) Chrysene-d12	21.293	240	15514	0.400	ng/ul	# 0.00
23) Perylene-d12	23.572	264	18194	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.116	96	45585	8.012	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.090	152	8892	0.286	ng/ul	-0.02
18) Fluoranthene-d10	19.113	212	29754	0.596	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.150	88	690	0.110	ng/ul#	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028754.D
Acq On : 19 Nov 2023 00:53
Operator : MA/JU
Sample : 05370-04
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDQ0

Quant Time: Nov 19 23:48:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

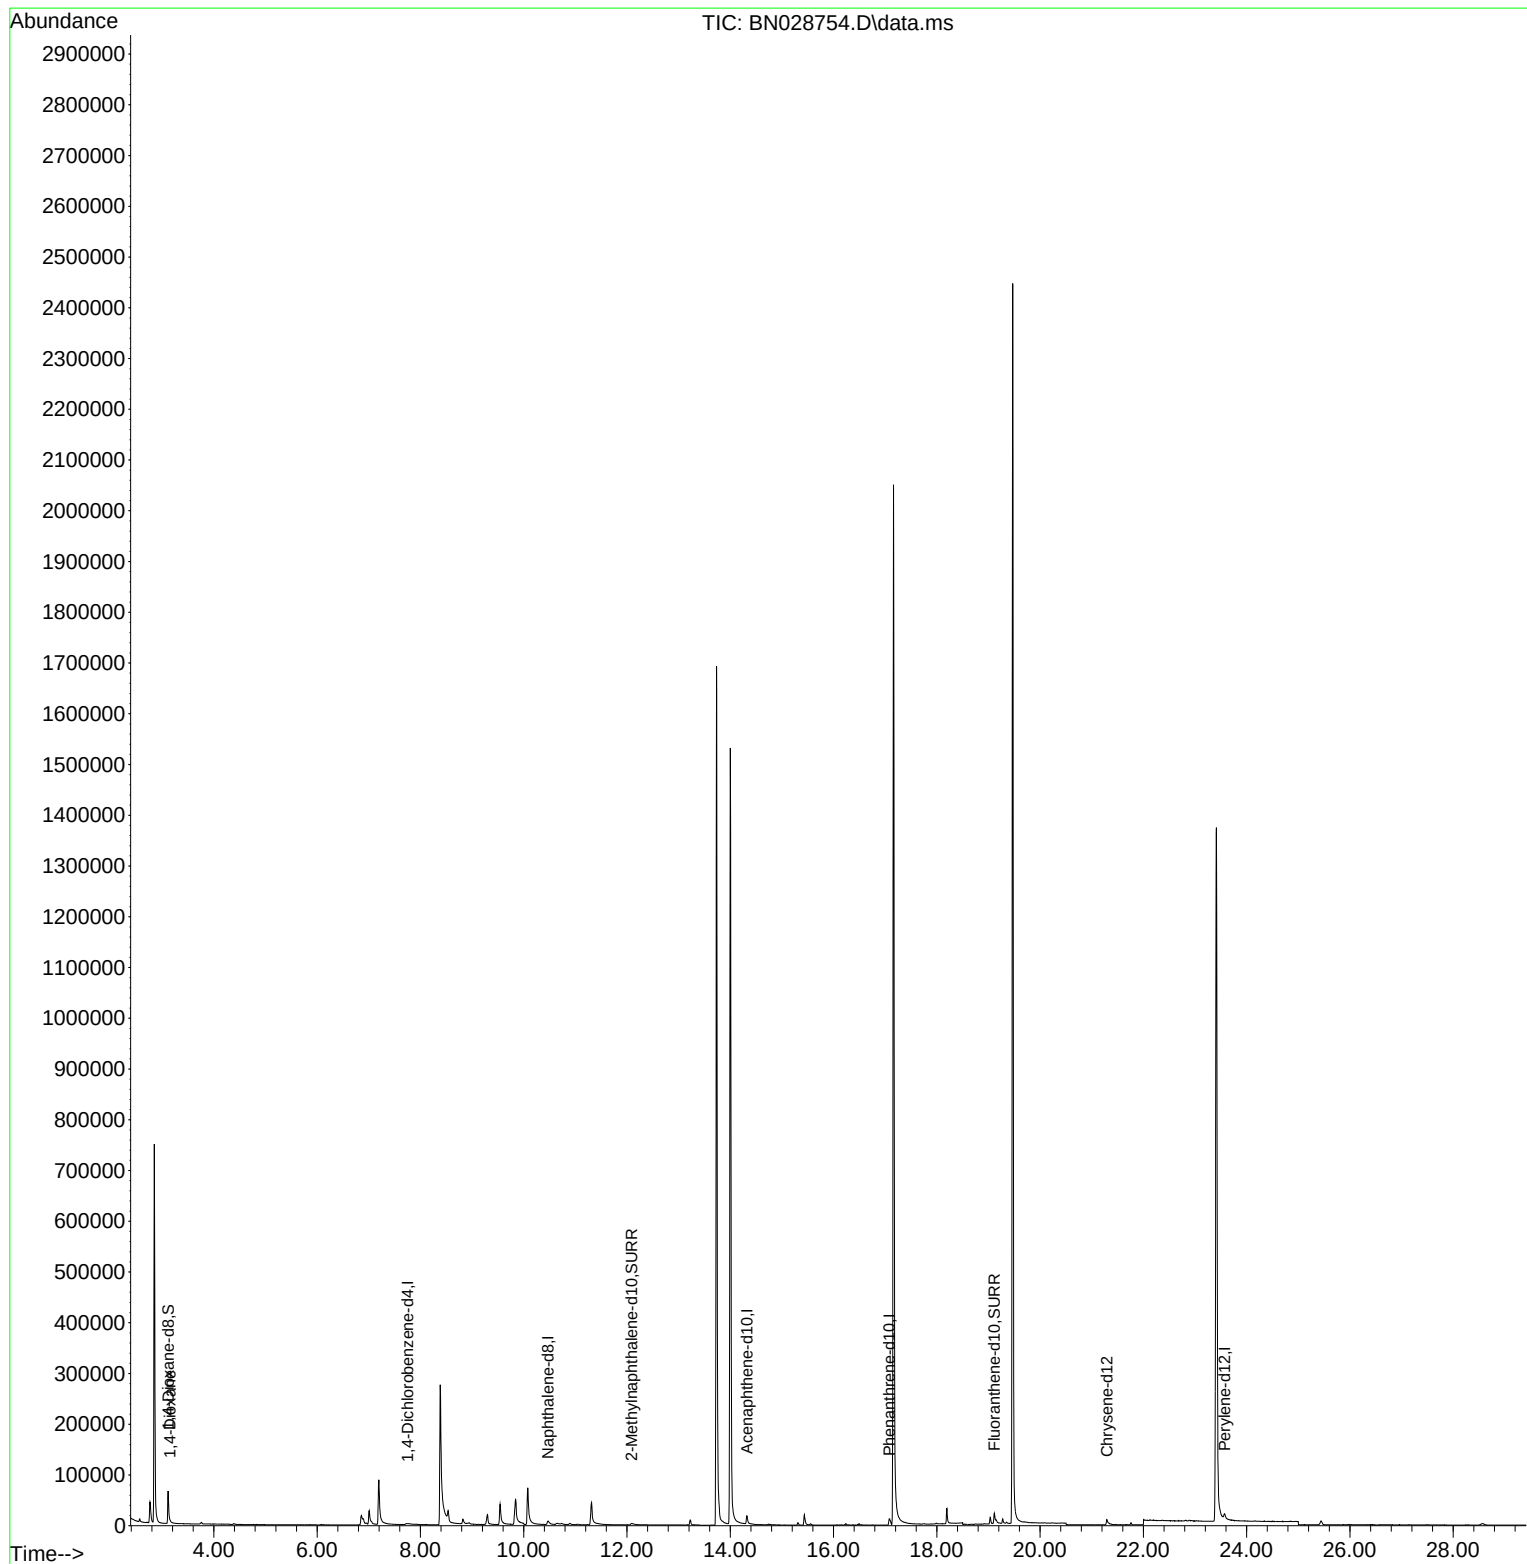

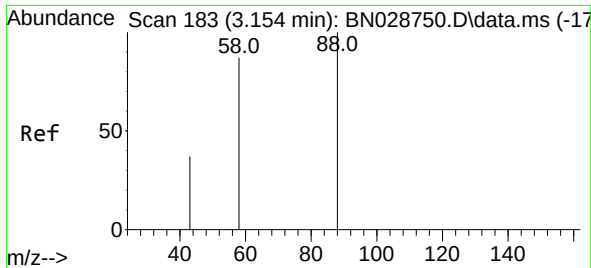

#2
1,4-Dioxane
Concen: 0.110 ng/ul
RT: 3.150 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN028754.D
Acq: 19 Nov 2023 00:53

Instrument :
BNA_N
ClientSampleId :
GCDQ0

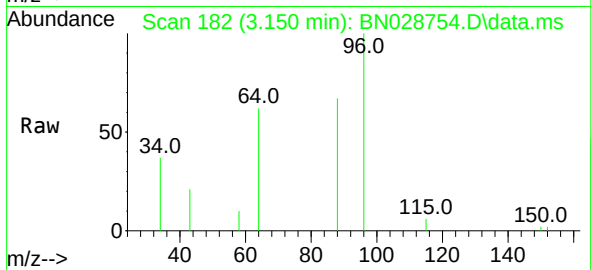

Tgt Ion: 88 Resp: 690
Ion Ratio Lower Upper
88 100
43 31.0 32.9 49.3
58 14.6 41.8 62.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

