

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028761.D
 Acq On : 19 Nov 2023 05:05
 Operator : MA/JU
 Sample : 05370-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDP7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 00:35:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.723	152	6040m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.473	136	23257m	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.320	164	13849m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.081	188	27731m	0.400	ng/ul	0.00
17) Chrysene-d12	21.292	240	21174m	0.400	ng/ul	0.00
23) Perylene-d12	23.569	264	27893m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	31048	4.651	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.107	152	8442m	0.241	ng/ul	0.00
18) Fluoranthene-d10	19.113	212	34692m	0.509	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.150	88	2182	0.296	ng/ul#	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028761.D
Acq On : 19 Nov 2023 05:05
Operator : MA/JU
Sample : 05370-01
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDP7

Quant Time: Nov 20 00:35:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

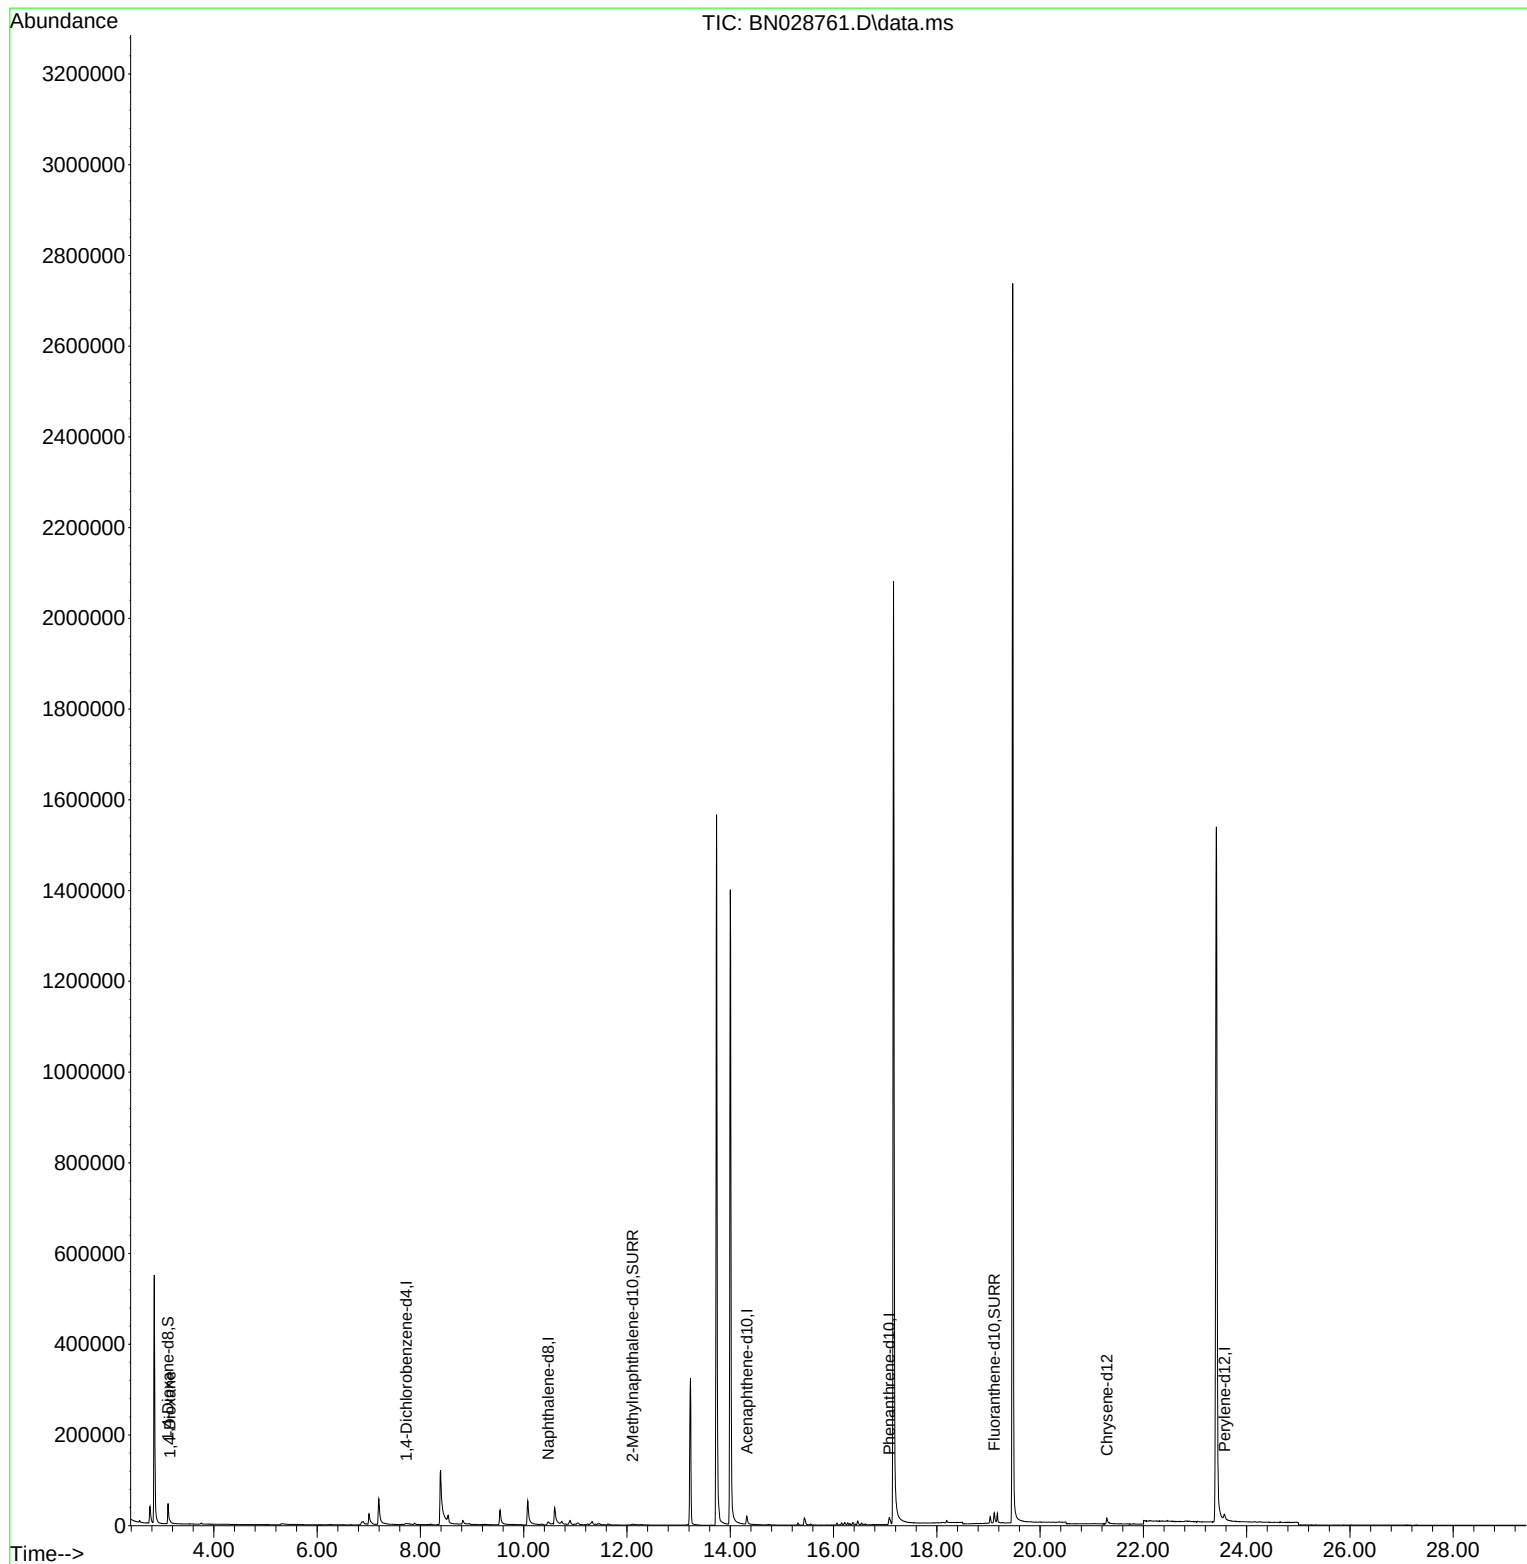

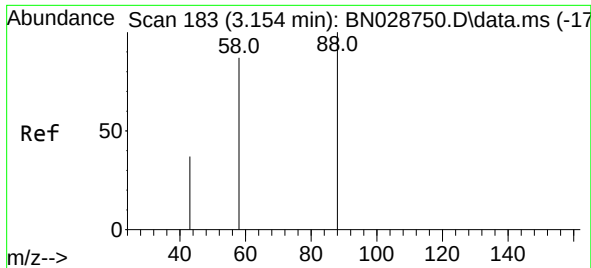

#2
1,4-Dioxane
Concen: 0.296 ng/ul
RT: 3.150 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN028761.D
Acq: 19 Nov 2023 05:05

Instrument :
BNA_N
ClientSampleId :
GCDP7

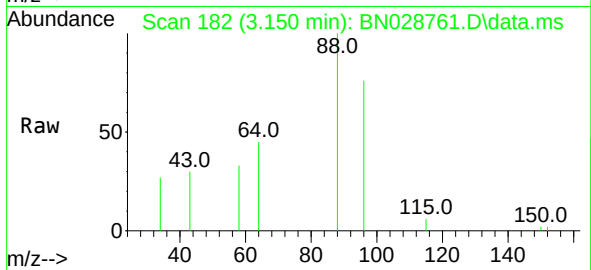

Tgt Ion: 88 Resp: 218
Ion Ratio Lower Upper
88 100
43 30.1 32.9 49.3
58 33.4 41.8 62.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

