

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028765.D
 Acq On : 19 Nov 2023 07:28
 Operator : MA/JU
 Sample : 05370-13
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDQ7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 01:09:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 09:39:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.727	152	5813m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.473	136	22970m	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.317	164	13478m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.078	188	24603m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.299	240	15868m	0.400	ng/ul	0.00
23) Perylene-d12	23.570	264	24873m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	39957	6.219	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.123	152	9416m	0.272	ng/ul	0.01
18) Fluoranthene-d10	19.113	212	30571m	0.599	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.154	88	680	0.096	ng/ul#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028765.D
Acq On : 19 Nov 2023 07:28
Operator : MA/JU
Sample : 05370-13
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDQ7

Quant Time: Nov 20 01:09:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 09:39:27 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

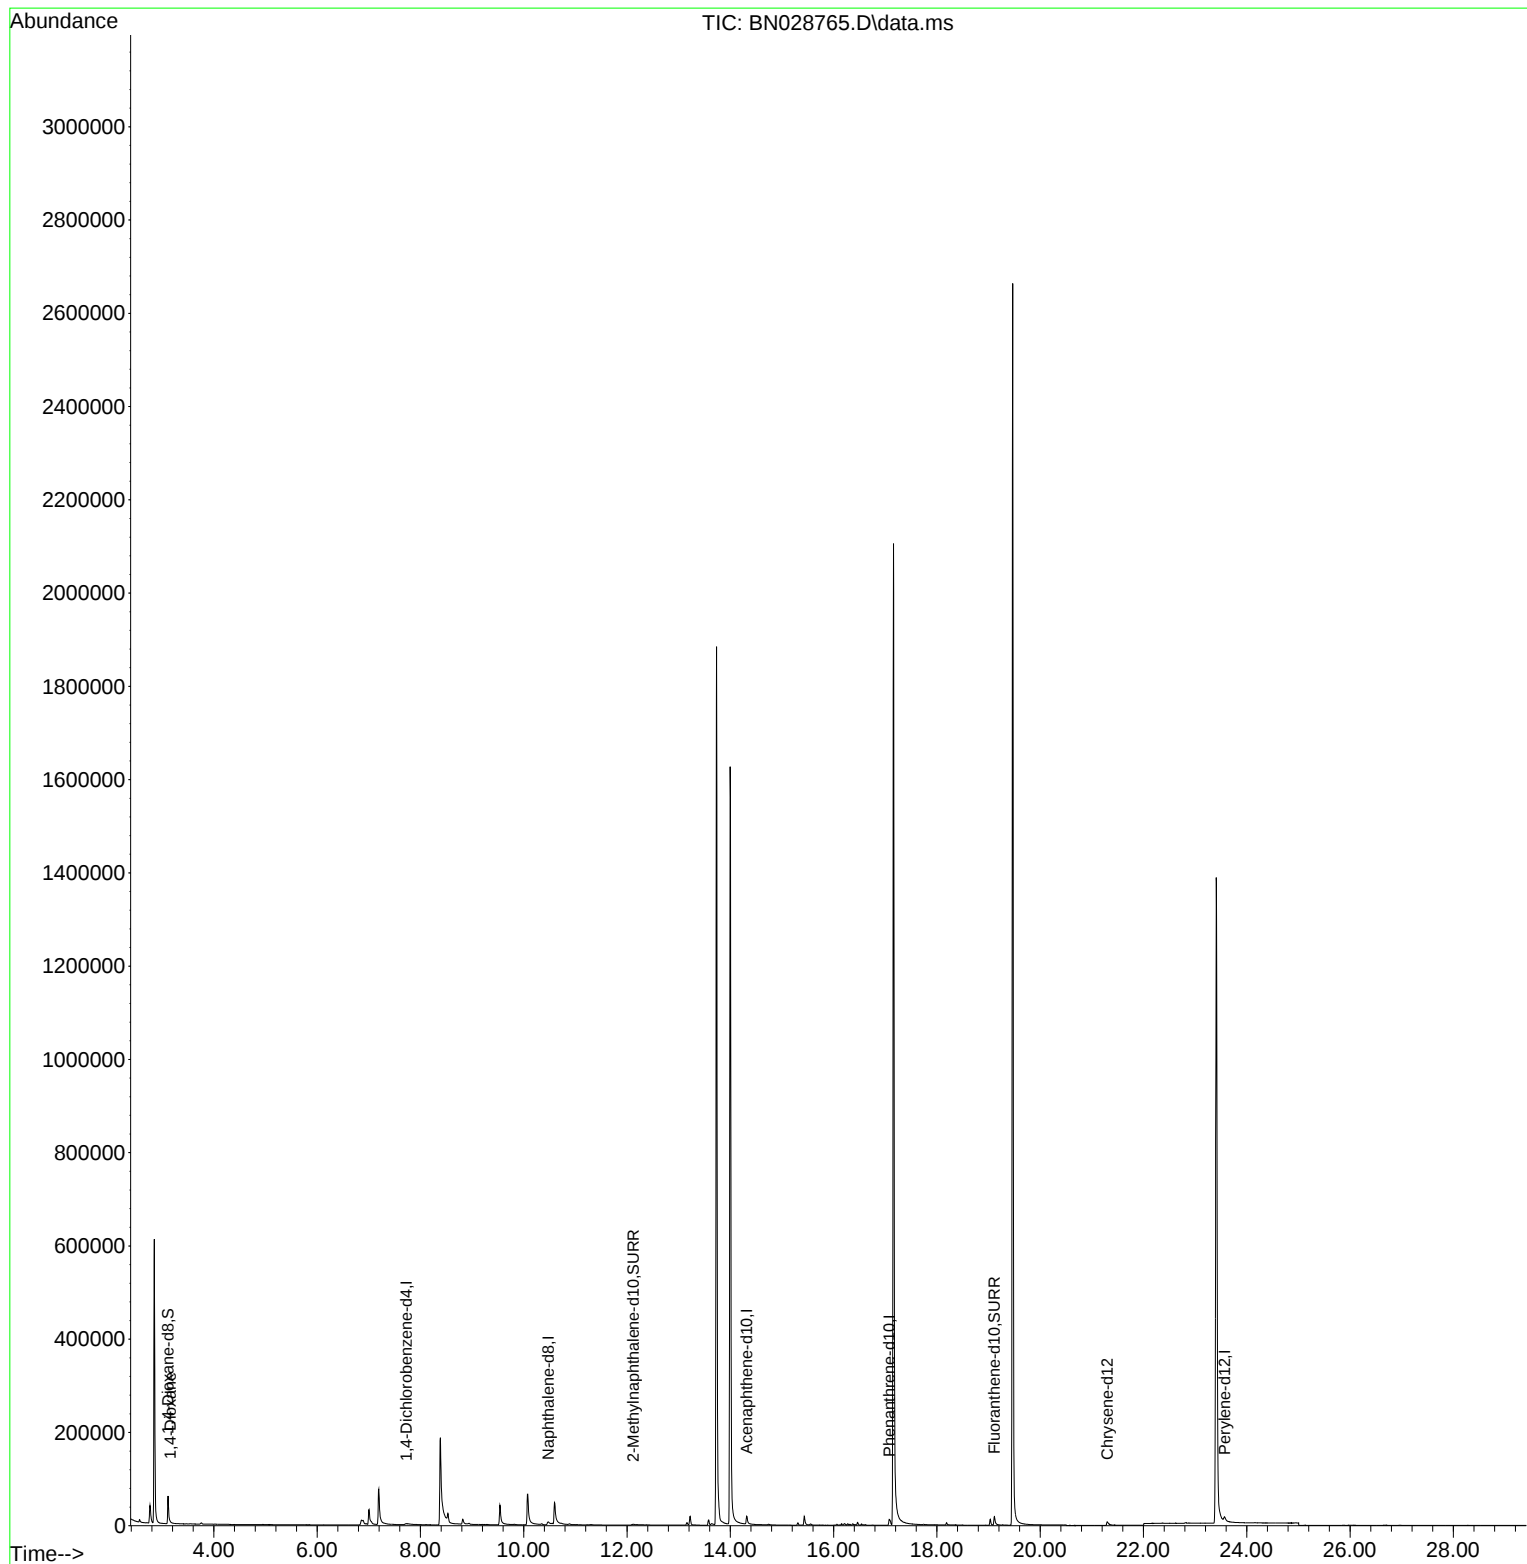

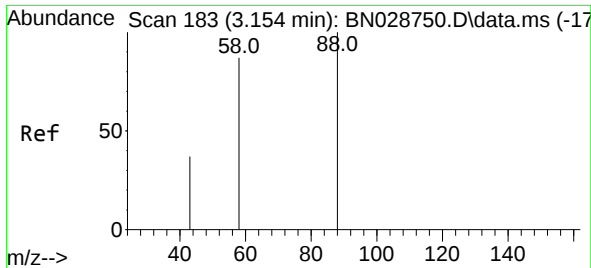

#2
1,4-Dioxane
Concen: 0.096 ng/ul
RT: 3.154 min Scan# 183
Delta R.T. -0.000 min
Lab File: BN028765.D
Acq: 19 Nov 2023 07:28

Instrument :
BNA_N
ClientSampleId :
GCDQ7

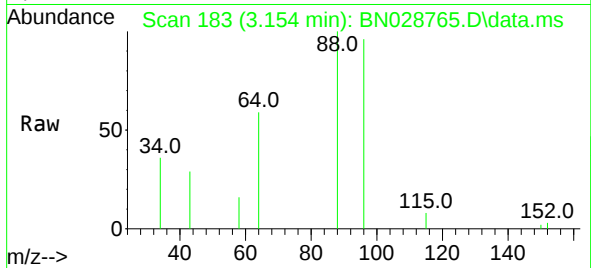

Tgt Ion: 88 Resp: 680
Ion Ratio Lower Upper
88 100
43 28.9 32.9 49.3
58 15.8 41.8 62.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

