

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
 Data File : BN028774.D
 Acq On : 19 Nov 2023 13:26
 Operator : MA/JU
 Sample : 05370-18
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDR2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :mohammad ahmed 11/20/2023

Quant Time: Nov 20 01:39:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 20 01:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	5609m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.479	136	20423m	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.321	164	12365m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.085	188	21576m	0.400	ng/ul	0.00
17) Chrysene-d12	21.298	240	14782m	0.400	ng/ul	0.00
23) Perylene-d12	23.569	264	19485m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	34641	5.588	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.118	152	7705m	0.251	ng/ul	0.00
18) Fluoranthene-d10	19.113	212	28170m	0.592	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.146	88	19637	2.866	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028774.D
Acq On : 19 Nov 2023 13:26
Operator : MA/JU
Sample : 05370-18
Misc :
ALS Vial : 76 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GCDR2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023


Quant Time: Nov 20 01:39:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 20 01:23:26 2023
Response via : Initial Calibration

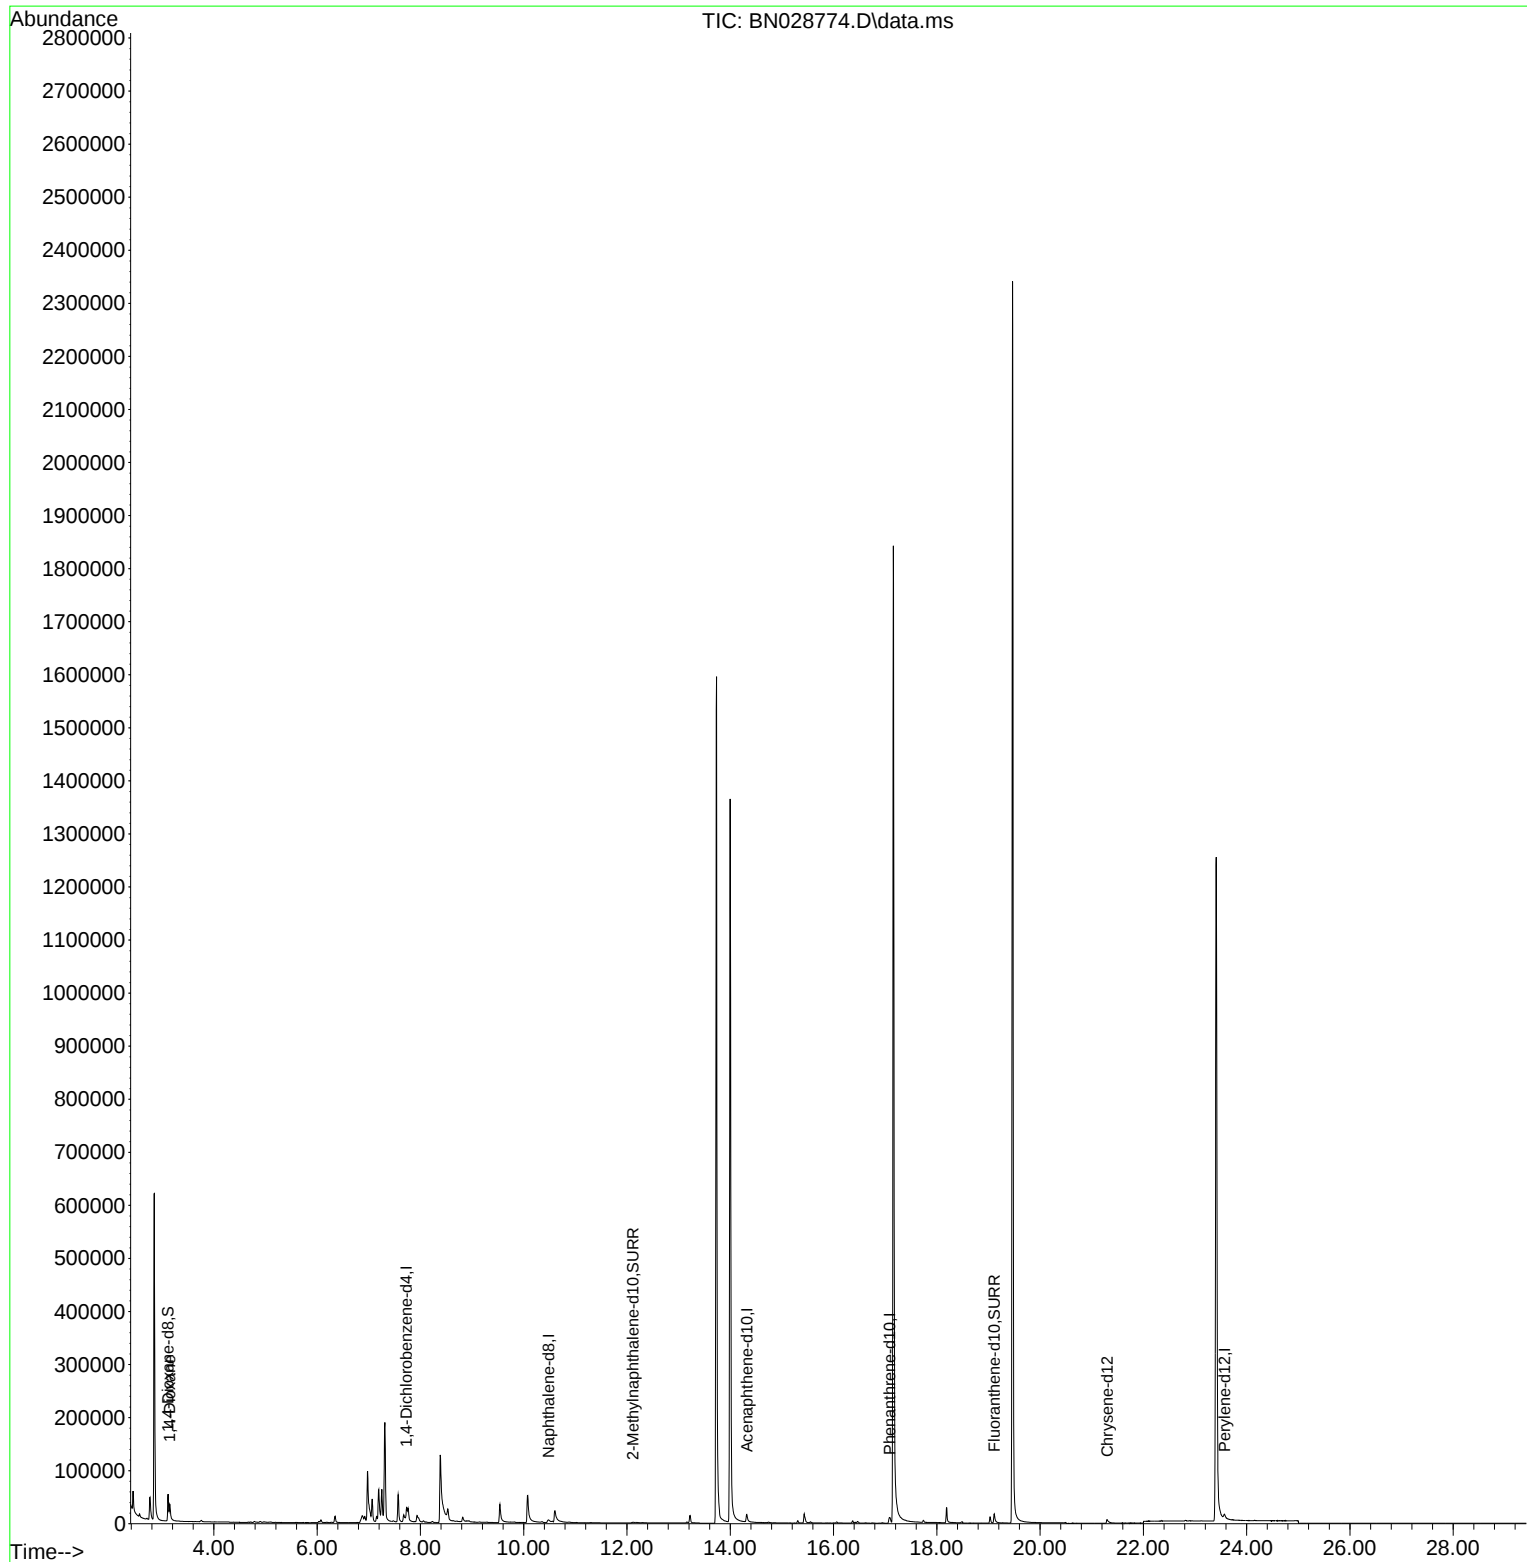

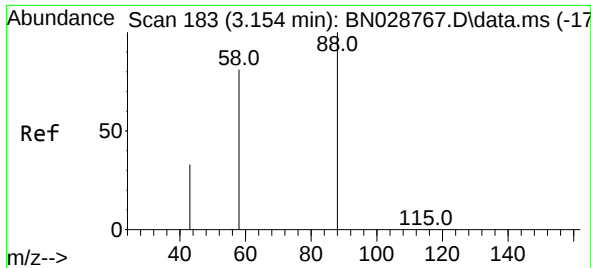

#2
1,4-Dioxane
Concen: 2.866 ng/ul
RT: 3.146 min Scan# 11
Delta R.T. -0.008 min
Lab File: BN028774.D
Acq: 19 Nov 2023 13:26

Instrument :
BNA_N
ClientSampleId :
GCDR2

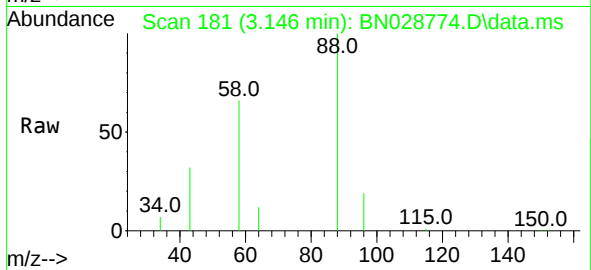

Tgt Ion: 88 Resp: 1963
Ion Ratio Lower Upper
88 100
43 32.1 32.9 49.3
58 65.8 41.8 62.8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :mohammad ahmed 11/20/2023

