




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035117.D
Acq On : 15 Nov 2024 22:24
Operator : RC/JU
Sample : P4715-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:55:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

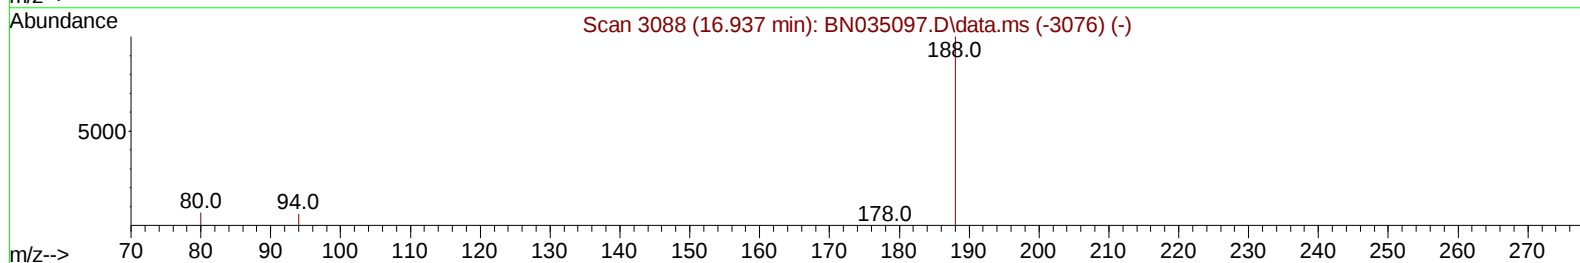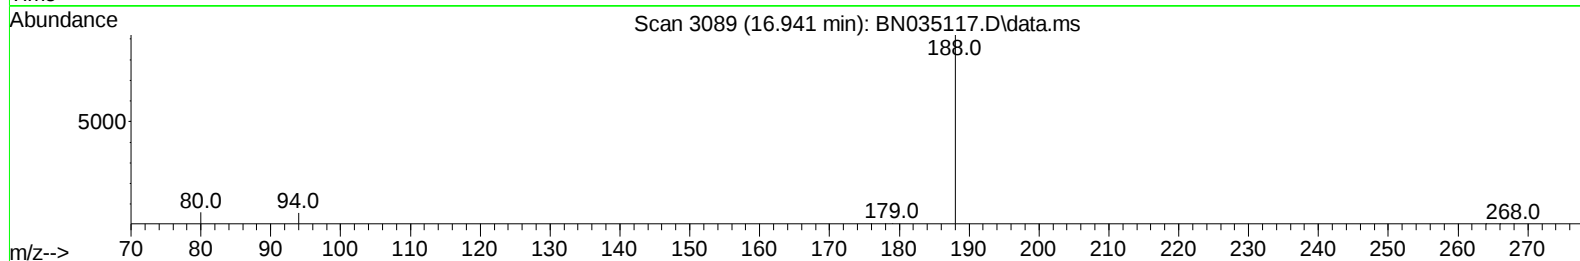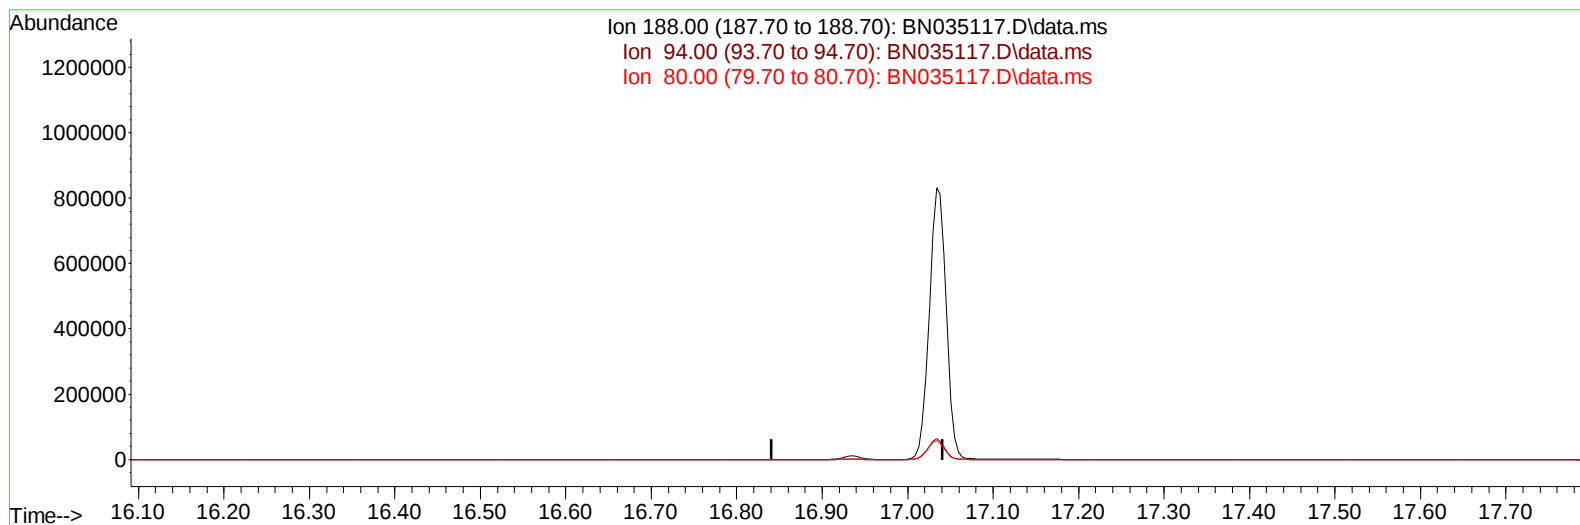

TIC: BN035117.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.10	0.00#
80.00	7.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035117.D
Acq On : 15 Nov 2024 22:24
Operator : RC/JU
Sample : P4715-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:55:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

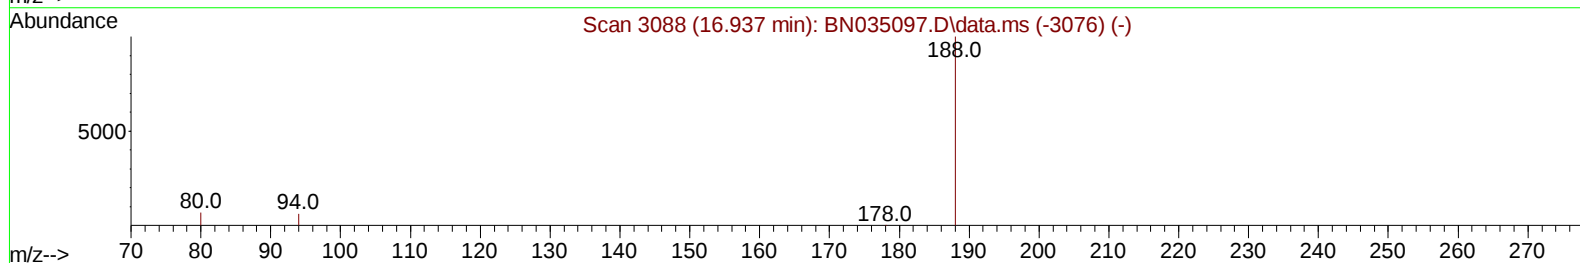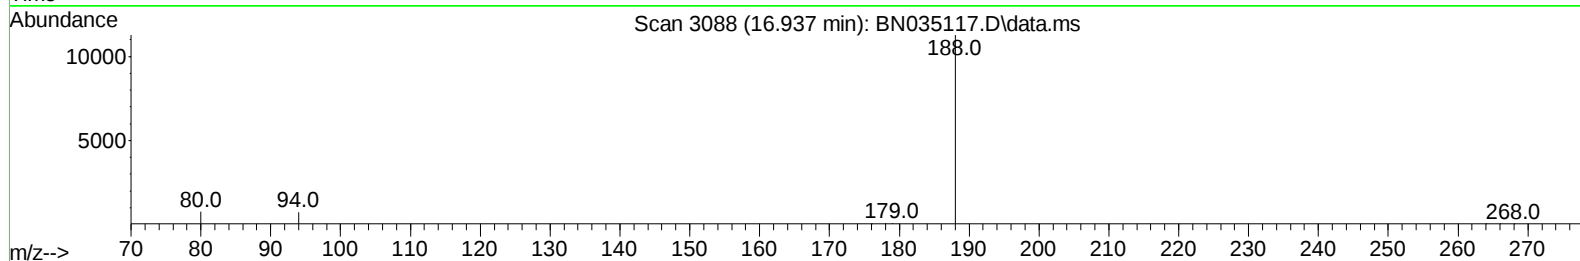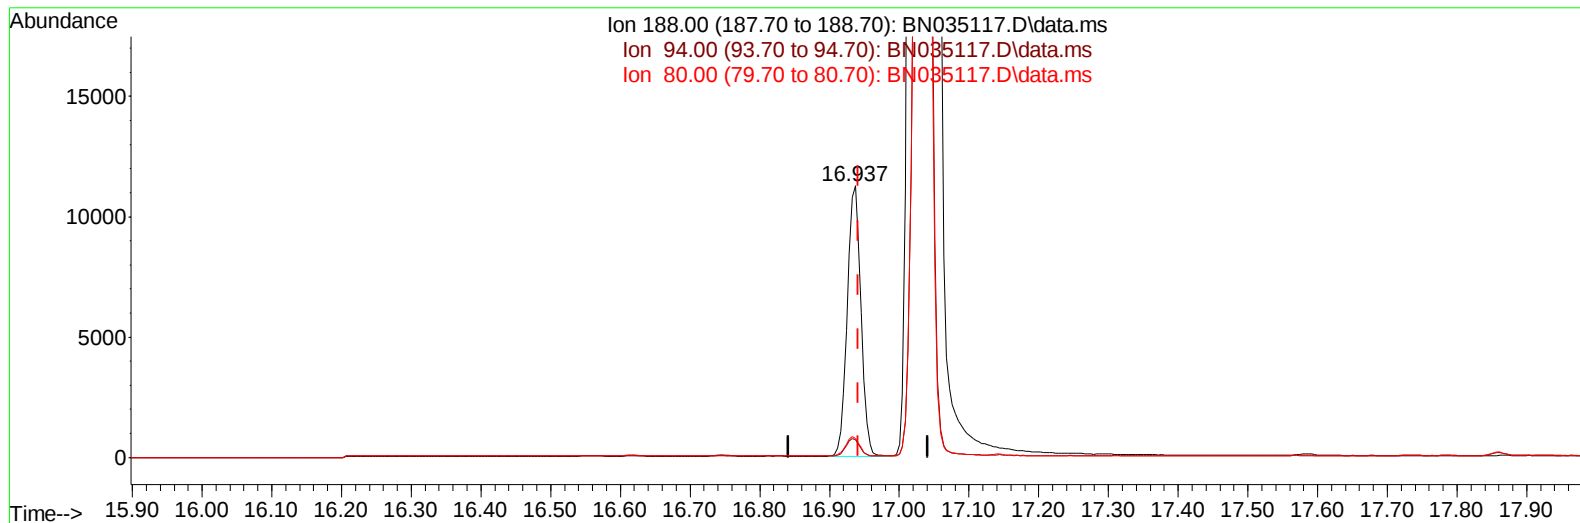

TIC: BN035117.D\data.ms

(13) Phenanthrene-d10 (I)

16.937min (-0.004) 0.40 ng/u1 m

response 15320

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.10	6.55
80.00	7.00	6.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035117.D
Acq On : 15 Nov 2024 22:24
Operator : RC/JU
Sample : P4715-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 22:55:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

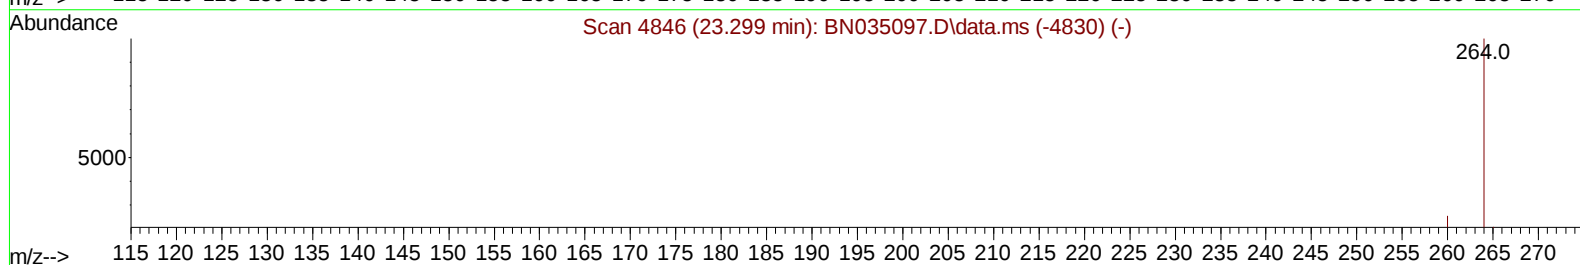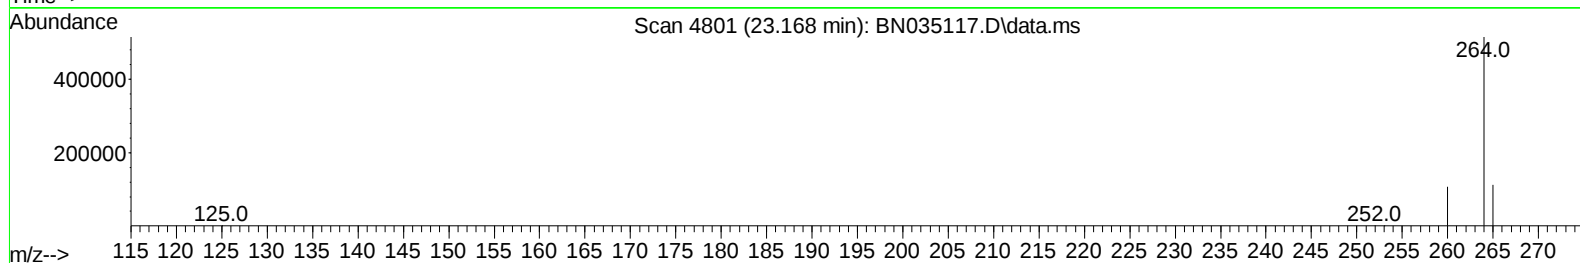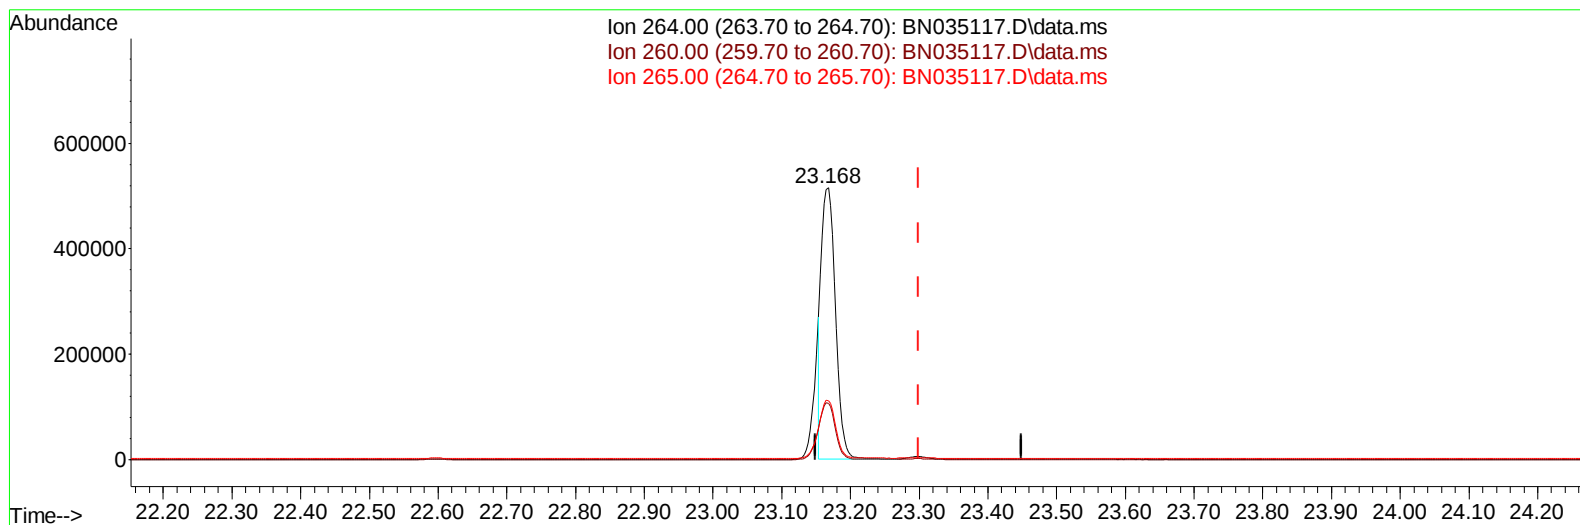

TIC: BN035117.D\data.ms

(23) Perylene-d12 (I)

23.168min (-0.132) 0.40 ng/u1

response 741792

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	20.72#
265.00	52.80	21.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035117.D
Acq On : 15 Nov 2024 22:24
Operator : RC/JU
Sample : P4715-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:55:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

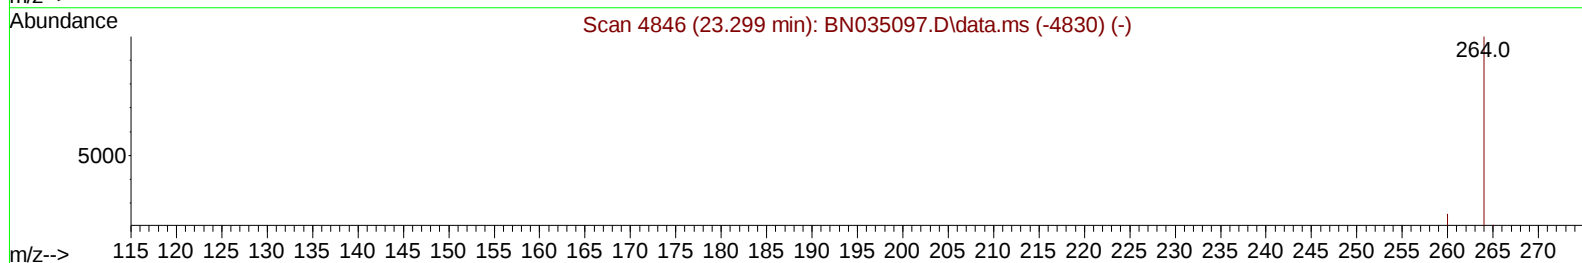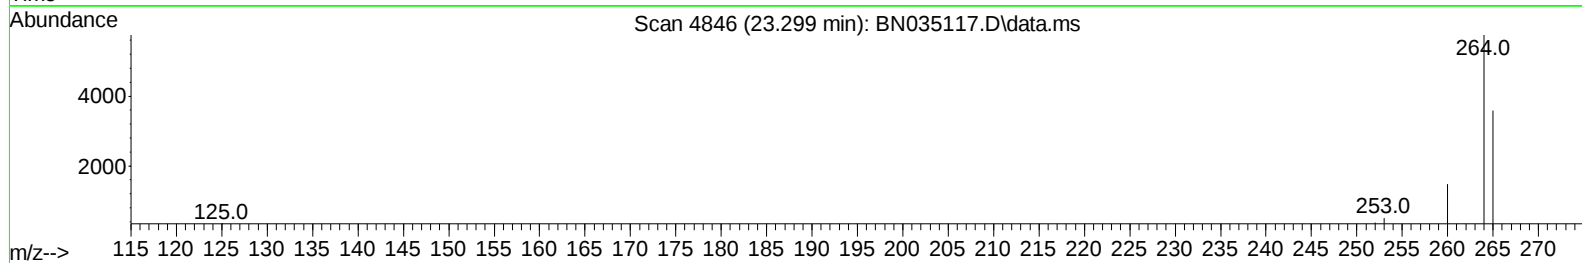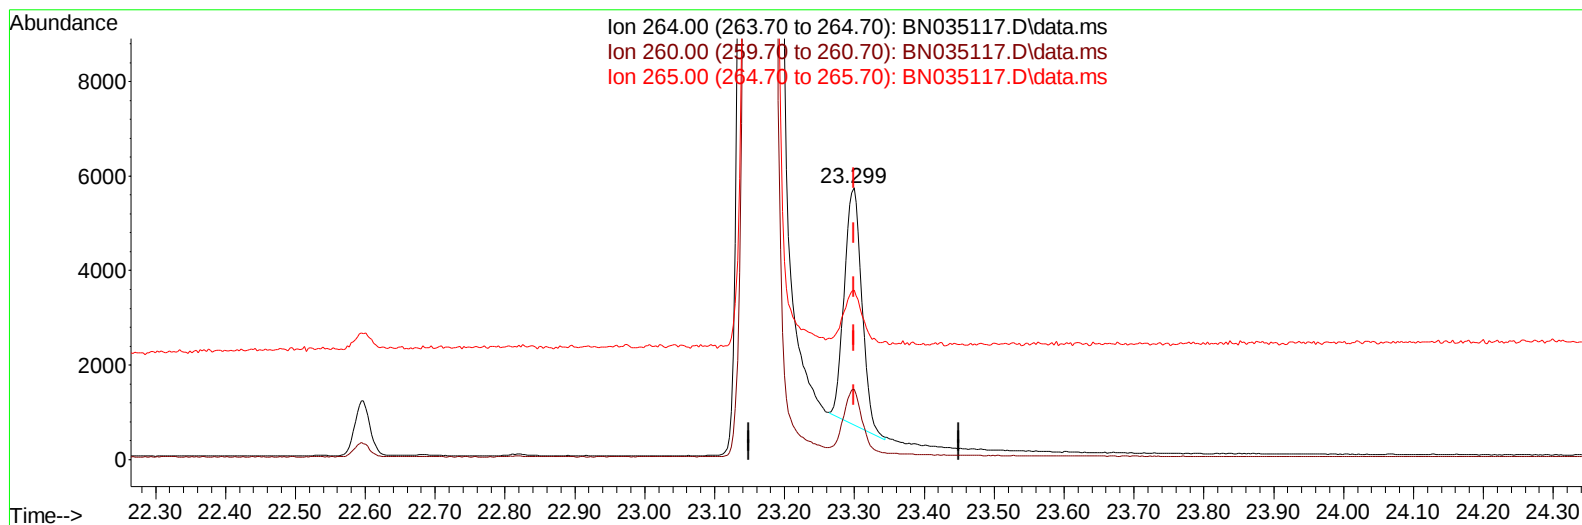

TIC: BN035117.D\data.ms

(23) Perylene-d12 (I)

23.299min (-0.000) 0.40 ng/ul m

response 8720

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	25.72
265.00	52.80	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
 Data File : BN035117.D
 Acq On : 15 Nov 2024 22:24
 Operator : RC/JU
 Sample : P4715-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 22:55:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 00:41:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.550	152	3045	0.400	ng/ul	0.00
4) Naphthalene-d8	10.311	136	8196	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.185	164	6687	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	15320m	0.400	ng/ul	0.00
17) Chrysene-d12	21.134	240	10483	0.400	ng/ul	# 0.00
23) Perylene-d12	23.299	264	8720m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	13716	4.734	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.906	152	3628	0.289	ng/ul	-0.01
18) Fluoranthene-d10	18.972	212	13763	0.511	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035117.D
Acq On : 15 Nov 2024 22:24
Operator : RC/JU
Sample : P4715-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:55:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

