




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035123.D
Acq On : 16 Nov 2024 02:01
Operator : RC/JU
Sample : P4715-15
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 02:31:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

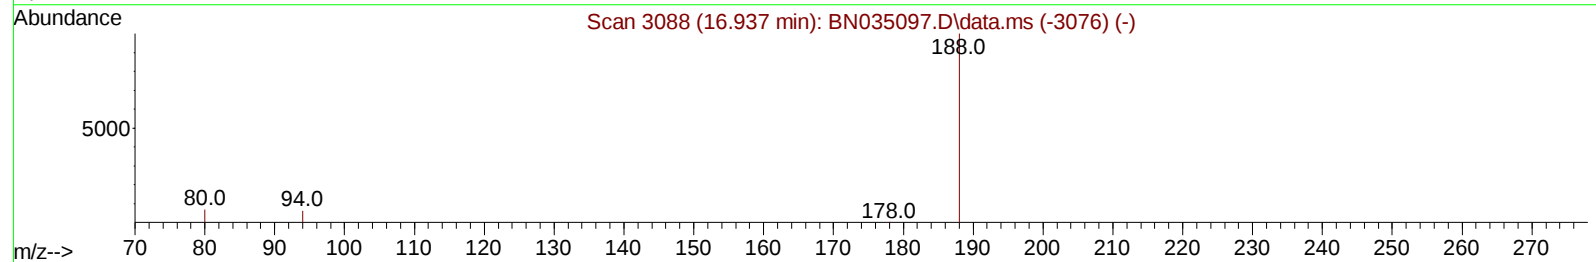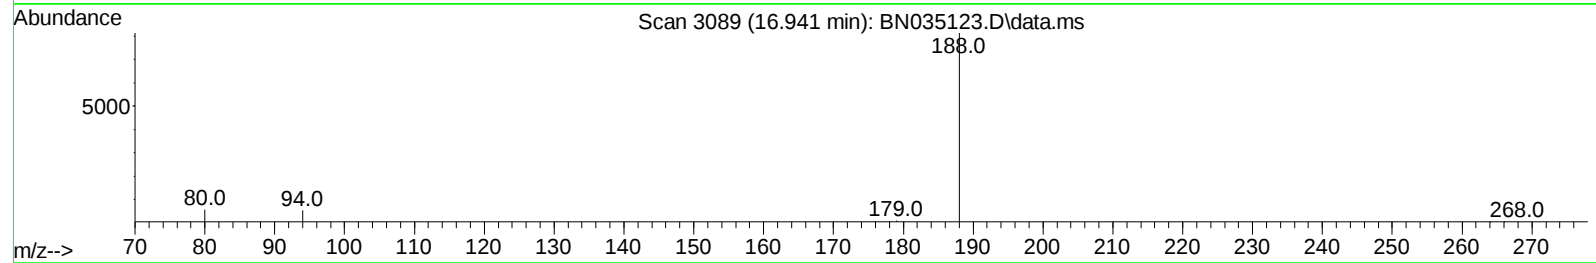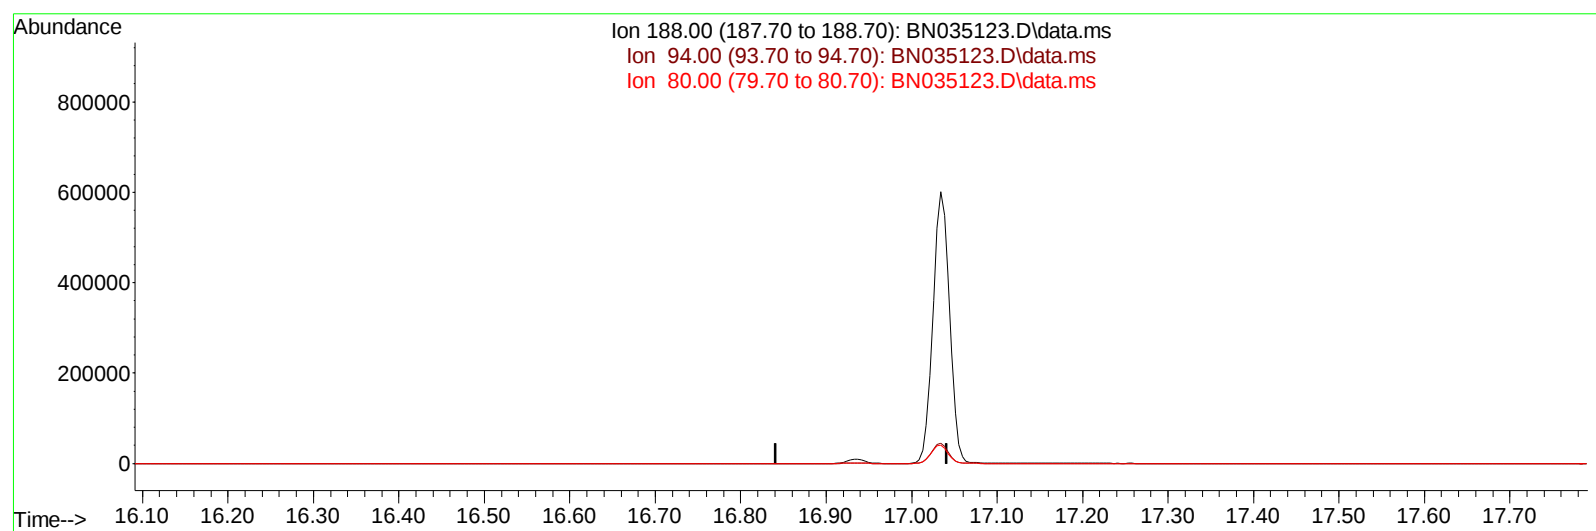

TIC: BN035123.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.10	0.00#
80.00	7.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035123.D
Acq On : 16 Nov 2024 02:01
Operator : RC/JU
Sample : P4715-15
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAL3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 02:31:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

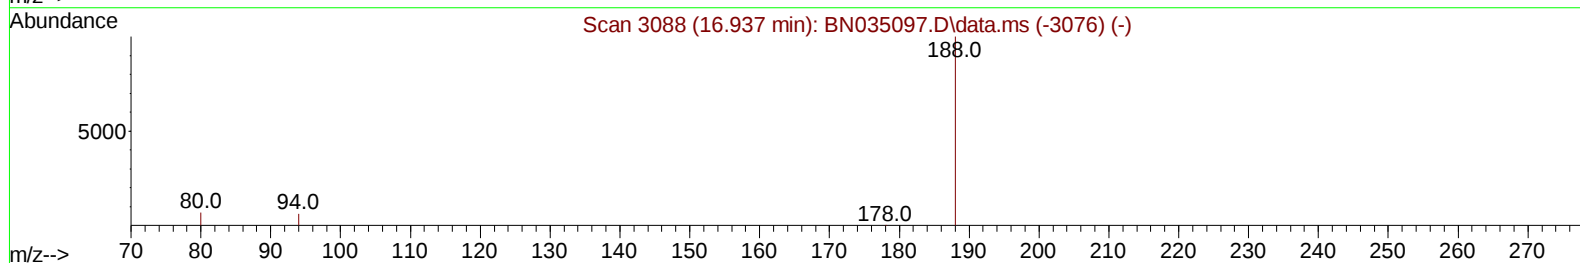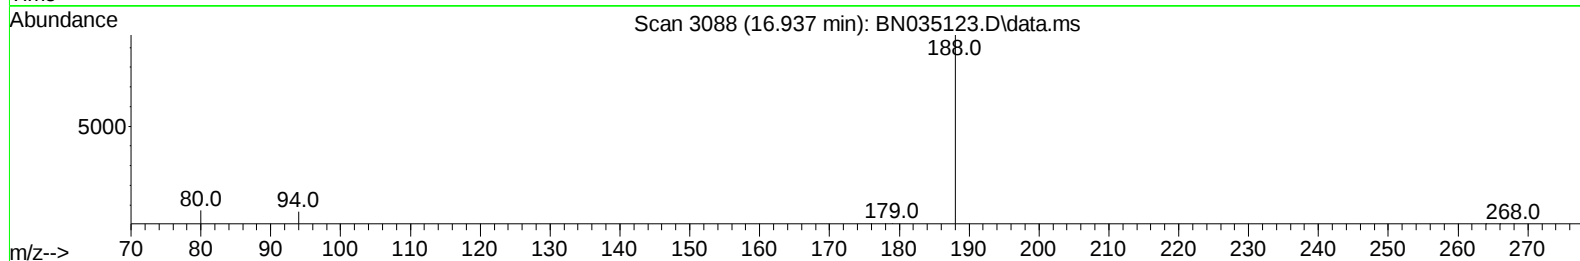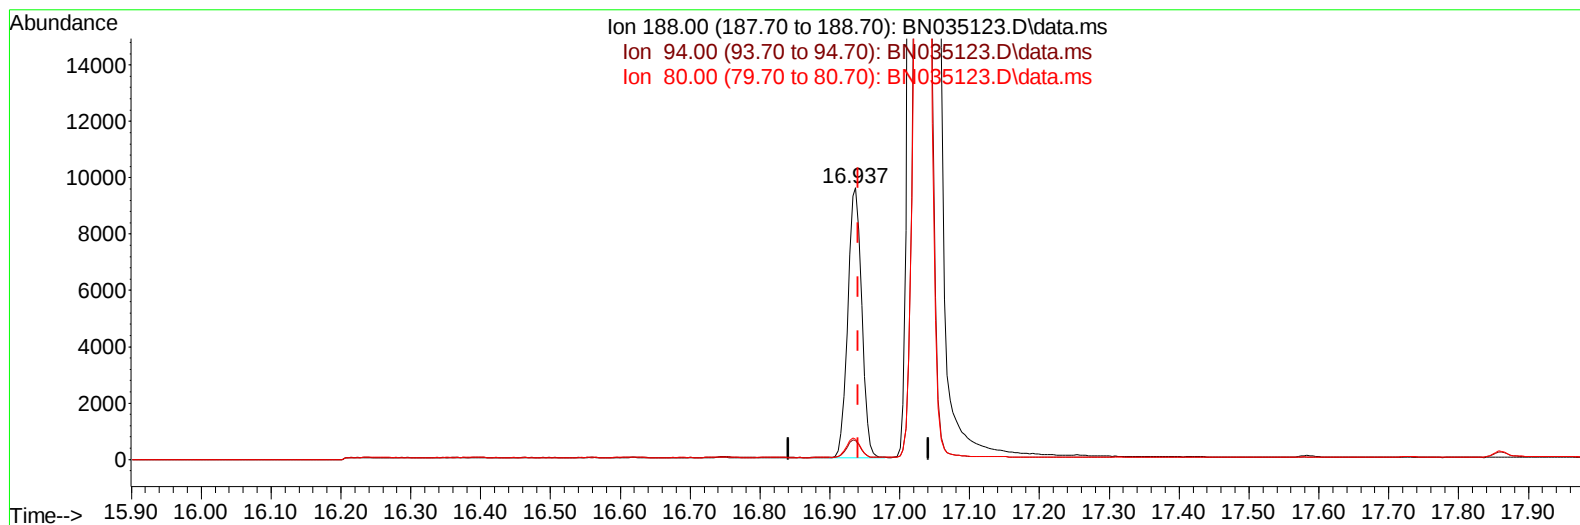

TIC: BN035123.D\data.ms

(13) Phenanthrene-d10 (I)

16.937min (-0.004) 0.40 ng/u1 m

response 13250

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.10	7.03
80.00	7.00	7.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035123.D
Acq On : 16 Nov 2024 02:01
Operator : RC/JU
Sample : P4715-15
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 02:31:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

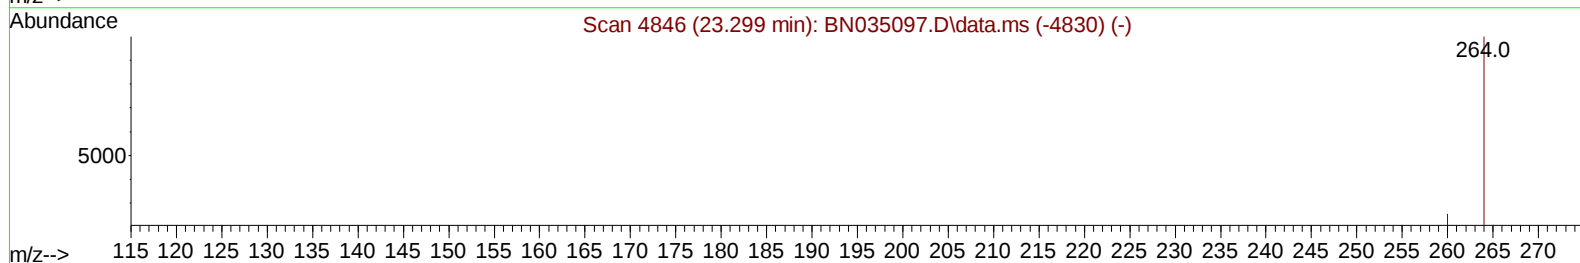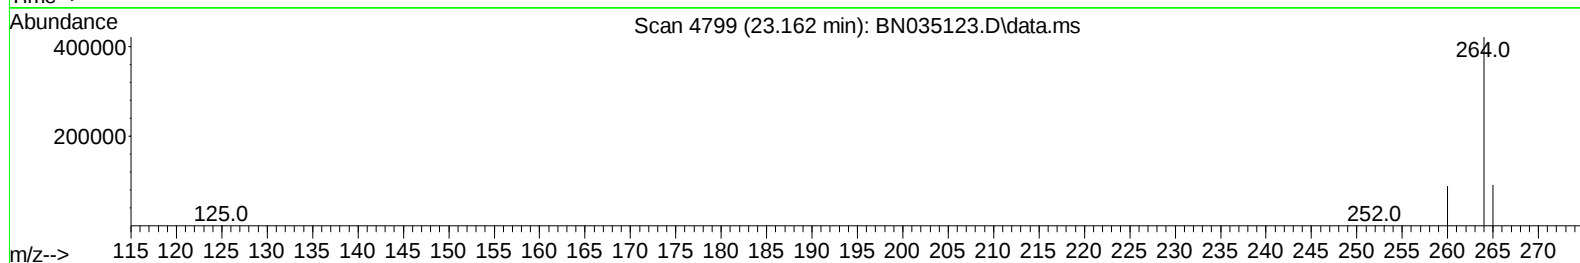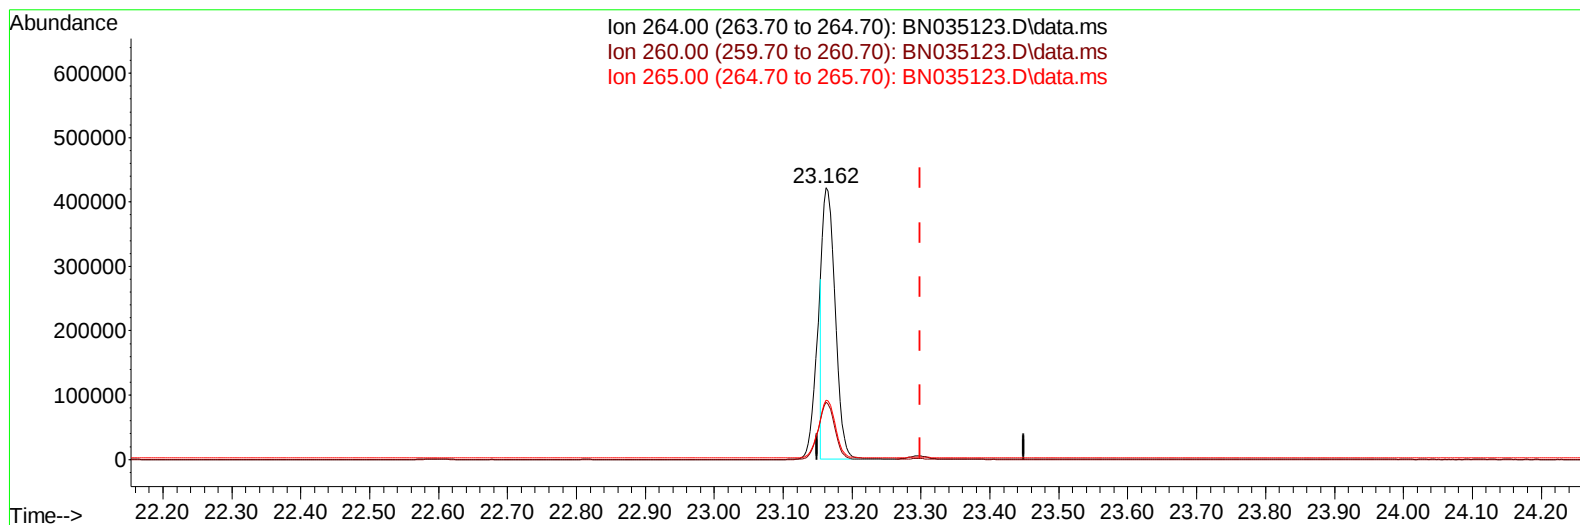

TIC: BN035123.D\data.ms

(23) Perylene-d12 (I)

23.162min (-0.137) 0.40 ng/u1

response 546675

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	21.02#
265.00	52.80	21.81#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035123.D
Acq On : 16 Nov 2024 02:01
Operator : RC/JU
Sample : P4715-15
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 02:31:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

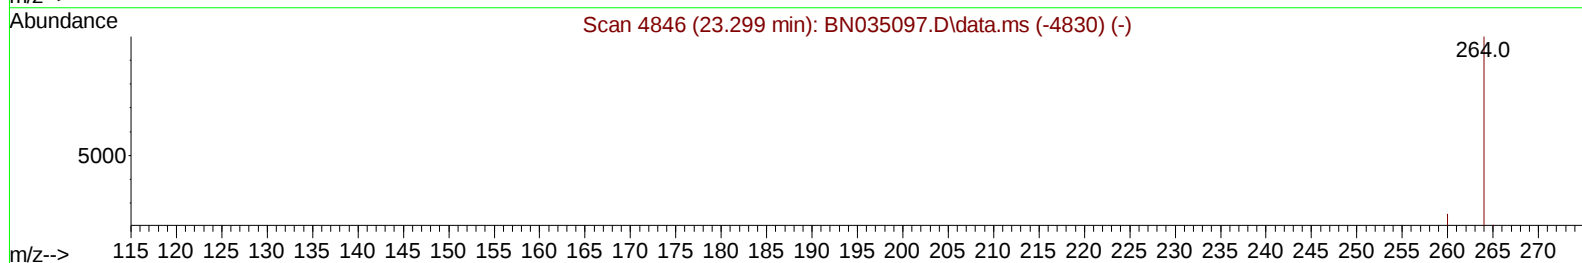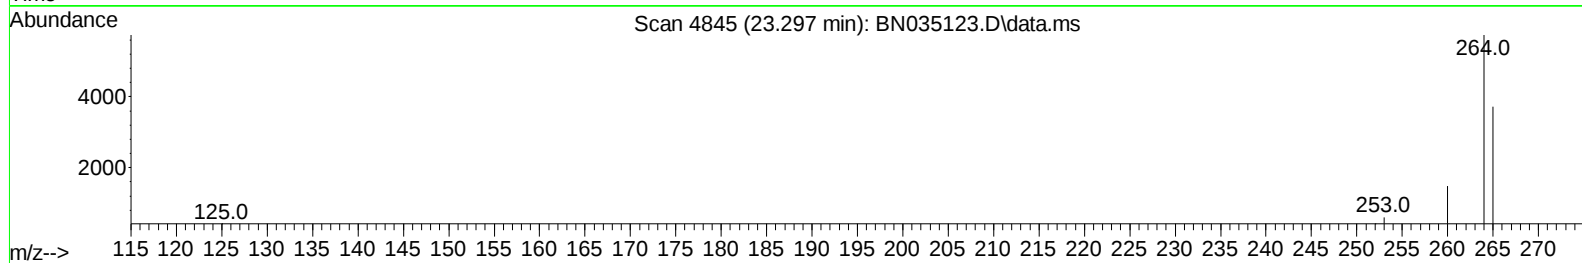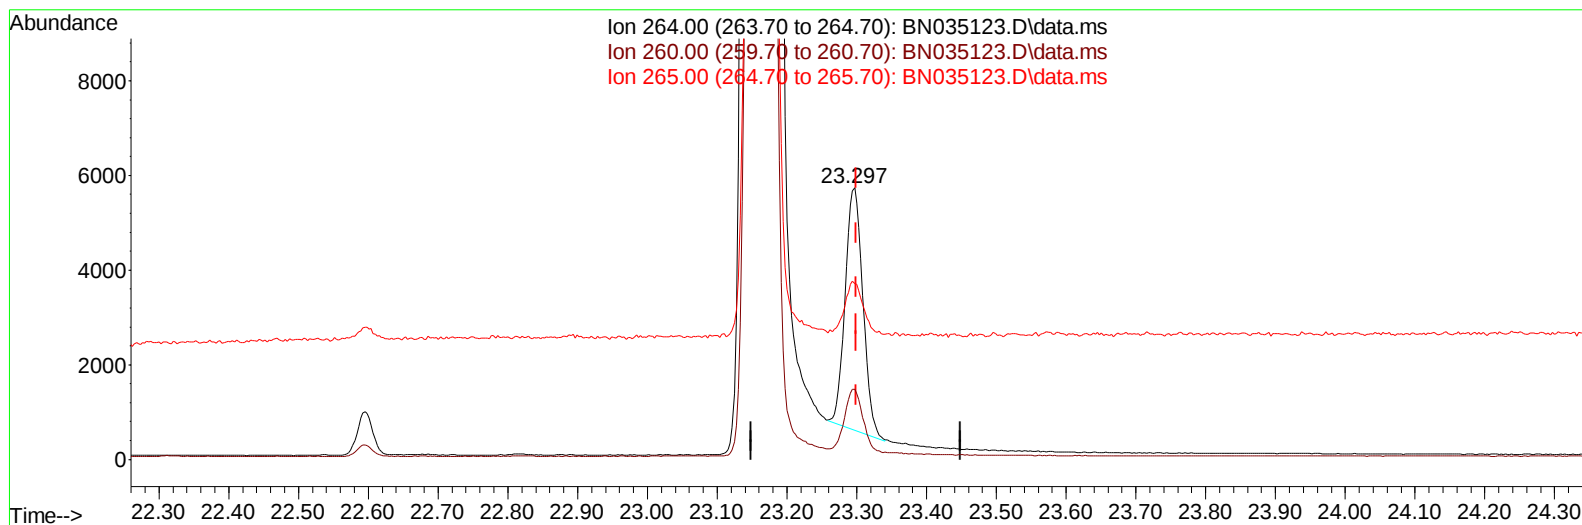

TIC: BN035123.D\data.ms

(23) Perylene-d12 (I)

23.297min (-0.003) 0.40 ng/ul m

response 9026

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	25.92
265.00	52.80	64.82#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
 Data File : BN035123.D
 Acq On : 16 Nov 2024 02:01
 Operator : RC/JU
 Sample : P4715-15
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 16 02:31:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 00:41:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.550	152	2914	0.400	ng/ul	0.00
4) Naphthalene-d8	10.312	136	7851	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.185	164	6251	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	13250m	0.400	ng/ul	0.00
17) Chrysene-d12	21.134	240	9341	0.400	ng/ul	# 0.00
23) Perylene-d12	23.297	264	9026m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	13963	5.036	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.906	152	3165	0.263	ng/ul	-0.01
18) Fluoranthene-d10	18.968	212	9190	0.383	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035123.D
Acq On : 16 Nov 2024 02:01
Operator : RC/JU
Sample : P4715-15
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 02:31:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

