

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
 Data File : BN035103.D
 Acq On : 15 Nov 2024 13:24
 Operator : RC/JU
 Sample : P4715-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 14:08:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 00:41:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.550	152	2714	0.400	ng/ul	0.00
4) Naphthalene-d8	10.311	136	6963	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.189	164	5198	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	10932m	0.400	ng/ul	0.00
17) Chrysene-d12	21.134	240	8609	0.400	ng/ul	# 0.00
23) Perylene-d12	23.302	264	8426m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	14075	5.450	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.912	152	3902	0.366	ng/ul	0.00
18) Fluoranthene-d10	18.972	212	10937	0.495	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.361	128	1005	0.058	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035103.D
Acq On : 15 Nov 2024 13:24
Operator : RC/JU
Sample : P4715-07
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AL7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024


Quant Time: Nov 15 14:08:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

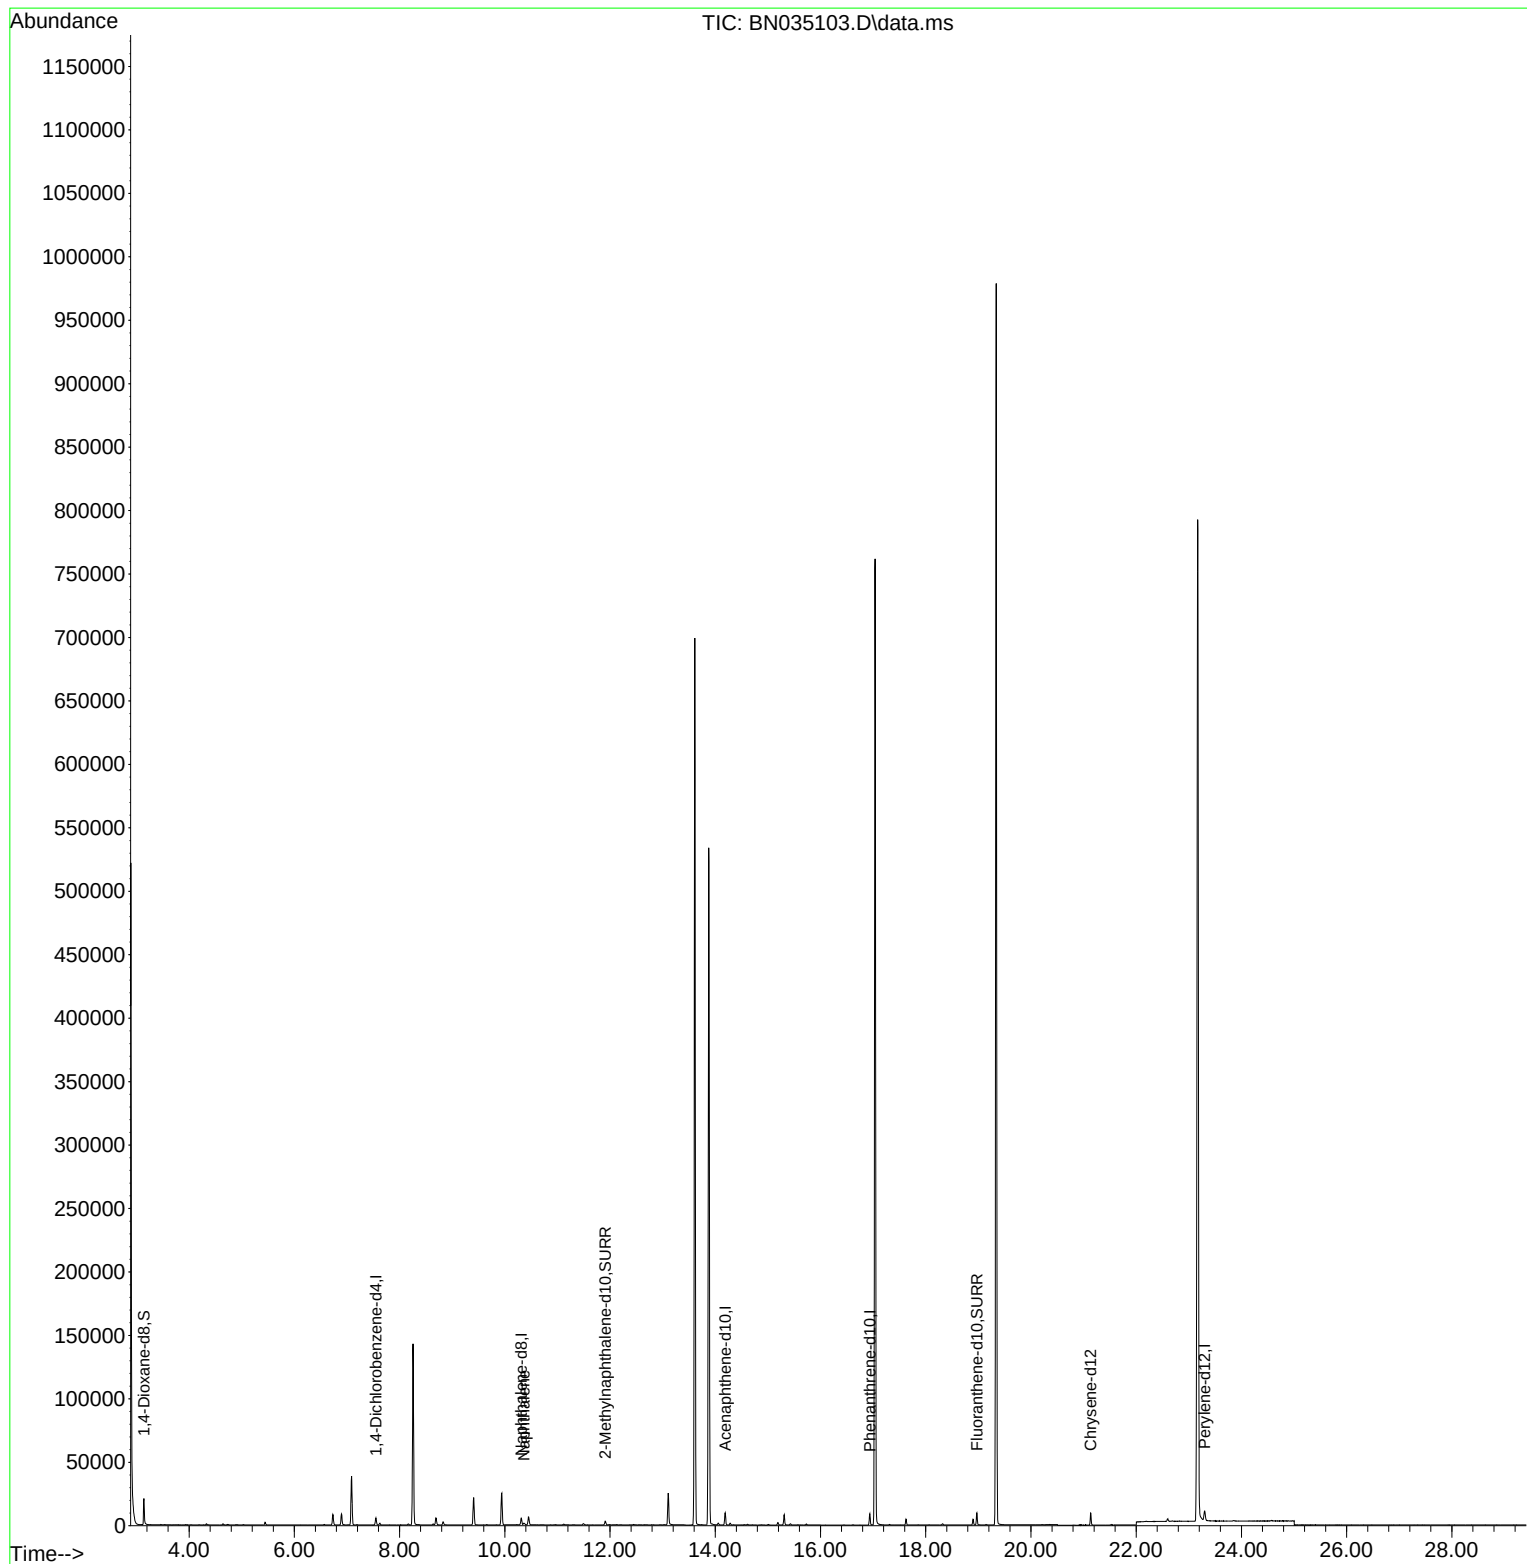

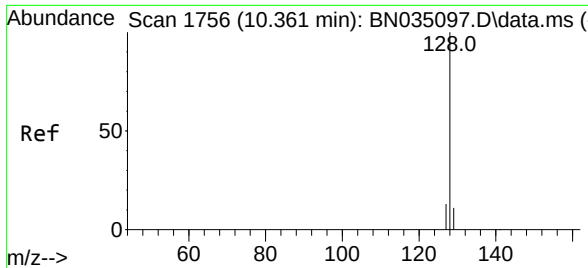

#5
Naphthalene
Concen: 0.058 ng/ul
RT: 10.361 min Scan# 1756
Delta R.T. -0.011 min
Lab File: BN035103.D
Acq: 15 Nov 2024 13:24

Instrument :
BNA_N
ClientSampleId :
C0AL7

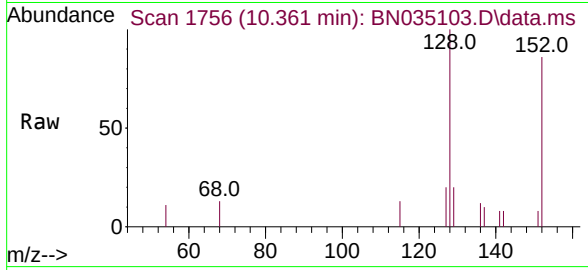

Tgt Ion:128 Resp: 100%

Ion	Ratio	Lower	Upper
128	100		
129	19.7	10.1	15.1
127	19.7	12.1	18.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

