

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
 Data File : BN035104.D
 Acq On : 15 Nov 2024 14:00
 Operator : RC/JU
 Sample : P4715-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAM0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 15:04:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 00:41:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.550	152	3294	0.400	ng/u1	0.00
4) Naphthalene-d8	10.311	136	8984	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.189	164	7062	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.937	188	15789m	0.400	ng/u1	0.00
17) Chrysene-d12	21.137	240	10890	0.400	ng/u1	# 0.00
23) Perylene-d12	23.305	264	9857m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	16145	5.151	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.912	152	4903	0.356	ng/u1	0.00
18) Fluoranthene-d10	18.972	212	14674	0.525	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.591	266	27557	7.549	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111524\
Data File : BN035104.D
Acq On : 15 Nov 2024 14:00
Operator : RC/JU
Sample : P4715-09
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
COAM0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024


Quant Time: Nov 15 15:04:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

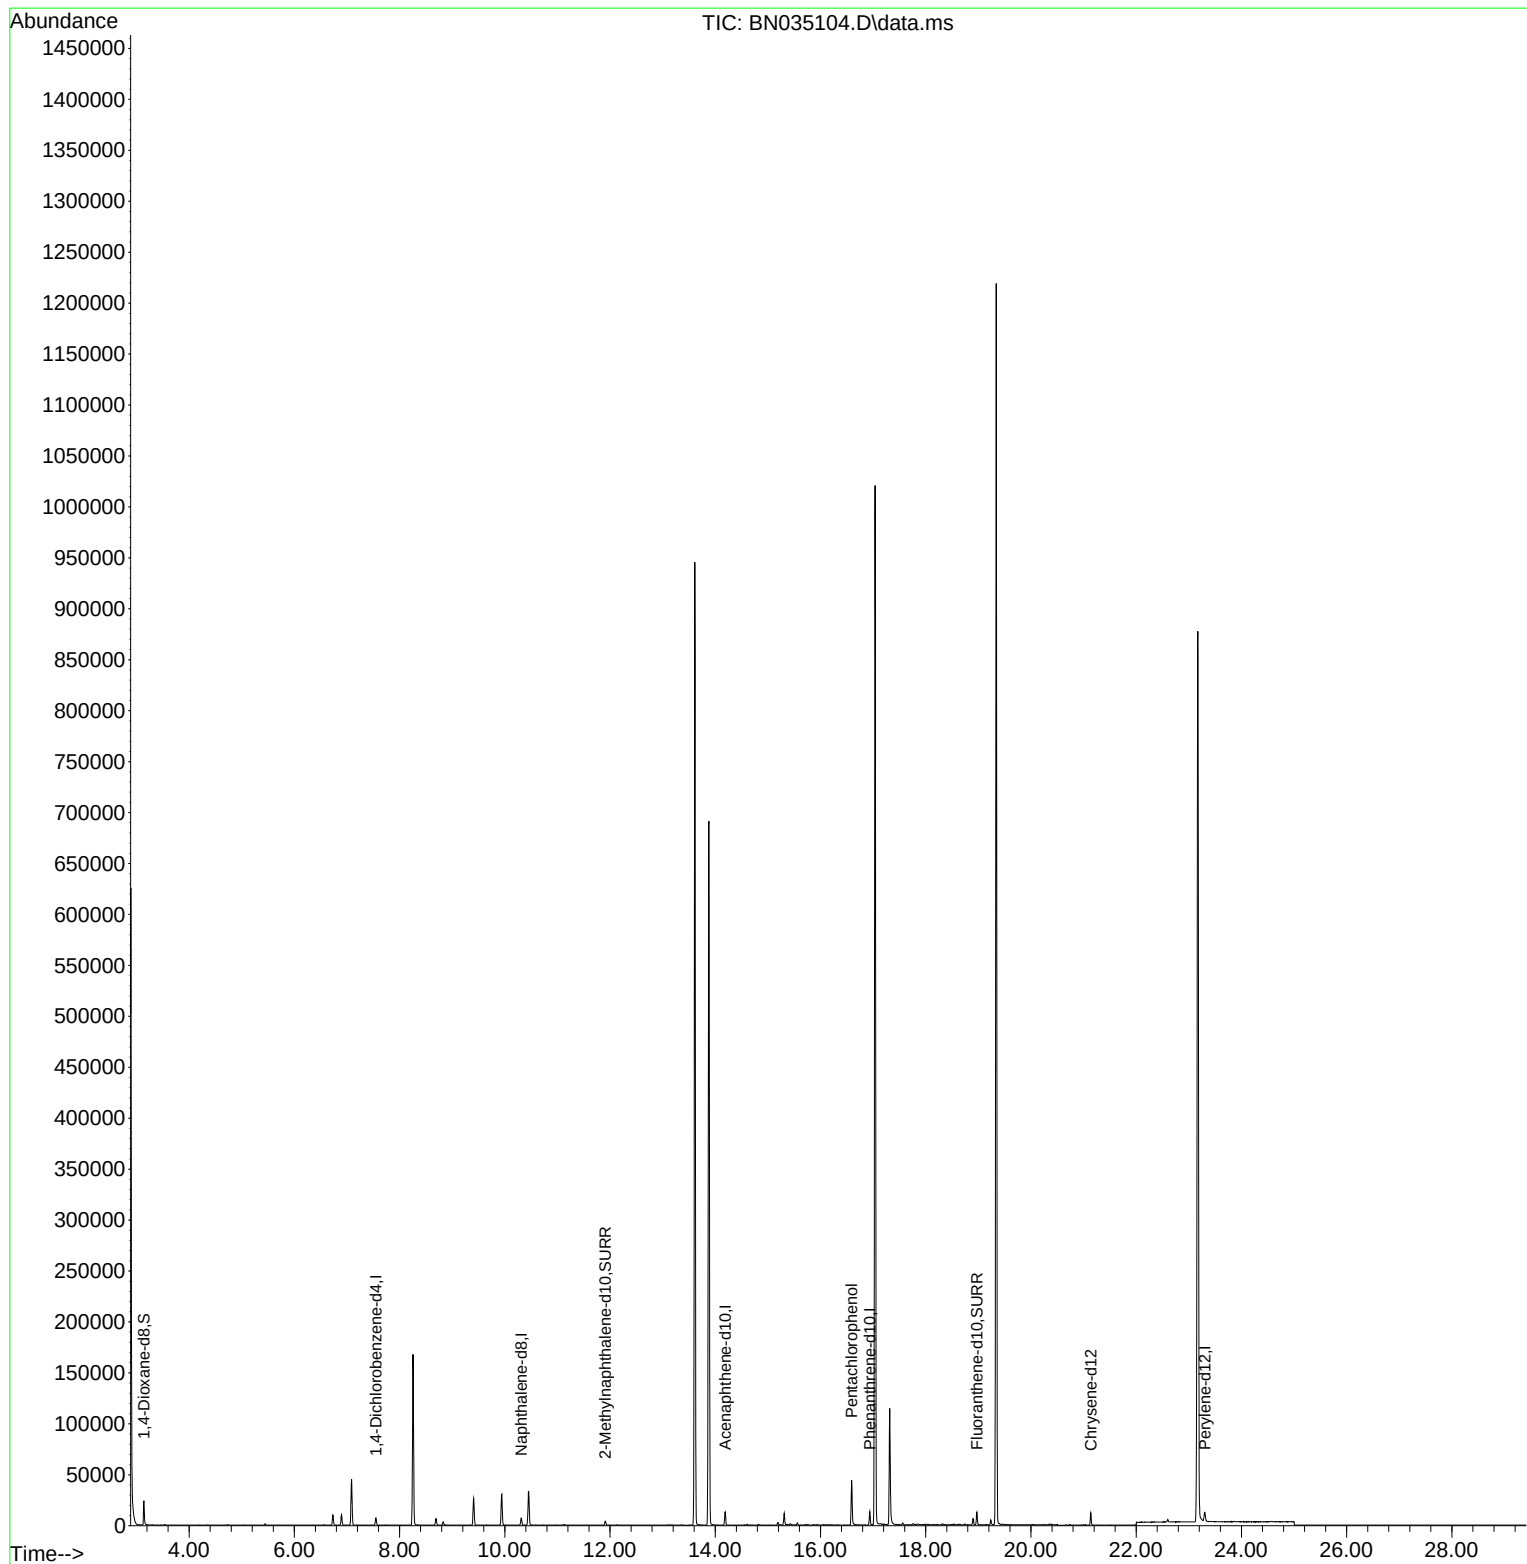

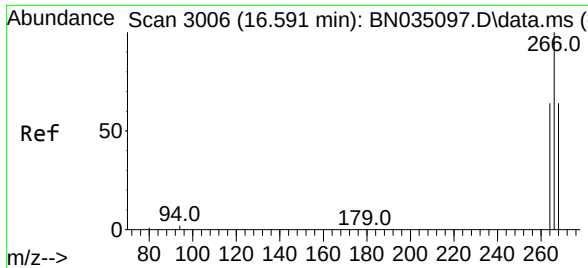

#14
Pentachlorophenol
Concen: 7.549 ng/ul
RT: 16.591 min Scan# 30
Delta R.T. -0.004 min
Lab File: BN035104.D
Acq: 15 Nov 2024 14:00

Instrument :
BNA_N
ClientSampleId :
COAM0

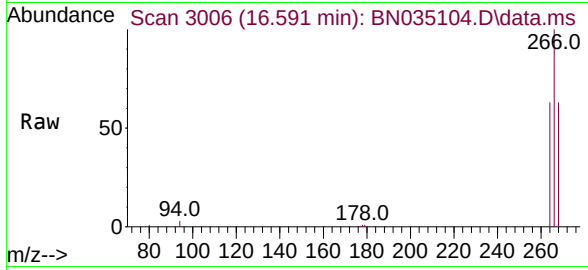

Tgt Ion:266 Resp: 2755
Ion Ratio Lower Upper
266 100
264 62.9 50.2 75.2
268 64.0 48.4 72.6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :mohammad ahmed 11/18/2024

