


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111818\
 Data File : BN003583.D
 Acq On : 19 Nov 2018 08:25
 Operator : MJ/SJ
 Sample : DFTPP53
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP53

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111418MA.M
 Title : SVOA CALIBRATION
 Last Update : Fri Nov 16 22:18:27 2018

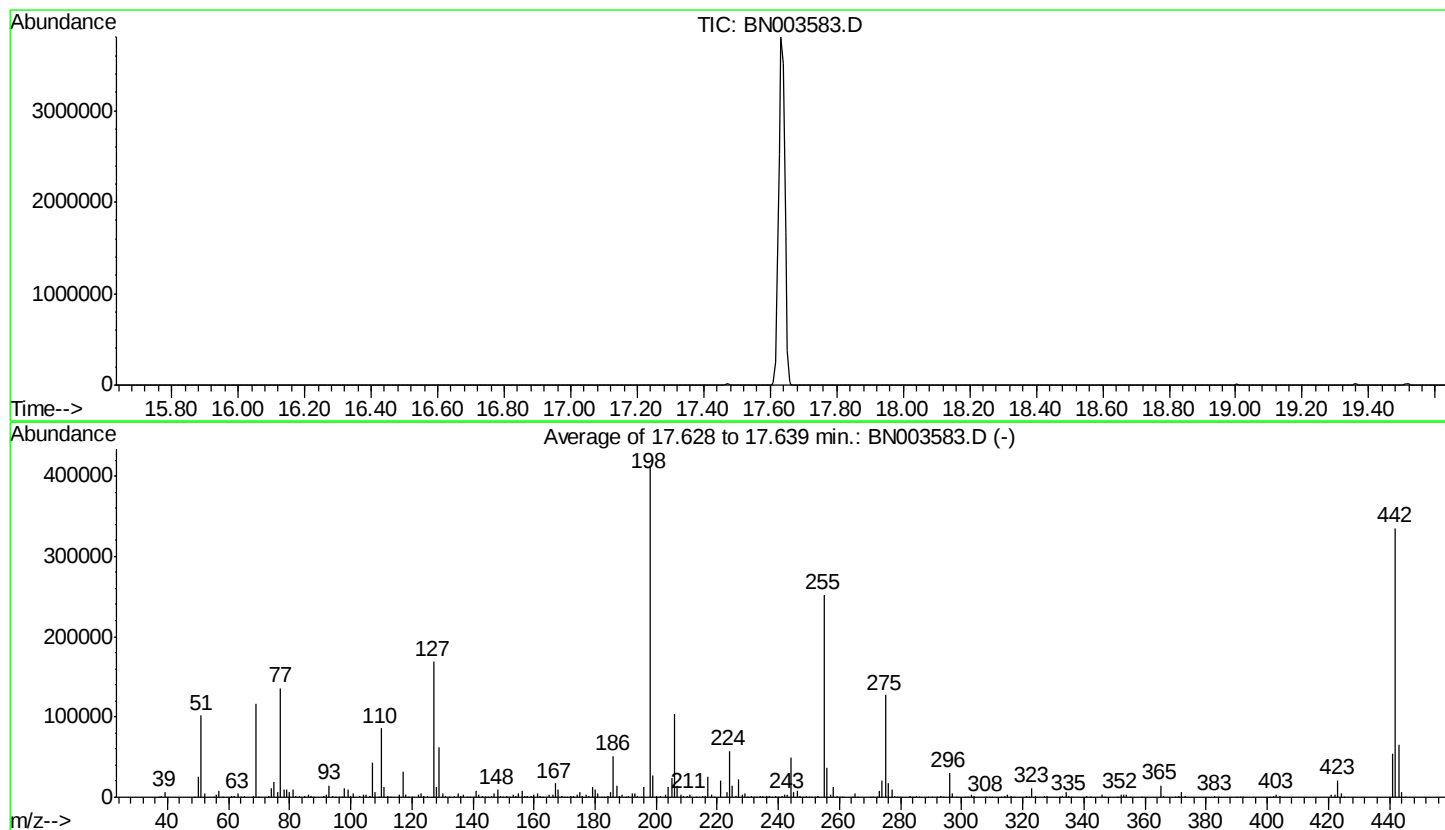

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	101853	PASS
68	69	0.00	2	1.9	2240	PASS
69	198	0.00	100	28.1	115906	PASS
70	69	0.00	2	0.5	611	PASS
127	198	10	80	40.8	168384	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	412970	PASS
199	198	5	9	6.8	27941	PASS
275	198	10	60	30.8	127069	PASS
365	198	1	100	3.5	14609	PASS
441	198	0.01	100	13.0	53858	PASS
442	198	50	100	81.2	335146	PASS
443	442	15	24	19.6	65624	PASS

m/z	Abundance
37.00	411.0
38.00	1036.0
39.00	6559.0
40.00	531.0
44.00	1187.0
49.00	779.0
50.00	23280.0
51.00	94472.0
52.00	4934.0
55.00	520.0
56.00	2910.0
57.00	6815.0
61.00	1292.0
62.00	1409.0
63.00	3936.0
64.00	626.0
65.00	2075.0
68.10	1964.0
69.00	105064.0
70.00	625.0
73.00	891.0
74.00	10457.0
75.00	17408.0
76.10	5889.0
77.00	122664.0
78.10	8473.0
79.00	8144.0
80.00	6221.0
81.00	8501.0
82.00	1944.0
83.00	2003.0
85.00	1620.0
86.00	2378.0
87.00	1203.0
88.00	426.0
91.00	1937.0
92.00	2266.0
93.00	13311.0
94.00	1006.0
96.00	492.0
97.00	309.0
98.00	10361.0
99.00	9132.0
100.00	881.0
101.00	4947.0
103.00	1860.0
104.00	3135.0
105.00	2678.0
106.10	942.0
107.00	37216.0
108.00	6143.0
110.00	73520.0
111.00	10956.0
112.00	1491.0
113.00	372.0
116.00	2321.0
117.00	28344.0
118.00	2291.0
120.00	535.0
122.00	2675.0
123.00	4116.0
124.00	1804.0
125.00	1625.0
127.00	145472.0
128.00	11031.0
129.00	53088.0
130.00	4850.0
131.00	829.0
132.00	474.0
134.00	1702.0
135.00	4226.0
136.00	1755.0
137.00	2467.0
138.00	513.0
139.00	307.0
140.00	678.0
141.00	6881.0
142.00	2473.0
143.00	1566.0
144.00	403.0
144.90	305.0
146.00	1341.0
147.00	3462.0
148.00	7638.0
149.00	1892.0
150.00	540.0
151.10	866.0
151.70	693.0
153.00	2278.0
154.00	1755.0
155.00	3945.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

156.00	6097.0
157.00	1153.0
157.90	1329.0
158.90	1041.0
160.00	2349.0
161.00	3313.0
162.00	969.0
164.00	363.0
165.00	2700.0
166.00	2170.0
167.00	14338.0
168.00	8526.0
169.00	1479.0
170.10	514.0
170.90	667.0
172.00	1234.0
173.00	1563.0
174.00	3082.0
175.00	5311.0
176.00	1905.0
177.00	2632.0
178.00	820.0
179.00	10404.0
180.00	7885.0
181.00	3365.0
181.90	561.0
182.90	329.0
184.00	755.0
185.00	5251.0
186.00	40672.0
187.00	12014.0
188.00	1458.0
189.00	2297.0
190.00	425.0
191.00	1257.0
192.00	3372.0
193.00	3559.0
194.00	809.0
195.10	487.0
196.00	9766.0
198.00	322496.0
199.00	22864.0
200.00	1635.0
201.50	1693.0
203.00	2005.0
204.00	10399.0
205.00	17928.0
206.10	80120.0
207.00	11581.0
208.00	2541.0
209.00	832.0
211.00	3005.0
215.00	824.0
216.00	1706.0
217.00	19448.0
218.00	2568.0
221.00	14972.0
223.00	4564.0
224.00	43648.0
225.00	11499.0
226.10	1441.0
227.00	16856.0
228.00	2387.0
229.00	3658.0
230.00	510.0
231.00	1683.0
232.00	363.0
233.00	312.0
234.00	1050.0
235.00	1414.0
236.00	777.0
237.00	1827.0
238.00	316.0
239.00	749.0
240.00	648.0
241.00	1128.0
242.00	2203.0
243.00	2616.0
244.00	36120.0
245.10	4689.0
246.00	6331.0
247.00	1265.0
248.00	317.0
249.00	1384.0
250.90	304.0
252.00	305.0
253.00	682.0
255.00	183872.0
256.00	27944.0
257.00	2403.0
258.00	9765.0
259.00	1783.0
265.00	3851.0
266.00	611.0
271.00	389.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

272.00	452.0
273.00	5786.0
274.00	14593.0
275.00	88920.0
276.00	12376.0
277.00	6808.0
278.00	1242.0
283.00	680.0
284.00	523.0
285.00	1292.0
289.00	331.0
291.90	333.0
293.00	1477.0
294.00	429.0
296.00	21984.0
297.00	3330.0
302.00	350.0
303.00	2465.0
304.00	761.0
308.00	352.0
310.00	332.0
314.00	1090.0
315.00	2363.0
316.00	1403.0
321.00	881.0
322.00	462.0
323.00	7378.0
324.00	1493.0
327.00	1458.0
328.00	750.0
332.00	518.0
333.00	729.0
334.00	4662.0
335.10	1402.0
341.10	904.0
346.00	1537.0
347.00	377.0
352.00	2201.0
353.00	1696.0
354.00	2380.0
355.00	505.0
365.00	9571.0
365.90	1468.0
371.00	586.0
372.00	3855.0
373.00	1039.0
383.00	1005.0
384.00	322.0
390.00	498.0
391.00	333.0
402.00	1298.0
403.00	2100.0
404.00	799.0
421.00	1647.0
422.10	1731.0
423.00	12256.0
424.10	3512.0
425.00	514.0
441.10	30288.0
442.10	192448.0
443.10	37664.0
444.00	3695.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

m/z	Abundance
37.00	387.0
38.00	1384.0
39.10	8183.0
40.00	547.0
44.00	1017.0
49.10	925.0
50.00	29744.0
51.00	116680.0
52.00	5758.0
54.90	661.0
56.00	3544.0
57.00	8254.0
57.90	422.0
61.00	1543.0
62.00	1815.0
63.00	5128.0
64.00	739.0
65.00	2510.0
68.10	2752.0
69.00	134656.0
70.00	669.0
73.00	1000.0
74.00	13682.0
75.00	21736.0
76.10	7884.0
77.10	158016.0
78.00	11129.0
79.00	10555.0
80.00	7921.0
81.00	10991.0
82.00	2747.0
83.00	2660.0
85.00	2082.0
86.00	3145.0
87.00	1478.0
88.00	521.0
91.00	2424.0
92.00	3078.0
93.00	17280.0
94.00	1228.0
95.10	301.0
96.10	876.0
97.10	378.0
98.00	13514.0
99.00	11370.0
100.00	1129.0
101.00	6284.0
103.00	2509.0
104.00	4128.0
105.00	3821.0
106.10	1260.0
107.00	51008.0
108.00	8145.0
109.10	1588.0
110.00	101312.0
111.00	14431.0
112.00	1730.0
113.00	538.0
116.00	2818.0
117.00	37304.0
118.00	3065.0
118.90	385.0
120.00	660.0
122.00	3523.0
123.00	5111.0
124.00	2412.0
125.00	2246.0
127.00	194240.0
128.00	14985.0
129.00	72824.0
130.00	6325.0
131.00	1116.0
132.10	593.0
134.00	2138.0
135.00	5960.0
136.00	2363.0
137.00	3143.0
137.90	743.0
138.90	469.0
140.00	923.0
141.00	9270.0
142.00	3327.0
143.00	2166.0
144.00	592.0
145.00	516.0
146.00	1847.0
147.00	4767.0
148.00	10513.0
149.00	2371.0
150.00	663.0
151.10	1463.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

151.80	960.0
153.00	3131.0
154.00	2508.0
155.00	5702.0
156.00	8628.0
157.00	1879.0
157.90	1931.0
159.00	1414.0
160.00	3090.0
161.00	4838.0
161.90	1290.0
162.90	390.0
164.00	572.0
165.00	3865.0
166.00	3248.0
167.00	20032.0
168.00	10414.0
169.00	1761.0
170.00	746.0
170.90	1021.0
172.00	1787.0
173.00	2421.0
174.00	4367.0
175.00	8072.0
176.00	2517.0
177.00	3631.0
178.00	1251.0
179.00	15344.0
180.00	11041.0
181.00	5336.0
182.00	844.0
183.00	573.0
184.00	1153.0
185.00	7381.0
186.00	60936.0
187.00	17368.0
188.00	1948.0
189.00	3611.0
190.00	575.0
191.00	1583.0
192.00	5245.0
193.00	5197.0
194.00	1147.0
196.00	14535.0
198.00	481792.0
199.00	33128.0
200.00	2334.0
201.40	2438.0
203.00	3063.0
204.00	15133.0
205.00	26904.0
206.00	122480.0
207.00	16448.0
208.00	3889.0
209.00	1220.0
210.30	2011.0
211.00	4812.0
213.00	330.0
215.00	1405.0
216.00	2708.0
217.00	30280.0
218.00	3984.0
219.00	448.0
221.00	24664.0
223.00	7005.0
224.00	68360.0
225.00	17760.0
226.00	2191.0
227.00	25416.0
228.00	3847.0
229.00	5618.0
230.00	804.0
231.00	2630.0
232.00	446.0
233.00	472.0
234.00	1726.0
235.00	2002.0
236.00	1248.0
237.00	2610.0
238.00	431.0
239.00	1048.0
240.00	824.0
241.00	1433.0
242.00	3804.0
243.00	4166.0
244.00	58680.0
245.00	8178.0
246.00	10042.0
247.00	2112.0
247.90	526.0
249.00	2224.0
249.90	374.0
251.00	407.0
252.00	577.0
253.00	1121.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

255.00	297280.0
256.00	44016.0
257.00	3454.0
258.00	14923.0
259.00	2593.0
260.00	433.0
261.00	557.0
264.10	530.0
265.00	6028.0
266.00	919.0
270.00	350.0
271.00	561.0
272.00	800.0
273.00	9829.0
274.00	24600.0
275.00	148416.0
276.00	20784.0
277.00	11016.0
278.00	1982.0
279.00	384.0
283.00	1296.0
284.10	938.0
285.00	2027.0
286.00	369.0
289.00	458.0
290.00	356.0
292.00	626.0
293.00	2628.0
294.00	692.0
296.00	35784.0
297.00	5173.0
298.00	317.0
301.00	541.0
302.00	682.0
303.00	4369.0
304.00	1263.0
308.00	616.0
308.90	431.0
310.00	565.0
312.90	377.0
314.00	1877.0
315.00	3983.0
316.00	2432.0
317.00	450.0
321.00	1322.0
322.00	772.0
323.00	12945.0
324.10	2446.0
327.00	2407.0
328.00	1296.0
331.90	914.0
333.00	1322.0
334.00	8208.0
335.00	2246.0
336.00	352.0
341.00	1477.0
342.00	443.0
346.00	2950.0
346.90	569.0
352.00	3881.0
353.00	2902.0
354.00	4605.0
355.10	911.0
365.00	16768.0
366.00	2479.0
370.00	304.0
371.00	1092.0
372.10	6822.0
373.00	1850.0
383.00	2013.0
384.00	633.0
390.00	953.0
391.00	625.0
392.00	530.0
401.00	423.0
402.00	2900.0
403.00	4196.0
404.00	1419.0
421.00	3473.0
422.00	3282.0
423.00	23896.0
424.10	6062.0
425.00	633.0
441.10	61568.0
442.00	368000.0
443.10	74024.0
444.10	7088.0
445.00	418.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

m/z	Abundance
36.90	343.0
38.10	1040.0
39.00	6709.0
40.00	480.0
44.00	1214.0
49.10	671.0
50.00	23680.0
51.00	94408.0
52.00	4677.0
55.00	494.0
56.00	2858.0
57.00	6807.0
58.00	302.0
61.00	1269.0
62.00	1479.0
63.00	4036.0
64.00	517.0
65.00	2187.0
68.10	2005.0
69.00	108000.0
70.00	539.0
73.00	1020.0
74.00	11142.0
75.00	17528.0
76.10	6154.0
77.10	128344.0
78.10	8630.0
79.00	8486.0
80.00	6210.0
81.00	8687.0
82.00	2077.0
83.00	2090.0
85.00	1726.0
86.00	2643.0
87.00	1255.0
88.00	439.0
91.00	2080.0
92.00	2316.0
93.00	14138.0
94.00	1070.0
96.00	638.0
97.00	351.0
98.00	11337.0
99.00	9081.0
100.00	892.0
101.00	5345.0
103.00	2005.0
104.00	3418.0
105.00	3153.0
106.10	1075.0
107.00	41264.0
108.00	6436.0
110.00	82896.0
111.00	12288.0
112.00	1351.0
112.90	480.0
116.00	2438.0
117.00	32144.0
118.00	2356.0
118.90	342.0
120.00	542.0
122.00	2969.0
123.00	4519.0
124.00	2117.0
125.00	1973.0
127.00	165440.0
128.00	12531.0
129.00	61424.0
130.00	4835.0
131.00	954.0
132.00	509.0
134.00	1832.0
135.00	5279.0
136.00	1967.0
137.00	2521.0
137.90	591.0
139.00	367.0
140.00	881.0
141.00	8073.0
142.00	2870.0
143.00	1865.0
144.00	478.0
145.00	485.0
146.00	1437.0
147.00	4582.0
148.00	9373.0
149.00	1858.0
150.00	564.0
151.20	960.0
151.70	772.0
153.00	2701.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

154.00	2007.0
155.00	4870.0
156.00	7321.0
157.10	1405.0
157.90	1595.0
159.00	1204.0
160.00	2609.0
161.00	4267.0
162.00	1265.0
164.00	512.0
165.00	3363.0
166.00	2624.0
167.00	17272.0
168.00	8859.0
169.00	1527.0
170.00	679.0
171.00	801.0
172.00	1662.0
173.00	2161.0
174.00	3891.0
175.00	7052.0
176.00	2283.0
177.00	3608.0
178.00	1044.0
179.00	13467.0
180.00	9435.0
181.00	4550.0
182.10	704.0
182.90	460.0
184.00	988.0
185.00	6351.0
186.00	53960.0
187.00	15259.0
188.00	1467.0
189.00	3342.0
190.00	581.0
191.00	1663.0
192.00	4260.0
193.00	4781.0
194.00	1043.0
195.10	697.0
196.00	12956.0
198.00	434624.0
199.00	27832.0
200.00	1998.0
201.40	2115.0
203.00	2711.0
204.00	13742.0
205.00	24672.0
206.00	110416.0
207.00	14069.0
208.00	3226.0
209.00	1141.0
210.30	1975.0
211.00	4227.0
215.00	1227.0
216.00	2115.0
217.00	27080.0
218.00	3301.0
219.00	304.0
221.00	21744.0
223.00	6628.0
224.00	61408.0
225.00	15982.0
226.10	1909.0
227.00	23424.0
228.00	3599.0
229.00	5224.0
230.00	798.0
231.00	2455.0
232.00	415.0
233.00	484.0
234.00	1642.0
235.00	1785.0
236.00	1191.0
237.00	2269.0
238.00	321.0
238.90	962.0
239.90	766.0
241.00	1385.0
242.00	3435.0
243.00	3805.0
244.00	53208.0
245.00	7048.0
246.00	9527.0
247.00	1759.0
248.00	506.0
249.00	2187.0
250.00	379.0
251.00	405.0
252.00	385.0
253.00	1107.0
255.00	275840.0
256.00	40000.0
257.00	3050.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

258.00	14469.0
259.00	2334.0
260.00	411.0
261.00	477.0
264.00	353.0
265.00	6124.0
266.00	890.0
269.90	316.0
270.90	553.0
272.00	814.0
273.00	8605.0
274.00	23472.0
275.00	143872.0
276.00	18976.0
277.00	10403.0
278.00	1715.0
278.90	350.0
283.00	1166.0
284.00	810.0
285.10	1912.0
286.00	302.0
288.90	472.0
290.00	306.0
291.90	501.0
293.00	2527.0
294.00	697.0
296.00	35296.0
297.00	4888.0
298.00	362.0
301.00	456.0
302.00	619.0
303.00	4513.0
304.00	1113.0
308.00	601.0
309.00	337.0
310.00	617.0
313.00	301.0
314.00	1844.0
315.00	4094.0
316.00	2359.0
317.00	435.0
321.00	1366.0
322.00	718.0
323.00	13364.0
324.00	2550.0
327.00	2378.0
328.00	1437.0
332.00	988.0
333.00	1276.0
334.00	8673.0
335.00	2113.0
341.00	1558.0
342.00	489.0
346.00	3021.0
347.00	590.0
351.00	318.0
352.00	4060.0
353.00	2958.0
354.10	4614.0
355.00	904.0
359.00	317.0
365.00	17488.0
366.00	2435.0
370.00	384.0
371.10	1161.0
372.00	7487.0
373.00	1859.0
383.00	1921.0
384.00	585.0
390.00	1021.0
391.00	742.0
392.00	585.0
401.00	461.0
402.00	2906.0
403.00	4484.0
404.00	1584.0
421.00	3594.0
422.10	3762.0
423.10	27064.0
424.10	6549.0
425.10	743.0
441.10	69720.0
442.10	444992.0
443.10	85184.0
444.10	7652.0
445.10	472.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53

m/z	Abundance
44.00	1458.0
207.00	382.0

Instrument :
BNA_N
ClientSampleId :
DFTPP53