
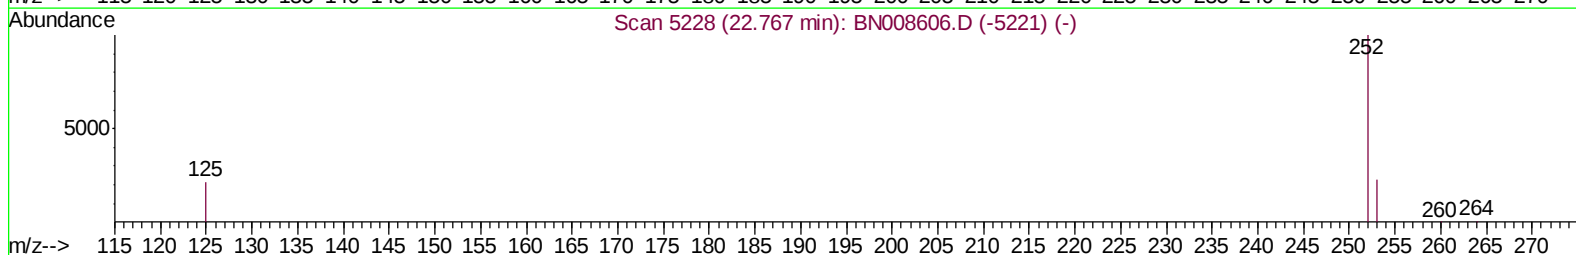
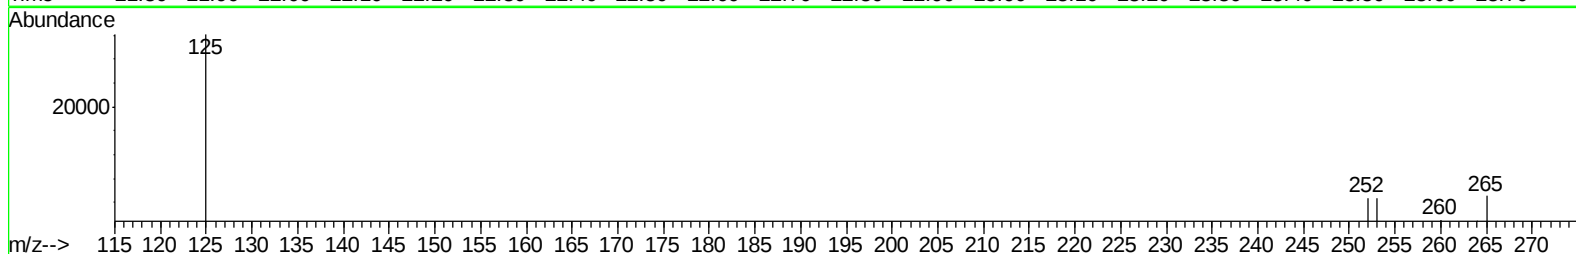


Data File : BN008609.D
Acq On : 18 Nov 2019 18:19
Operator : JU
Sample : K5678-05DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 19 01:51:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

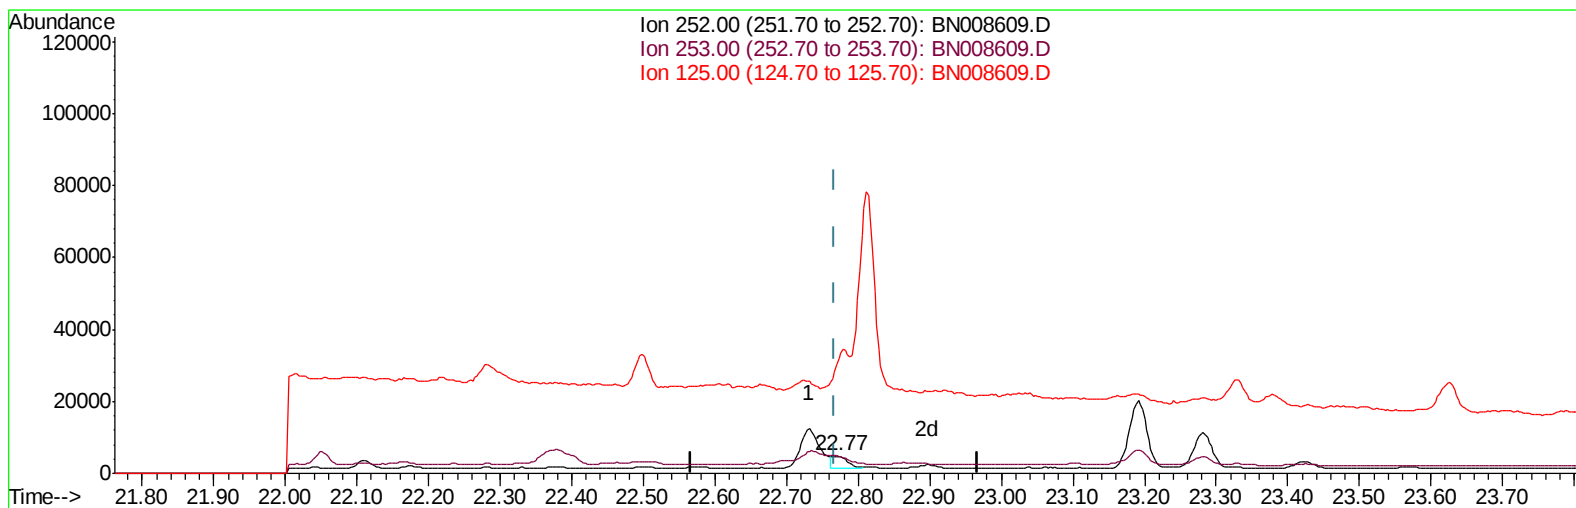

TIC: BN008609.D

(22) Benzo(k)fluoranthene

22.773min (+0.006) 0.08ng/ul m

response 4634

Ion	Exp%	Act%
252.00	100	100
253.00	25.60	97.11#
125.00	18.70	668.19#
0.00	0.00	0.00