
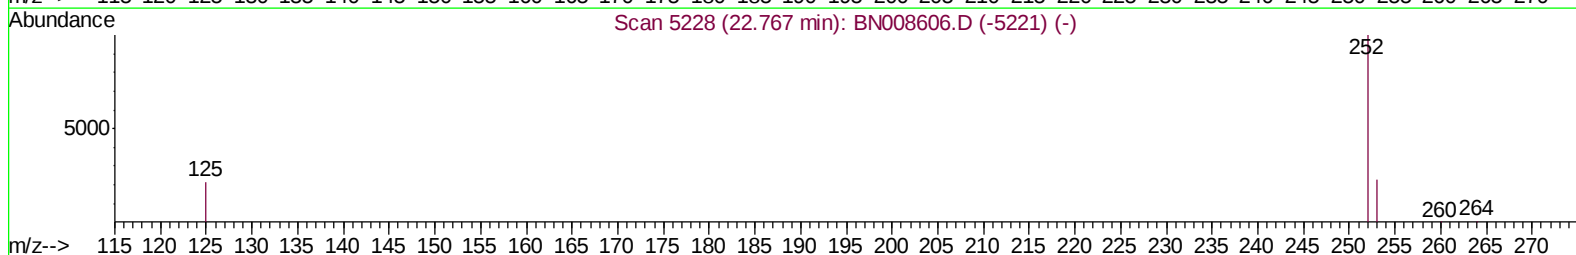
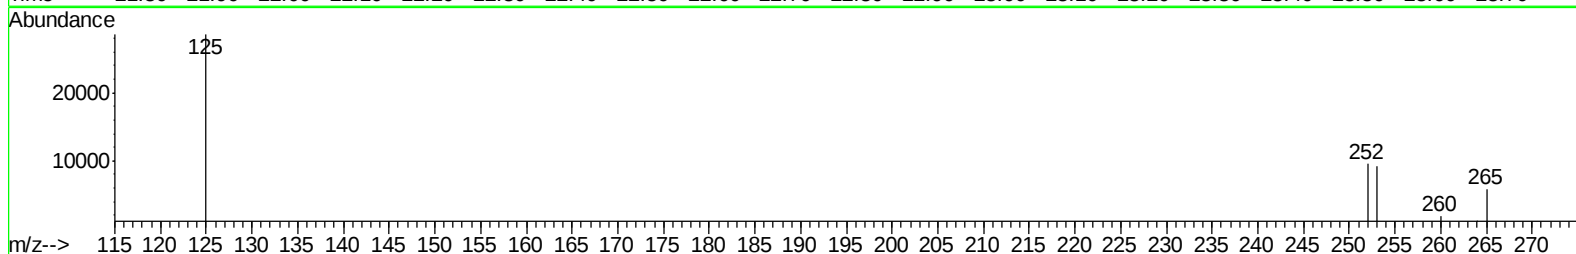


Data File : BN008610.D
Acq On : 18 Nov 2019 18:55
Operator : JU
Sample : K5678-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 19 01:51:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

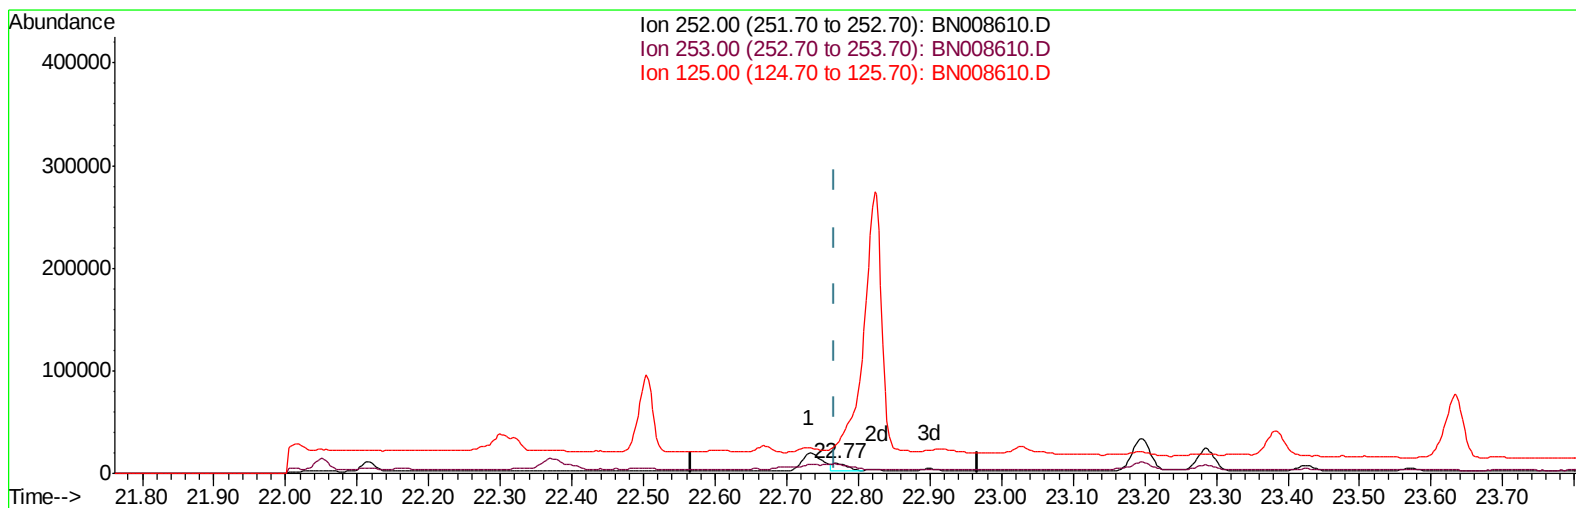

TIC: BN008610.D

(22) Benzo(k)fluoranthene

22.770min (+0.003) 0.29ng/ul m

response 11436

Ion	Exp%	Act%
252.00	100	100
253.00	25.60	97.20#
125.00	18.70	300.11#
0.00	0.00	0.00