
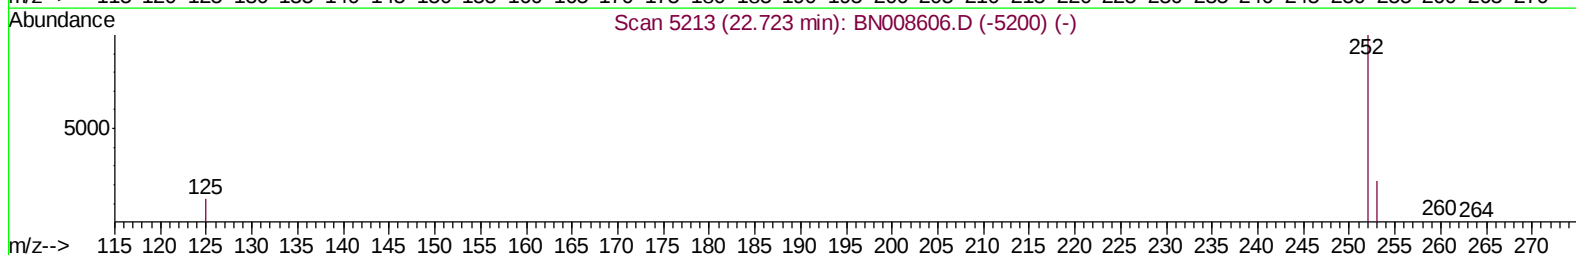
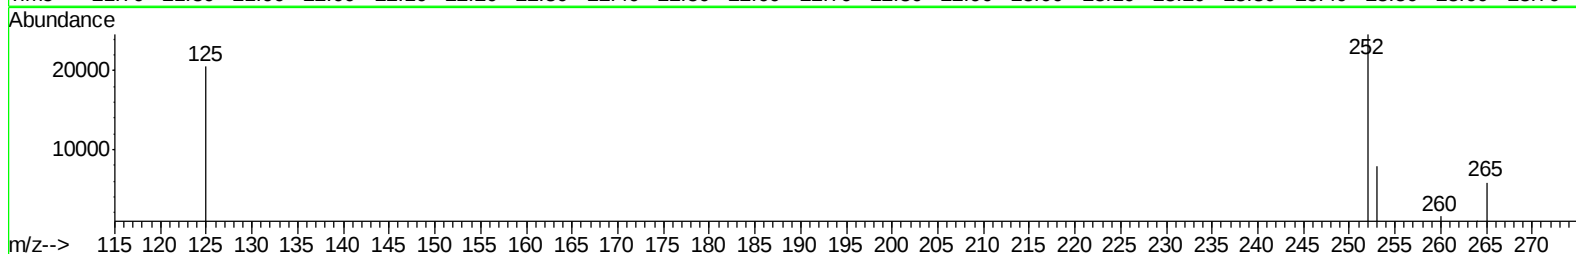


Data File : BN008613.D
Acq On : 18 Nov 2019 20:43
Operator : JU
Sample : K5678-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Nov 19 01:51:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 19 01:47:58 2019
Response via : Initial Calibration

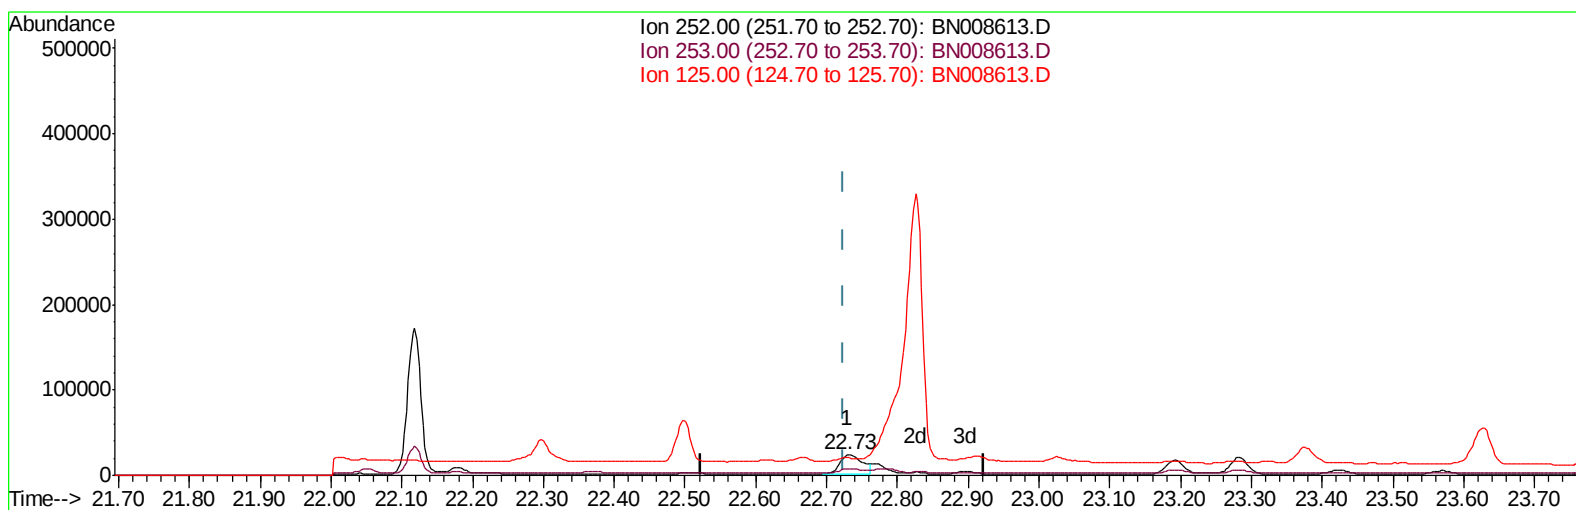

TIC: BN008613.D

(21) Benzo(b)fluoranthene

22.729min (+0.006) 1.21ng/ul m

response 51552

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	32.49
125.00	15.00	83.45#
0.00	0.00	0.00